

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083121\
 Data File : P0080864.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2021 10:00
 Operator : DD\AJ
 Sample : PB138783BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB138783BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:00:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 27 12:15:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.935	4.060	1811335	582751	22.071	21.624
2)	SA Decachlor...	11.000	9.423	1514420	621600	24.153	22.779
Target Compounds							
8)	L2 AR-1221-1	5.187	0.000	48368	0	52.109	N.D. #
9)	L2 AR-1221-2	5.291	4.394f	24887	3774	35.176	15.950 #
28)	L6 AR-1254-3	7.812f	0.000	91743	0	16.953	N.D. #
32)	L7 AR-1260-2	8.203f	7.112f	99218	29910	20.866	15.204 #
33)	L7 AR-1260-3	0.000	7.300	0	35228	N.D.	18.287 #
38)	L8 AR-1262-3	0.000	8.323	0	72670	N.D.	49.597 #
41)	L9 AR-1268-1	0.000	8.323	0	72670	N.D.	18.128 #
43)	L9 AR-1268-3	0.000	8.586	0	14802	N.D.	4.854 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083121\
Data File : PO080864.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2021 10:00
Operator : DD\AJ
Sample : PB138783BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
PB138783BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:00:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 27 12:15:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

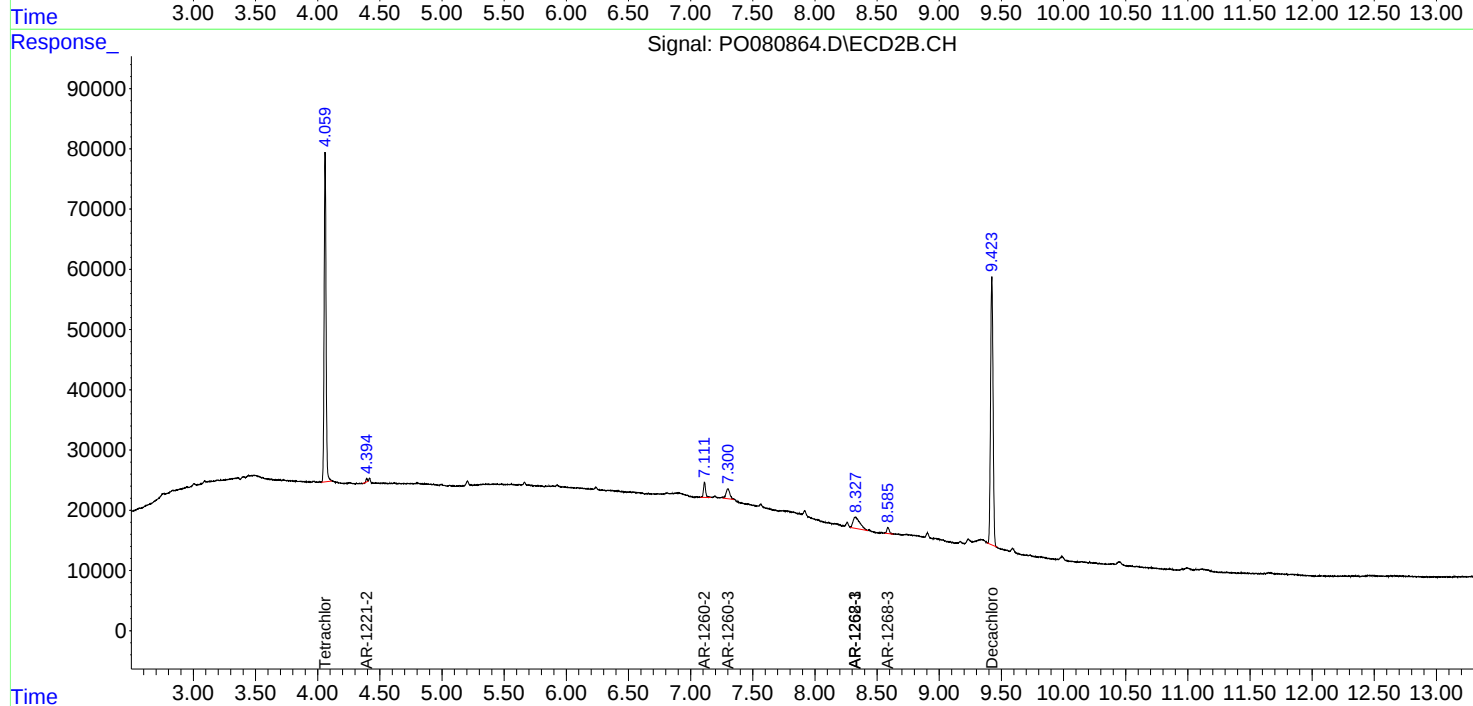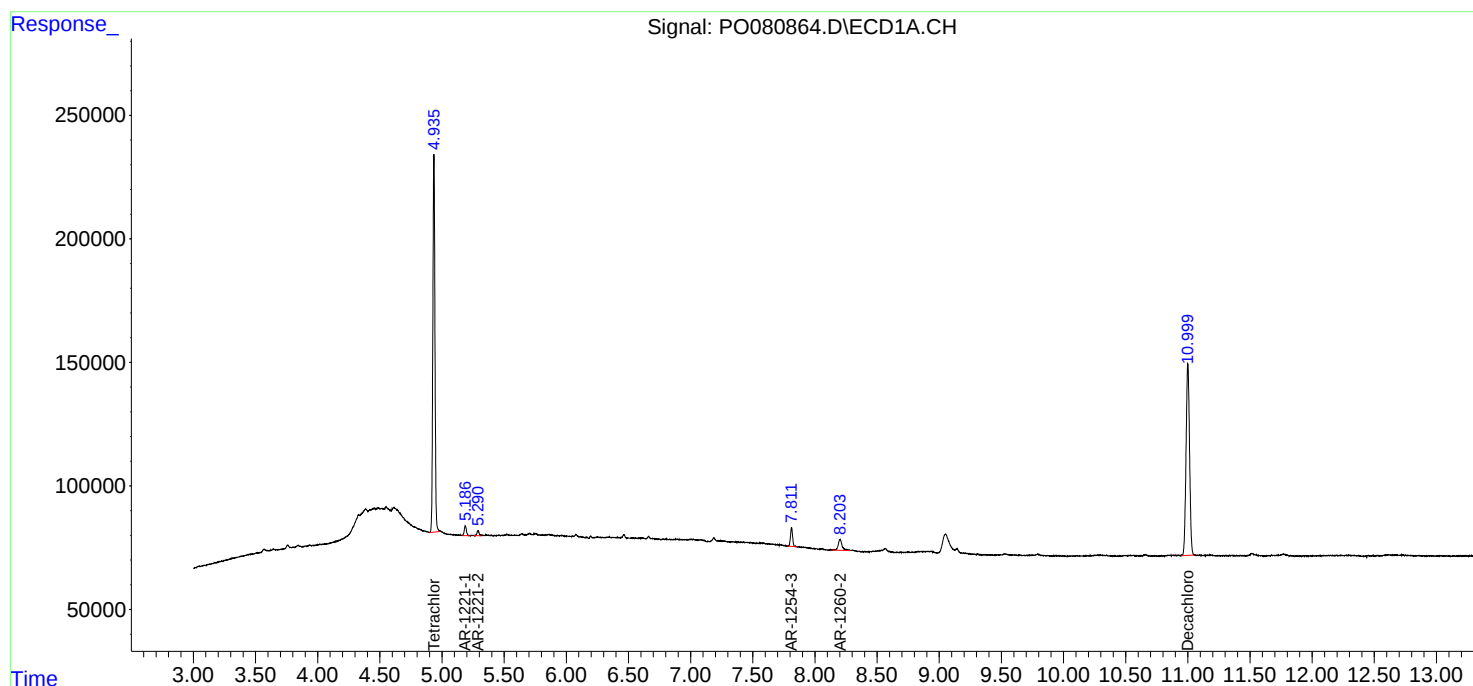


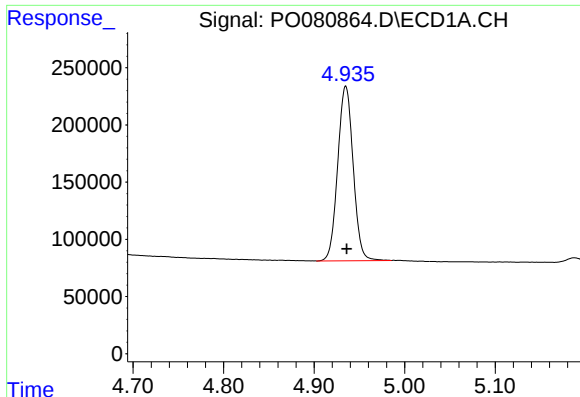

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: -0.001 min
Response: 1811335
Conc: 22.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB138783BL

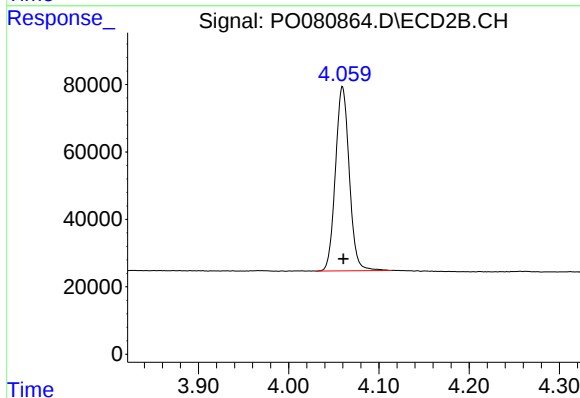


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.001 min
Response: 582751
Conc: 21.62 ng/ml

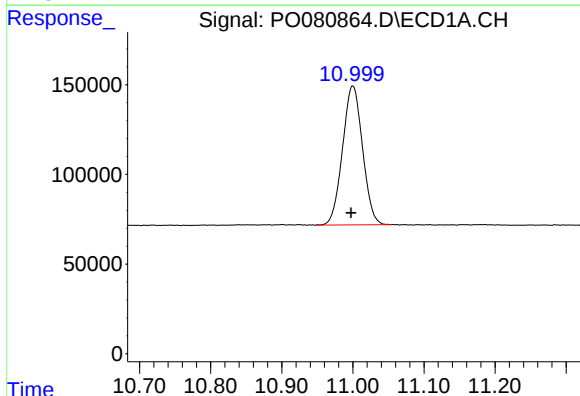


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.002 min
Response: 1514420
Conc: 24.15 ng/ml

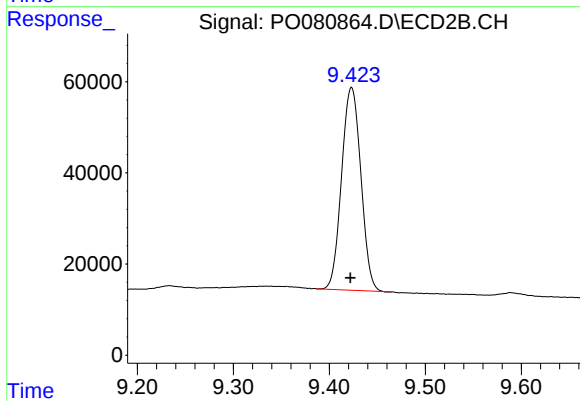

#2 Decachlorobiphenyl


R.T.: 9.423 min
Delta R.T.: 0.000 min
Response: 621600
Conc: 22.78 ng/ml

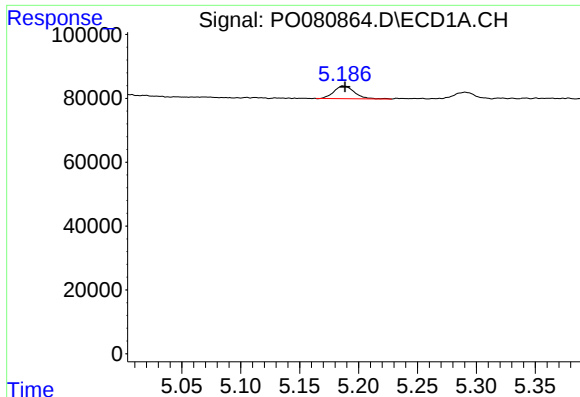

#8 AR-1221-1


R.T.: 5.187 min
Delta R.T.: -0.001 min
Response: 48368
Conc: 52.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB138783BL

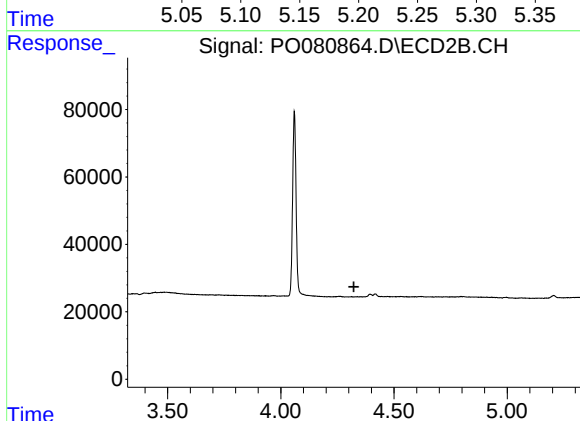


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.322 min
Response: 0
Conc: N.D.

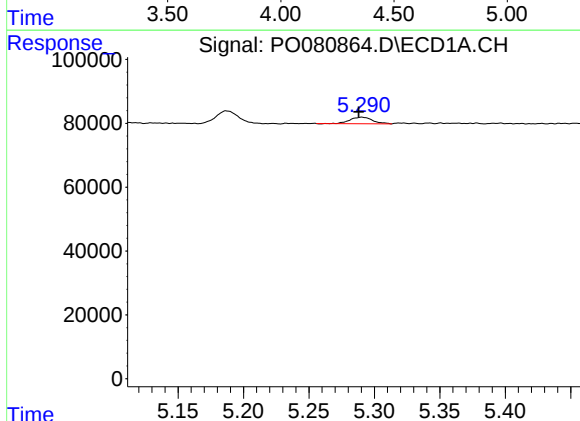


#9 AR-1221-2

R.T.: 5.291 min
Delta R.T.: 0.003 min
Response: 24887
Conc: 35.18 ng/ml

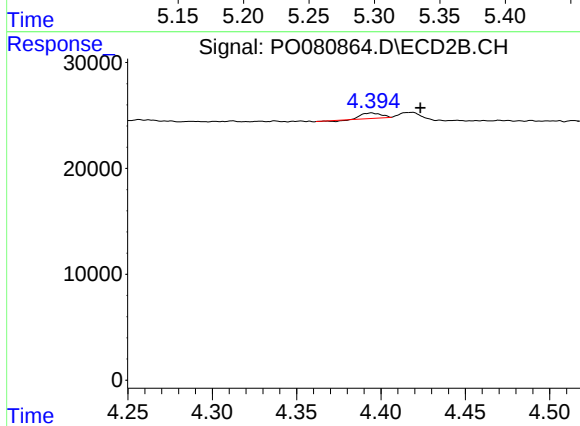

#9 AR-1221-2


R.T.: 4.394 min
Delta R.T.: -0.029 min
Response: 3774
Conc: 15.95 ng/ml

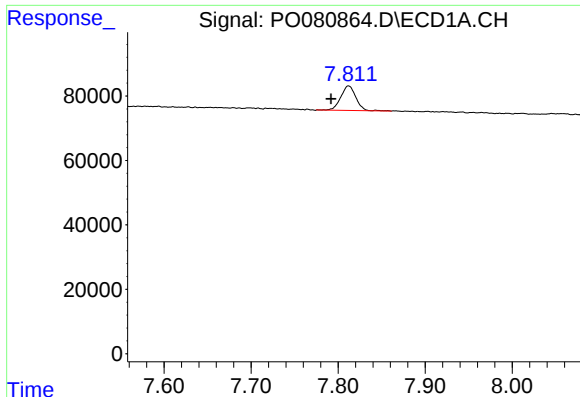

#28 AR-1254-3


R.T.: 7.812 min
Delta R.T.: 0.020 min
Response: 91743
Conc: 16.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB138783BL

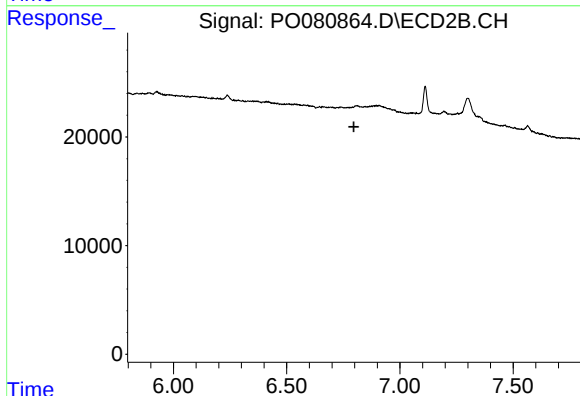


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.797 min
Response: 0
Conc: N.D.

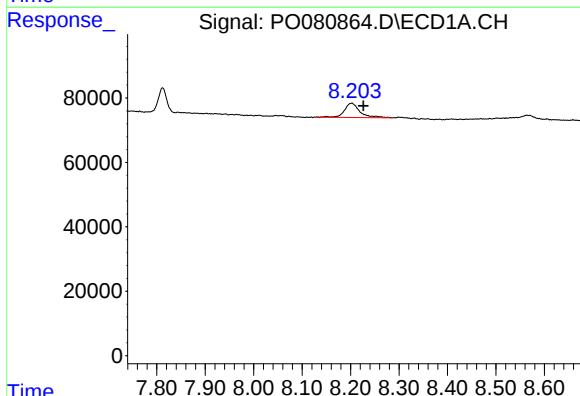


#32 AR-1260-2

R.T.: 8.203 min
Delta R.T.: -0.024 min
Response: 99218
Conc: 20.87 ng/ml

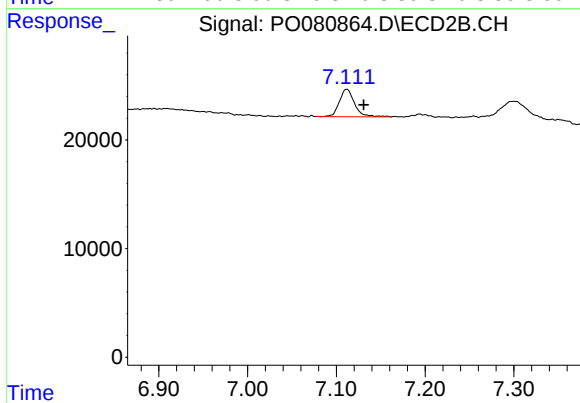

#32 AR-1260-2


R.T.: 7.112 min
Delta R.T.: -0.019 min
Response: 29910
Conc: 15.20 ng/ml

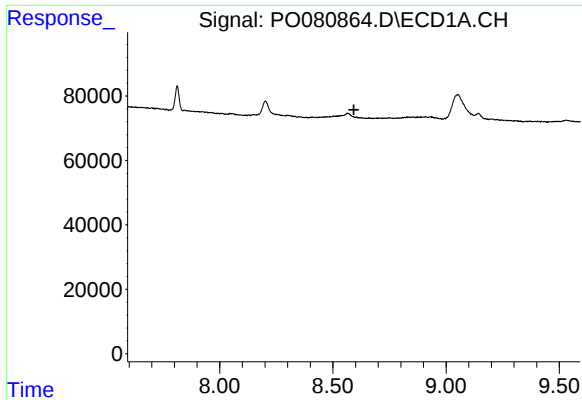

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.593 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB138783BL

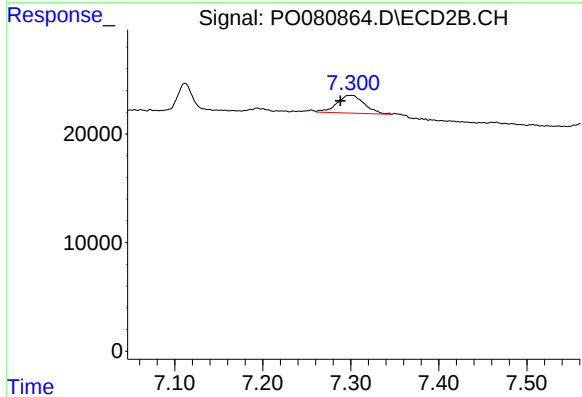


#33 AR-1260-3

R.T.: 7.300 min
Delta R.T.: 0.012 min
Response: 35228
Conc: 18.29 ng/ml

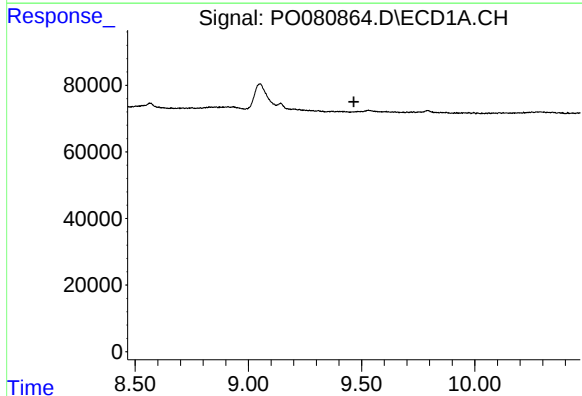


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.466 min
Response: 0
Conc: N.D.

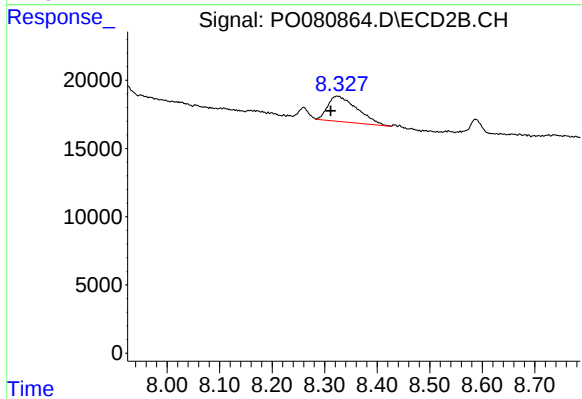

#38 AR-1262-3


R.T.: 8.323 min
Delta R.T.: 0.012 min
Response: 72670
Conc: 49.60 ng/ml

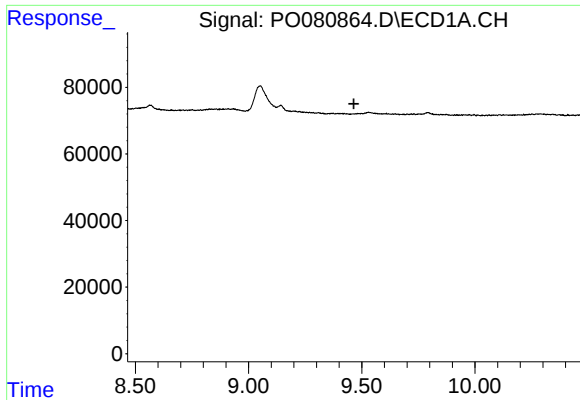

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB138783BL

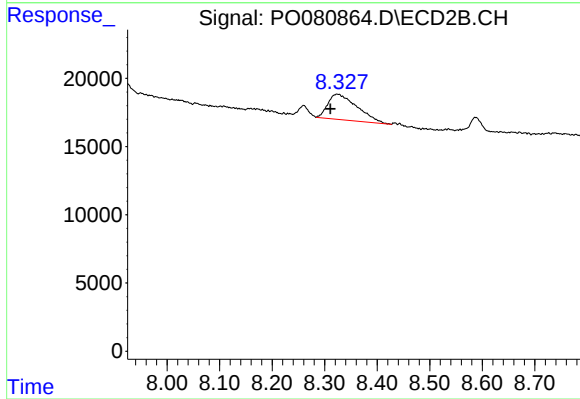


#41 AR-1268-1

R.T.: 8.323 min
Delta R.T.: 0.012 min
Response: 72670
Conc: 18.13 ng/ml

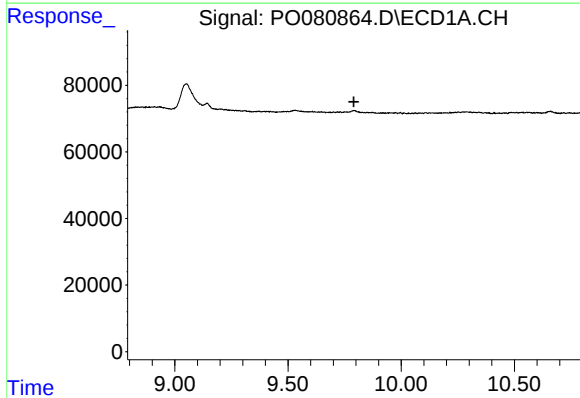

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.791 min
Response: 0
Conc: N.D.

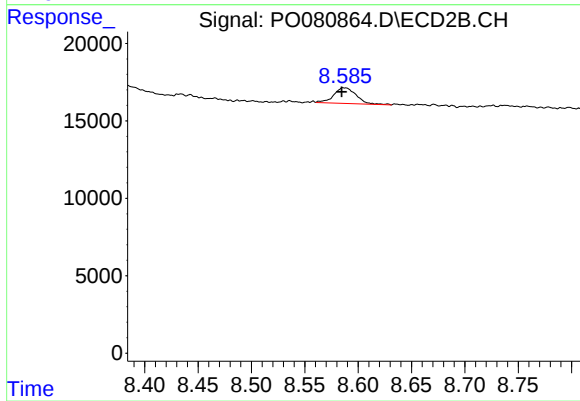

#43 AR-1268-3

R.T.: 8.586 min
Delta R.T.: 0.001 min
Response: 14802
Conc: 4.85 ng/ml