

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083121\
 Data File : P0080865.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Aug 2021 10:17
 Operator : DD\AJ
 Sample : M3569-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-2

Manual Integrations
 APPROVED

mohammad
 9/1/2021 4:28:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 03:48:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 27 12:15:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	4.061	2136148	685203	26.029	25.426
2) SA Decachlor...	11.001	9.425	1628173	661106	25.967	24.227

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083121\
Data File : PO080865.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Aug 2021 10:17
Operator : DD\AJ
Sample : M3569-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S-2


Manual Integrations
APPROVED

mohammad
9/1/2021 4:28:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 03:48:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 27 12:15:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

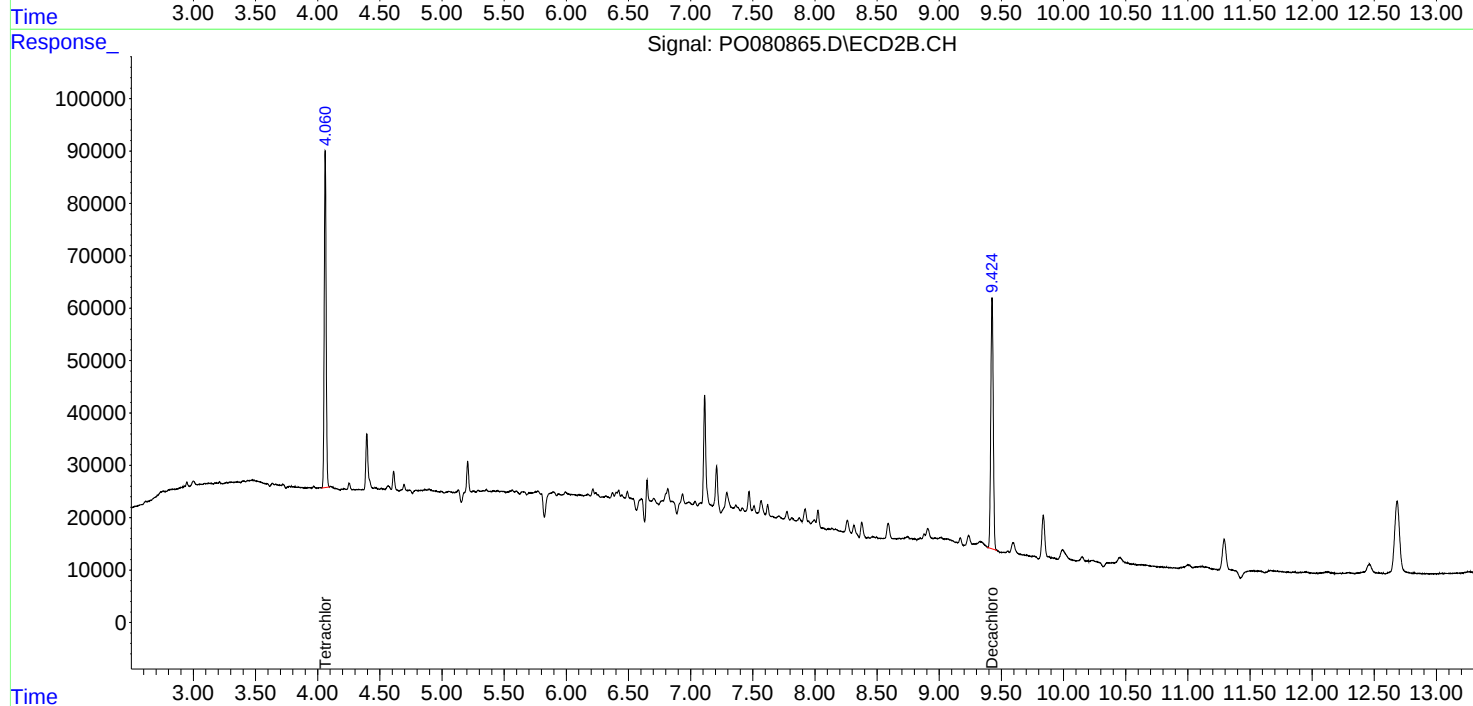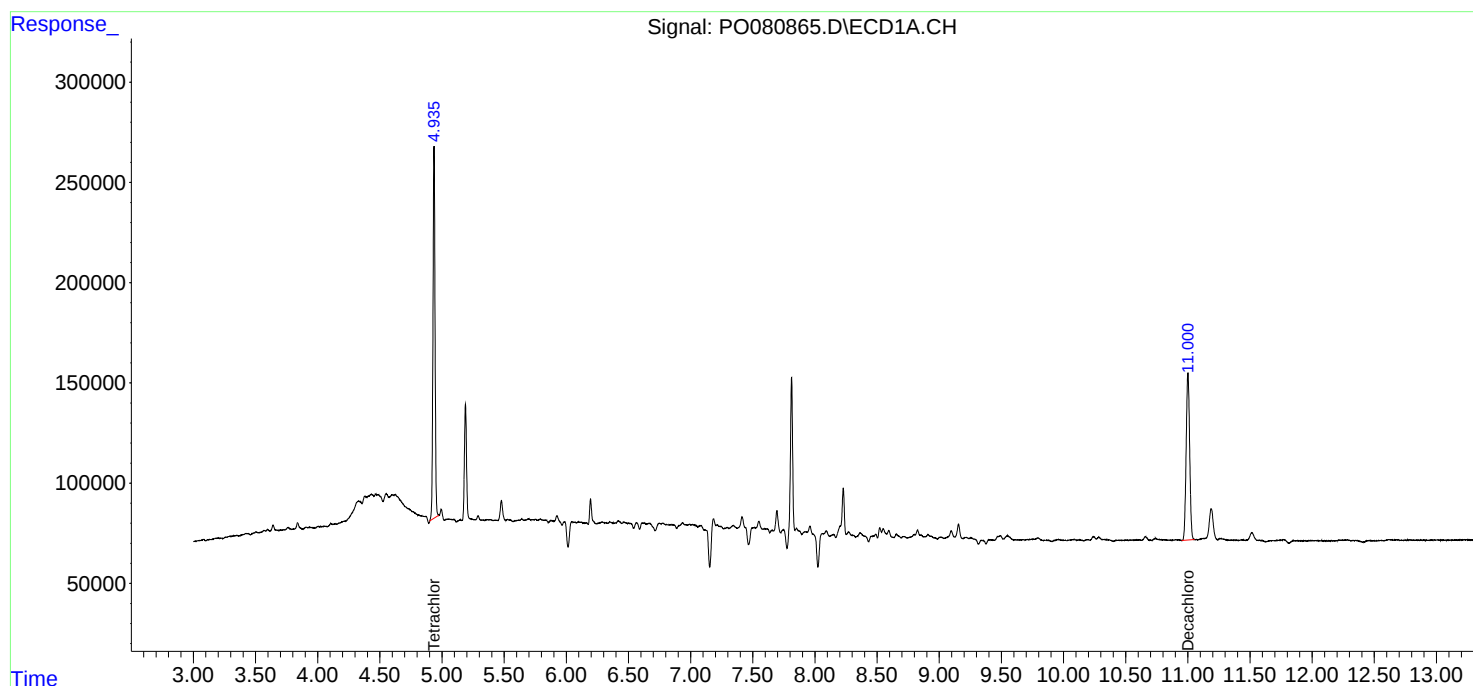

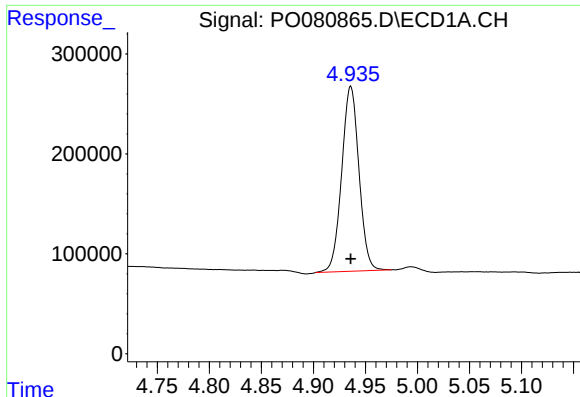


#1 Tetrachloro-m-xylene

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 2136148
Conc: 26.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-2


Manual Integrations
APPROVED

mohammad
9/1/2021 4:28:11 PM

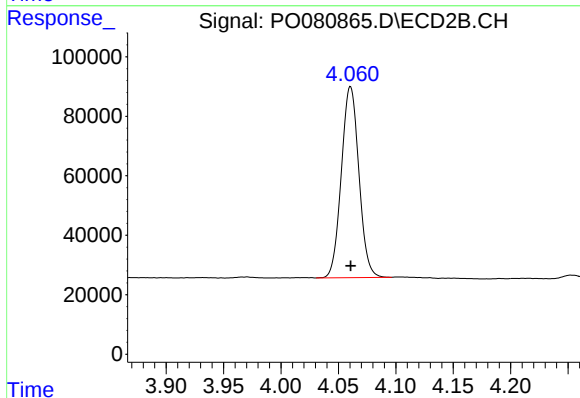


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 685203
Conc: 25.43 ng/ml

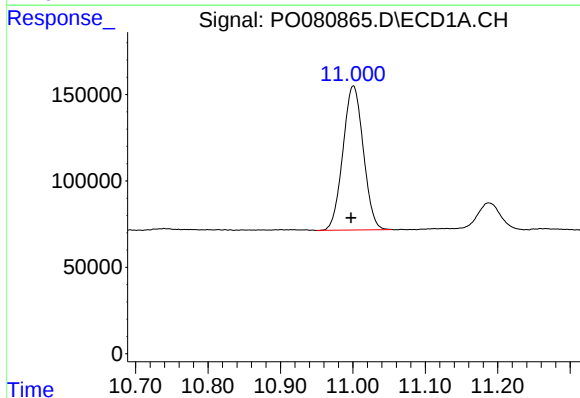

#2 Decachlorobiphenyl

R.T.: 11.001 min
Delta R.T.: 0.003 min
Response: 1628173
Conc: 25.97 ng/ml

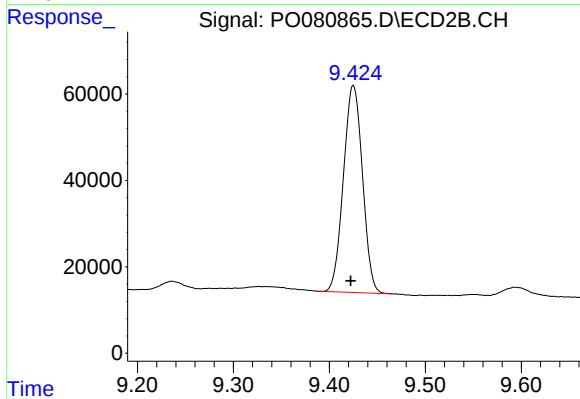

#2 Decachlorobiphenyl

R.T.: 9.425 min
Delta R.T.: 0.003 min
Response: 661106
Conc: 24.23 ng/ml