

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0083122\
 Data File : P0089196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2022 22:55
 Operator : YP/AJ
 Sample : N4427-01 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 D-171

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/01/2022
 Supervised By :Ankita Jodhani 09/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:22:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 29 17:48:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.430	3.588	3096216	1225773	0.826	1.270m#
2) SA Decachlor...	10.253	8.571	3117428	1089104	1.354	1.232

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO083122\
Data File : PO089196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2022 22:55
Operator : YP/AJ
Sample : N4427-01 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
D-171


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/01/2022
Supervised By :Ankita Jodhani 09/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:22:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082922.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 29 17:48:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

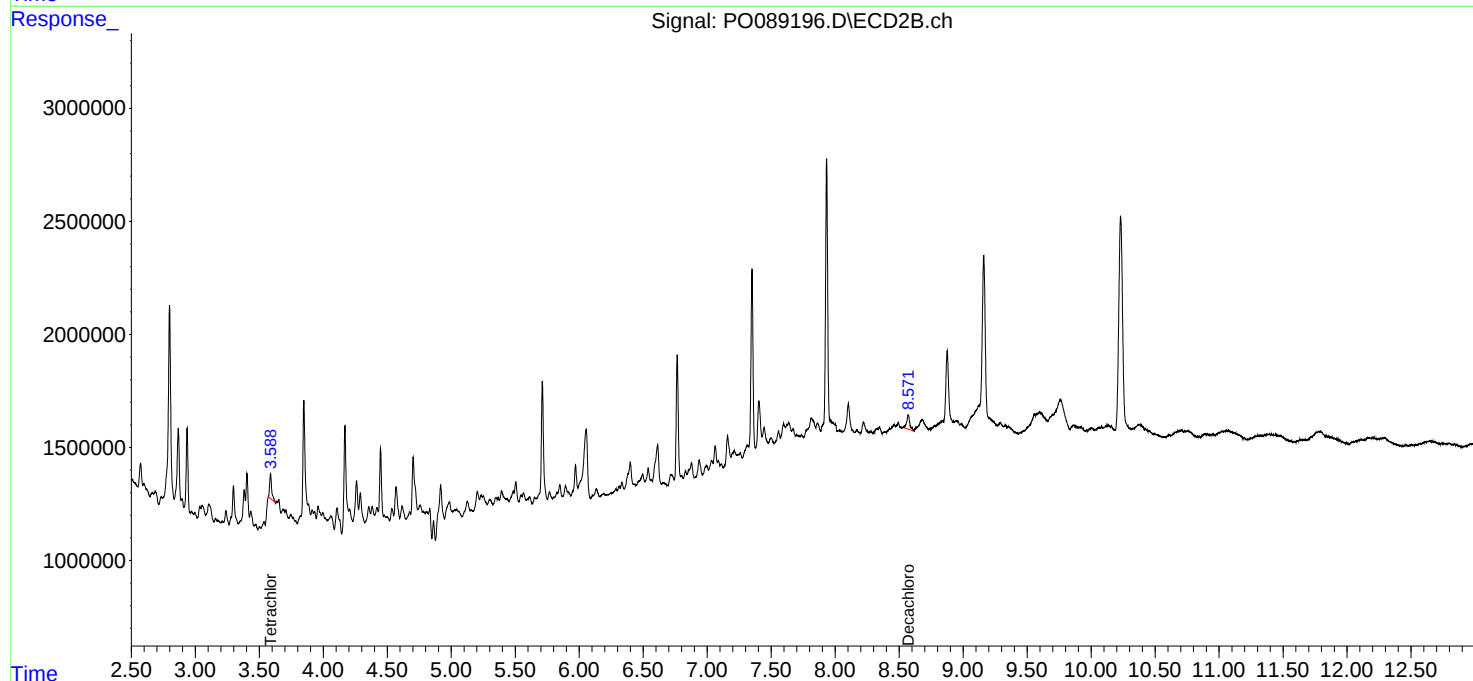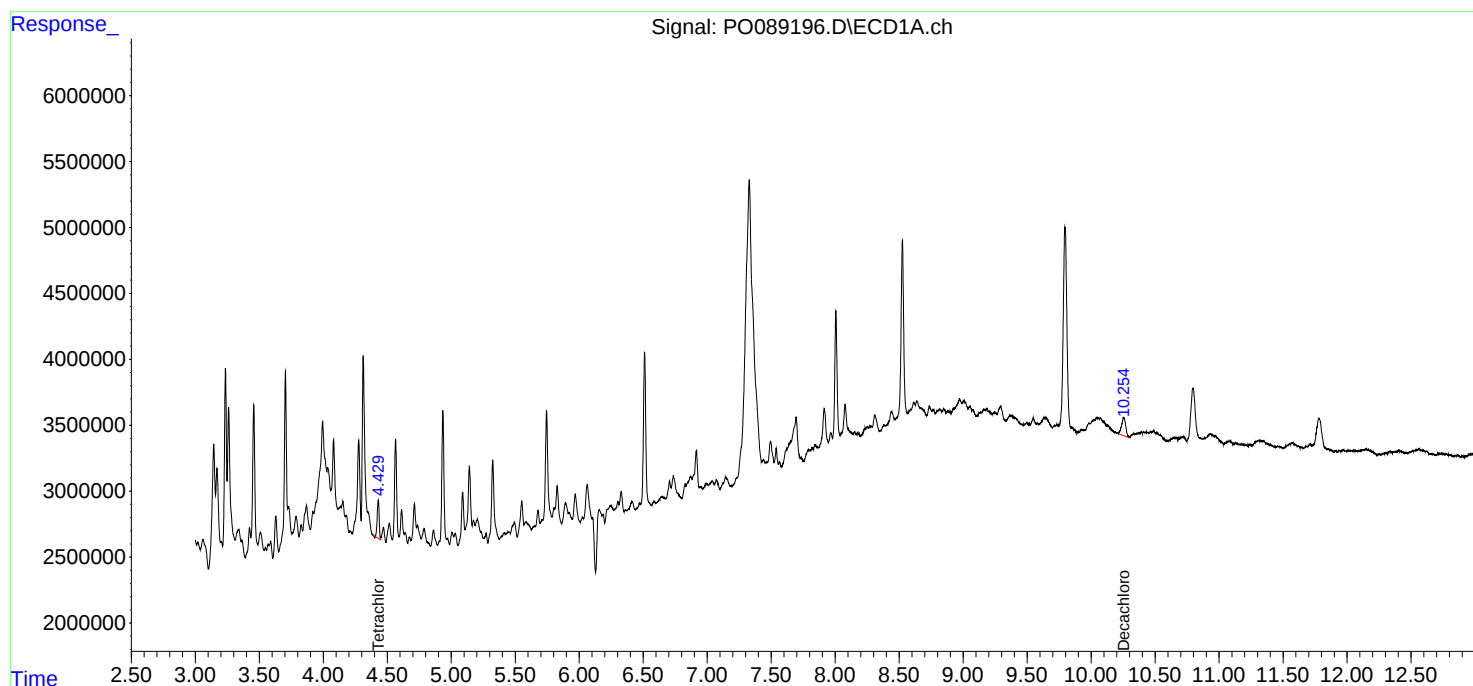

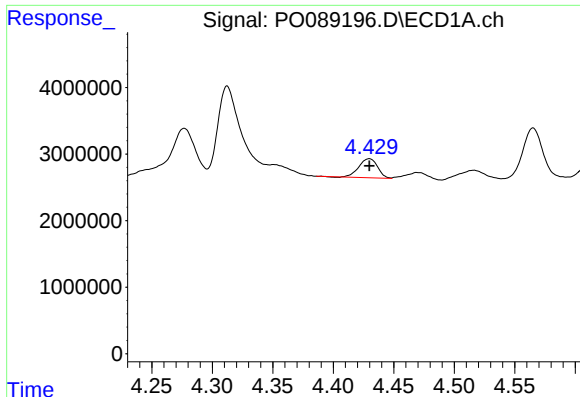


#1 Tetrachloro-m-xylene

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 3096216
Conc: 0.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
D-171


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/01/2022
Supervised By :Ankita Jodhani 09/01/2022

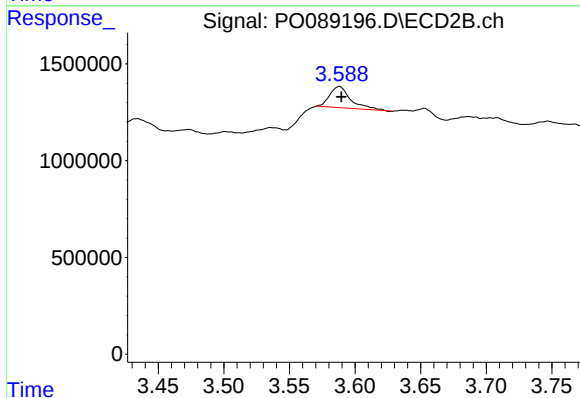


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.002 min
Response: 1225773
Conc: 1.27 ng/ml m

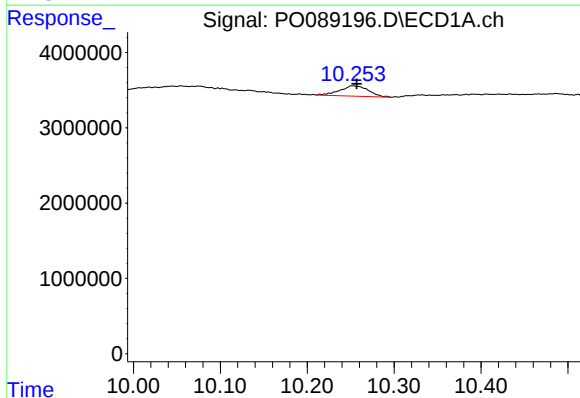

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: -0.004 min
Response: 3117428
Conc: 1.35 ng/ml

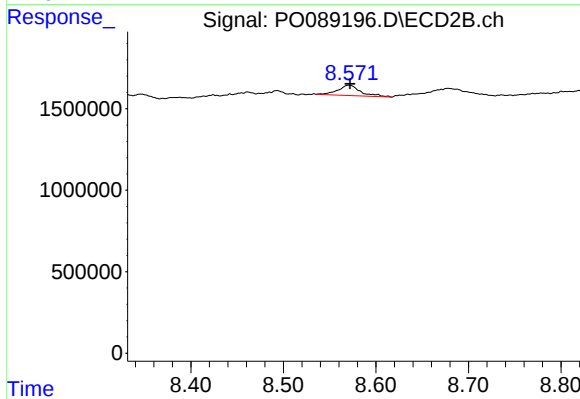

#2 Decachlorobiphenyl

R.T.: 8.571 min
Delta R.T.: 0.000 min
Response: 1089104
Conc: 1.23 ng/ml