

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090120\
 Data File : P0071076.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Sep 2020 15:13
 Operator : DD\AJ
 Sample : L3849-05RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 16:48:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.538	2272848	1326284	29.430	29.918
2) SA Decachlor...	9.969	8.719	2495803	1412719	27.276	24.595
Target Compounds						
24) L5 AR-1248-4	6.563f	0.000	62754	0	17.112	N.D. #
26) L6 AR-1254-1	6.563	0.000	62754	0	17.285	N.D. #
27) L6 AR-1254-2	6.785	0.000	199579	0	35.477	N.D. #
28) L6 AR-1254-3	7.170f	6.211f	38611	67690	6.705	16.871 #
32) L7 AR-1260-2	7.588	0.000	196260	0	29.471	N.D. #
33) L7 AR-1260-3	7.968f	0.000	988215	0	177.431	N.D. #
34) L7 AR-1260-4	8.157	0.000	32234	0	6.084	N.D. #
36) L8 AR-1262-1	7.968f	0.000	988215	0	123.899	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090120\
Data File : PO071076.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Sep 2020 15:13
Operator : DD\AJ
Sample : L3849-05RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 16:48:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

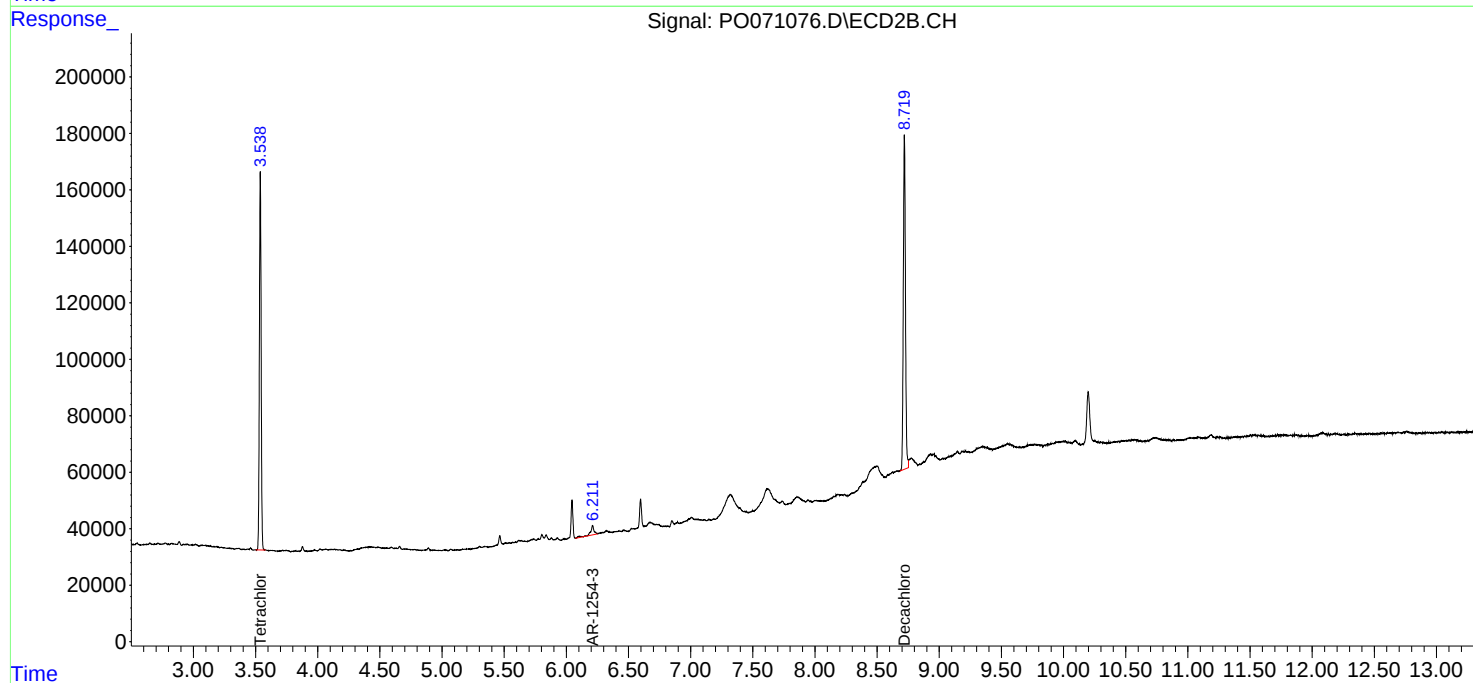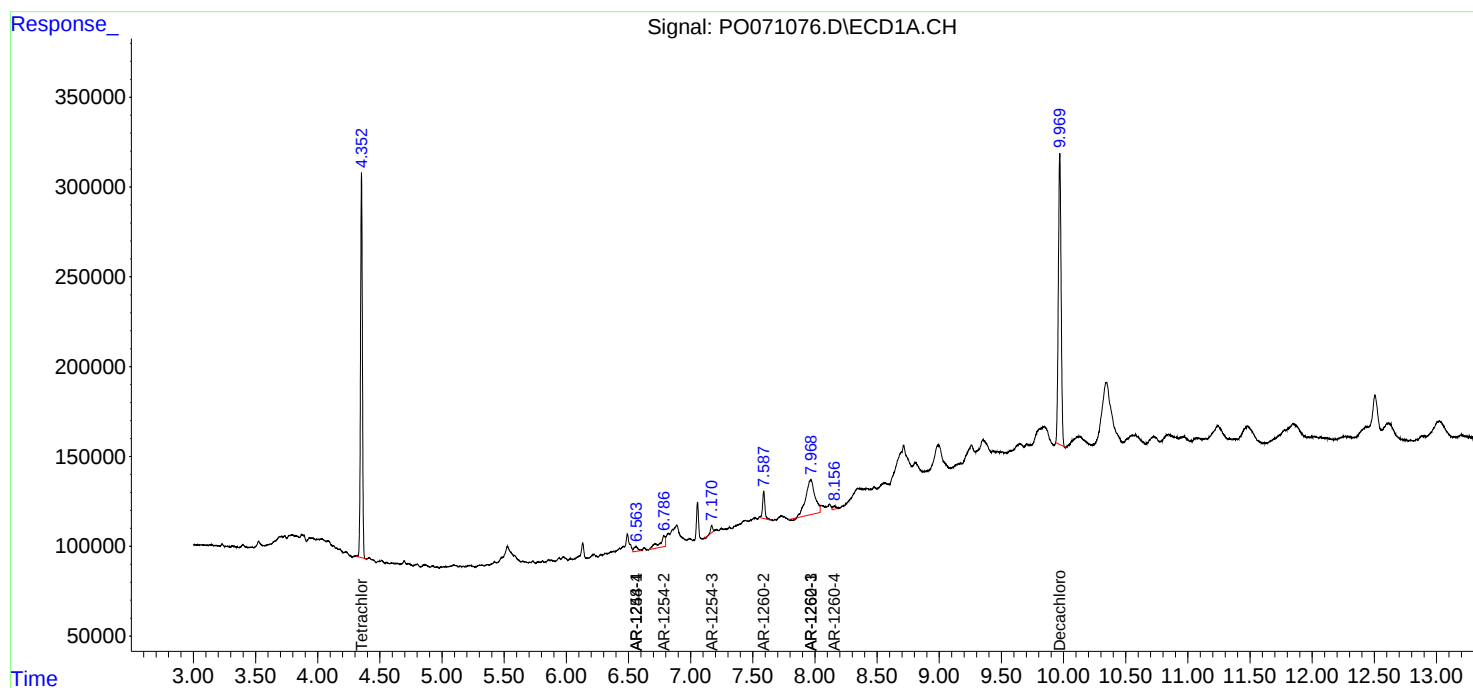


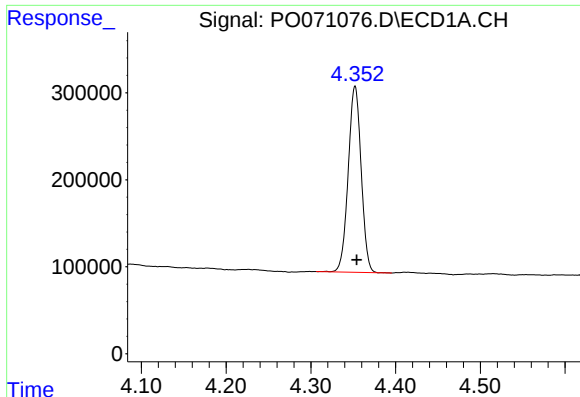

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: -0.002 min
Response: 2272848
Conc: 29.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

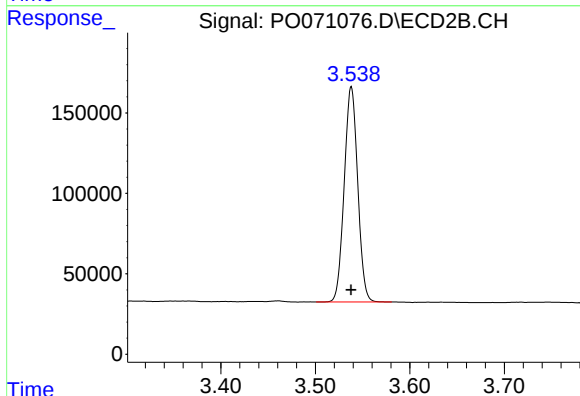


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 1326284
Conc: 29.92 ng/ml

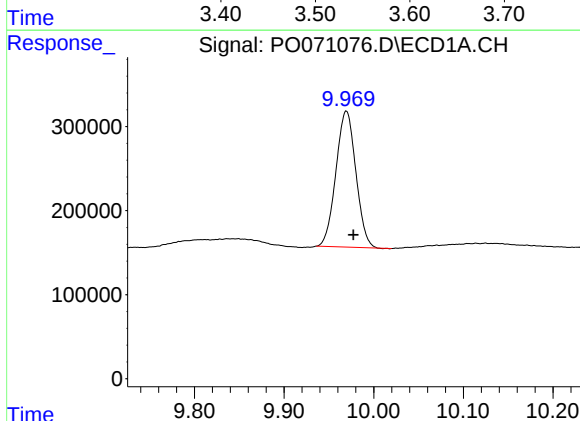


#2 Decachlorobiphenyl

R.T.: 9.969 min
Delta R.T.: -0.008 min
Response: 2495803
Conc: 27.28 ng/ml

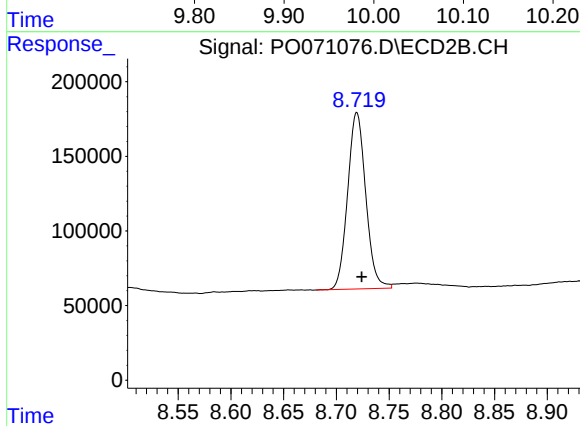

#2 Decachlorobiphenyl


R.T.: 8.719 min
Delta R.T.: -0.005 min
Response: 1412719
Conc: 24.60 ng/ml

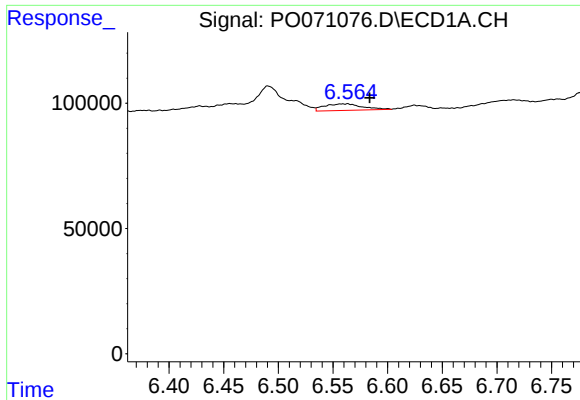

#24 AR-1248-4


R.T.: 6.563 min
Delta R.T.: -0.021 min
Response: 62754
Conc: 17.11 ng/ml

Instrument :
ECD_O
ClientSampleId :

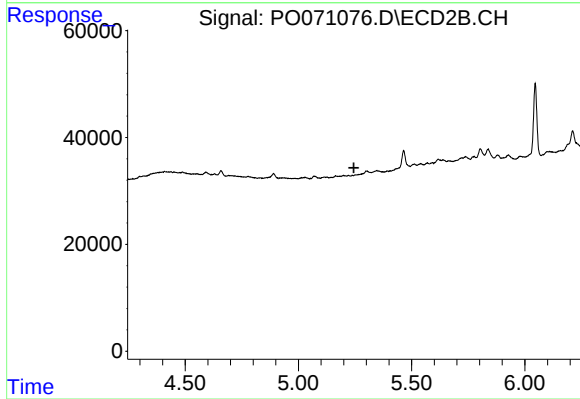


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.245 min
Response: 0
Conc: N.D.

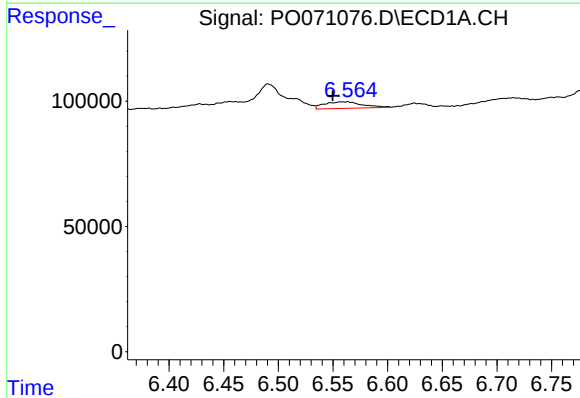


#26 AR-1254-1

R.T.: 6.563 min
Delta R.T.: 0.013 min
Response: 62754
Conc: 17.29 ng/ml

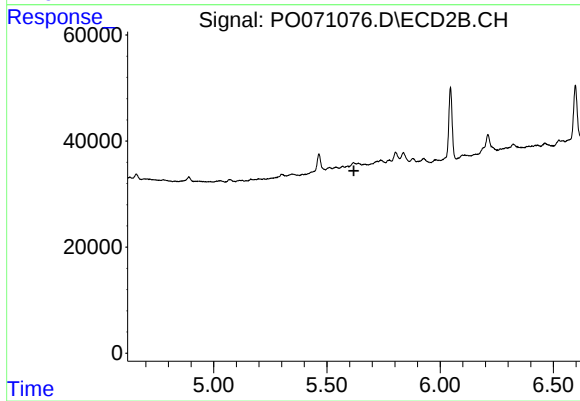

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.619 min
Response: 0
Conc: N.D.

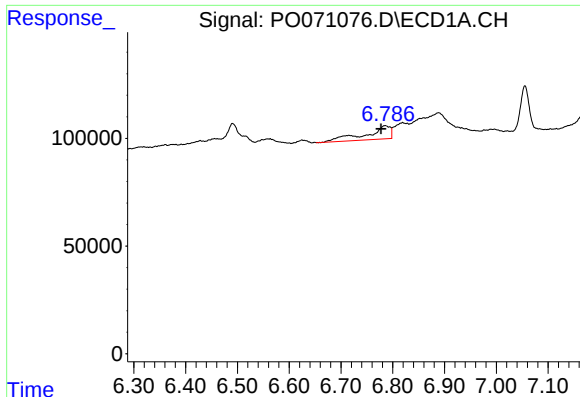

#27 AR-1254-2


R.T.: 6.785 min
Delta R.T.: 0.007 min
Response: 199579
Conc: 35.48 ng/ml

Instrument :
ECD_O
ClientSampleId :

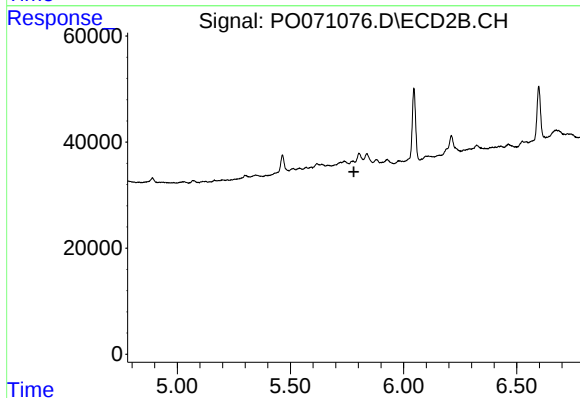


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.780 min
Response: 0
Conc: N.D.

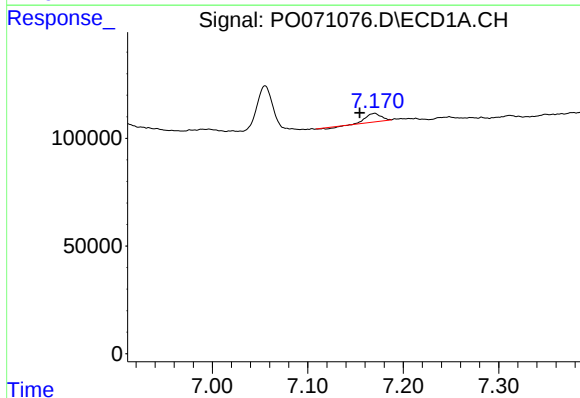


#28 AR-1254-3

R.T.: 7.170 min
Delta R.T.: 0.016 min
Response: 38611
Conc: 6.70 ng/ml

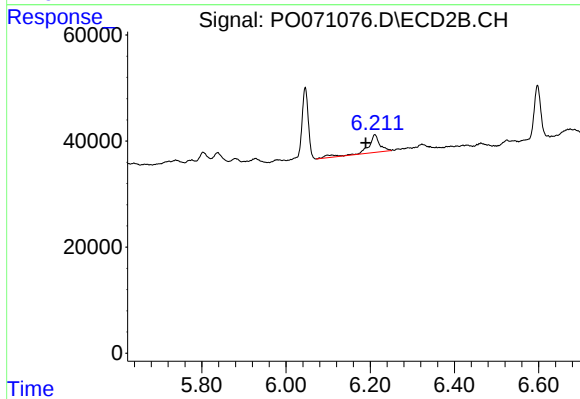

#28 AR-1254-3


R.T.: 6.211 min
Delta R.T.: 0.021 min
Response: 67690
Conc: 16.87 ng/ml

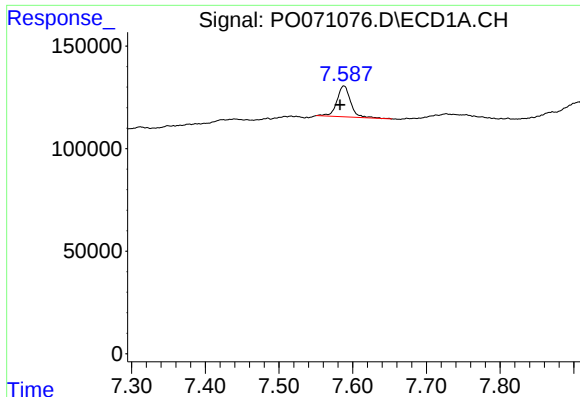

#32 AR-1260-2


R.T.: 7.588 min
Delta R.T.: 0.005 min
Response: 196260
Conc: 29.47 ng/ml

Instrument :
ECD_O
ClientSampleId :

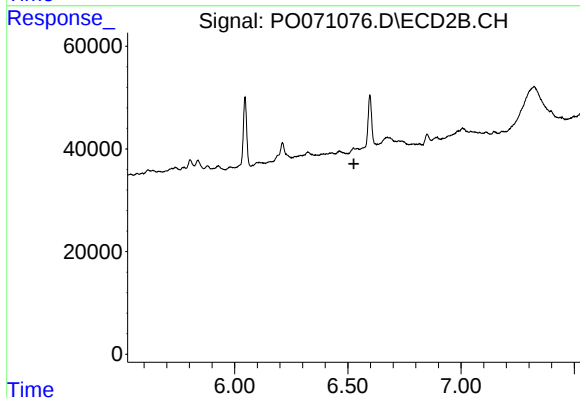


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

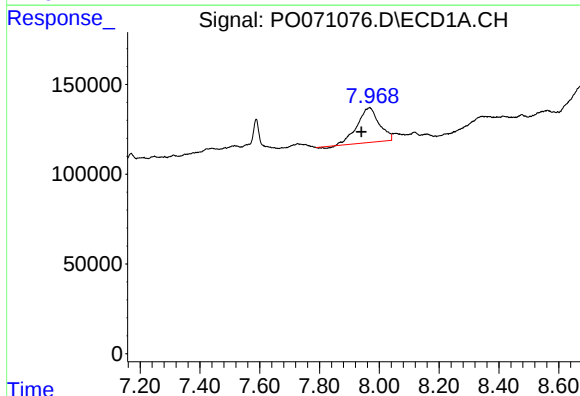


#33 AR-1260-3

R.T.: 7.968 min
Delta R.T.: 0.027 min
Response: 988215
Conc: 177.43 ng/ml

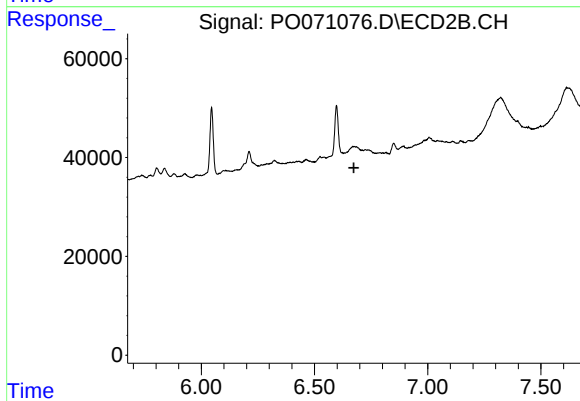

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.674 min
Response: 0
Conc: N.D.

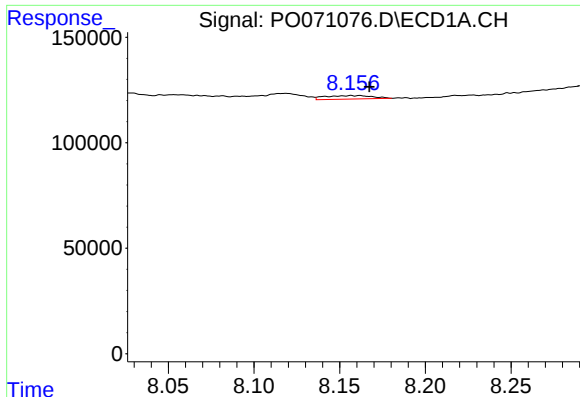

#34 AR-1260-4


R.T.: 8.157 min
Delta R.T.: -0.010 min
Response: 32234
Conc: 6.08 ng/ml

Instrument :
ECD_O
ClientSampleId :

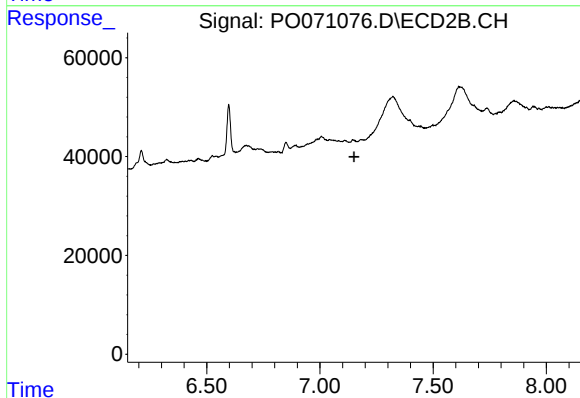


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.150 min
Response: 0
Conc: N.D.

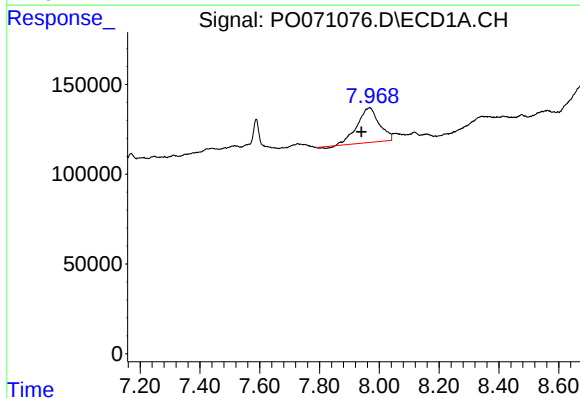

#36 AR-1262-1

R.T.: 7.968 min
Delta R.T.: 0.027 min
Response: 988215
Conc: 123.90 ng/ml

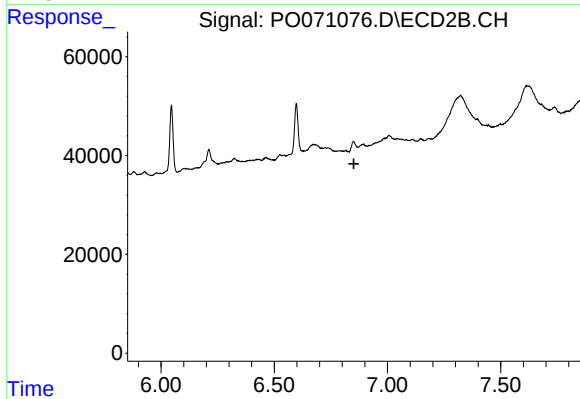

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.851 min
Response: 0
Conc: N.D.