

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P00902220\
 Data File : P0071130.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Sep 2020 17:51
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 02:30:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.351	3.537	1828624	1029484	23.678	23.223
2)	SA Decachlor...	9.970	8.720	1754334	1051777	19.172	18.311
Target Compounds							
20)	L4 AR-1242-5	0.000	5.637f	0	278795	N.D.	211.230 #
24)	L5 AR-1248-4	6.559f	0.000	1091206	0	297.552	N.D. #
25)	L5 AR-1248-5	0.000	5.637f	0	278795	N.D.	160.857 #
26)	L6 AR-1254-1	6.559	5.637f	1091206	278795	300.571	97.871 #
28)	L6 AR-1254-3	7.177f	0.000	36266	0	6.297	N.D. #
30)	L6 AR-1254-5	7.850f	0.000	110592	0	21.020	N.D. #
33)	L7 AR-1260-3	7.965f	0.000	64947	0	11.661	N.D. #
36)	L8 AR-1262-1	7.965f	0.000	64947	0	8.143	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090220\
Data File : PO071130.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Sep 2020 17:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 02:30:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

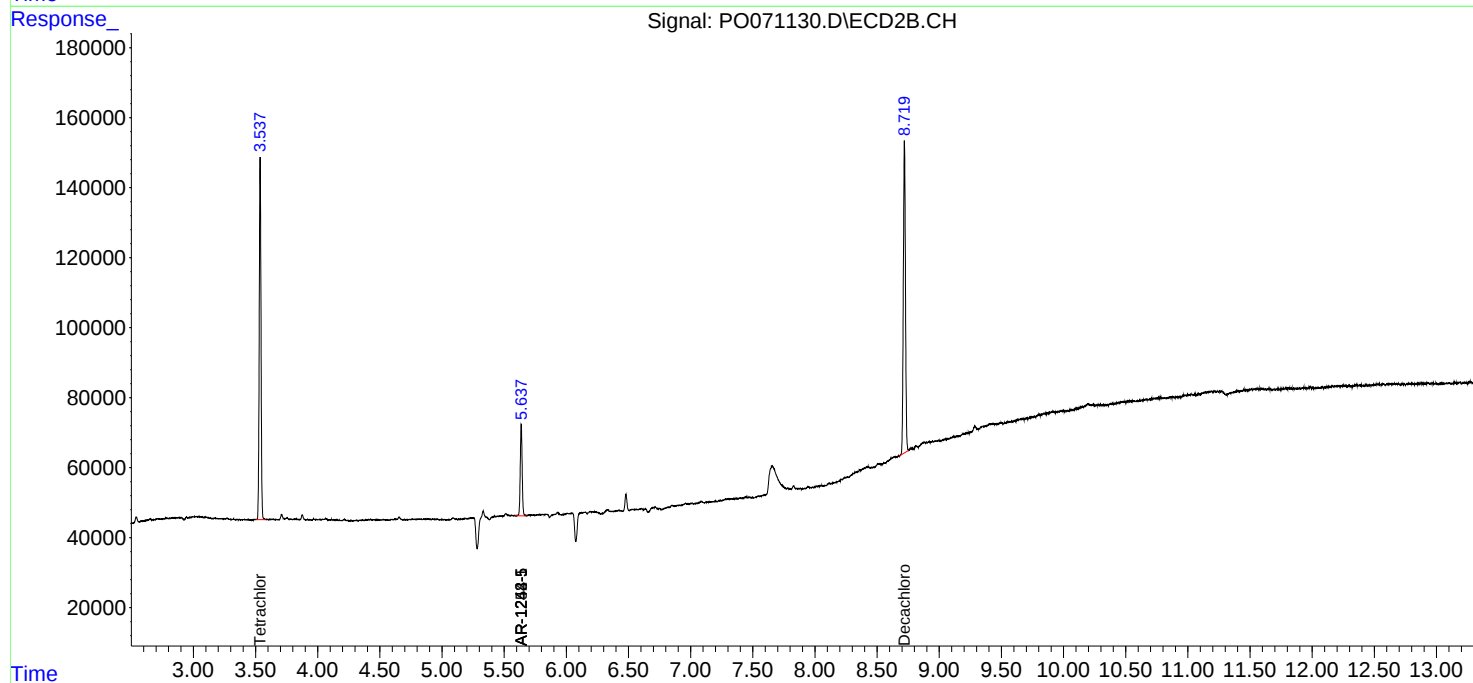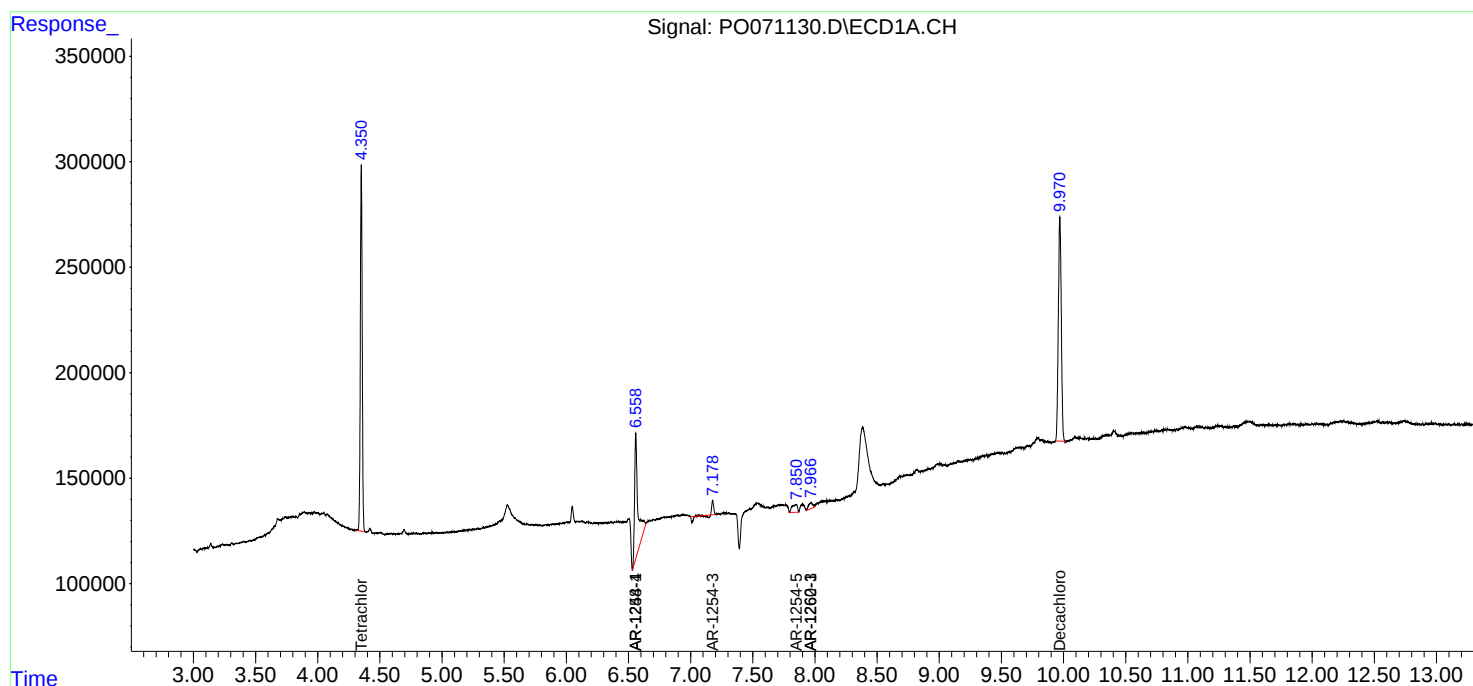


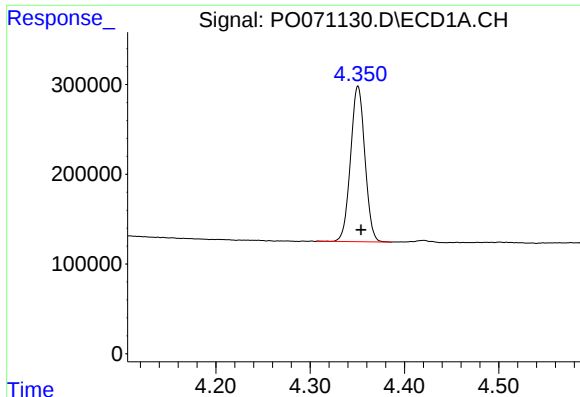

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.003 min
Response: 1828624
Conc: 23.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

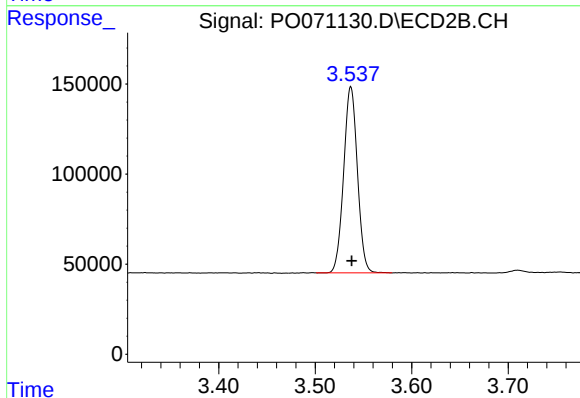


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 1029484
Conc: 23.22 ng/ml

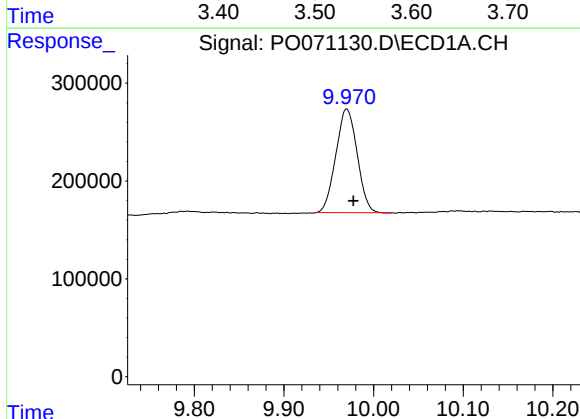


#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.007 min
Response: 1754334
Conc: 19.17 ng/ml

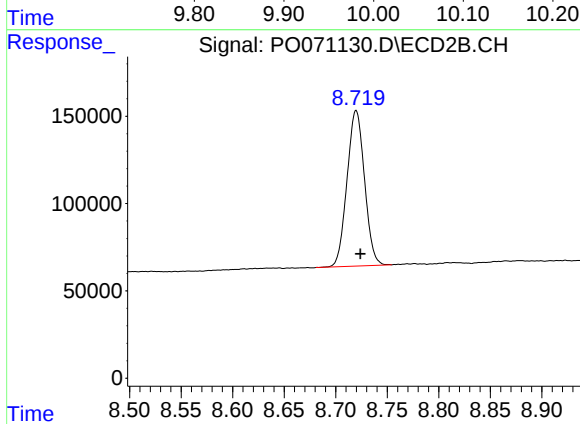

#2 Decachlorobiphenyl


R.T.: 8.720 min
Delta R.T.: -0.004 min
Response: 1051777
Conc: 18.31 ng/ml

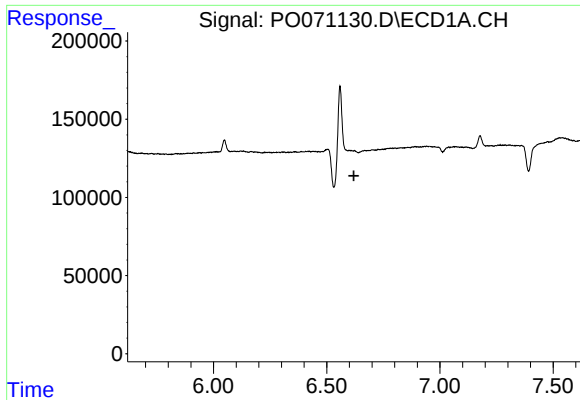

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

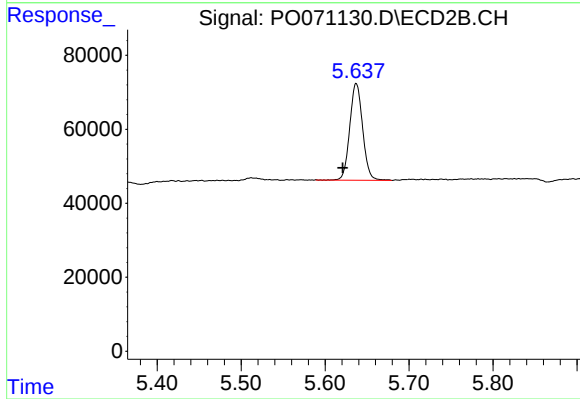


#20 AR-1242-5

R.T.: 5.637 min
Delta R.T.: 0.016 min
Response: 278795
Conc: 211.23 ng/ml

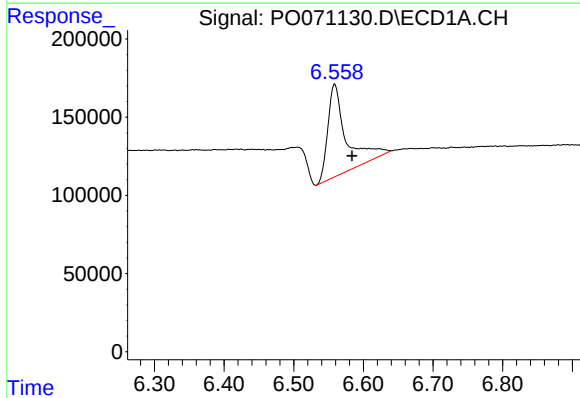


#24 AR-1248-4

R.T.: 6.559 min
Delta R.T.: -0.025 min
Response: 1091206
Conc: 297.55 ng/ml

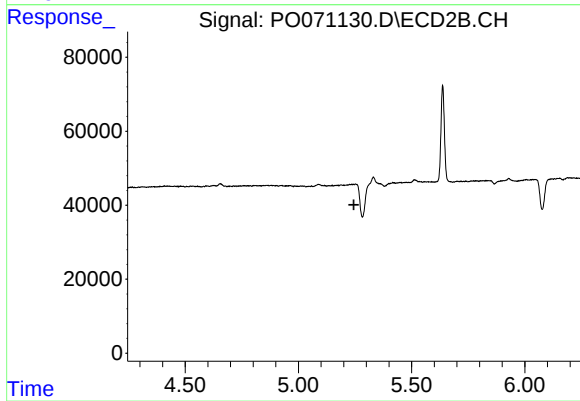

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.245 min
Response: 0
Conc: N.D.

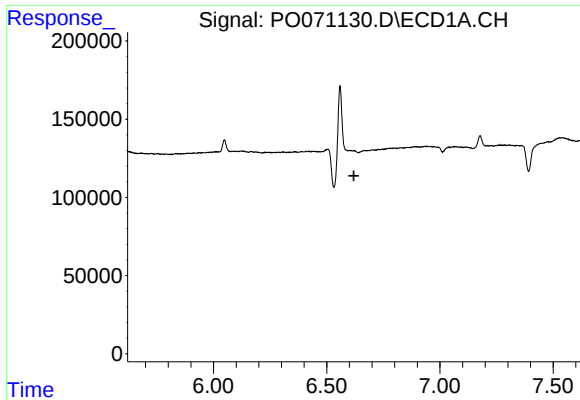

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

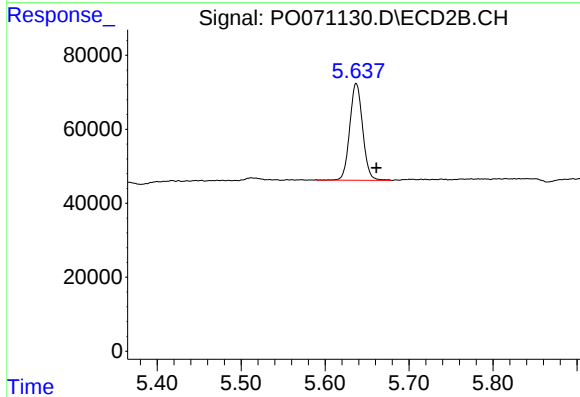


#25 AR-1248-5

R.T.: 5.637 min
Delta R.T.: -0.024 min
Response: 278795
Conc: 160.86 ng/ml

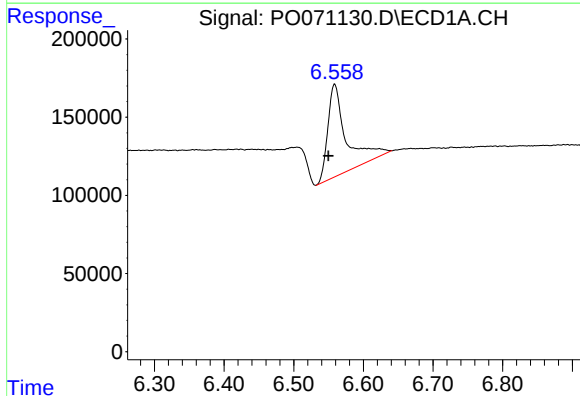


#26 AR-1254-1

R.T.: 6.559 min
Delta R.T.: 0.009 min
Response: 1091206
Conc: 300.57 ng/ml

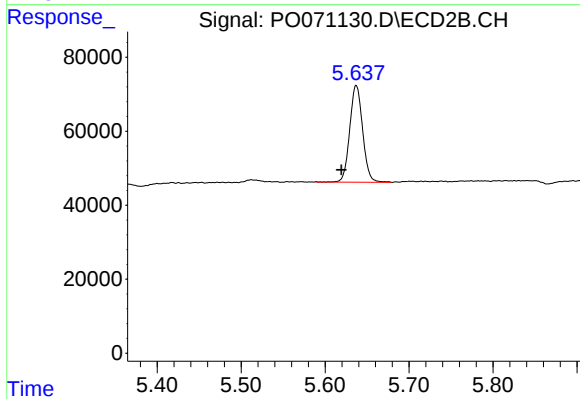

#26 AR-1254-1


R.T.: 5.637 min
Delta R.T.: 0.018 min
Response: 278795
Conc: 97.87 ng/ml

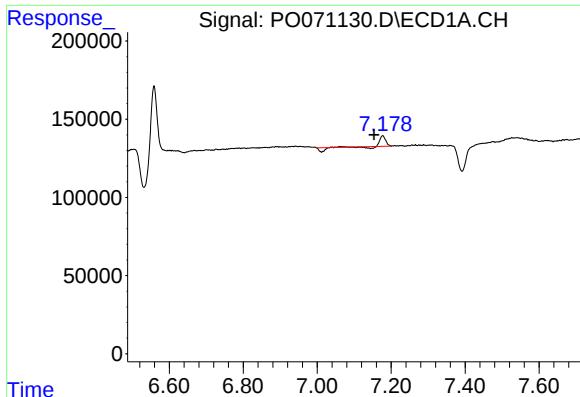

#28 AR-1254-3


R.T.: 7.177 min
Delta R.T.: 0.023 min
Response: 36266
Conc: 6.30 ng/ml

Instrument :
ECD_O
ClientSampleId :

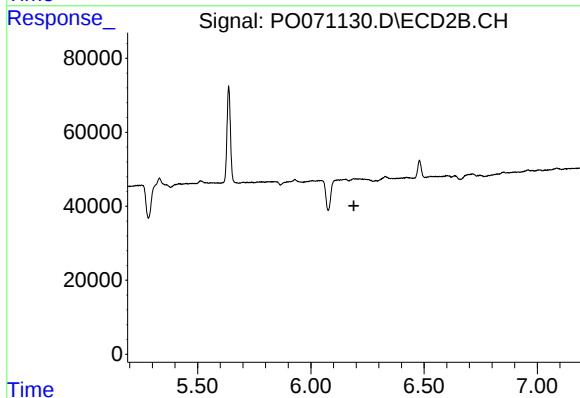


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.190 min
Response: 0
Conc: N.D.

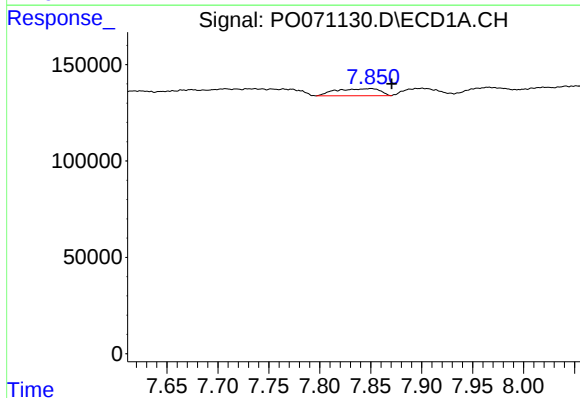


#30 AR-1254-5

R.T.: 7.850 min
Delta R.T.: -0.020 min
Response: 110592
Conc: 21.02 ng/ml

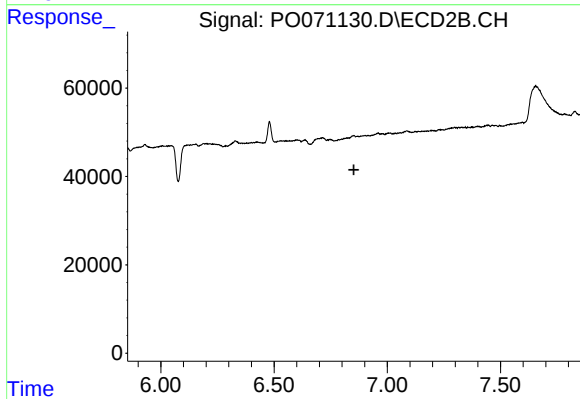

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

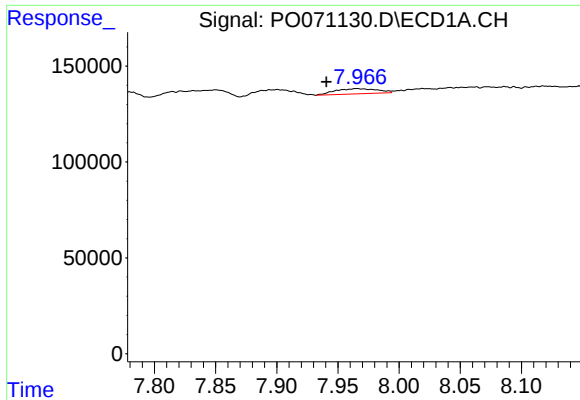

#33 AR-1260-3


R.T.: 7.965 min
Delta R.T.: 0.025 min
Response: 64947
Conc: 11.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

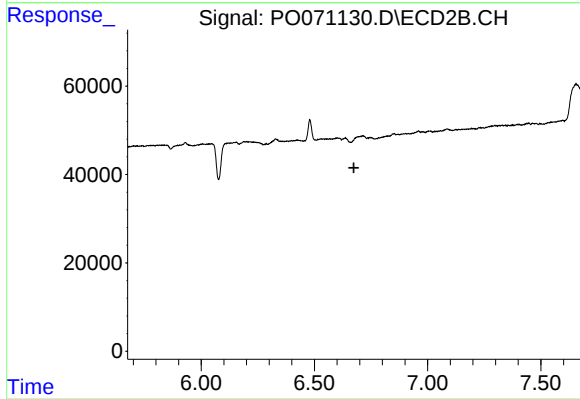


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.674 min
Response: 0
Conc: N.D.

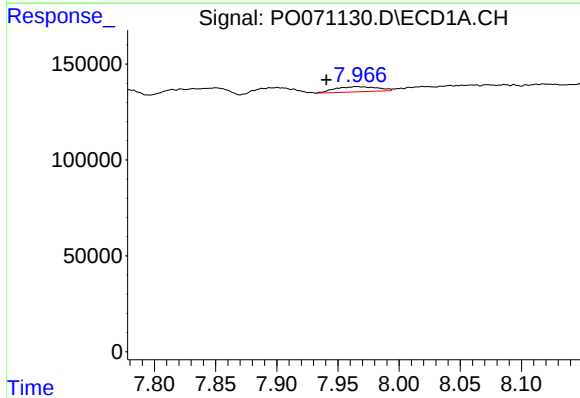

#36 AR-1262-1

R.T.: 7.965 min
Delta R.T.: 0.025 min
Response: 64947
Conc: 8.14 ng/ml

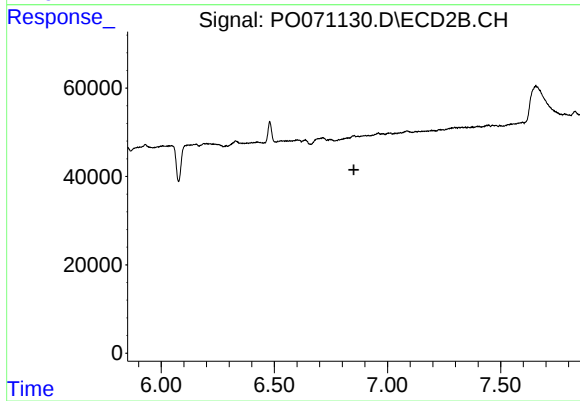

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.851 min
Response: 0
Conc: N.D.