

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090220\
 Data File : P0071109.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Sep 2020 10:00
 Operator : DD\AJ
 Sample : L3506-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-083120

Manual Integrations
 APPROVED

Ankita
 9/3/2020 10:41:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 15:47:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.536	1806273	1111035	23.389m	25.062
2) SA Decachlor...	9.968	8.719	1784794	971752	19.505	16.918

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090220\
Data File : PO071109.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Sep 2020 10:00
Operator : DD\AJ
Sample : L3506-11
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-083120


Manual Integrations
APPROVED

Ankita
9/3/2020 10:41:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 15:47:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

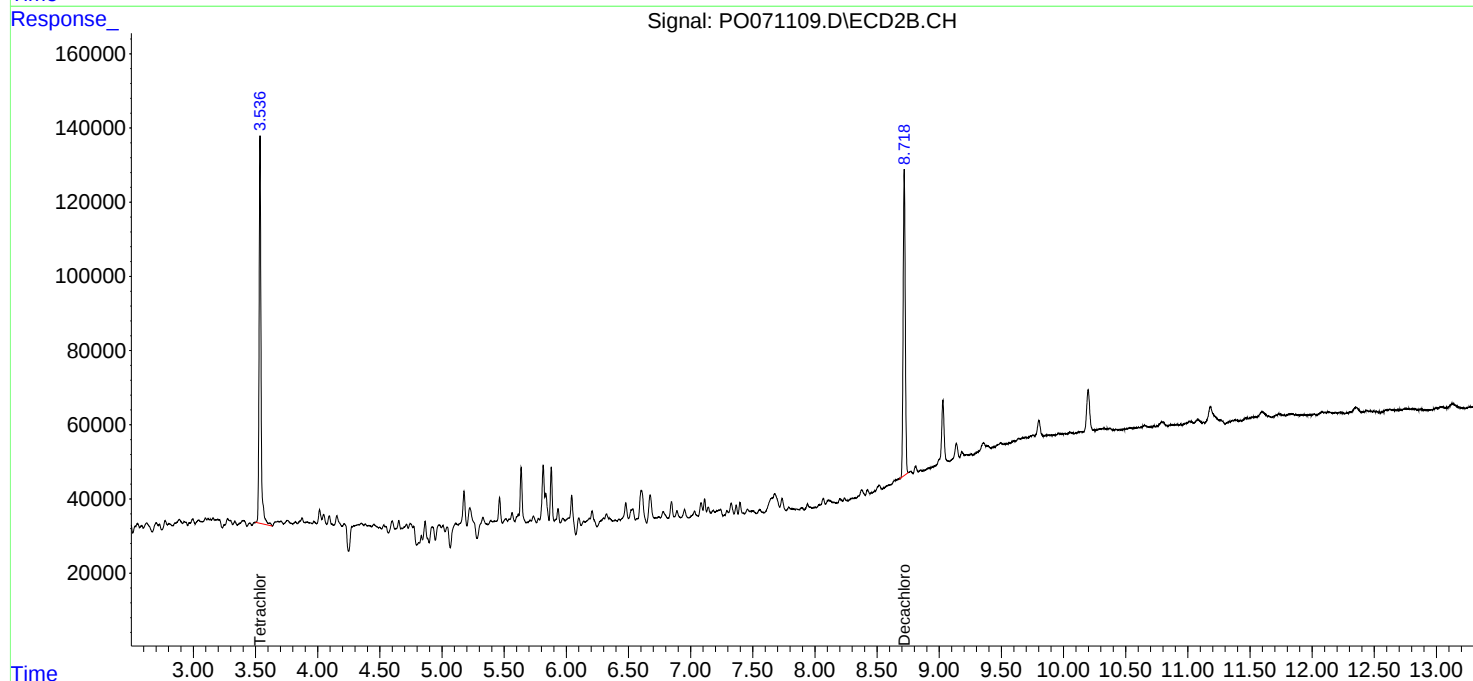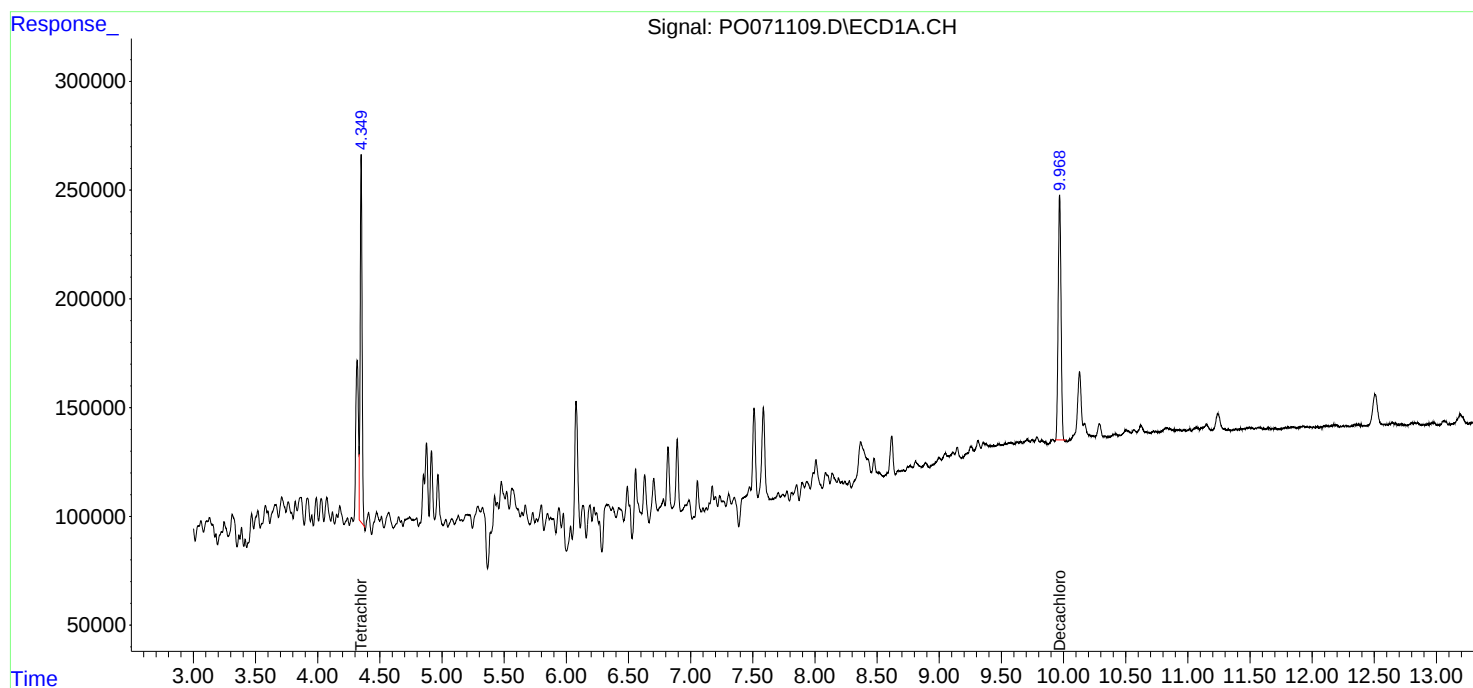

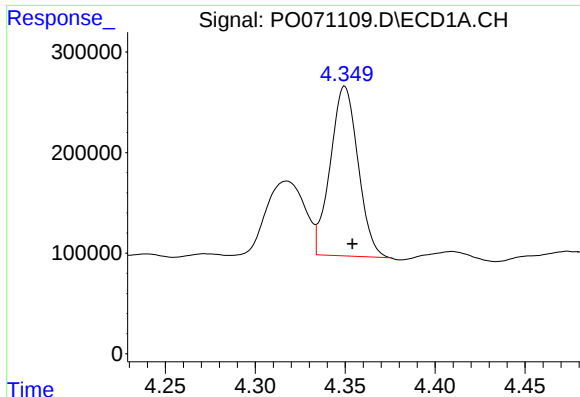


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.005 min
Response: 1806273
Conc: 23.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-02-083120


Manual Integrations
APPROVED

Ankita
9/3/2020 10:41:03 AM

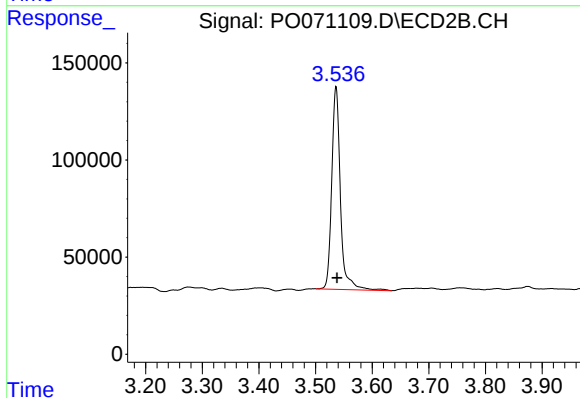


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 1111035
Conc: 25.06 ng/ml

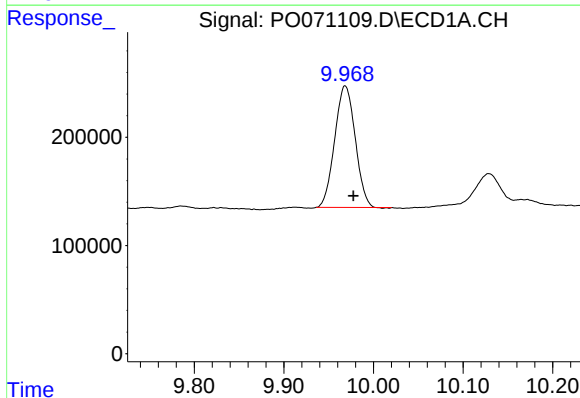

#2 Decachlorobiphenyl

R.T.: 9.968 min
Delta R.T.: -0.009 min
Response: 1784794
Conc: 19.51 ng/ml

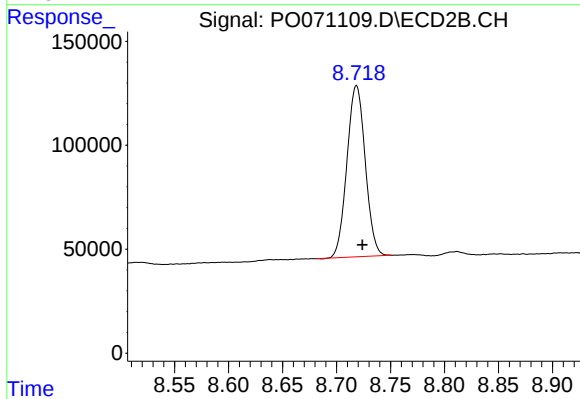

#2 Decachlorobiphenyl

R.T.: 8.719 min
Delta R.T.: -0.006 min
Response: 971752
Conc: 16.92 ng/ml