

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090220\
 Data File : P0071120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Sep 2020 15:00
 Operator : DD\AJ
 Sample : L3876-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1500

Manual Integrations
 APPROVED

Ankita
 9/3/2020 10:41:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 16:54:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.537	2281510	1337239	29.542	30.165
2) SA Decachlor...	9.972	8.718	2090379	4522057	22.845	78.729 #
Target Compounds						
26) L6 AR-1254-1	6.547	5.617	931453	792425	256.567m	278.181
27) L6 AR-1254-2	6.774	5.779	1317745	474368	234.239m	189.219
28) L6 AR-1254-3	7.151	6.187	1183609	825416	205.525	205.720m
29) L6 AR-1254-4	7.446	6.428	1175881	673175	215.280	230.107
30) L6 AR-1254-5	7.866	6.850	1281622	835570	243.595	215.336

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090220\
Data File : PO071120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Sep 2020 15:00
Operator : DD\AJ
Sample : L3876-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
1500


Manual Integrations
APPROVED

Ankita
9/3/2020 10:41:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 16:54:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

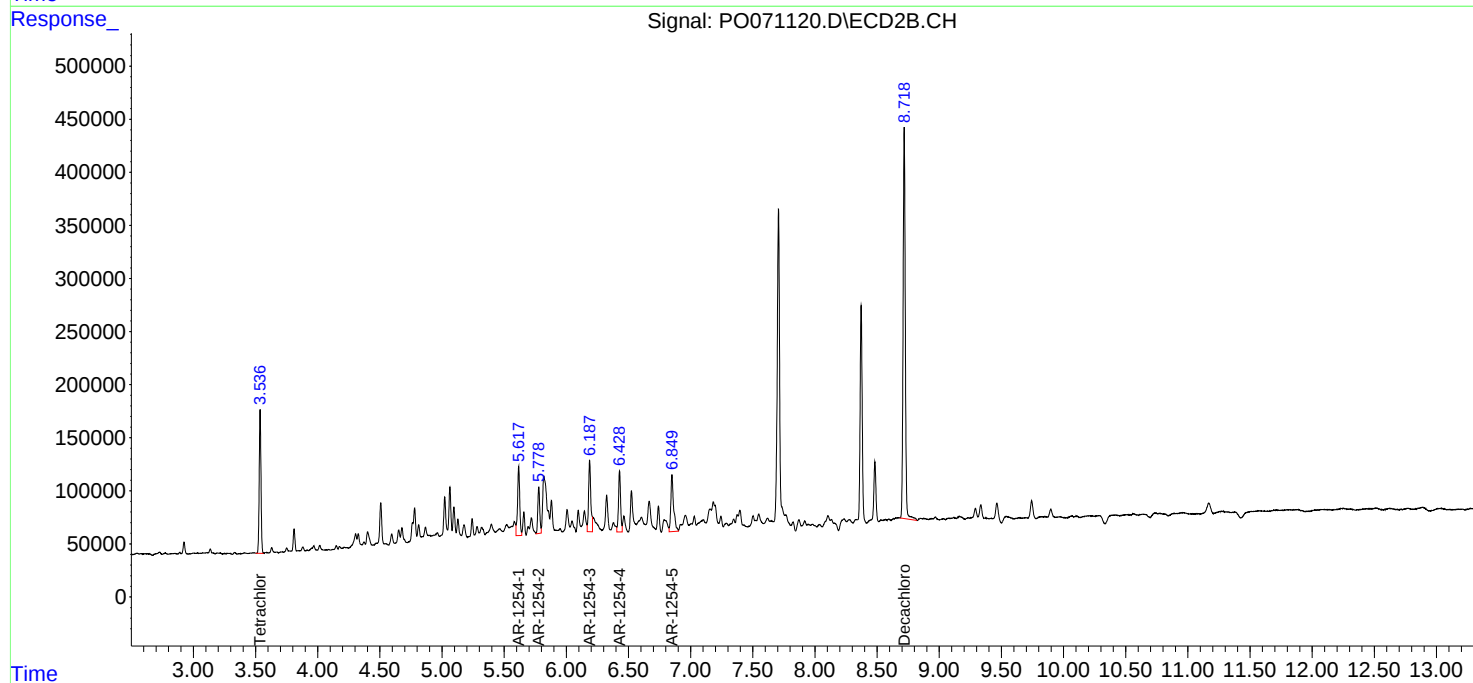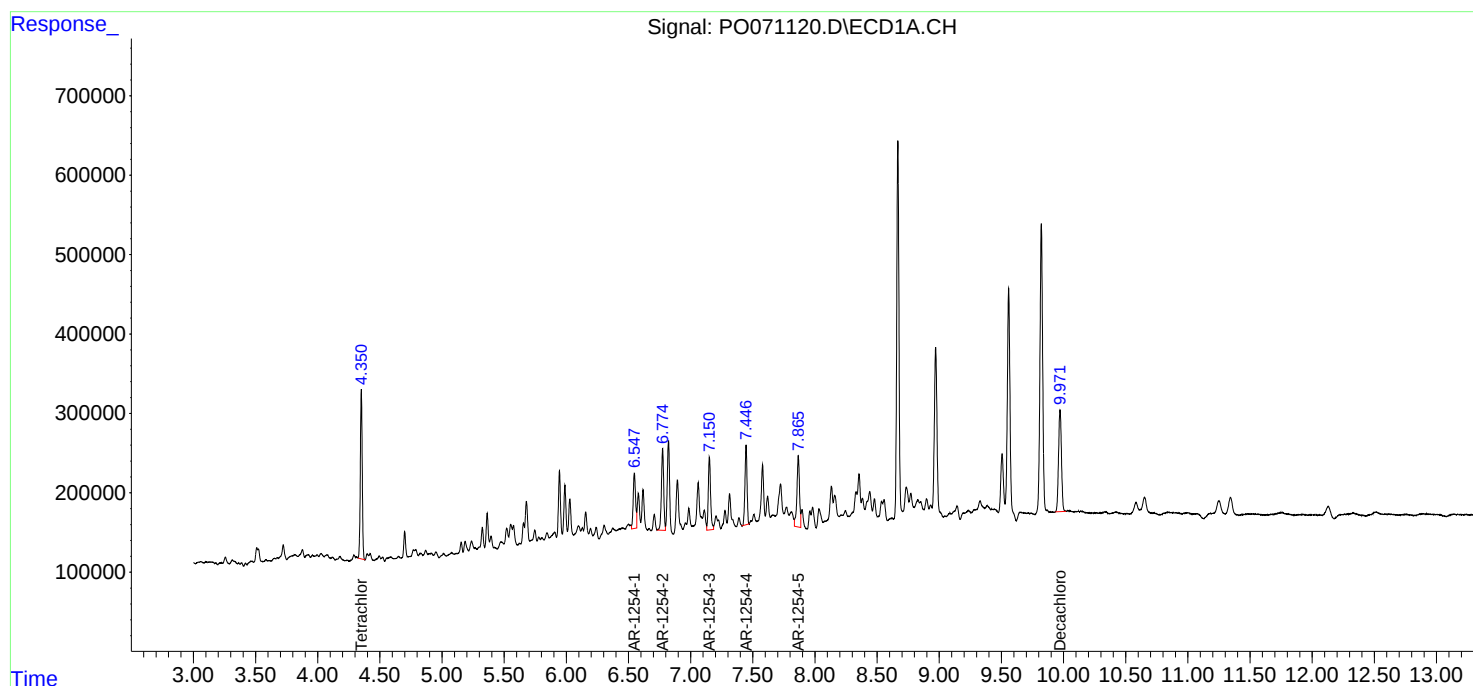

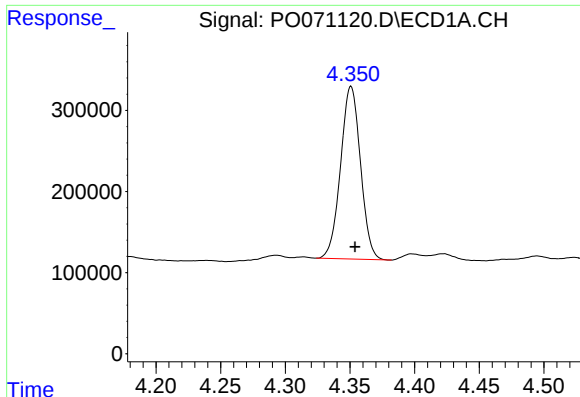


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.003 min
Response: 2281510
Conc: 29.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
1500


Manual Integrations
APPROVED

Ankita
9/3/2020 10:41:08 AM

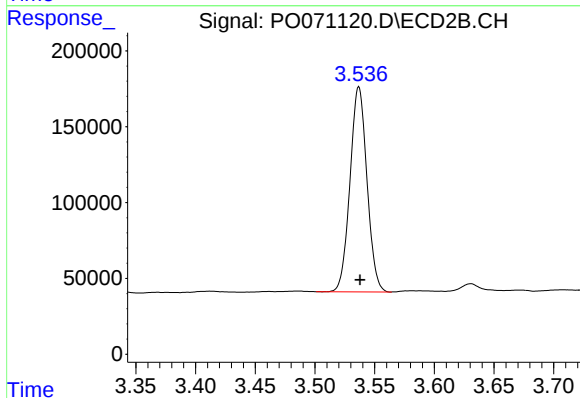


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.001 min
Response: 1337239
Conc: 30.16 ng/ml

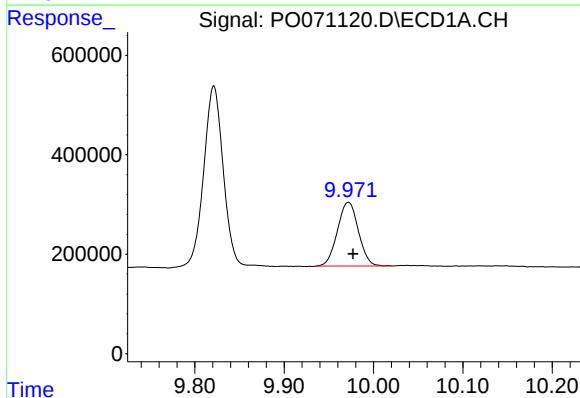


#2 Decachlorobiphenyl

R.T.: 9.972 min
Delta R.T.: -0.005 min
Response: 2090379
Conc: 22.84 ng/ml

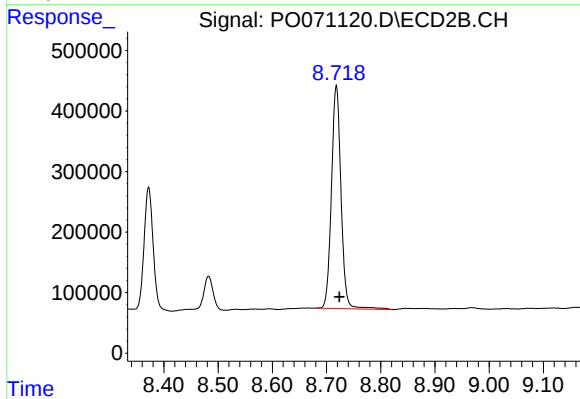

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: -0.006 min
Response: 4522057
Conc: 78.73 ng/ml

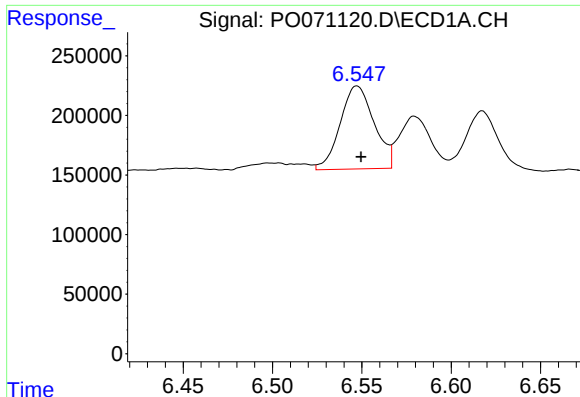


#26 AR-1254-1

R.T.: 6.547 min
Delta R.T.: -0.003 min
Response: 931453
Conc: 256.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1500


Manual Integrations
APPROVED

Ankita
9/3/2020 10:41:08 AM

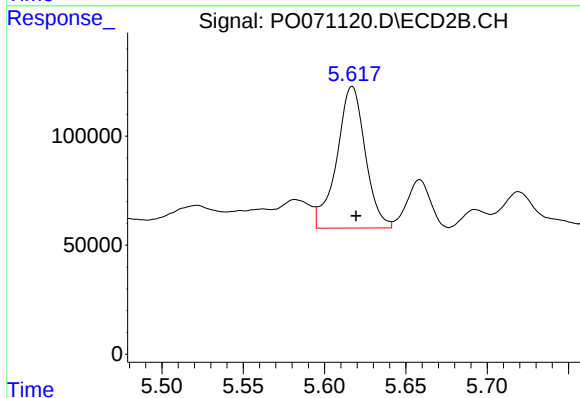


#26 AR-1254-1

R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 792425
Conc: 278.18 ng/ml

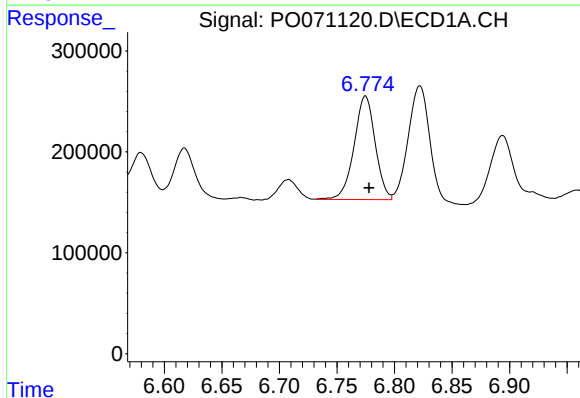


#27 AR-1254-2

R.T.: 6.774 min
Delta R.T.: -0.004 min
Response: 1317745
Conc: 234.24 ng/ml m

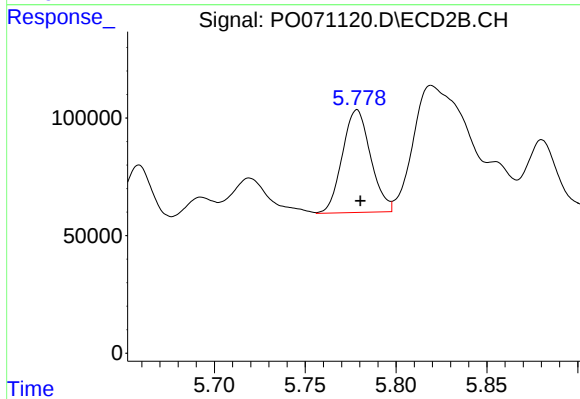

#27 AR-1254-2

R.T.: 5.779 min
Delta R.T.: -0.002 min
Response: 474368
Conc: 189.22 ng/ml

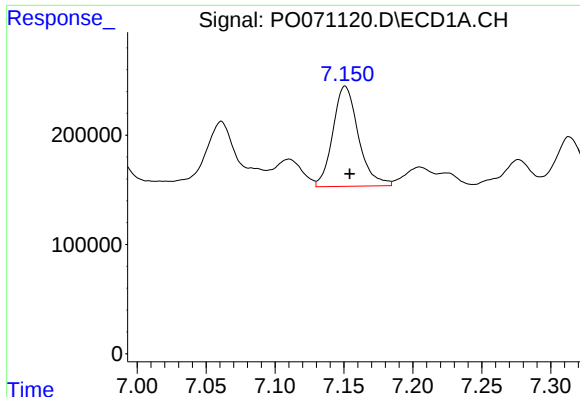


#28 AR-1254-3

R.T.: 7.151 min
Delta R.T.: -0.003 min
Response: 1183609
Conc: 205.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
1500


Manual Integrations
APPROVED

Ankita
9/3/2020 10:41:08 AM

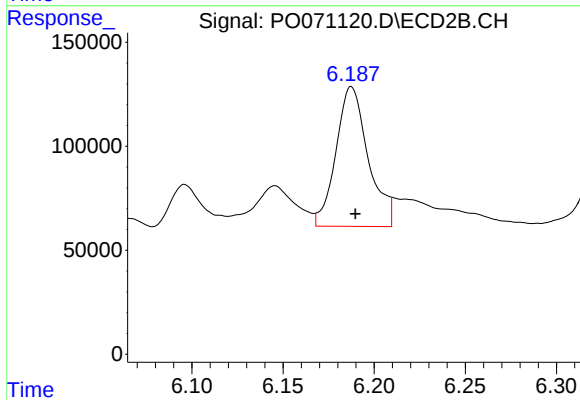


#28 AR-1254-3

R.T.: 6.187 min
Delta R.T.: -0.003 min
Response: 825416
Conc: 205.72 ng/ml m

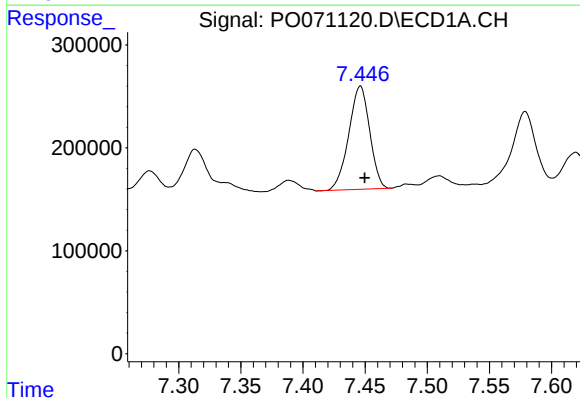


#29 AR-1254-4

R.T.: 7.446 min
Delta R.T.: -0.003 min
Response: 1175881
Conc: 215.28 ng/ml

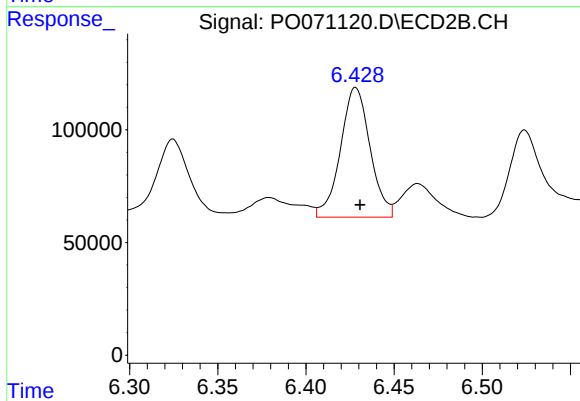

#29 AR-1254-4

R.T.: 6.428 min
Delta R.T.: -0.003 min
Response: 673175
Conc: 230.11 ng/ml

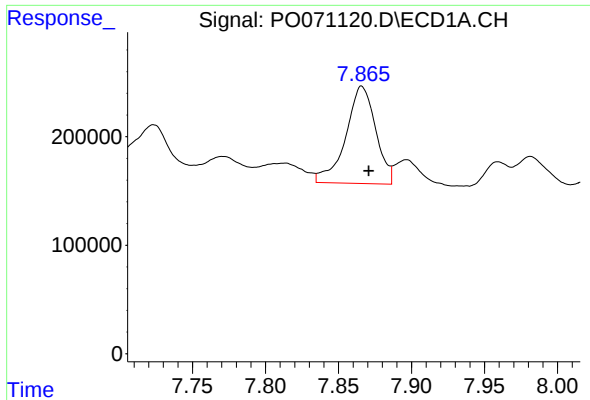


#30 AR-1254-5

R.T.: 7.866 min
Delta R.T.: -0.005 min
Response: 1281622
Conc: 243.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
1500

Manual Integrations
APPROVED

Ankita
9/3/2020 10:41:08 AM

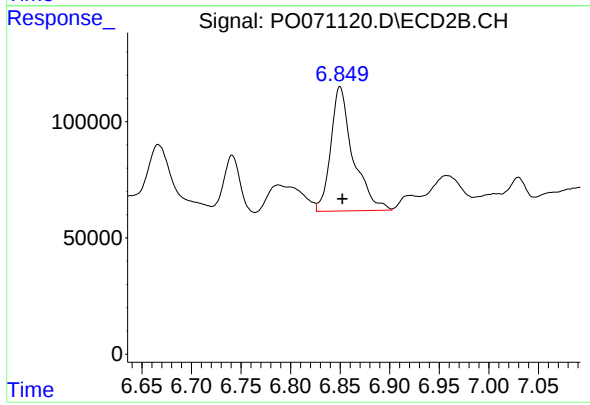

#30 AR-1254-5

R.T.: 6.850 min
Delta R.T.: -0.003 min
Response: 835570
Conc: 215.34 ng/ml