

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090222\
 Data File : P0089236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 20:02
 Operator : YP/AJ
 Sample : N4489-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRIP-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 10:21:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 29 17:48:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.587	53750702	18323864	14.335	18.983 #
2) SA Decachlor...	10.252	8.567	28191638	11826834	12.245	13.374
Target Compounds						
16) L4 AR-1242-1	5.604	4.663	66561231	24087427	753.033	826.881
17) L4 AR-1242-2	5.627	4.682	76521689	23931777	618.275	604.115
18) L4 AR-1242-3	5.690	4.857	35409220	10991431	460.671	515.853
19) L4 AR-1242-4	5.789	4.941	30145864	11316537	485.379	520.088
20) L4 AR-1242-5	6.531	5.462	4937963	2514175	76.709	92.036



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090222\
Data File : PO089236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 20:02
Operator : YP/AJ
Sample : N4489-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DRIP-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 10:21:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082922.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 29 17:48:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

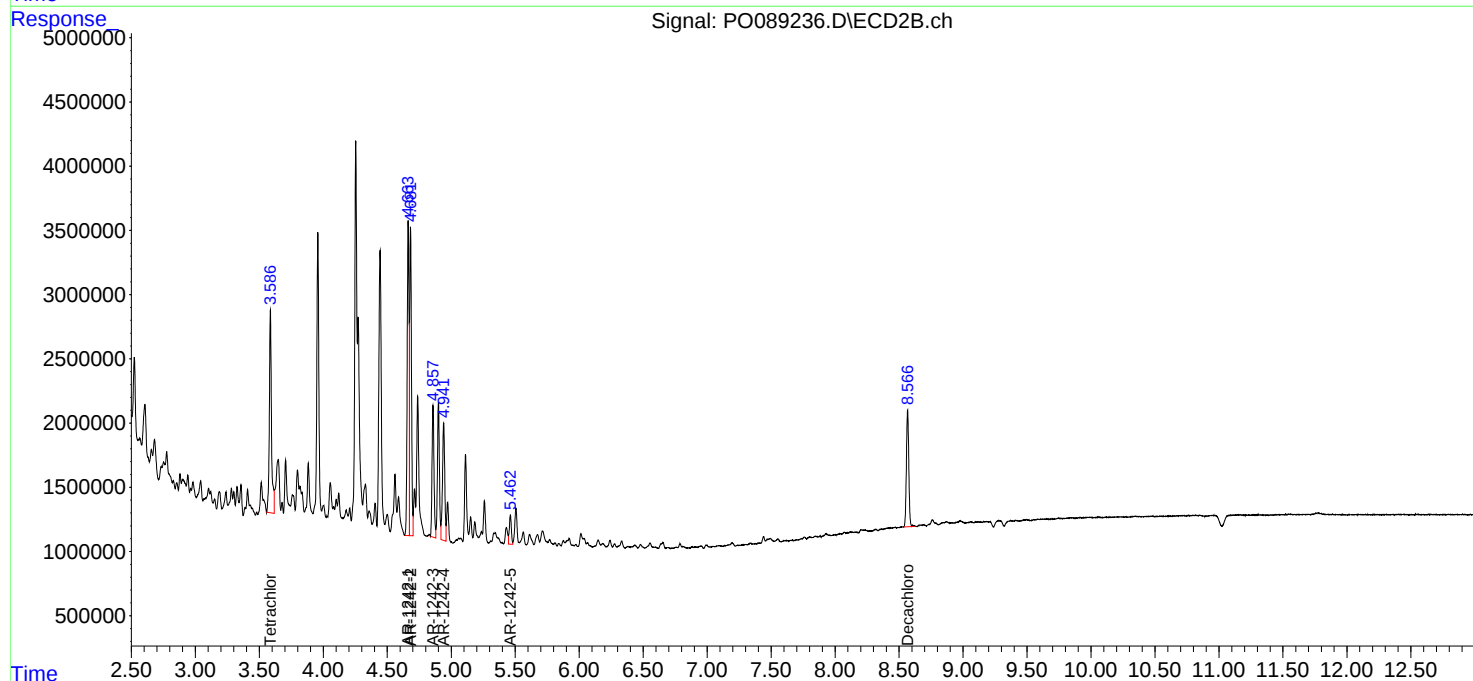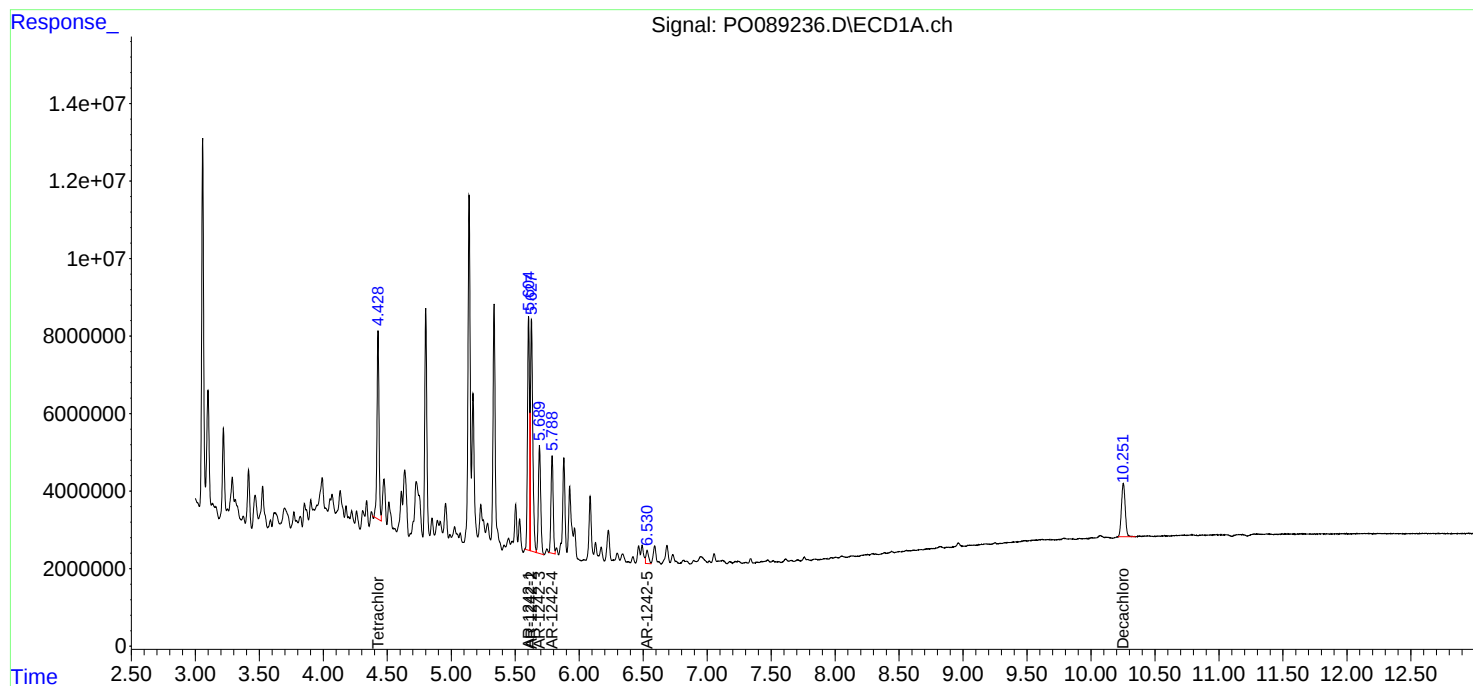


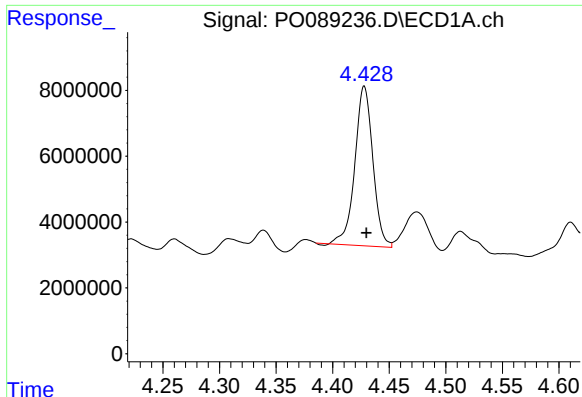

#1 Tetrachloro-m-xylene


R.T.: 4.428 min
Delta R.T.: -0.002 min
Response: 53750702
Conc: 14.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRIP-COMP

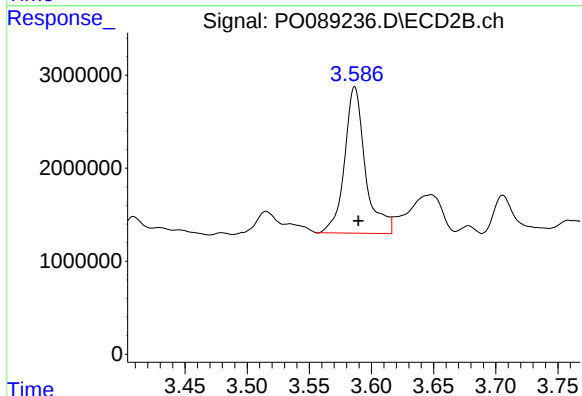


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: -0.003 min
Response: 18323864
Conc: 18.98 ng/ml

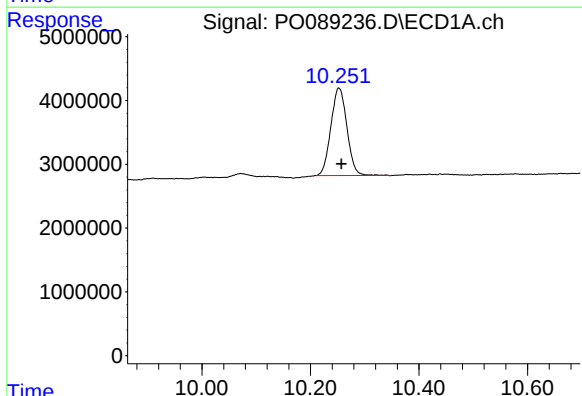


#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: -0.005 min
Response: 28191638
Conc: 12.24 ng/ml

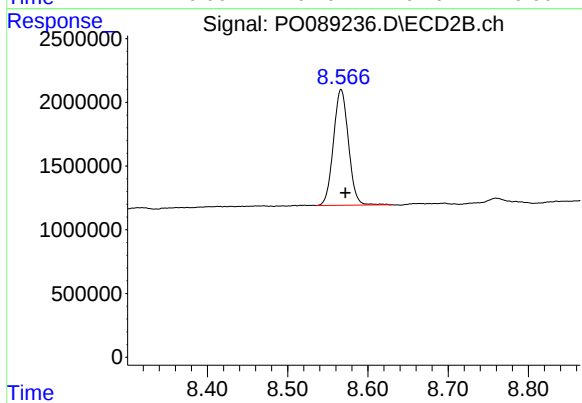

#2 Decachlorobiphenyl


R.T.: 8.567 min
Delta R.T.: -0.006 min
Response: 11826834
Conc: 13.37 ng/ml

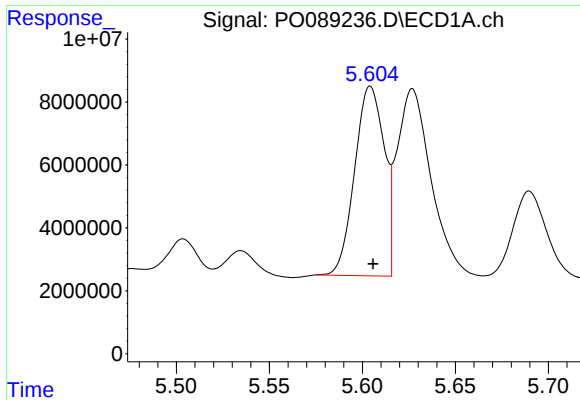

#16 AR-1242-1


R.T.: 5.604 min
Delta R.T.: -0.001 min
Response: 66561231
Conc: 753.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRIP-COMP

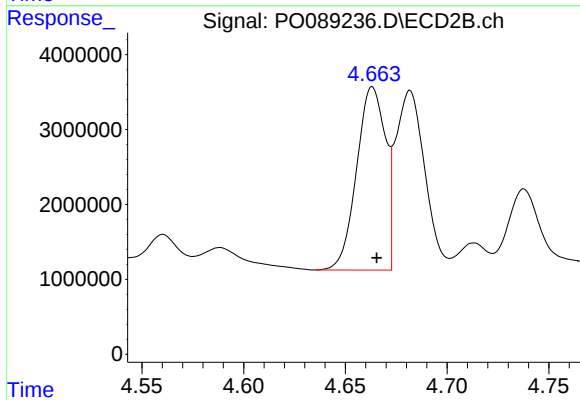


#16 AR-1242-1

R.T.: 4.663 min
Delta R.T.: -0.002 min
Response: 24087427
Conc: 826.88 ng/ml

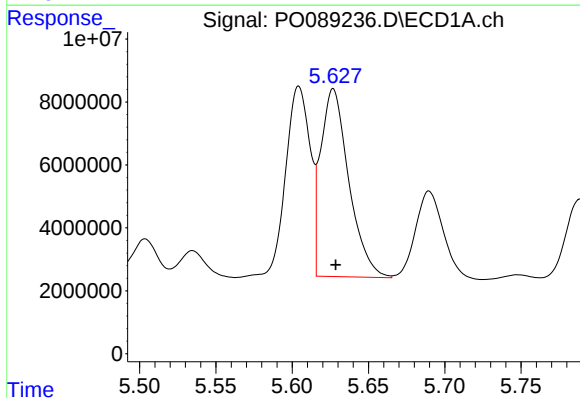


#17 AR-1242-2

R.T.: 5.627 min
Delta R.T.: -0.002 min
Response: 76521689
Conc: 618.27 ng/ml

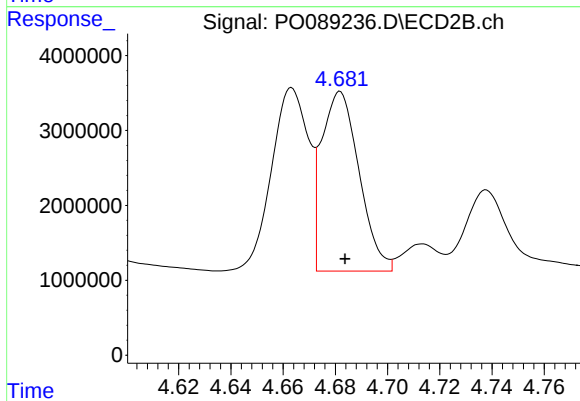

#17 AR-1242-2


R.T.: 4.682 min
Delta R.T.: -0.002 min
Response: 23931777
Conc: 604.11 ng/ml

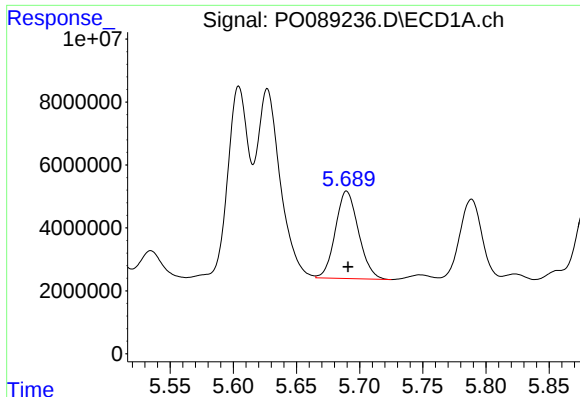

#18 AR-1242-3


R.T.: 5.690 min
Delta R.T.: -0.001 min
Response: 35409220
Conc: 460.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRIP-COMP

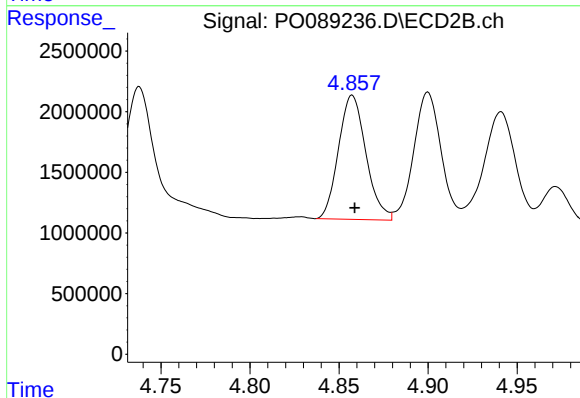


#18 AR-1242-3

R.T.: 4.857 min
Delta R.T.: -0.001 min
Response: 10991431
Conc: 515.85 ng/ml

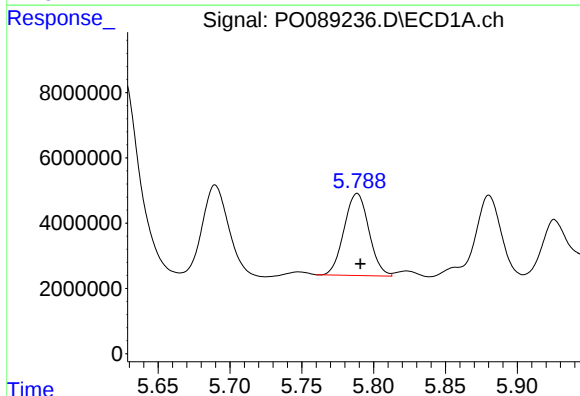


#19 AR-1242-4

R.T.: 5.789 min
Delta R.T.: -0.002 min
Response: 30145864
Conc: 485.38 ng/ml

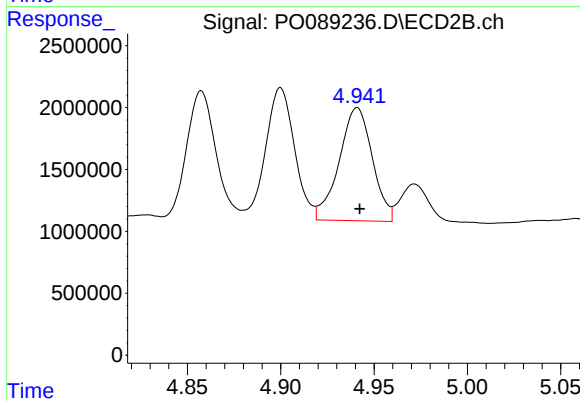

#19 AR-1242-4


R.T.: 4.941 min
Delta R.T.: -0.001 min
Response: 11316537
Conc: 520.09 ng/ml

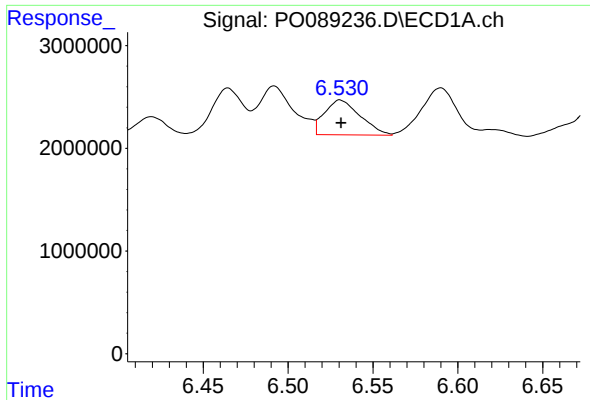

#20 AR-1242-5

R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 4937963
Conc: 76.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRIP-COMP

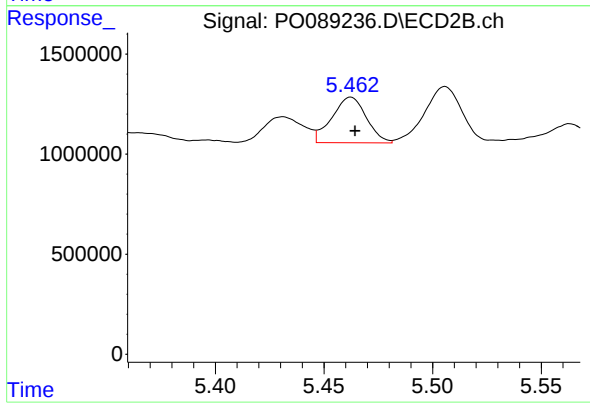

#20 AR-1242-5

R.T.: 5.462 min
Delta R.T.: -0.002 min
Response: 2514175
Conc: 92.04 ng/ml