

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090222\
 Data File : P0089257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2022 05:09
 Operator : YP/AJ
 Sample : N4489-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ORA-0067

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/06/2022
 Supervised By :Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 21:54:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 29 17:48:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.586	46205827	14486125	12.323m	15.007
2) SA Decachlor...	10.249	8.564	27390634	8872091	11.897	10.033

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090222\
Data File : PO089257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2022 05:09
Operator : YP/AJ
Sample : N4489-07
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ORA-0067


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2022
Supervised By :Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 21:54:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082922.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 29 17:48:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

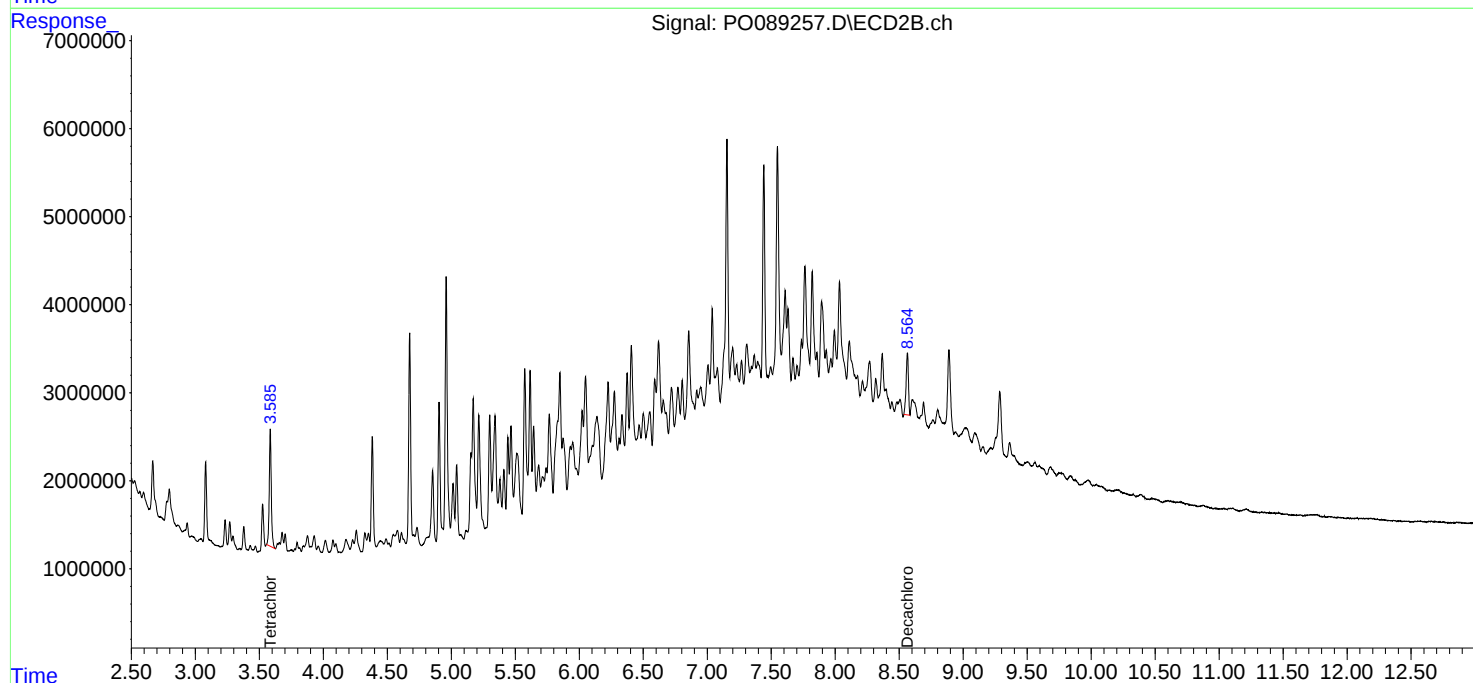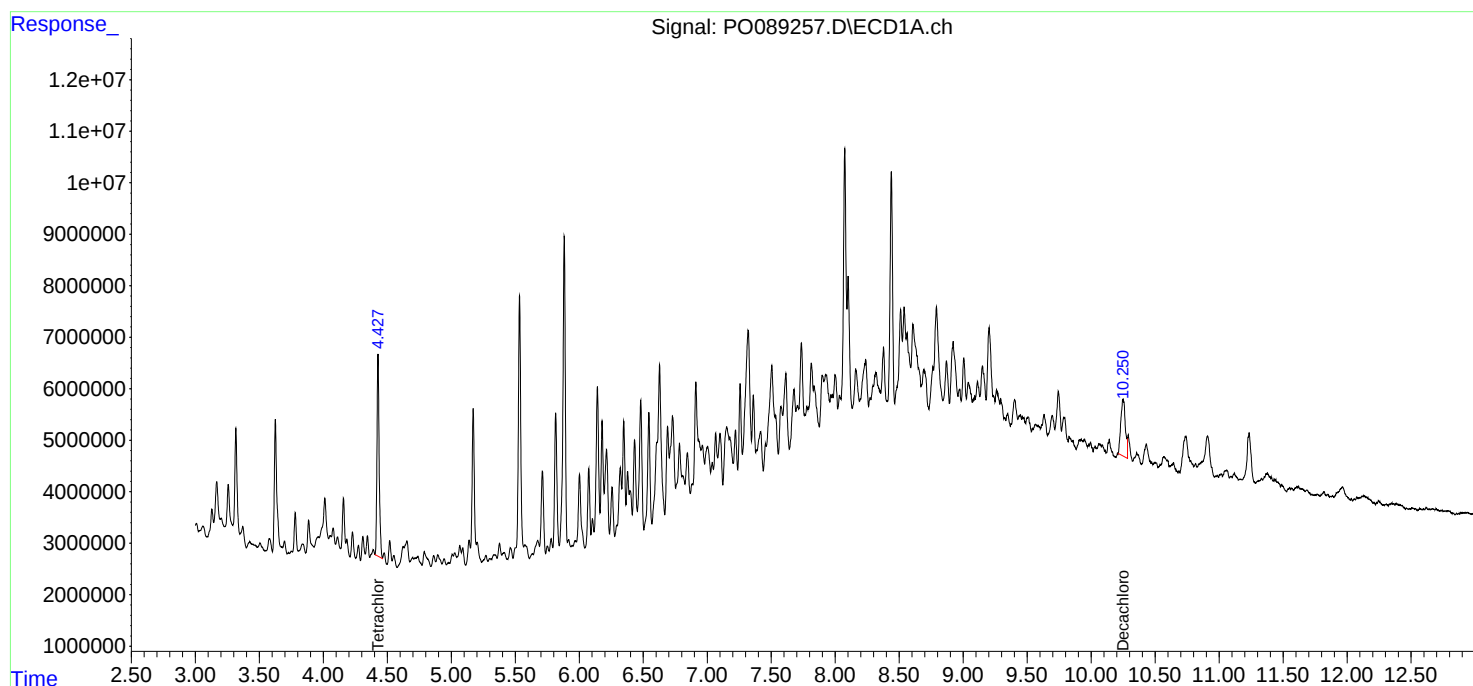

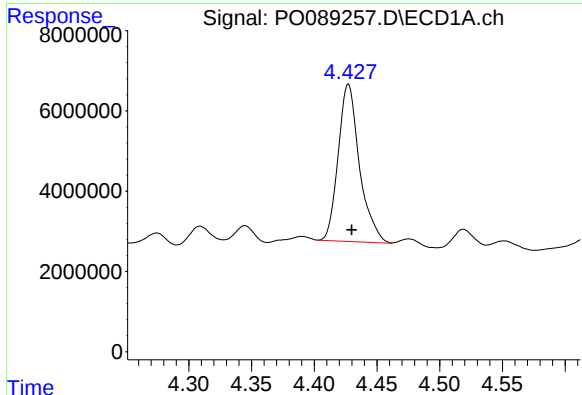


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: -0.003 min
Response: 46205827
Conc: 12.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
ORA-0067


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2022
Supervised By :Ankita Jodhani 09/06/2022

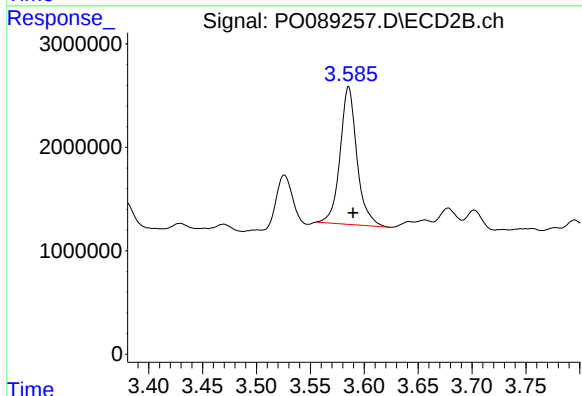


#1 Tetrachloro-m-xylene

R.T.: 3.586 min
Delta R.T.: -0.004 min
Response: 14486125
Conc: 15.01 ng/ml

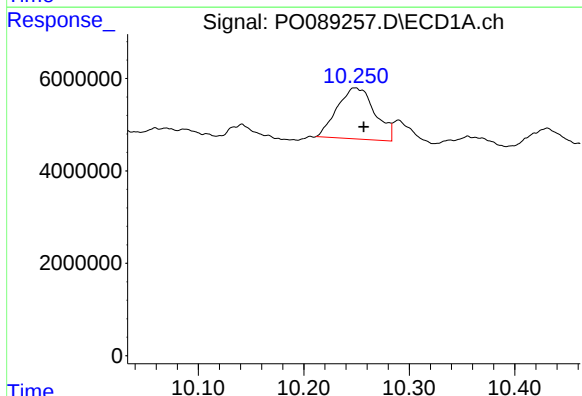

#2 Decachlorobiphenyl

R.T.: 10.249 min
Delta R.T.: -0.008 min
Response: 27390634
Conc: 11.90 ng/ml

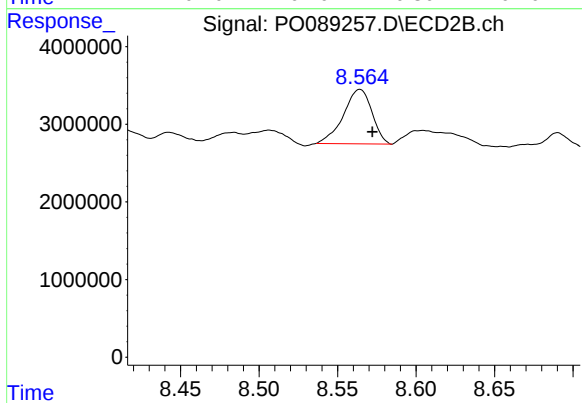

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.008 min
Response: 8872091
Conc: 10.03 ng/ml