

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090222\
 Data File : P0089273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2022 10:19
 Operator : YP/AJ
 Sample : N4489-09 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ORA-73-74-W

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/06/2022
 Supervised By :Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 22:02:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 29 17:48:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.583	3013685	1277075	0.804	1.323m#
2) SA Decachlor...	10.245	8.565	2994193	639708	1.301m	0.723 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090222\
Data File : PO089273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2022 10:19
Operator : YP/AJ
Sample : N4489-09 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ORA-73-74-W


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2022
Supervised By :Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 22:02:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082922.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 29 17:48:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

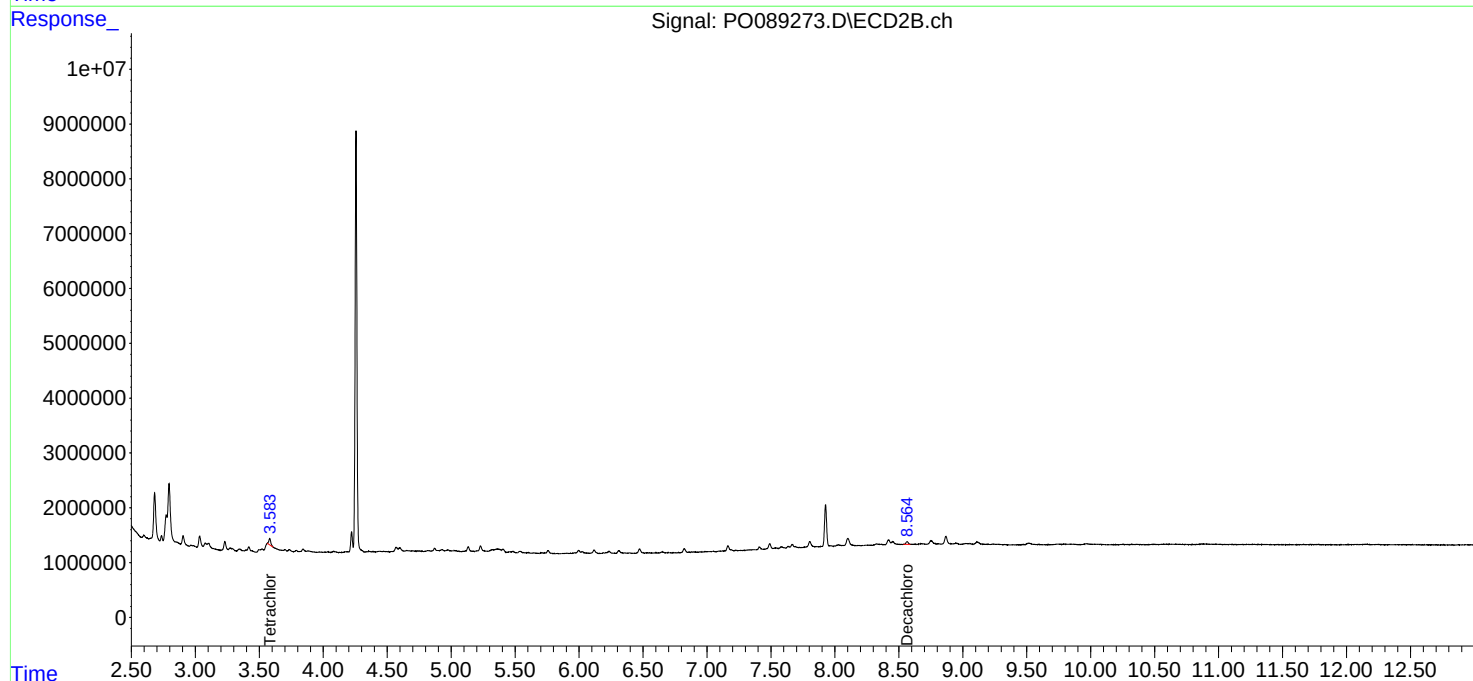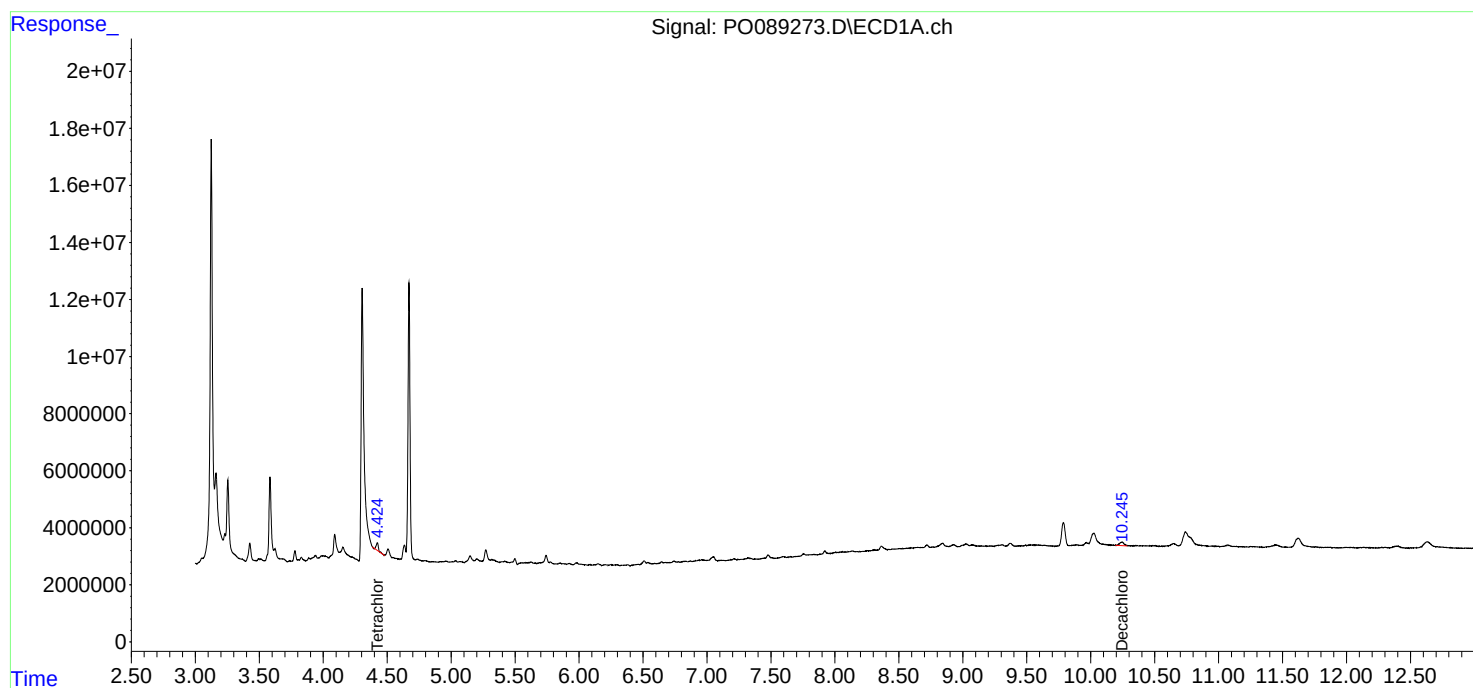

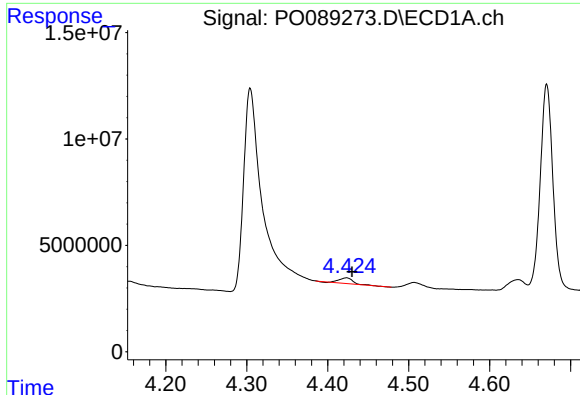


#1 Tetrachloro-m-xylene

R.T.: 4.423 min
Delta R.T.: -0.007 min
Response: 3013685
Conc: 0.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
ORA-73-74-W


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2022
Supervised By :Ankita Jodhani 09/06/2022

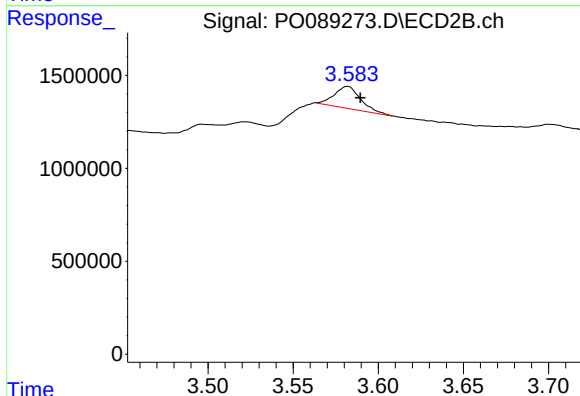


#1 Tetrachloro-m-xylene

R.T.: 3.583 min
Delta R.T.: -0.007 min
Response: 1277075
Conc: 1.32 ng/ml m

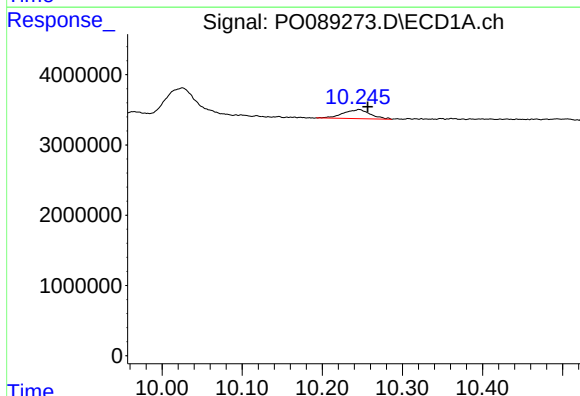

#2 Decachlorobiphenyl

R.T.: 10.245 min
Delta R.T.: -0.012 min
Response: 2994193
Conc: 1.30 ng/ml m

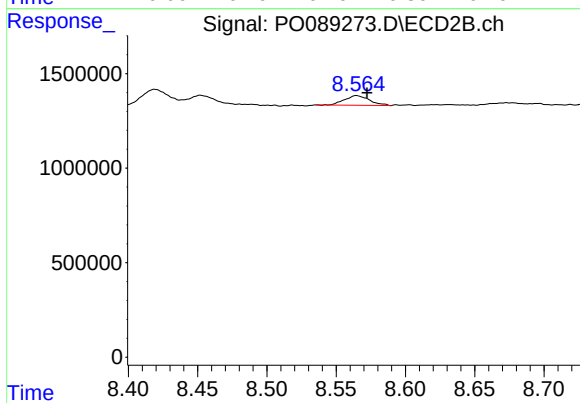

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: -0.007 min
Response: 639708
Conc: 0.72 ng/ml