

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 10:24
 Operator : SM/AJ
 Sample : K4479-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU19-FLDDCAP1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:13:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.117	3.493	763551	675547	21.808	18.767
2)	SA Decachlor...	9.569	8.344	534114	420528	10.040	10.429
Target Compounds							
3)	L1 AR-1016-1	5.285	0.000	5039	0	3.142	N.D. #
4)	L1 AR-1016-2	5.285	0.000	5039	0	2.106	N.D. #
5)	L1 AR-1016-3	5.310	0.000	451	0	0.303	N.D. #
6)	L1 AR-1016-4	5.443	0.000	1026	0	0.848	N.D. #
7)	L1 AR-1016-5	5.730	0.000	4914	0	3.826	N.D. #
8)	L2 AR-1221-1	4.365	0.000	1175	0	2.775	N.D. #
9)	L2 AR-1221-2	4.417	0.000	12338	0	37.988	N.D. #
10)	L2 AR-1221-3	4.494	0.000	5597	0	5.321	N.D. #
11)	L3 AR-1232-1	4.494	0.000	5597	0	4.490	N.D. #
12)	L3 AR-1232-2	4.997	0.000	3571	0	5.055	N.D. #
13)	L3 AR-1232-3	5.285	0.000	5039	0	3.291	N.D. #
14)	L3 AR-1232-4	5.529	0.000	6890	0	8.812	N.D. #
15)	L3 AR-1232-5	5.573	0.000	5351	0	8.902	N.D. #
16)	L4 AR-1242-1	5.285	0.000	5039	0	3.969	N.D. #
17)	L4 AR-1242-2	5.285	0.000	5039	0	2.716	N.D. #
18)	L4 AR-1242-3	5.373	0.000	4679	0	4.003	N.D. #
19)	L4 AR-1242-4	5.529	0.000	6890	0	7.118	N.D. #
20)	L4 AR-1242-5	6.248	5.320	9894	23119	7.874	20.667 #
21)	L5 AR-1248-1	5.285	0.000	5039	0	5.026	N.D. #
22)	L5 AR-1248-2	5.529	0.000	6890	0	4.749	N.D. #
23)	L5 AR-1248-3	5.730	0.000	4914	0	2.956	N.D. #
24)	L5 AR-1248-4	6.125	0.000	7705	0	3.769	N.D. #
25)	L5 AR-1248-5	6.166	5.320	15738	23119	7.936	16.152 #
26)	L6 AR-1254-1	6.099	5.320	33017	23119	15.825	9.747 #
27)	L6 AR-1254-2	6.316	5.522	37486	39743	11.236	18.940 #
28)	L6 AR-1254-3	6.680	5.872	26272	46341	7.404	13.782 #
29)	L6 AR-1254-4	6.960	6.113	14444	36326	4.904	17.618 #
30)	L6 AR-1254-5	7.374	6.493	120511	75243	38.970	24.233 #
31)	L7 AR-1260-1	6.835	5.985	98514	70182	36.543	30.796
32)	L7 AR-1260-2	7.091	6.173	117698	72324	31.720	24.685
33)	L7 AR-1260-3	7.445	6.320	90682	61002	27.678	23.027
34)	L7 AR-1260-4	7.671	6.783	105773	50302	34.439	22.232 #
35)	L7 AR-1260-5	7.978	7.025	217128	101707	30.664	18.481 #
36)	L8 AR-1262-1	7.502	6.527	50055	62459	10.314	16.756 #
37)	L8 AR-1262-2	8.031	7.025	43354	101707	5.619	17.300 #
38)	L8 AR-1262-3	8.277	7.299	119159	57533	23.354	22.642
39)	L8 AR-1262-4	8.325	7.364	183160	81055	47.516	18.343 #
40)	L8 AR-1262-5	8.954	7.858	32130	34871	12.519	19.313 #
41)	L9 AR-1268-1	8.277	7.299	119159	57533	12.662	8.079 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 10:24
 Operator : SM/AJ
 Sample : K4479-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU19-FLDDCAP1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:13:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.325	7.364	183160	81055	23.236	12.571 #
43) L9	AR-1268-3	8.613	0.000	56197	0	7.972	N.D. #
44) L9	AR-1268-4	8.954	7.858	32130	34871	11.557	17.083 #
45) L9	AR-1268-5	9.363	8.124	16872	11007	0.915	0.758



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
Data File : P0060222.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2019 10:24
Operator : SM/AJ
Sample : K4479-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
SU19-FLDDCAP1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:13:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

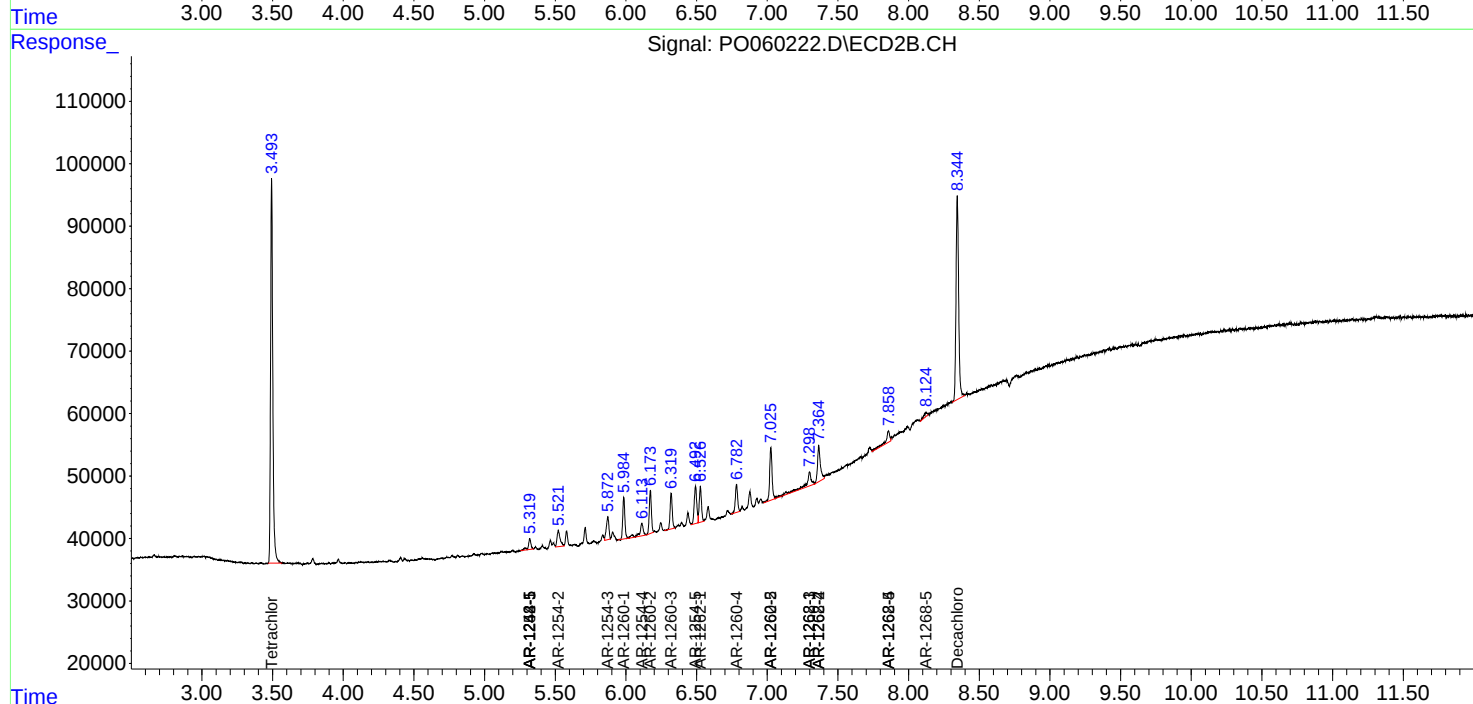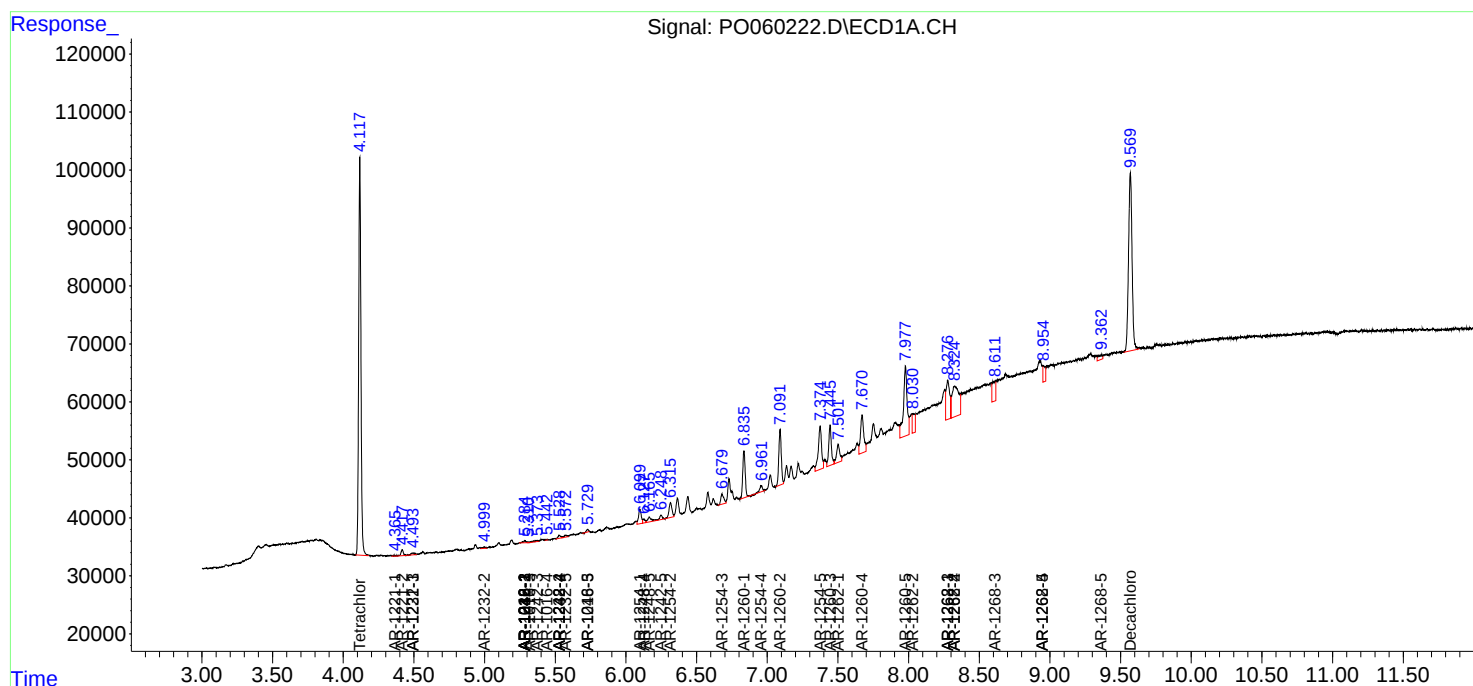


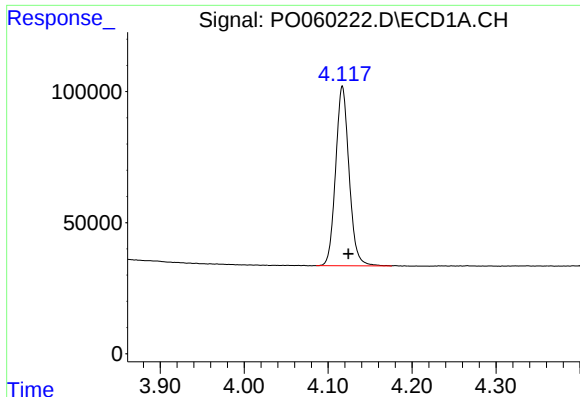

#1 Tetrachloro-m-xylene


R.T.: 4.117 min
Delta R.T.: -0.007 min
Response: 763551
Conc: 21.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

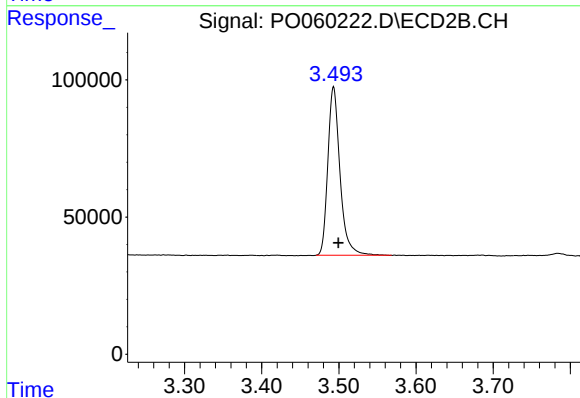


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: -0.006 min
Response: 675547
Conc: 18.77 ng/ml

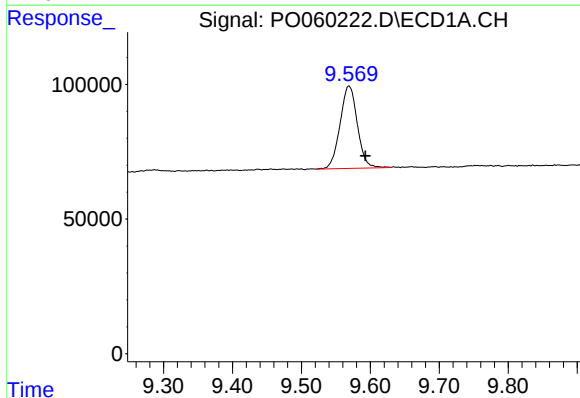


#2 Decachlorobiphenyl

R.T.: 9.569 min
Delta R.T.: -0.024 min
Response: 534114
Conc: 10.04 ng/ml

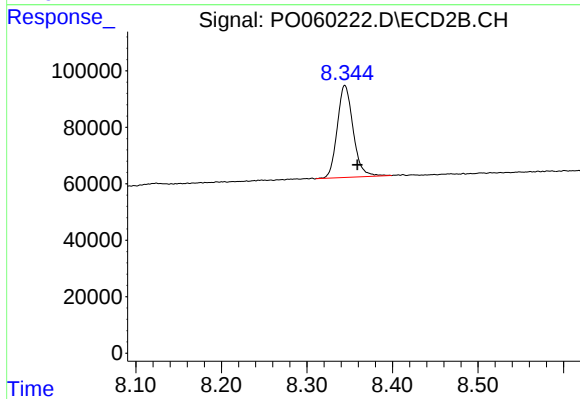

#2 Decachlorobiphenyl


R.T.: 8.344 min
Delta R.T.: -0.015 min
Response: 420528
Conc: 10.43 ng/ml

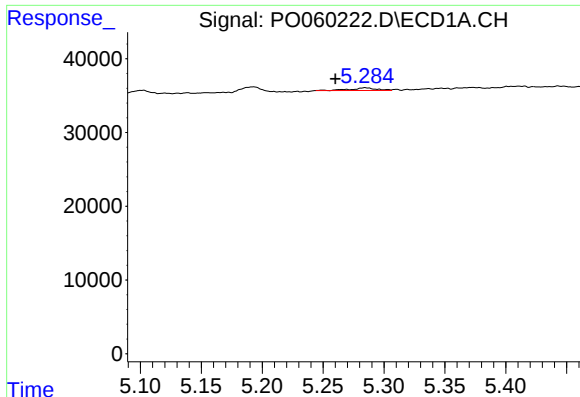

#3 AR-1016-1


R.T.: 5.285 min
Delta R.T.: 0.025 min
Response: 5039
Conc: 3.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

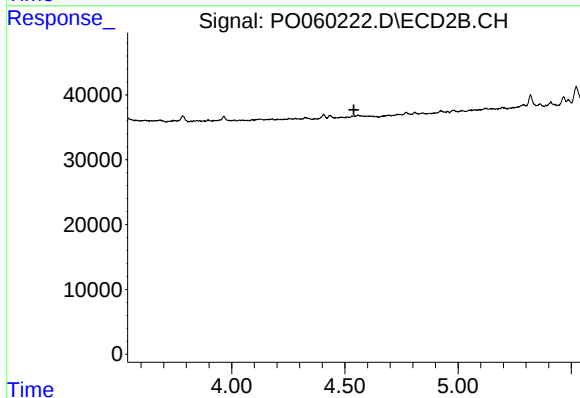


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.540 min
Response: 0
Conc: N.D.

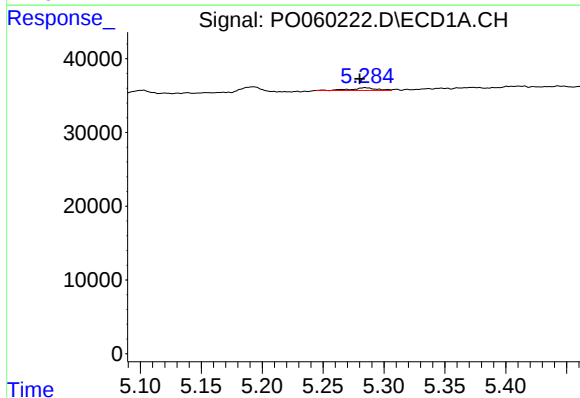


#4 AR-1016-2

R.T.: 5.285 min
Delta R.T.: 0.005 min
Response: 5039
Conc: 2.11 ng/ml

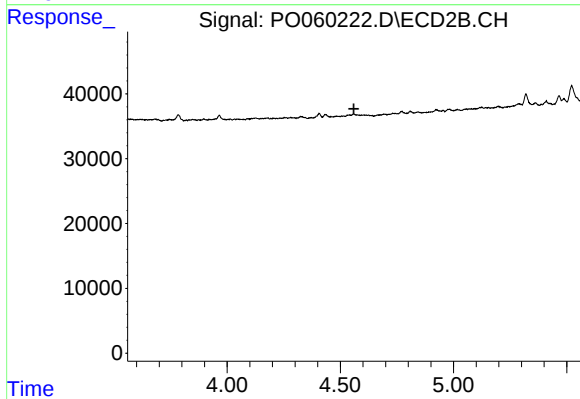

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

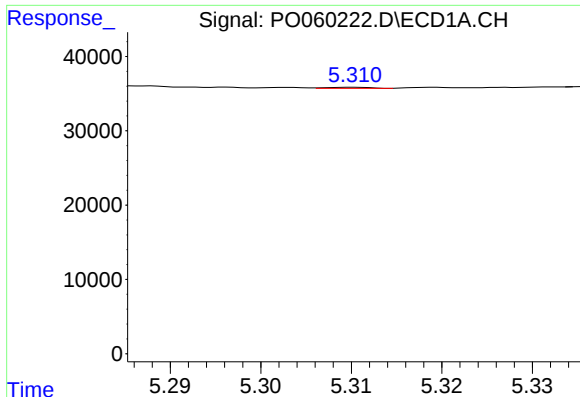

#5 AR-1016-3


R.T.: 5.310 min
Delta R.T.: -0.030 min
Response: 451
Conc: 0.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

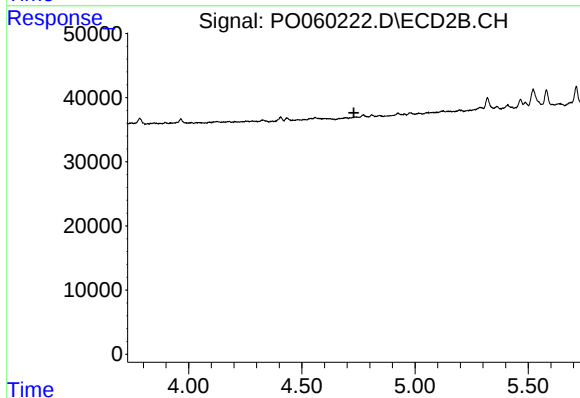


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.730 min
Response: 0
Conc: N.D.

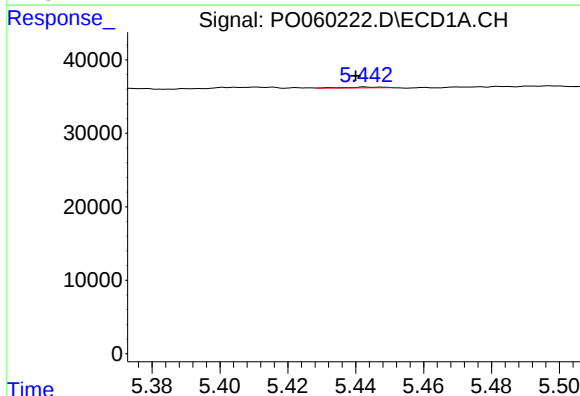


#6 AR-1016-4

R.T.: 5.443 min
Delta R.T.: 0.003 min
Response: 1026
Conc: 0.85 ng/ml

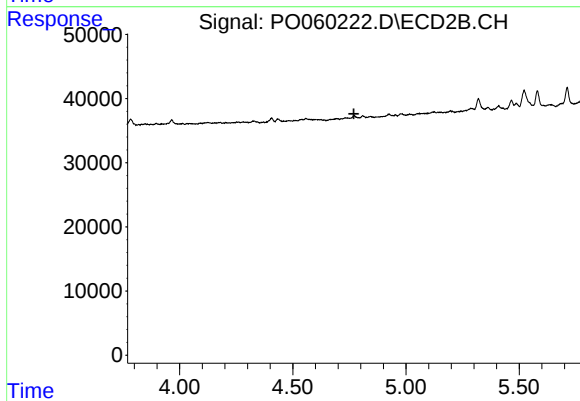

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.770 min
Response: 0
Conc: N.D.

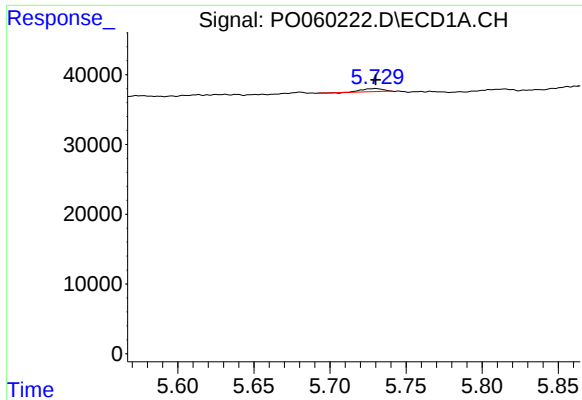

#7 AR-1016-5


R.T.: 5.730 min
Delta R.T.: 0.000 min
Response: 4914
Conc: 3.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

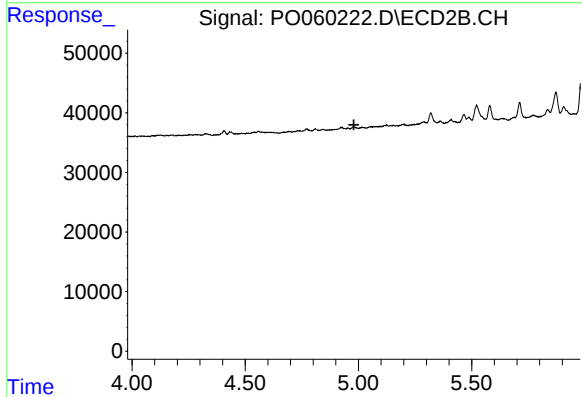


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 4.980 min
Response: 0
Conc: N.D.

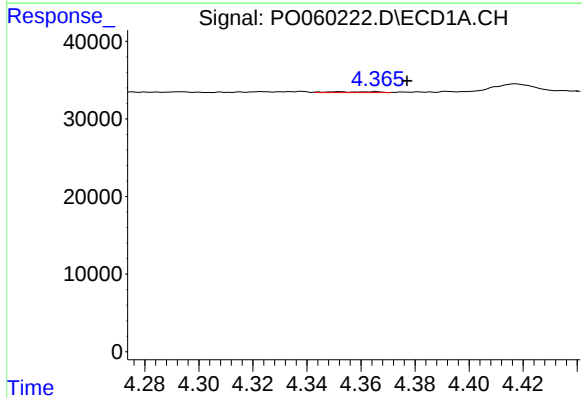


#8 AR-1221-1

R.T.: 4.365 min
Delta R.T.: -0.012 min
Response: 1175
Conc: 2.78 ng/ml

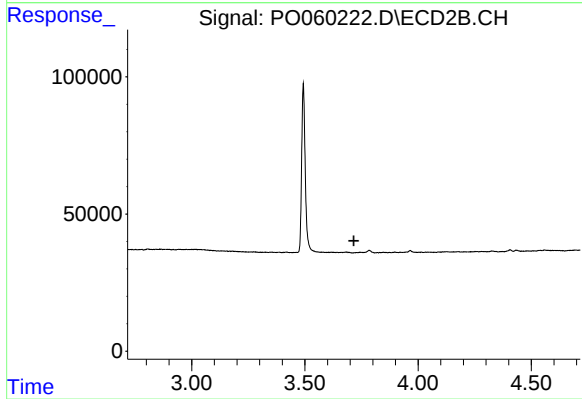

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.717 min
Response: 0
Conc: N.D.

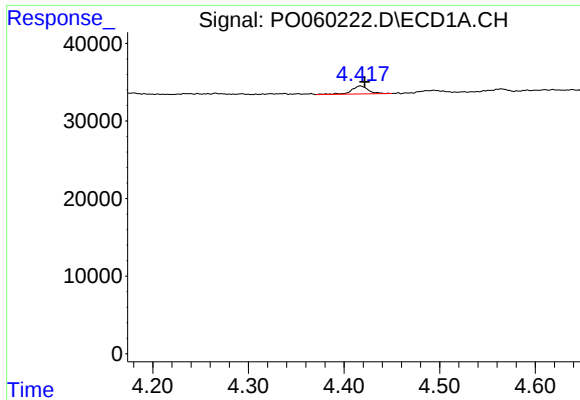

#9 AR-1221-2


R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 12338
Conc: 37.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

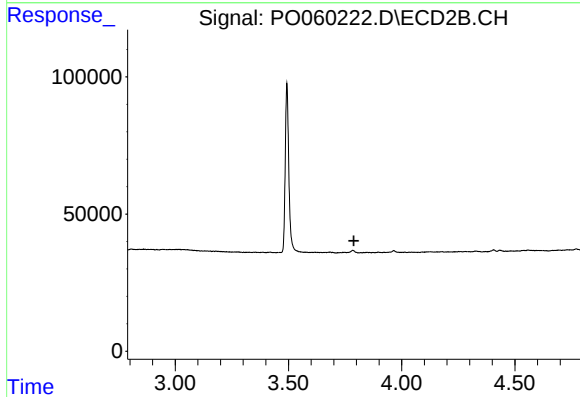


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.789 min
Response: 0
Conc: N.D.

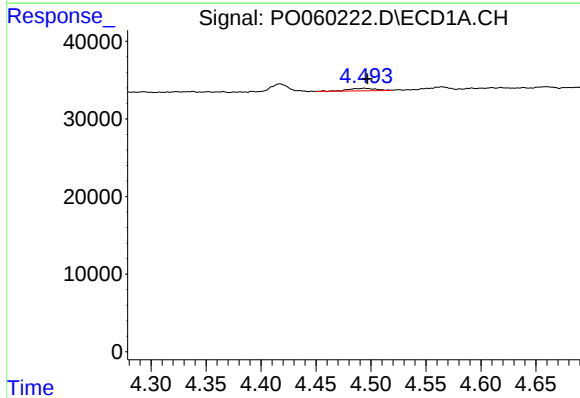


#10 AR-1221-3

R.T.: 4.494 min
Delta R.T.: -0.003 min
Response: 5597
Conc: 5.32 ng/ml

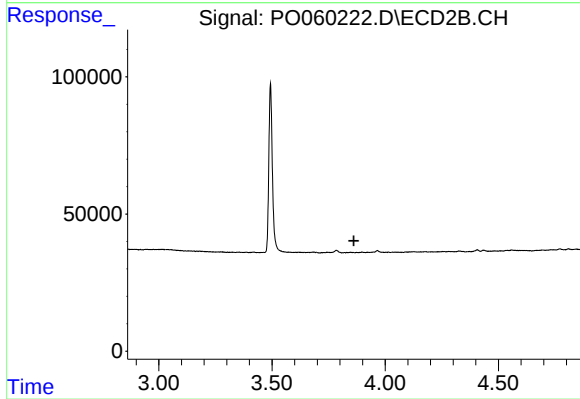

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

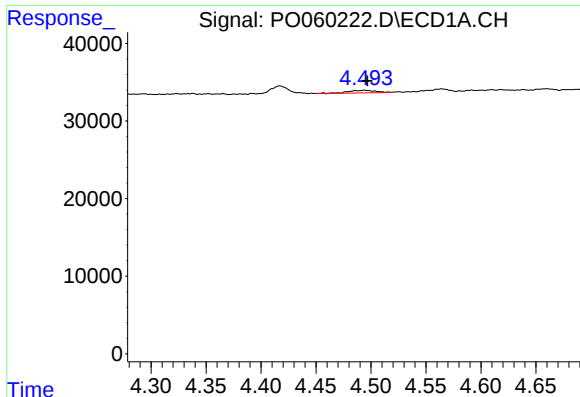

#11 AR-1232-1


R.T.: 4.494 min
Delta R.T.: -0.003 min
Response: 5597
Conc: 4.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

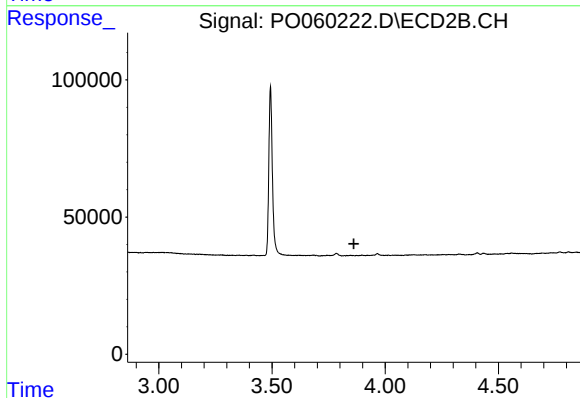


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

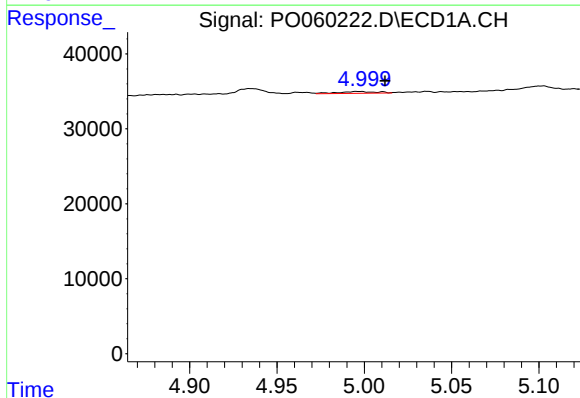


#12 AR-1232-2

R.T.: 4.997 min
Delta R.T.: -0.015 min
Response: 3571
Conc: 5.06 ng/ml

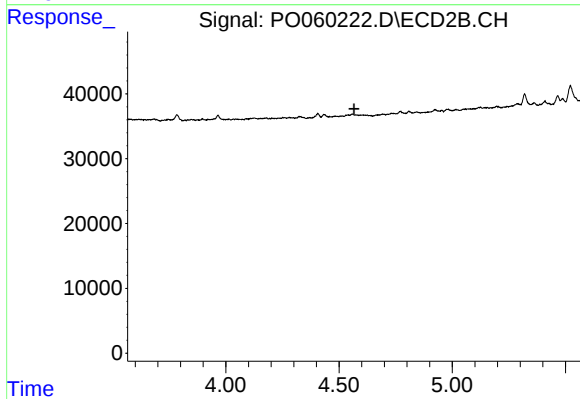

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

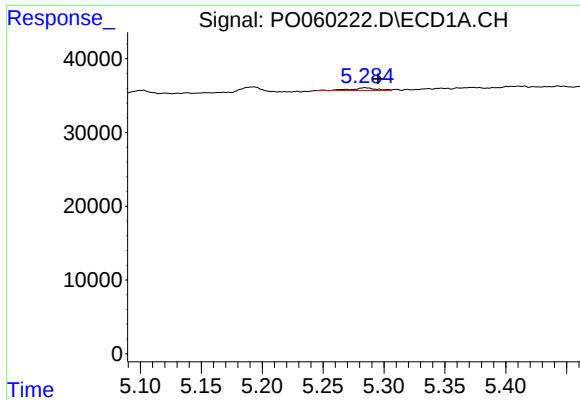

#13 AR-1232-3


R.T.: 5.285 min
Delta R.T.: -0.011 min
Response: 5039
Conc: 3.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

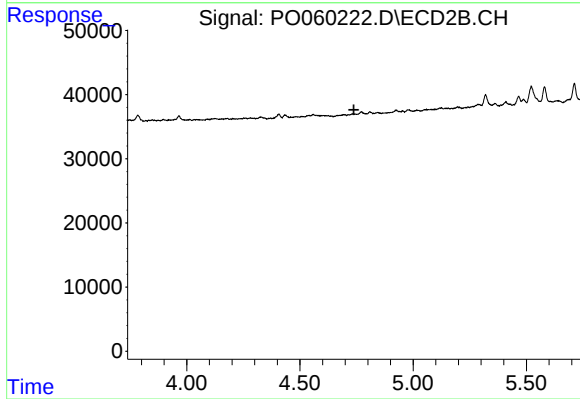


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

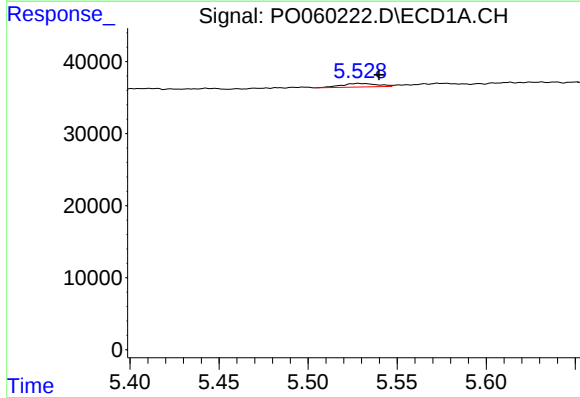


#14 AR-1232-4

R.T.: 5.529 min
Delta R.T.: -0.011 min
Response: 6890
Conc: 8.81 ng/ml

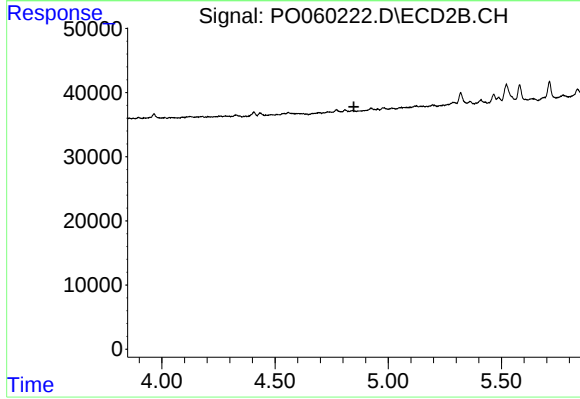

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

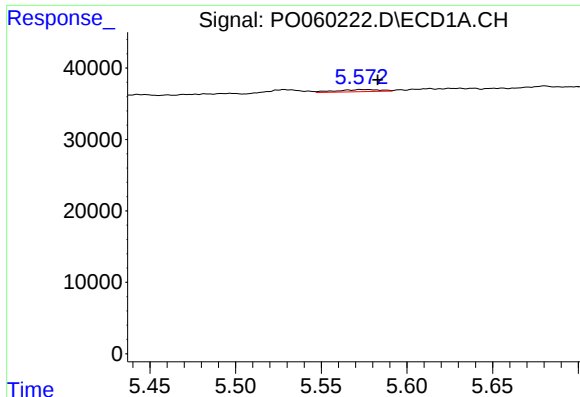

#15 AR-1232-5


R.T.: 5.573 min
Delta R.T.: -0.010 min
Response: 5351
Conc: 8.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

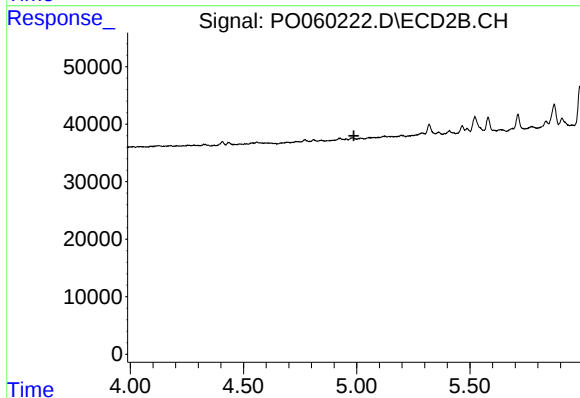


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

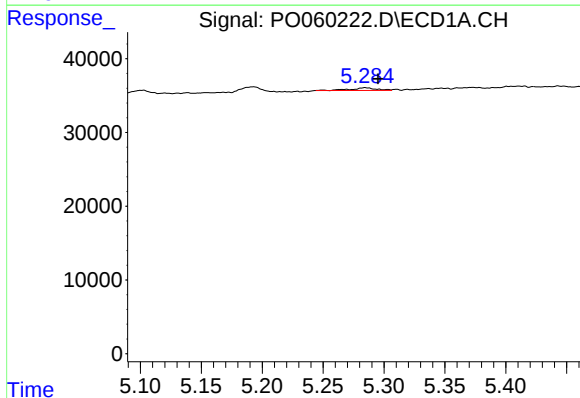


#16 AR-1242-1

R.T.: 5.285 min
Delta R.T.: -0.011 min
Response: 5039
Conc: 3.97 ng/ml

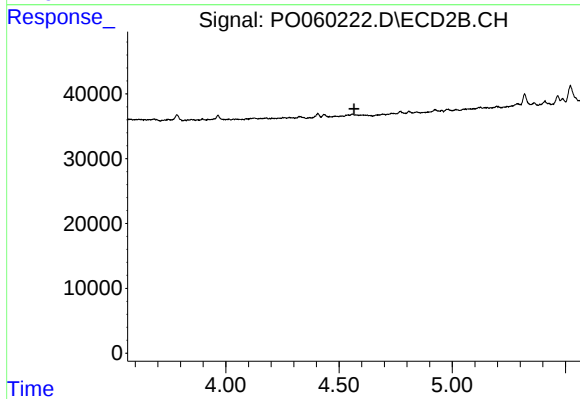

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

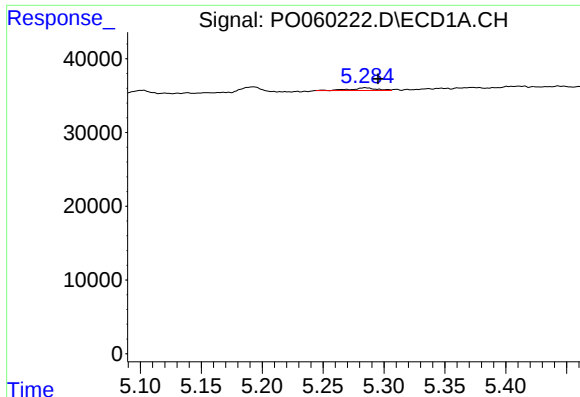

#17 AR-1242-2


R.T.: 5.285 min
Delta R.T.: -0.011 min
Response: 5039
Conc: 2.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

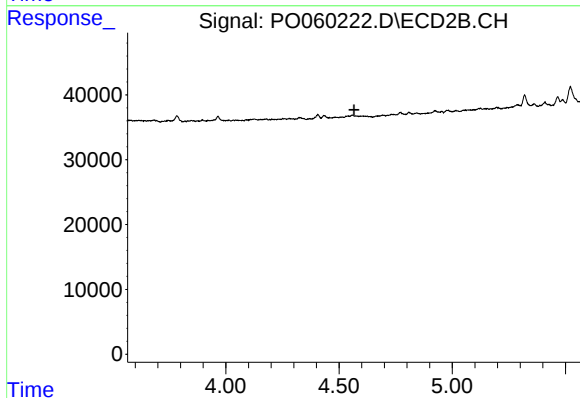


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

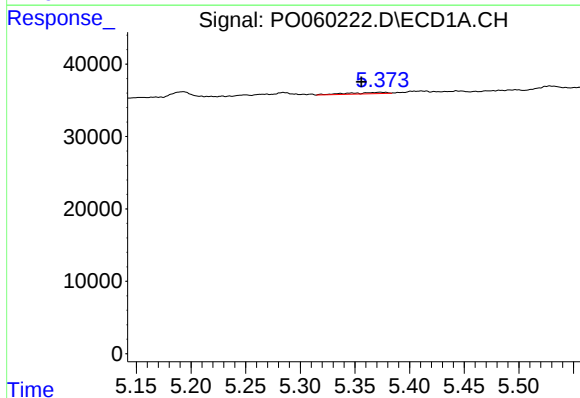


#18 AR-1242-3

R.T.: 5.373 min
Delta R.T.: 0.017 min
Response: 4679
Conc: 4.00 ng/ml

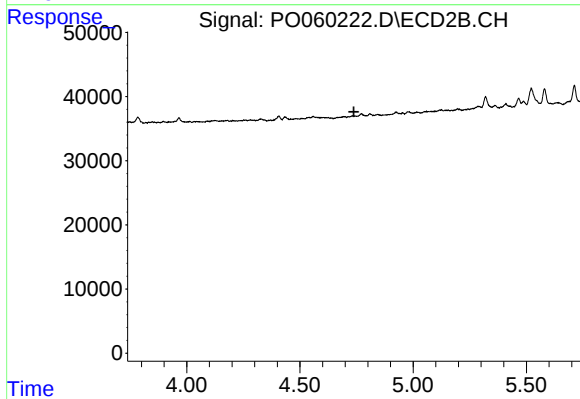

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

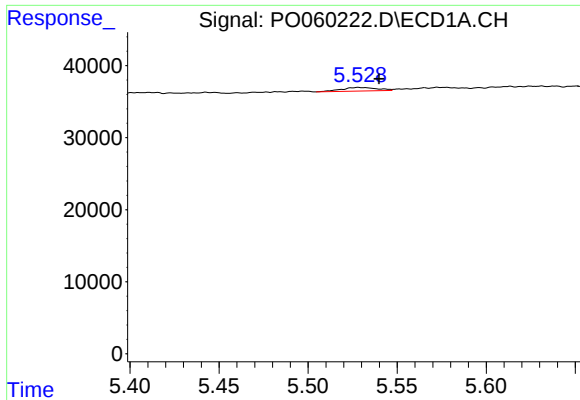

#19 AR-1242-4


R.T.: 5.529 min
Delta R.T.: -0.011 min
Response: 6890
Conc: 7.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

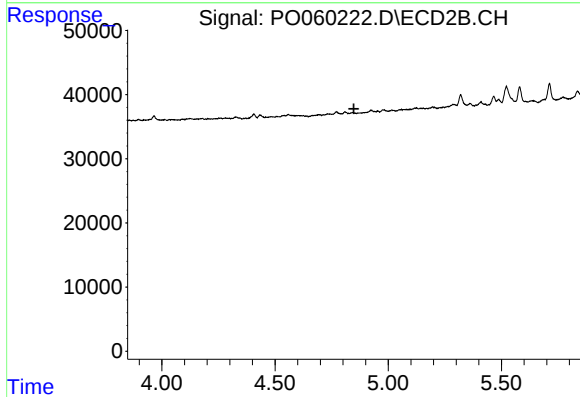


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

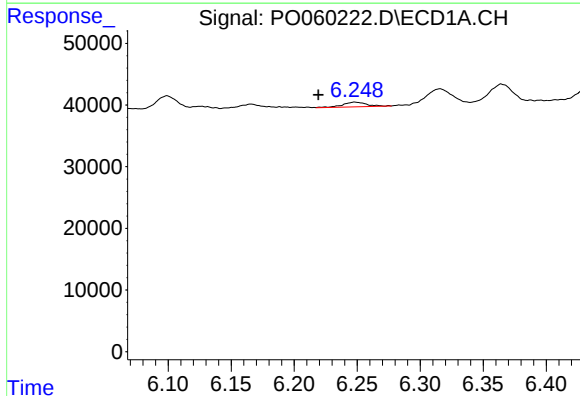


#20 AR-1242-5

R.T.: 6.248 min
Delta R.T.: 0.029 min
Response: 9894
Conc: 7.87 ng/ml

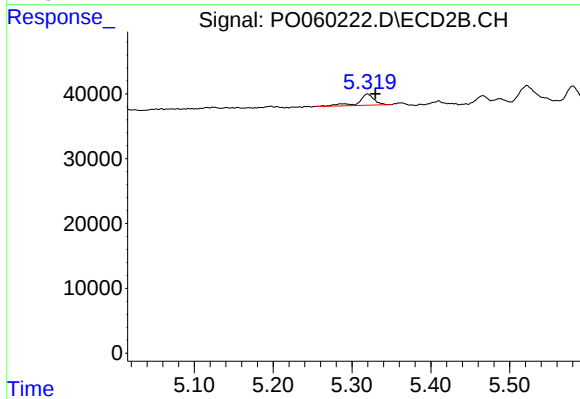

#20 AR-1242-5


R.T.: 5.320 min
Delta R.T.: -0.010 min
Response: 23119
Conc: 20.67 ng/ml

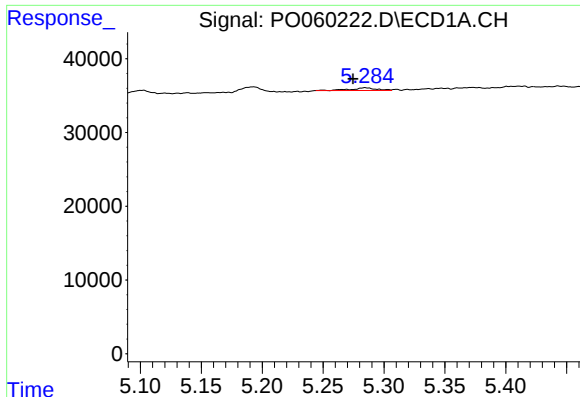

#21 AR-1248-1


R.T.: 5.285 min
Delta R.T.: 0.010 min
Response: 5039
Conc: 5.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

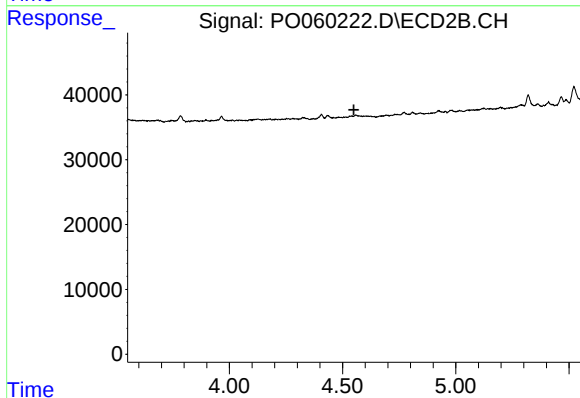


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

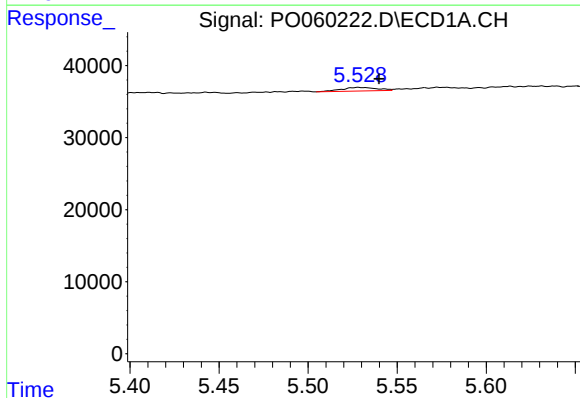


#22 AR-1248-2

R.T.: 5.529 min
Delta R.T.: -0.011 min
Response: 6890
Conc: 4.75 ng/ml

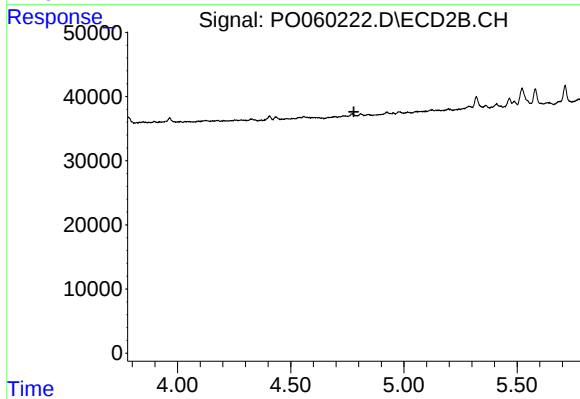

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

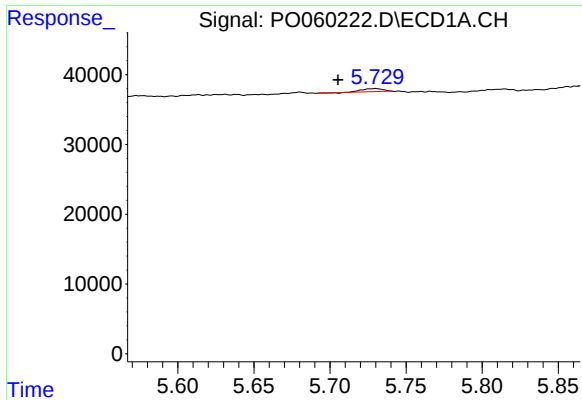

#23 AR-1248-3


R.T.: 5.730 min
Delta R.T.: 0.025 min
Response: 4914
Conc: 2.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

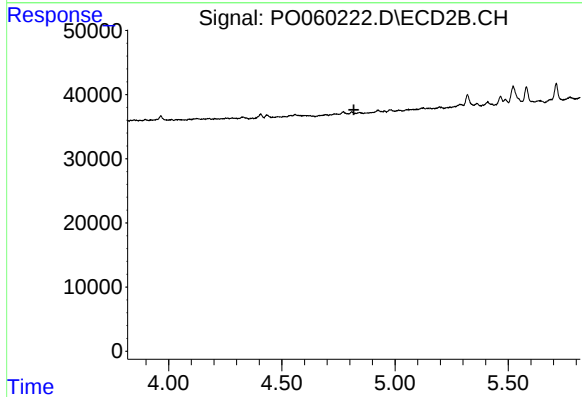


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

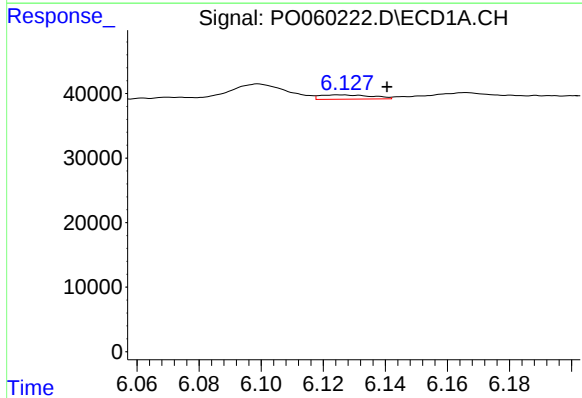


#24 AR-1248-4

R.T.: 6.125 min
Delta R.T.: -0.015 min
Response: 7705
Conc: 3.77 ng/ml

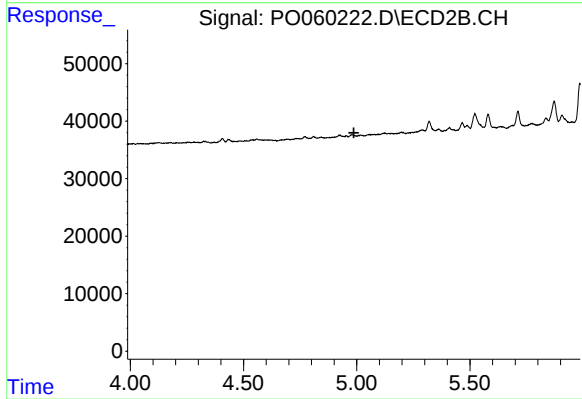

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

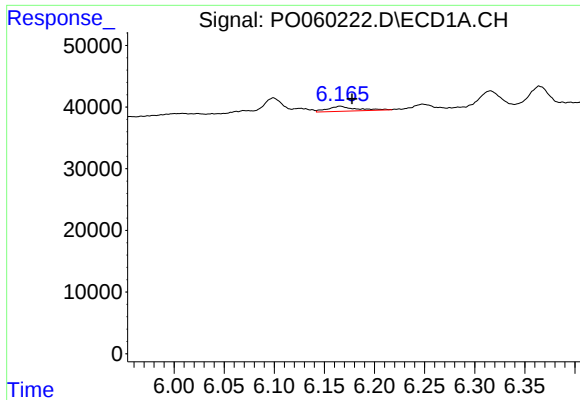

#25 AR-1248-5


R.T.: 6.166 min
Delta R.T.: -0.012 min
Response: 15738
Conc: 7.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

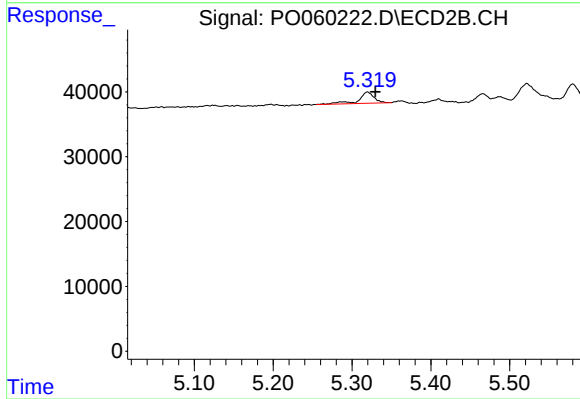


#25 AR-1248-5

R.T.: 5.320 min
Delta R.T.: -0.010 min
Response: 23119
Conc: 16.15 ng/ml

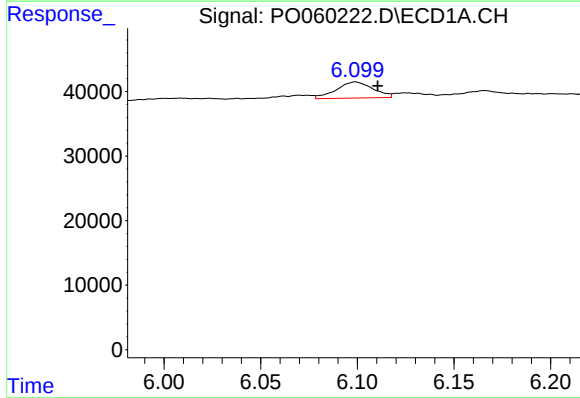


#26 AR-1254-1

R.T.: 6.099 min
Delta R.T.: -0.011 min
Response: 33017
Conc: 15.82 ng/ml

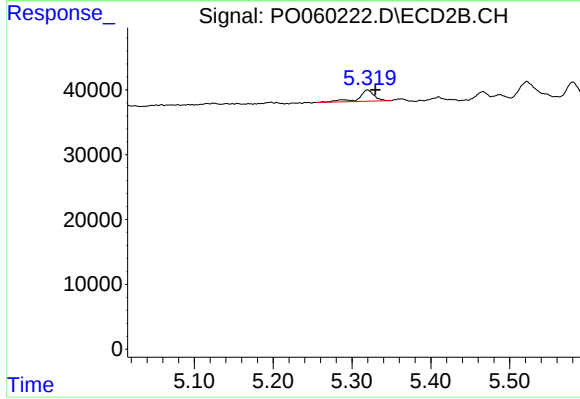

#26 AR-1254-1


R.T.: 5.320 min
Delta R.T.: -0.010 min
Response: 23119
Conc: 9.75 ng/ml

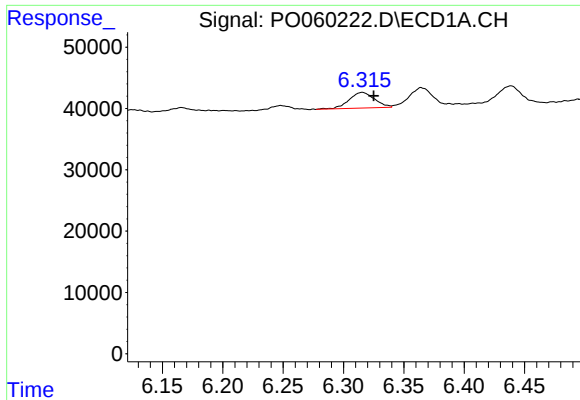

#27 AR-1254-2


R.T.: 6.316 min
Delta R.T.: -0.010 min
Response: 37486
Conc: 11.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

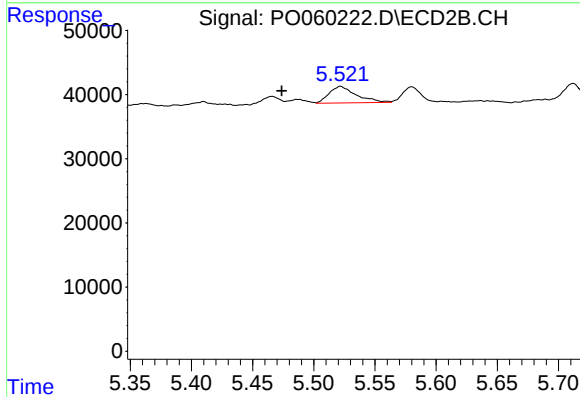


#27 AR-1254-2

R.T.: 5.522 min
Delta R.T.: 0.048 min
Response: 39743
Conc: 18.94 ng/ml

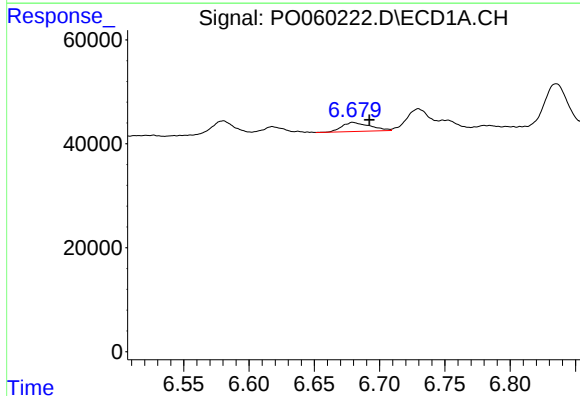


#28 AR-1254-3

R.T.: 6.680 min
Delta R.T.: -0.013 min
Response: 26272
Conc: 7.40 ng/ml

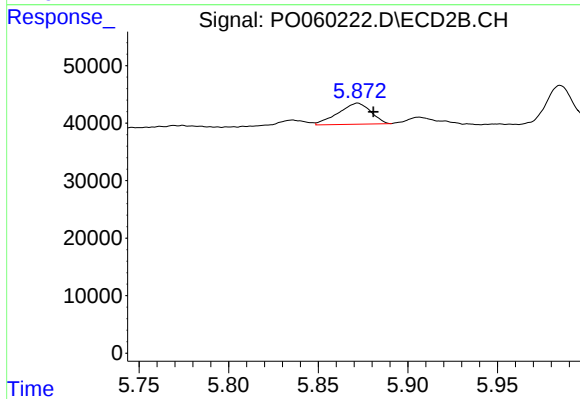

#28 AR-1254-3


R.T.: 5.872 min
Delta R.T.: -0.009 min
Response: 46341
Conc: 13.78 ng/ml

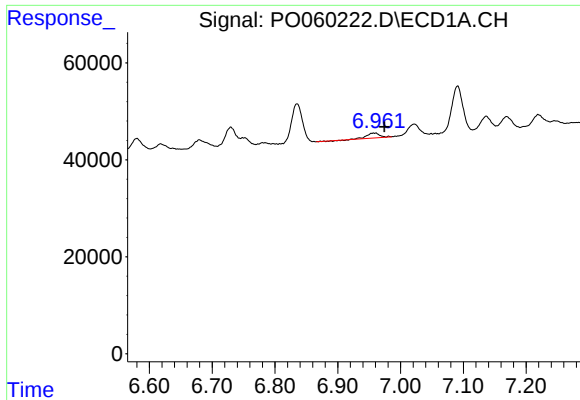

#29 AR-1254-4


R.T.: 6.960 min
Delta R.T.: -0.014 min
Response: 14444
Conc: 4.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

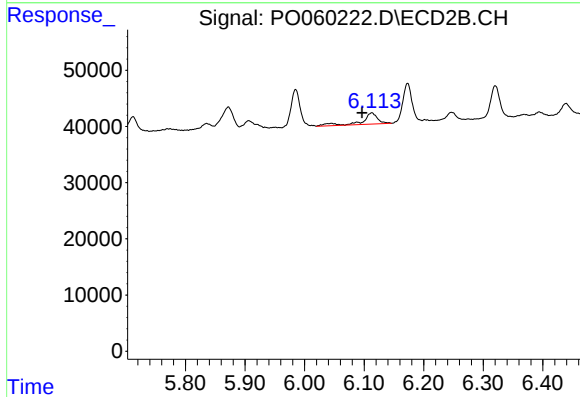


#29 AR-1254-4

R.T.: 6.113 min
Delta R.T.: 0.016 min
Response: 36326
Conc: 17.62 ng/ml

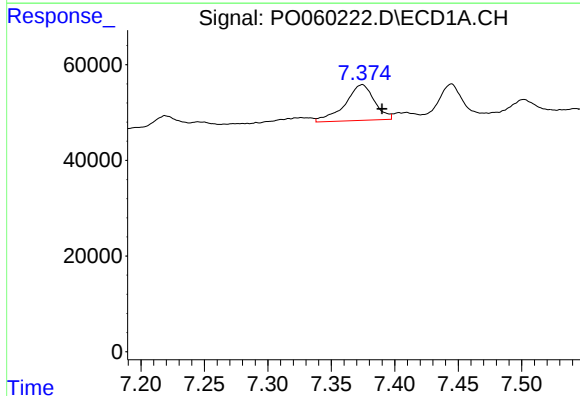


#30 AR-1254-5

R.T.: 7.374 min
Delta R.T.: -0.016 min
Response: 120511
Conc: 38.97 ng/ml

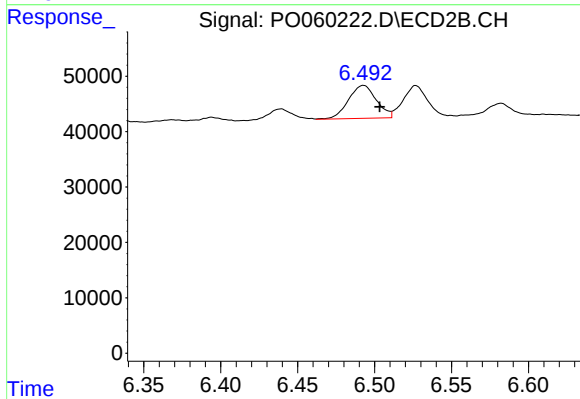

#30 AR-1254-5


R.T.: 6.493 min
Delta R.T.: -0.011 min
Response: 75243
Conc: 24.23 ng/ml

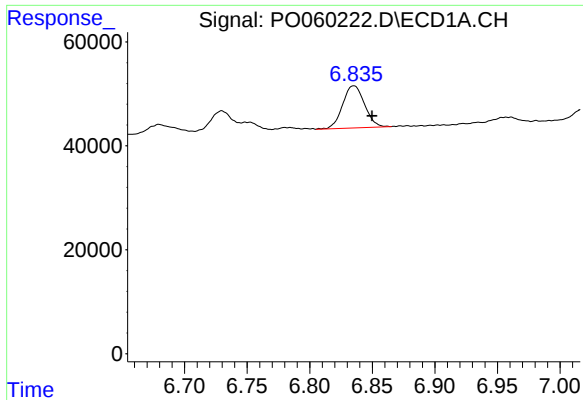

#31 AR-1260-1


R.T.: 6.835 min
Delta R.T.: -0.015 min
Response: 98514
Conc: 36.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

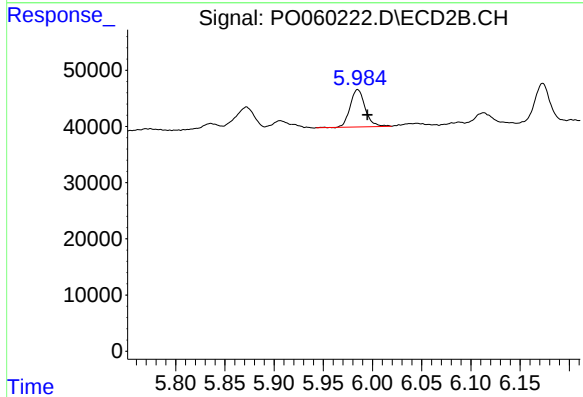


#31 AR-1260-1

R.T.: 5.985 min
Delta R.T.: -0.010 min
Response: 70182
Conc: 30.80 ng/ml

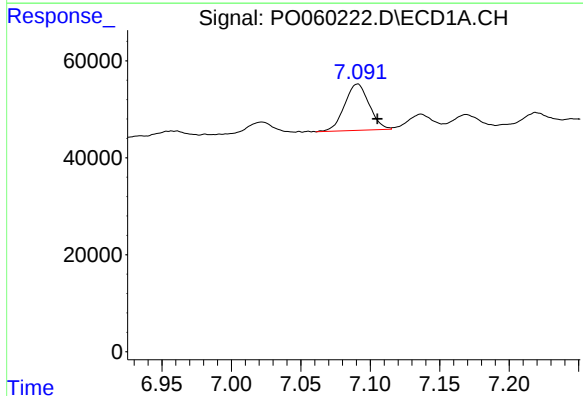


#32 AR-1260-2

R.T.: 7.091 min
Delta R.T.: -0.014 min
Response: 117698
Conc: 31.72 ng/ml

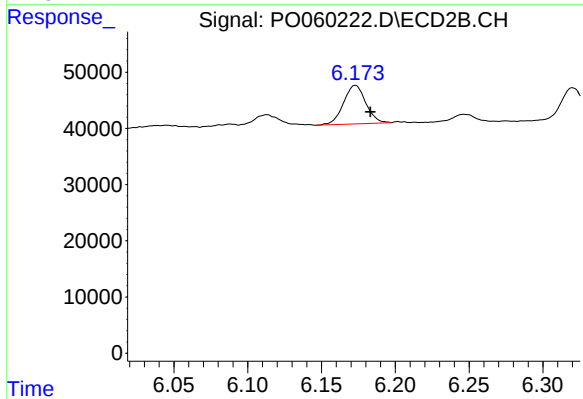

#32 AR-1260-2


R.T.: 6.173 min
Delta R.T.: -0.010 min
Response: 72324
Conc: 24.69 ng/ml

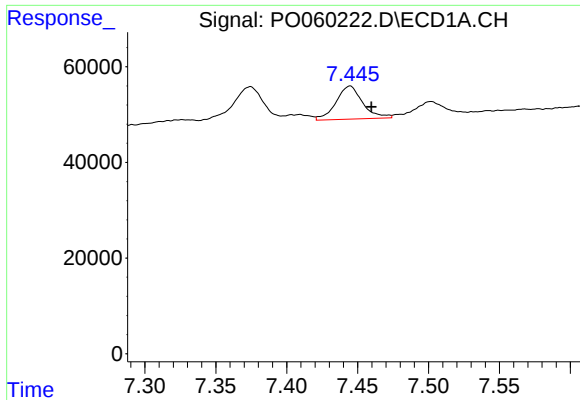

#33 AR-1260-3


R.T.: 7.445 min
Delta R.T.: -0.015 min
Response: 90682
Conc: 27.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

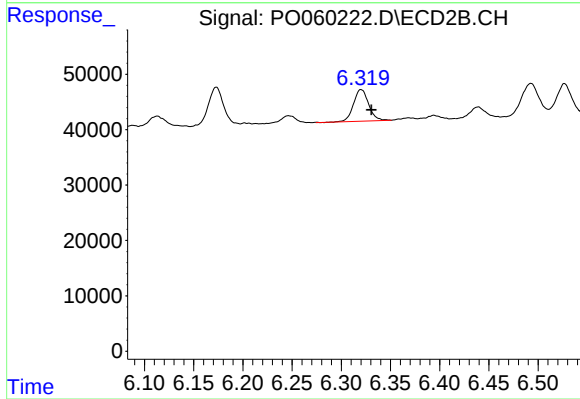


#33 AR-1260-3

R.T.: 6.320 min
Delta R.T.: -0.011 min
Response: 61002
Conc: 23.03 ng/ml

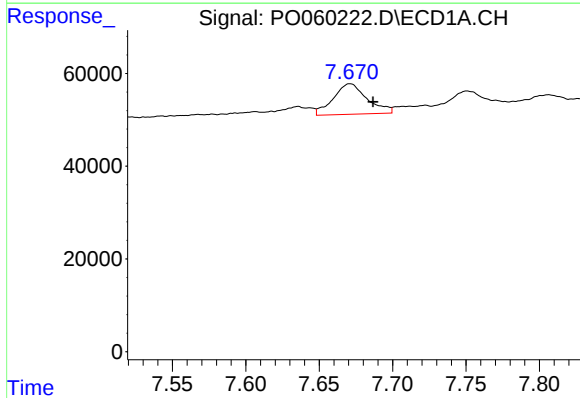


#34 AR-1260-4

R.T.: 7.671 min
Delta R.T.: -0.016 min
Response: 105773
Conc: 34.44 ng/ml

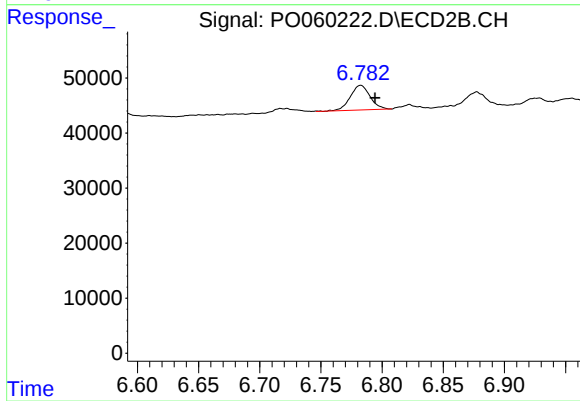

#34 AR-1260-4


R.T.: 6.783 min
Delta R.T.: -0.012 min
Response: 50302
Conc: 22.23 ng/ml

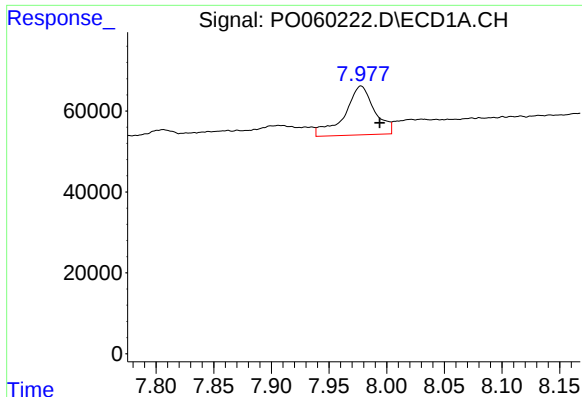

#35 AR-1260-5


R.T.: 7.978 min
Delta R.T.: -0.016 min
Response: 217128
Conc: 30.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

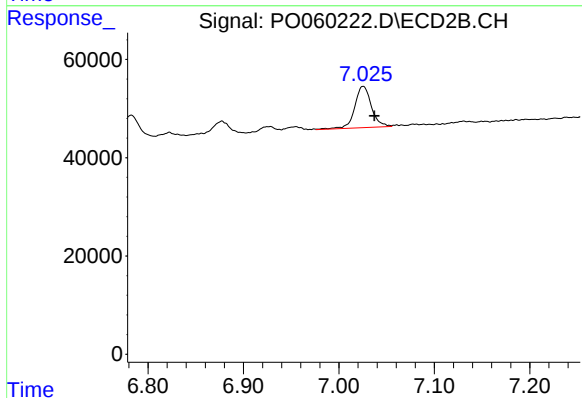


#35 AR-1260-5

R.T.: 7.025 min
Delta R.T.: -0.012 min
Response: 101707
Conc: 18.48 ng/ml

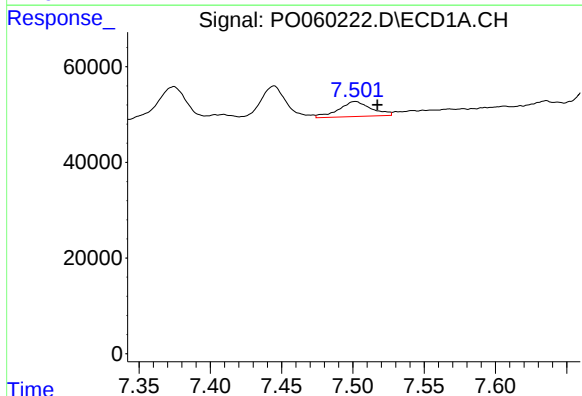


#36 AR-1262-1

R.T.: 7.502 min
Delta R.T.: -0.016 min
Response: 50055
Conc: 10.31 ng/ml

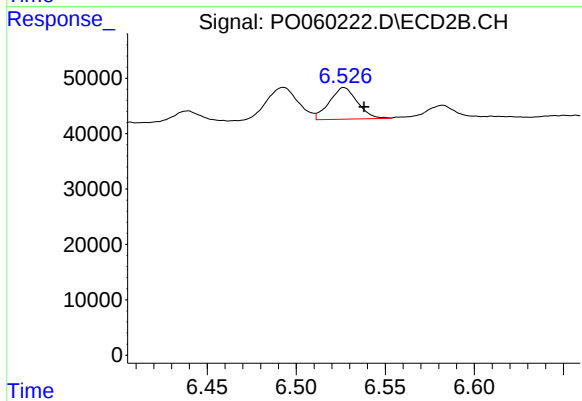

#36 AR-1262-1


R.T.: 6.527 min
Delta R.T.: -0.011 min
Response: 62459
Conc: 16.76 ng/ml

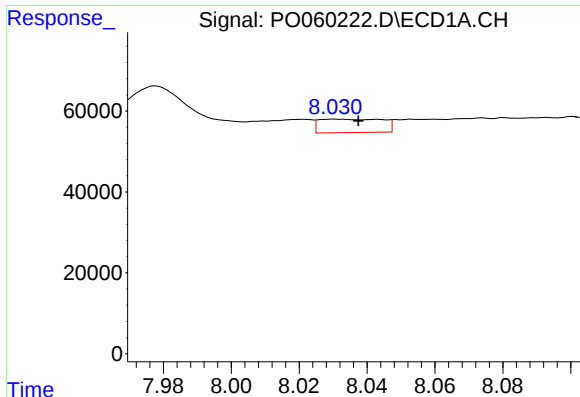

#37 AR-1262-2


R.T.: 8.031 min
Delta R.T.: -0.007 min
Response: 43354
Conc: 5.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

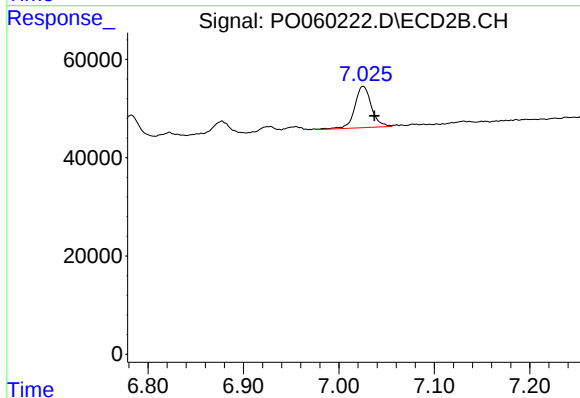


#37 AR-1262-2

R.T.: 7.025 min
Delta R.T.: -0.012 min
Response: 101707
Conc: 17.30 ng/ml

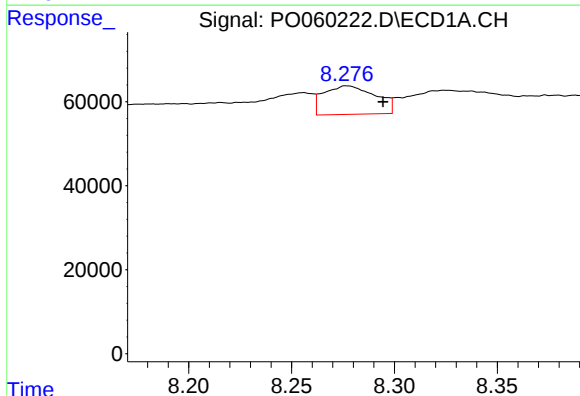


#38 AR-1262-3

R.T.: 8.277 min
Delta R.T.: -0.017 min
Response: 119159
Conc: 23.35 ng/ml

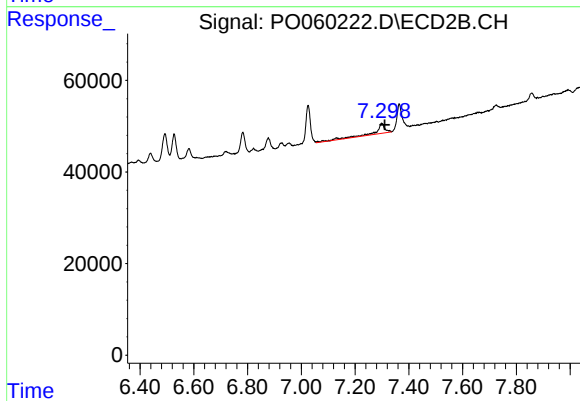

#38 AR-1262-3


R.T.: 7.299 min
Delta R.T.: -0.011 min
Response: 57533
Conc: 22.64 ng/ml

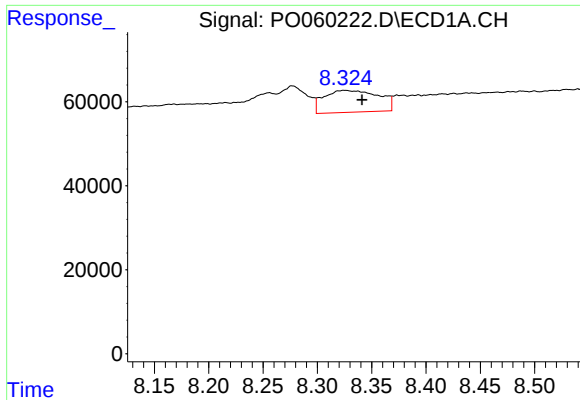

#39 AR-1262-4


R.T.: 8.325 min
Delta R.T.: -0.016 min
Response: 183160
Conc: 47.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

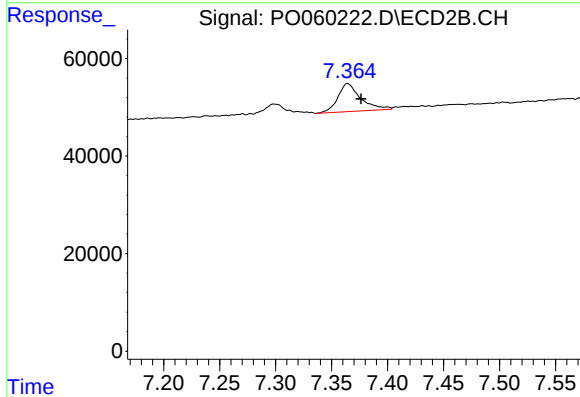


#39 AR-1262-4

R.T.: 7.364 min
Delta R.T.: -0.012 min
Response: 81055
Conc: 18.34 ng/ml

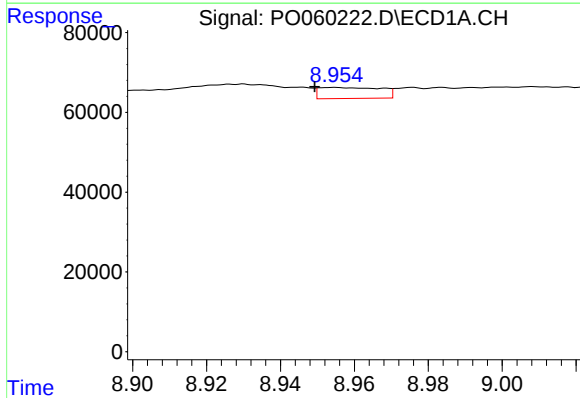


#40 AR-1262-5

R.T.: 8.954 min
Delta R.T.: 0.005 min
Response: 32130
Conc: 12.52 ng/ml

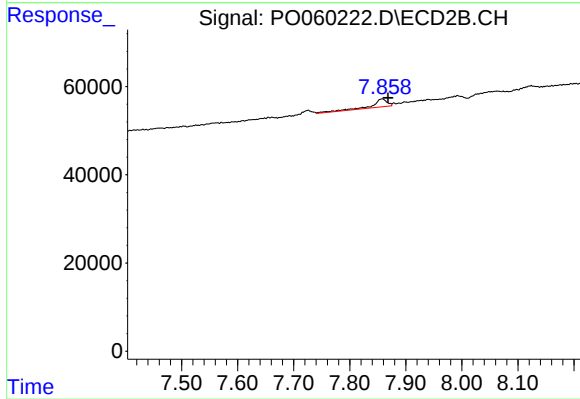

#40 AR-1262-5


R.T.: 7.858 min
Delta R.T.: -0.011 min
Response: 34871
Conc: 19.31 ng/ml

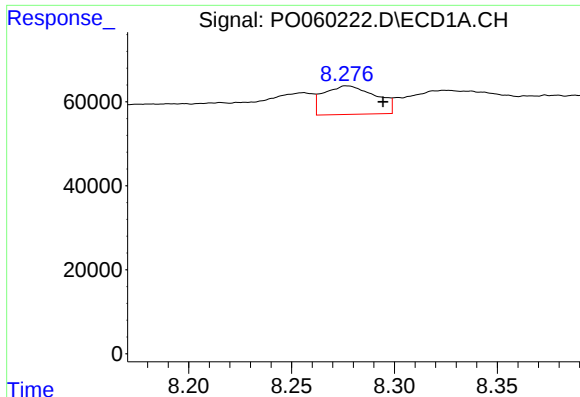

#41 AR-1268-1


R.T.: 8.277 min
Delta R.T.: -0.017 min
Response: 119159
Conc: 12.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

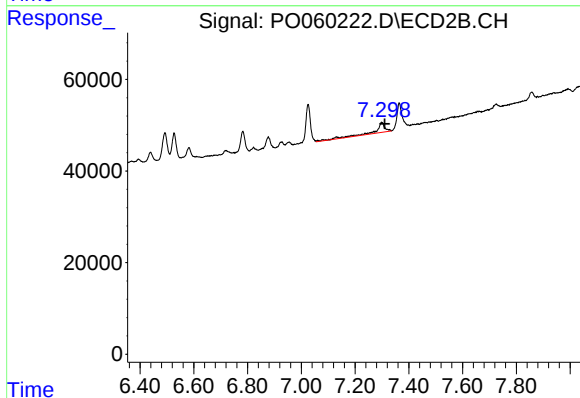


#41 AR-1268-1

R.T.: 7.299 min
Delta R.T.: -0.011 min
Response: 57533
Conc: 8.08 ng/ml

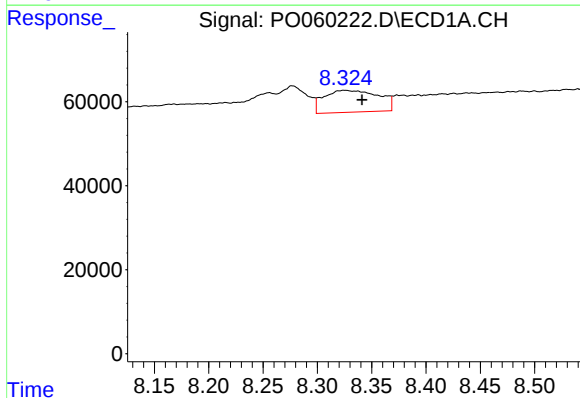


#42 AR-1268-2

R.T.: 8.325 min
Delta R.T.: -0.016 min
Response: 183160
Conc: 23.24 ng/ml

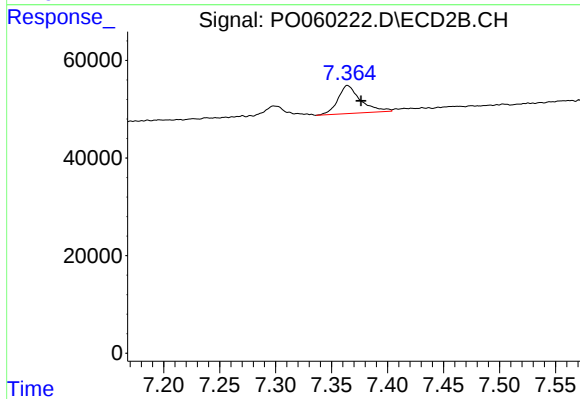

#42 AR-1268-2


R.T.: 7.364 min
Delta R.T.: -0.012 min
Response: 81055
Conc: 12.57 ng/ml

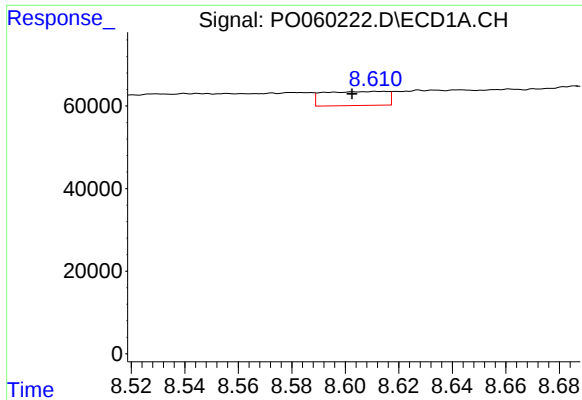

#43 AR-1268-3


R.T.: 8.613 min
Delta R.T.: 0.010 min
Response: 56197
Conc: 7.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

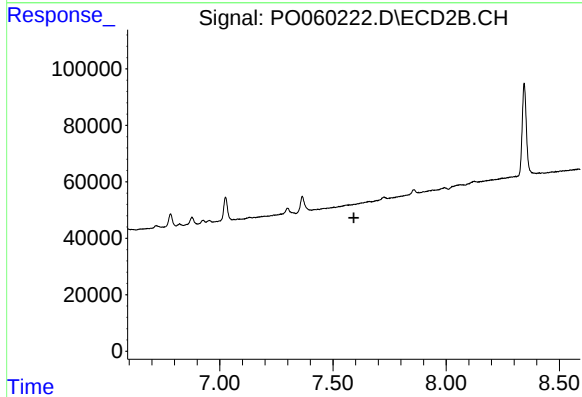


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

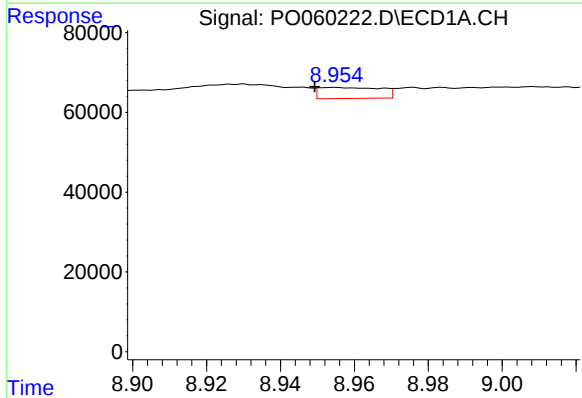


#44 AR-1268-4

R.T.: 8.954 min
Delta R.T.: 0.005 min
Response: 32130
Conc: 11.56 ng/ml

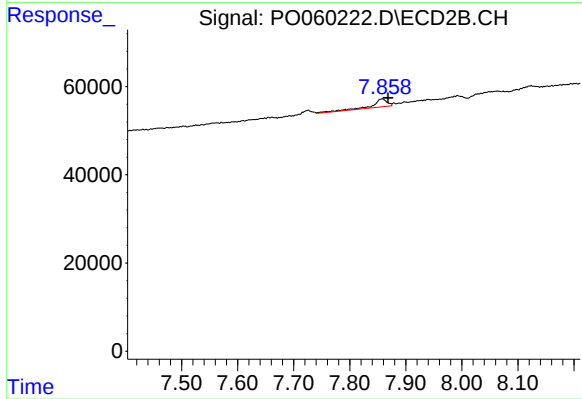

#44 AR-1268-4


R.T.: 7.858 min
Delta R.T.: -0.011 min
Response: 34871
Conc: 17.08 ng/ml

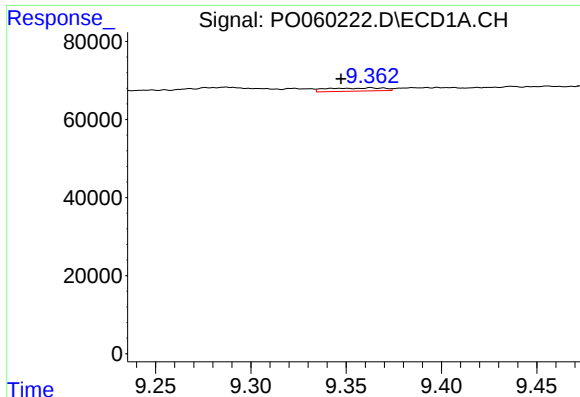

#45 AR-1268-5

R.T.: 9.363 min
Delta R.T.: 0.015 min
Response: 16872
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

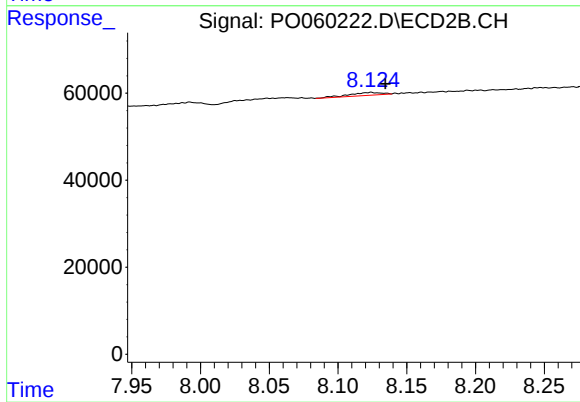

#45 AR-1268-5

R.T.: 8.124 min
Delta R.T.: -0.011 min
Response: 11007
Conc: 0.76 ng/ml