

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090319\
 Data File : P0060225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 11:16
 Operator : SM/AJ
 Sample : K4479-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SU19-FLDDCAP1RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:14:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.117	3.493	759319	673752	21.687	18.718
2)	SA Decachlor...	9.566	8.344	548561	427735	10.311	10.608
Target Compounds							
3)	L1 AR-1016-1	5.286	0.000	5986	0	3.732	N.D. #
4)	L1 AR-1016-2	5.286	0.000	5986	0	2.502	N.D. #
5)	L1 AR-1016-3	5.343	0.000	3079	0	2.067	N.D. #
6)	L1 AR-1016-4	5.413	0.000	2275	0	1.880	N.D. #
7)	L1 AR-1016-5	5.729	0.000	5257	0	4.094	N.D. #
8)	L2 AR-1221-1	4.417	0.000	12130	0	28.645	N.D. #
9)	L2 AR-1221-2	4.417	0.000	12130	0	37.348	N.D. #
10)	L2 AR-1221-3	4.491	0.000	5176	0	4.920	N.D. #
11)	L3 AR-1232-1	4.491	0.000	5176	0	4.152	N.D. #
12)	L3 AR-1232-2	5.000	0.000	2876	0	4.071	N.D. #
13)	L3 AR-1232-3	5.286	0.000	5986	0	3.909	N.D. #
14)	L3 AR-1232-4	5.529	0.000	2474	0	3.164	N.D. #
15)	L3 AR-1232-5	5.571	0.000	2807	0	4.669	N.D. #
16)	L4 AR-1242-1	5.286	0.000	5986	0	4.715	N.D. #
17)	L4 AR-1242-2	5.286	0.000	5986	0	3.226	N.D. #
18)	L4 AR-1242-3	5.343	0.000	3079	0	2.634	N.D. #
19)	L4 AR-1242-4	5.529	0.000	2474	0	2.556	N.D. #
20)	L4 AR-1242-5	6.249	5.320	14541	23785	11.571	21.263 #
21)	L5 AR-1248-1	5.286	0.000	5986	0	5.970	N.D. #
22)	L5 AR-1248-2	5.529	0.000	2474	0	1.705	N.D. #
23)	L5 AR-1248-3	5.682	0.000	3759	0	2.262	N.D. #
24)	L5 AR-1248-4	6.167	0.000	11705	0	5.726	N.D. #
25)	L5 AR-1248-5	6.167	5.320	11705	23785	5.902	16.618 #
26)	L6 AR-1254-1	6.100	5.320	59270	23785	28.408	10.028 #
27)	L6 AR-1254-2	6.315	5.521	41908	43922	12.561	20.932 #
28)	L6 AR-1254-3	6.679	5.871	28988	48481	8.169	14.418 #
29)	L6 AR-1254-4	6.959	6.113	16601	28930	5.636	14.031 #
30)	L6 AR-1254-5	7.374	6.493	134846	74446	43.606	23.976 #
31)	L7 AR-1260-1	6.835	5.985	101398	71094	37.613	31.196
32)	L7 AR-1260-2	7.091	6.173	120943	72448	32.595	24.727
33)	L7 AR-1260-3	7.444	6.321	91283	62476	27.861	23.584
34)	L7 AR-1260-4	7.671	6.782	104026	50280	33.870	22.223 #
35)	L7 AR-1260-5	7.977	7.027	237337	107440	33.518	19.523 #
36)	L8 AR-1262-1	7.501	6.527	48122	63143	9.916	16.940 #
37)	L8 AR-1262-2	8.024	7.027	78011	107440	10.110	18.275 #
38)	L8 AR-1262-3	8.276	7.299	283197	54929	55.504	21.618 #
39)	L8 AR-1262-4	8.322	7.364	174035	85450	45.148	19.337 #
40)	L8 AR-1262-5	8.925	7.857	208973	65247	81.421	36.137 #
41)	L9 AR-1268-1	8.276	7.299	283197	54929	30.093	7.714 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 11:16
 Operator : SM/AJ
 Sample : K4479-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU19-FLDDCAP1RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:14:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.322	7.364	174035	85450	22.078	13.252 #
43) L9	AR-1268-3	8.639	0.000	330049	0	46.823	N.D. #
44) L9	AR-1268-4	8.925	7.857	208973	65247	75.169	31.964 #
45) L9	AR-1268-5	9.350	8.119	17222	43560	0.934	2.998 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
Data File : P0060225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2019 11:16
Operator : SM/AJ
Sample : K4479-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:14:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

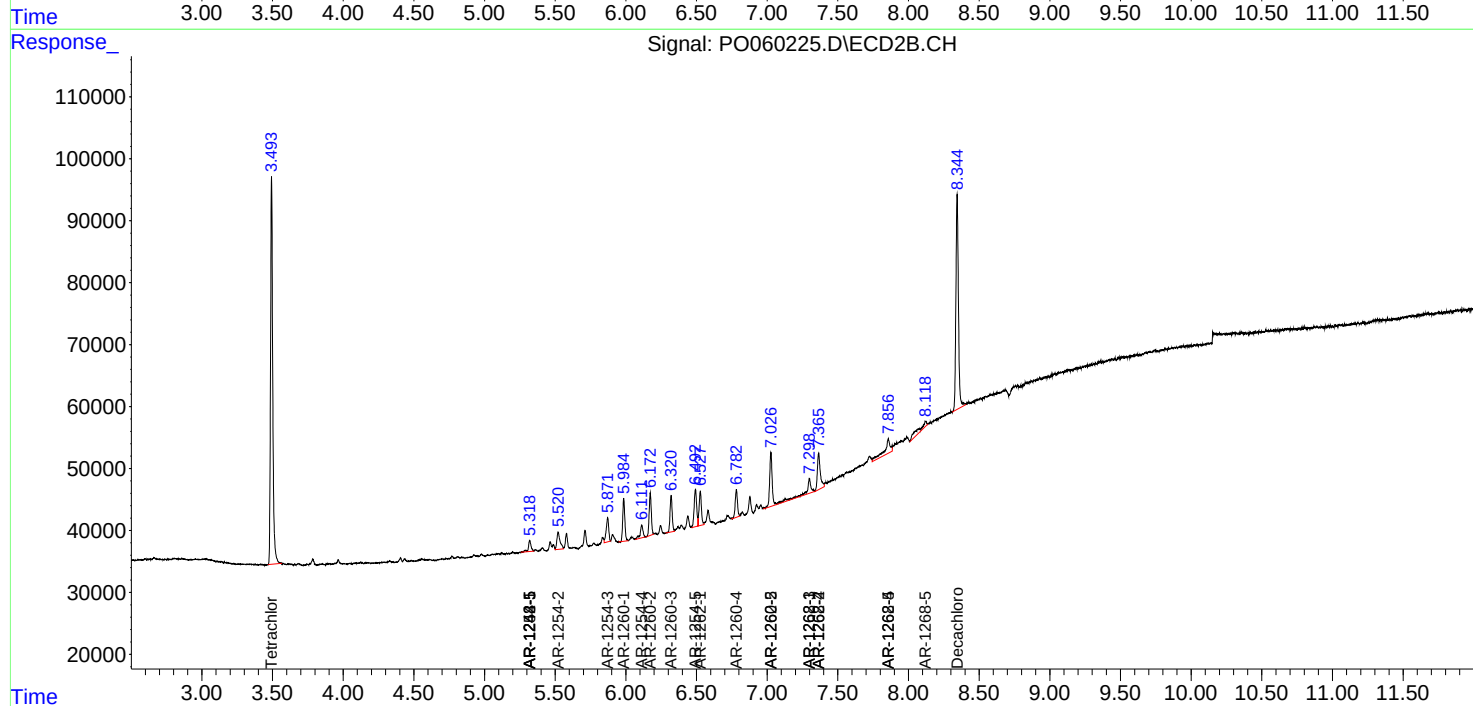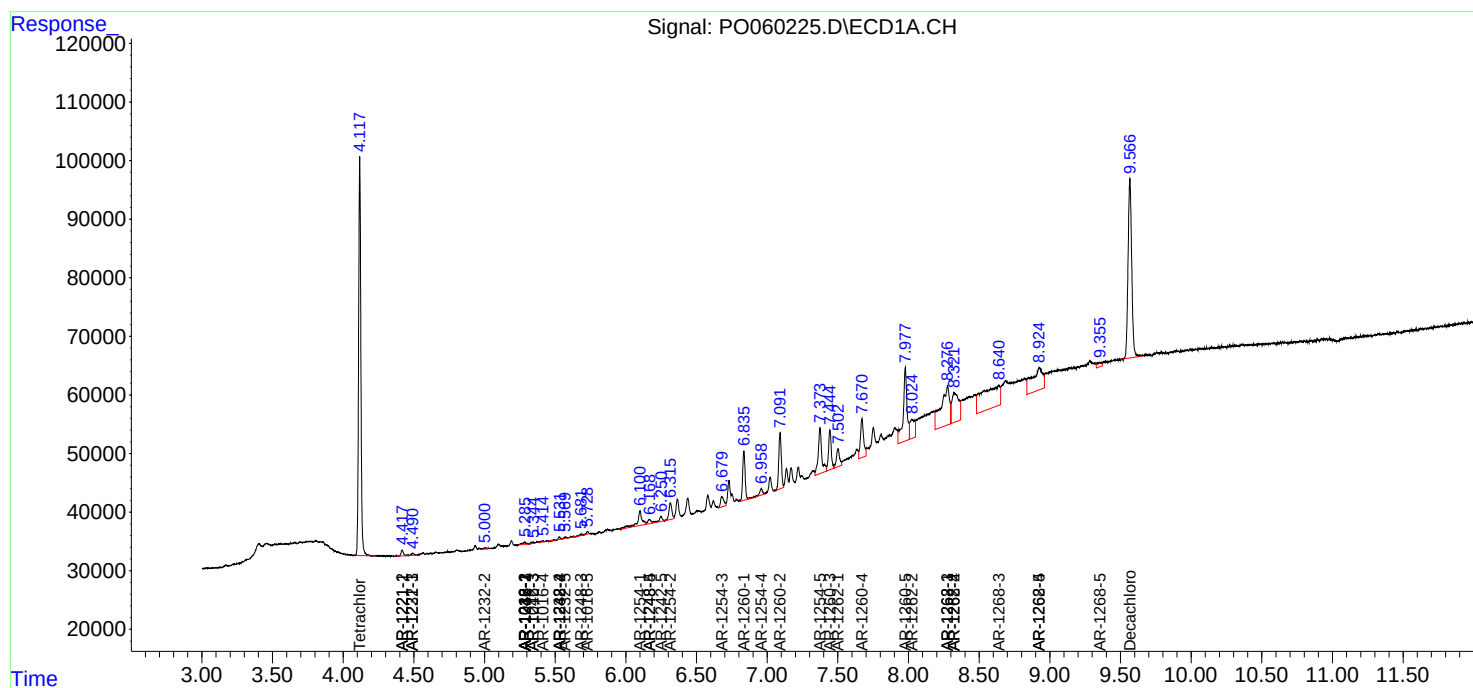


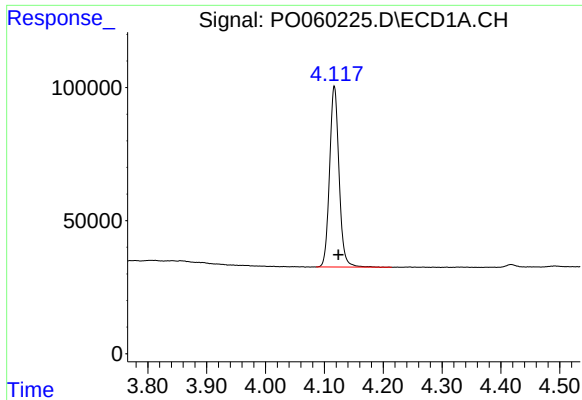

#1 Tetrachloro-m-xylene


R.T.: 4.117 min
Delta R.T.: -0.007 min
Response: 759319
Conc: 21.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

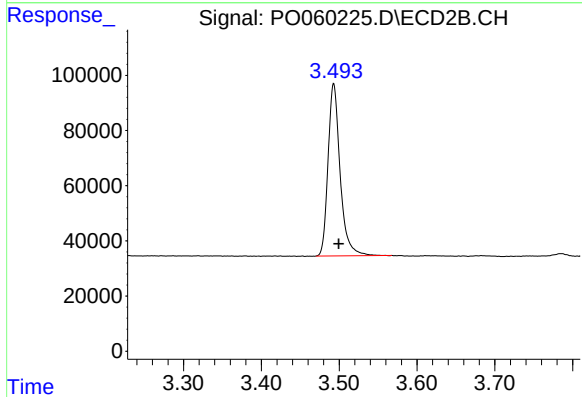


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: -0.006 min
Response: 673752
Conc: 18.72 ng/ml

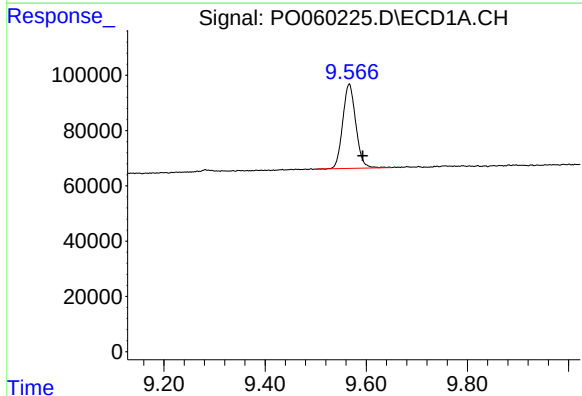


#2 Decachlorobiphenyl

R.T.: 9.566 min
Delta R.T.: -0.027 min
Response: 548561
Conc: 10.31 ng/ml

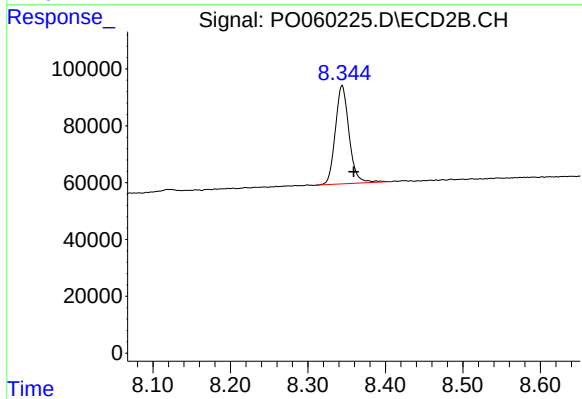

#2 Decachlorobiphenyl


R.T.: 8.344 min
Delta R.T.: -0.015 min
Response: 427735
Conc: 10.61 ng/ml

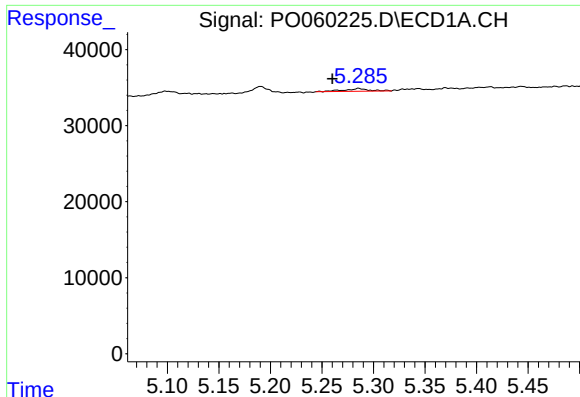

#3 AR-1016-1


R.T.: 5.286 min
Delta R.T.: 0.026 min
Response: 5986
Conc: 3.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

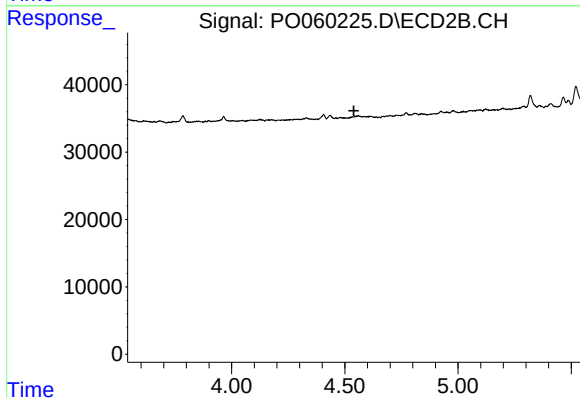


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.540 min
Response: 0
Conc: N.D.

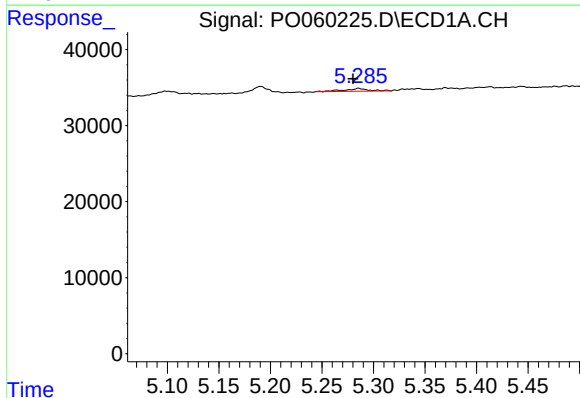


#4 AR-1016-2

R.T.: 5.286 min
Delta R.T.: 0.006 min
Response: 5986
Conc: 2.50 ng/ml

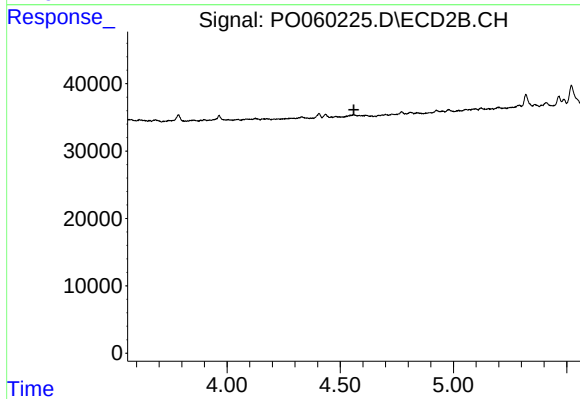

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

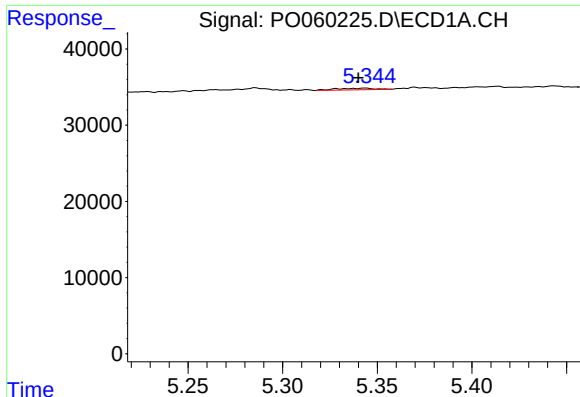

#5 AR-1016-3


R.T.: 5.343 min
Delta R.T.: 0.003 min
Response: 3079
Conc: 2.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

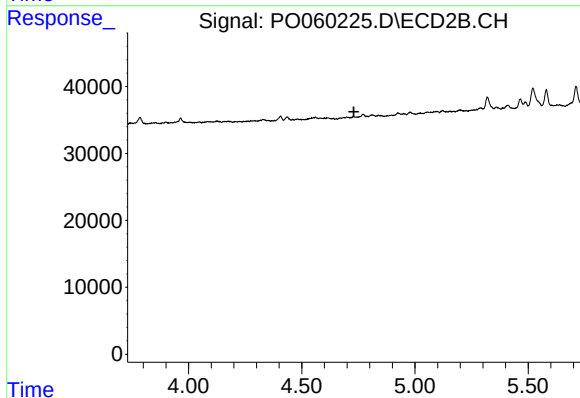


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.730 min
Response: 0
Conc: N.D.

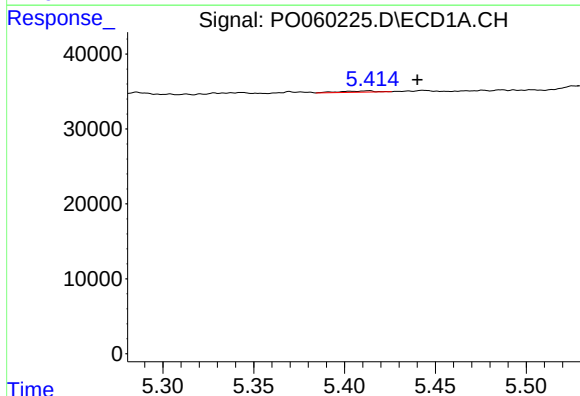


#6 AR-1016-4

R.T.: 5.413 min
Delta R.T.: -0.027 min
Response: 2275
Conc: 1.88 ng/ml

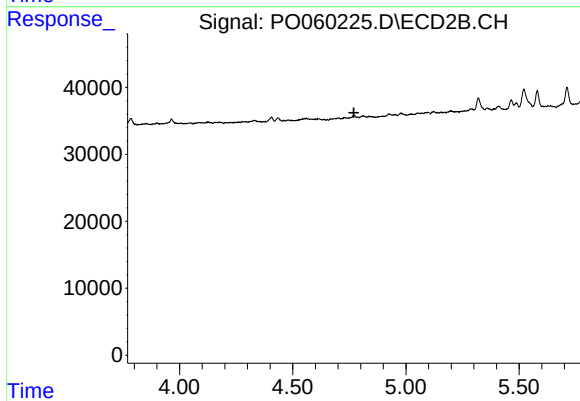

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.770 min
Response: 0
Conc: N.D.

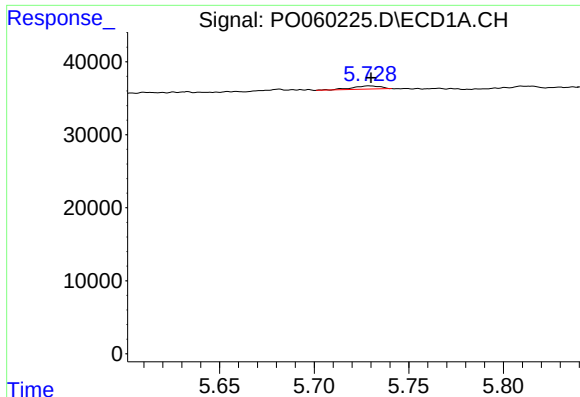

#7 AR-1016-5


R.T.: 5.729 min
Delta R.T.: 0.000 min
Response: 5257
Conc: 4.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

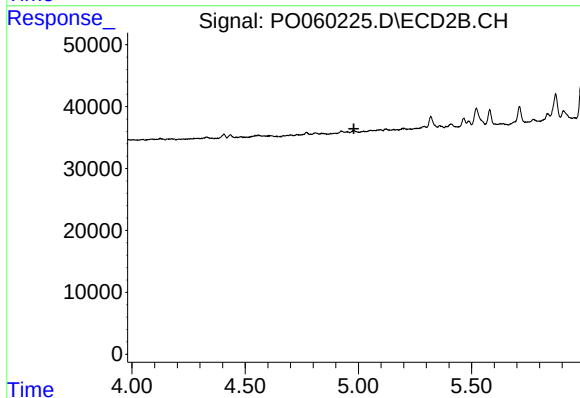


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 4.980 min
Response: 0
Conc: N.D.

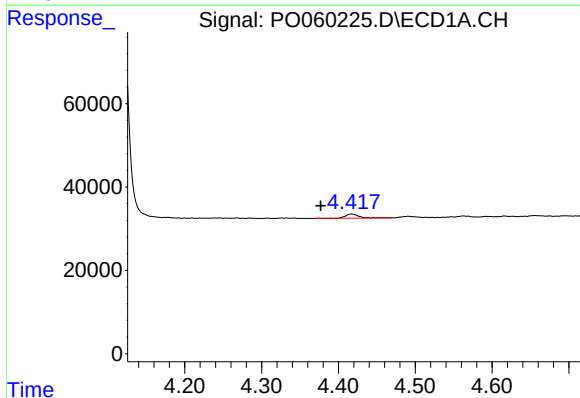


#8 AR-1221-1

R.T.: 4.417 min
Delta R.T.: 0.040 min
Response: 12130
Conc: 28.65 ng/ml

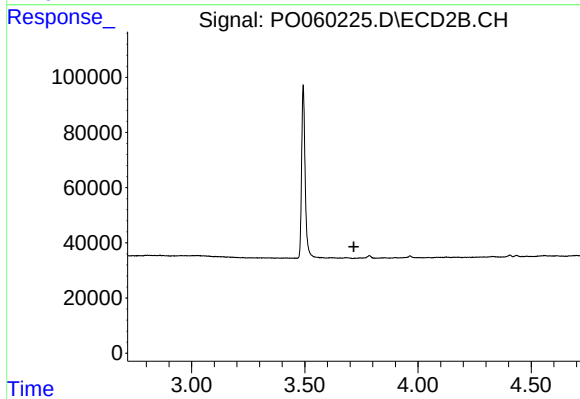

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.717 min
Response: 0
Conc: N.D.

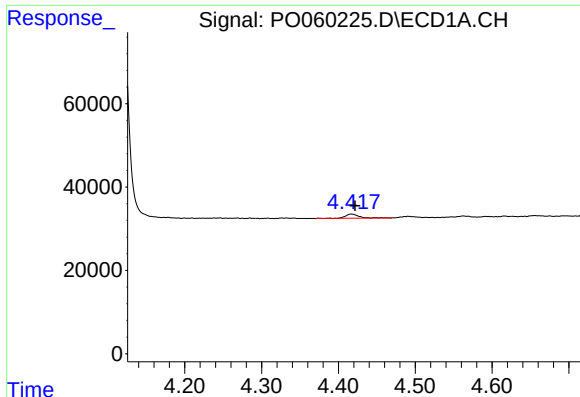

#9 AR-1221-2


R.T.: 4.417 min
Delta R.T.: -0.004 min
Response: 12130
Conc: 37.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

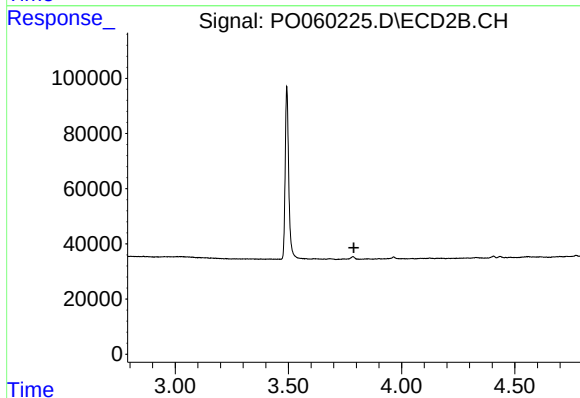


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.789 min
Response: 0
Conc: N.D.

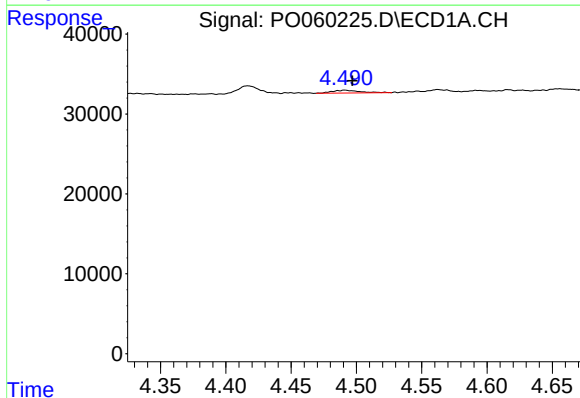


#10 AR-1221-3

R.T.: 4.491 min
Delta R.T.: -0.006 min
Response: 5176
Conc: 4.92 ng/ml

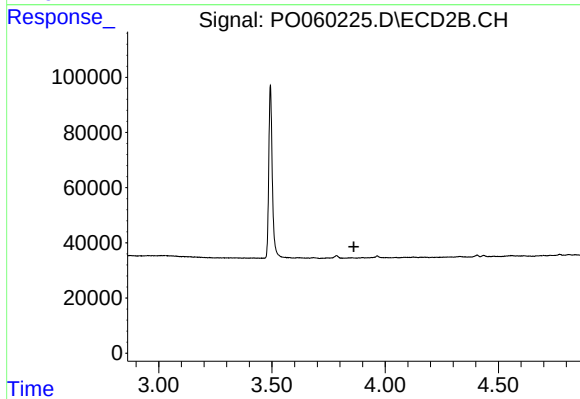

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

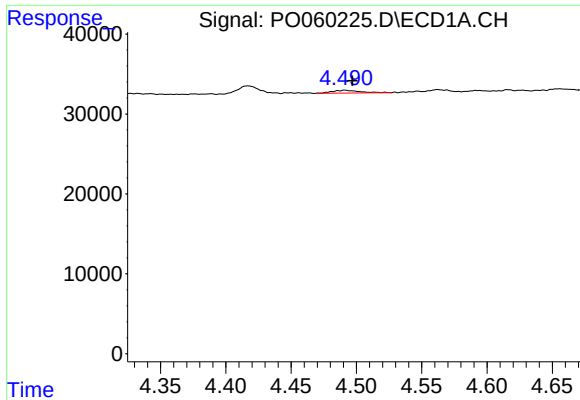

#11 AR-1232-1


R.T.: 4.491 min
Delta R.T.: -0.006 min
Response: 5176
Conc: 4.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

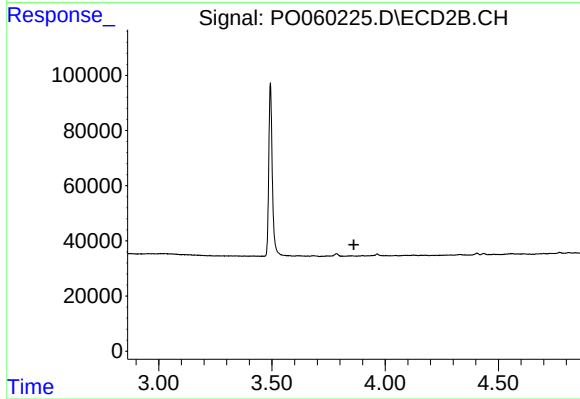


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

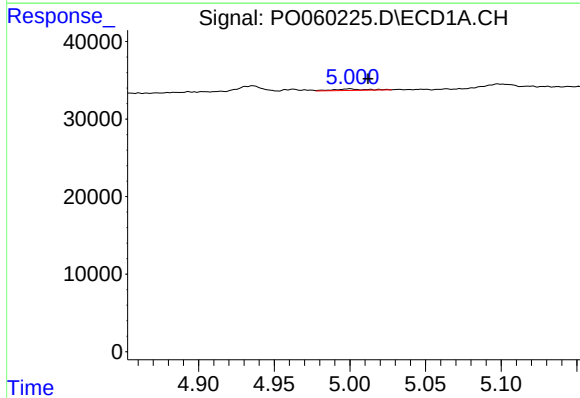


#12 AR-1232-2

R.T.: 5.000 min
Delta R.T.: -0.012 min
Response: 2876
Conc: 4.07 ng/ml

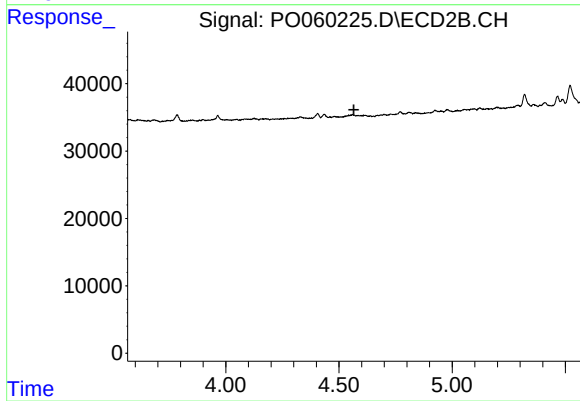

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

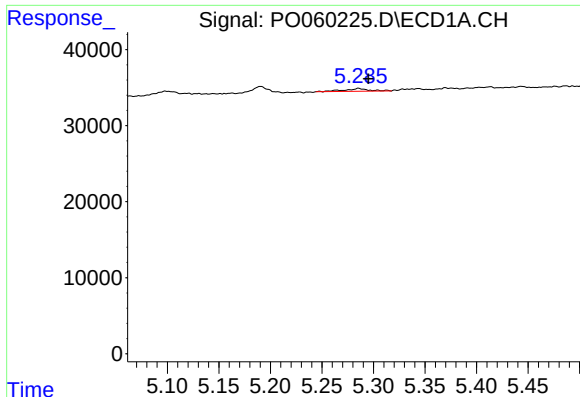

#13 AR-1232-3


R.T.: 5.286 min
Delta R.T.: -0.009 min
Response: 5986
Conc: 3.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

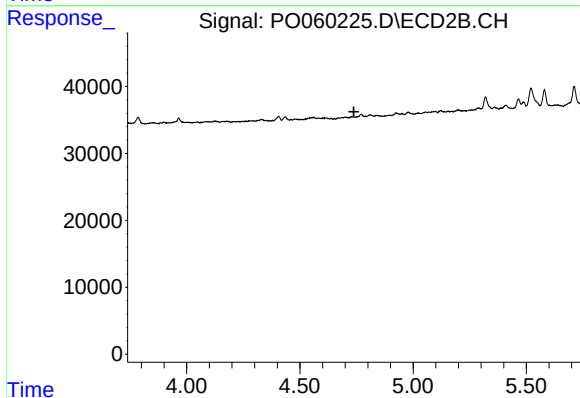


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

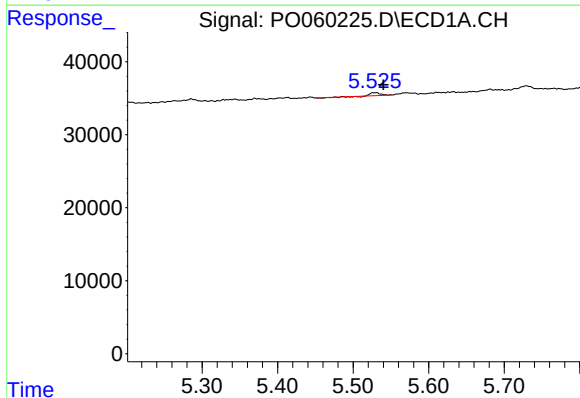


#14 AR-1232-4

R.T.: 5.529 min
Delta R.T.: -0.011 min
Response: 2474
Conc: 3.16 ng/ml

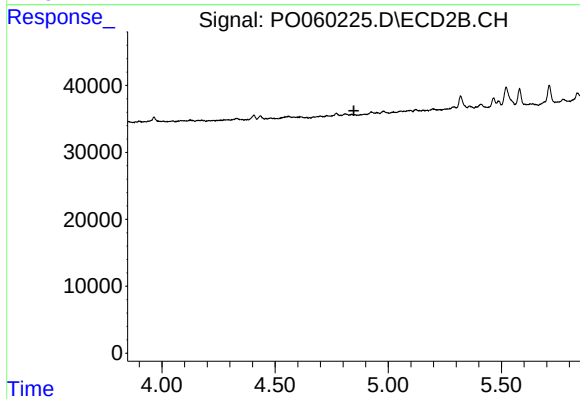

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

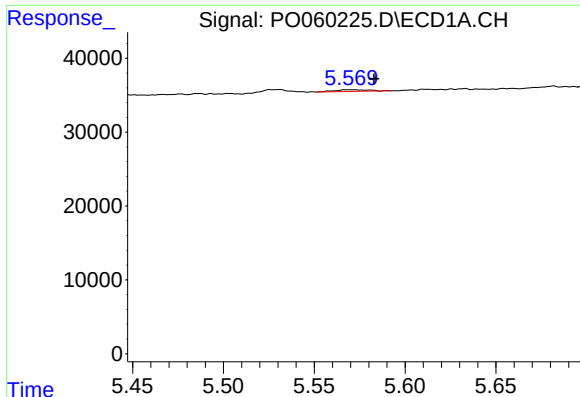

#15 AR-1232-5


R.T.: 5.571 min
Delta R.T.: -0.012 min
Response: 2807
Conc: 4.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

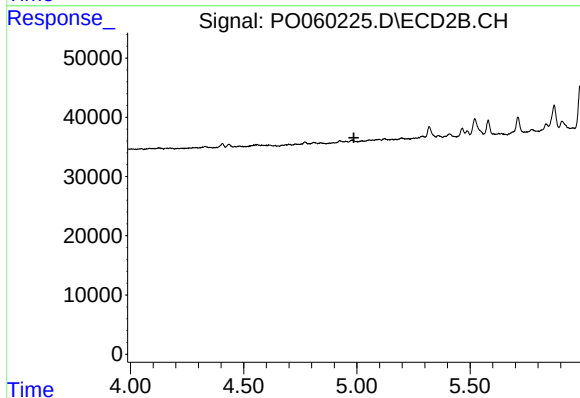


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

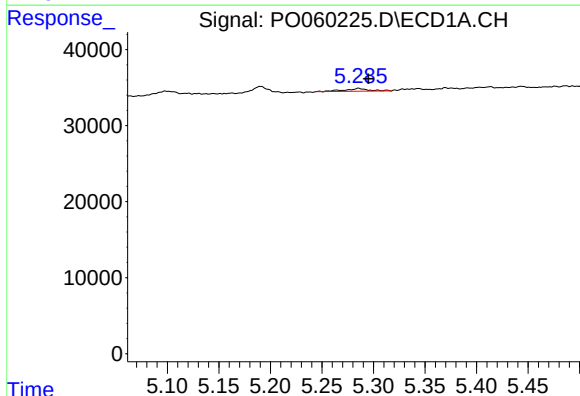


#16 AR-1242-1

R.T.: 5.286 min
Delta R.T.: -0.009 min
Response: 5986
Conc: 4.71 ng/ml

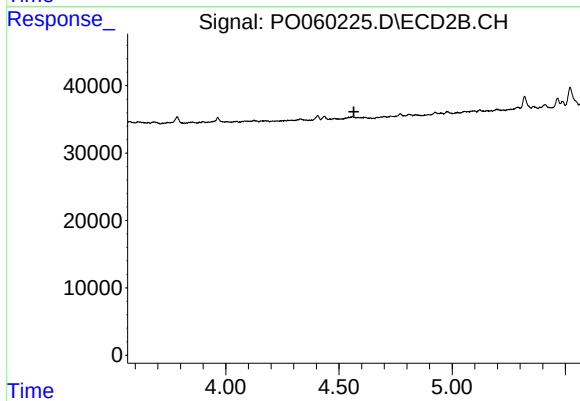

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

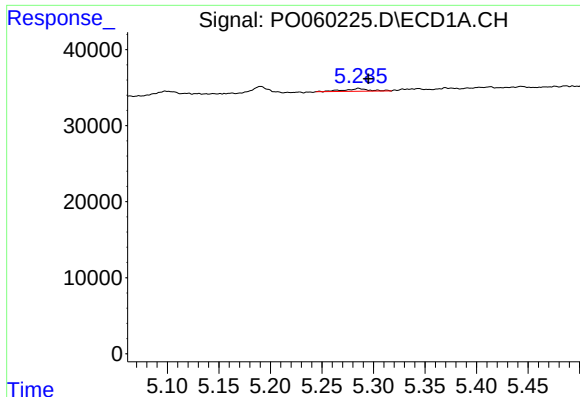

#17 AR-1242-2


R.T.: 5.286 min
Delta R.T.: -0.009 min
Response: 5986
Conc: 3.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

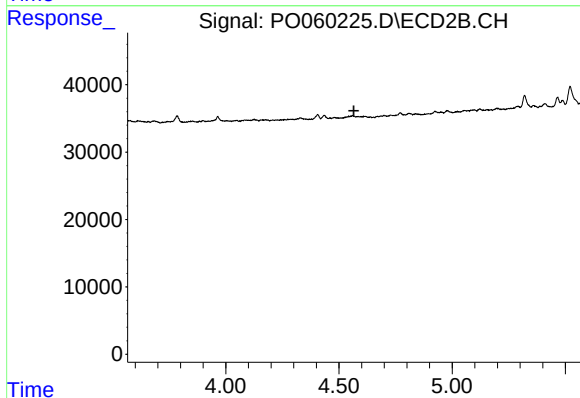


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

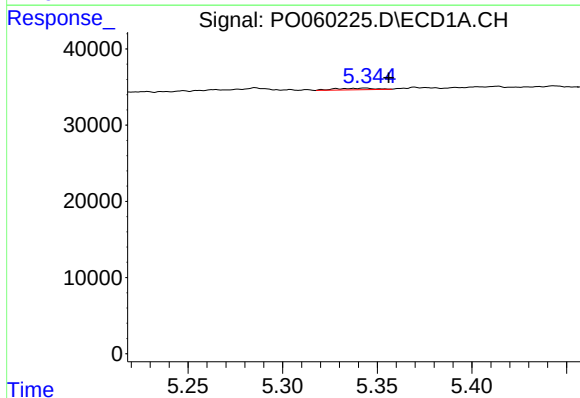


#18 AR-1242-3

R.T.: 5.343 min
Delta R.T.: -0.014 min
Response: 3079
Conc: 2.63 ng/ml

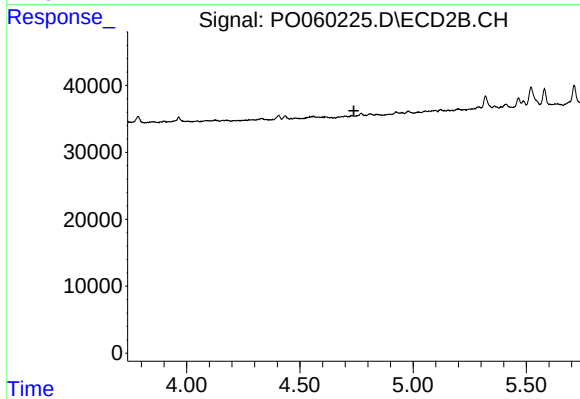

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

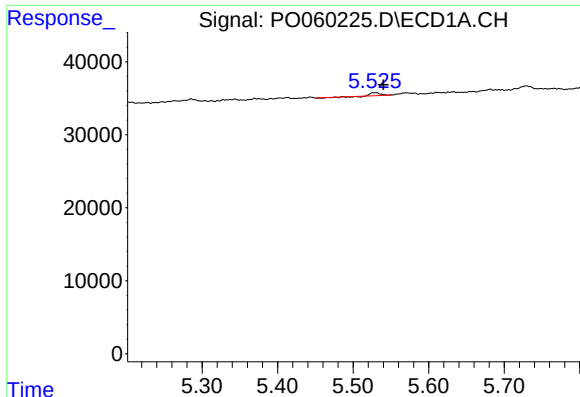

#19 AR-1242-4


R.T.: 5.529 min
Delta R.T.: -0.011 min
Response: 2474
Conc: 2.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

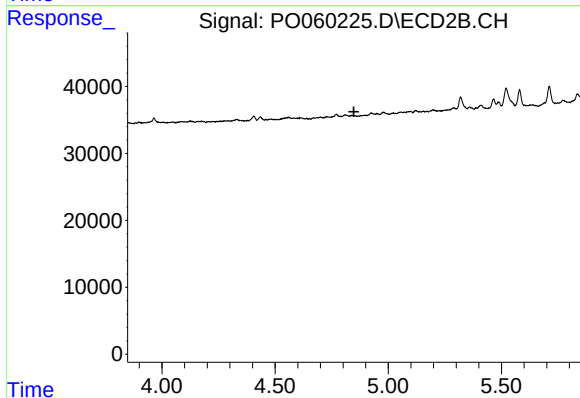


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.848 min
Response: 0
Conc: N.D.

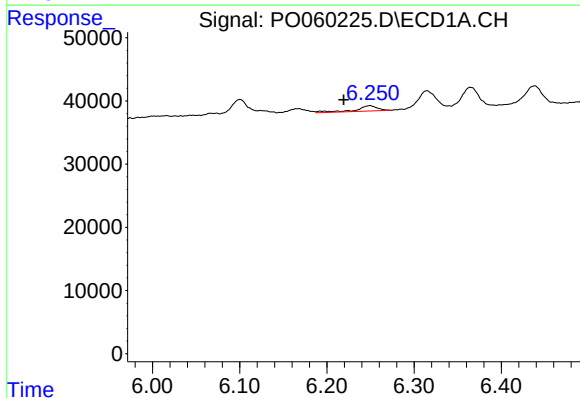


#20 AR-1242-5

R.T.: 6.249 min
Delta R.T.: 0.030 min
Response: 14541
Conc: 11.57 ng/ml

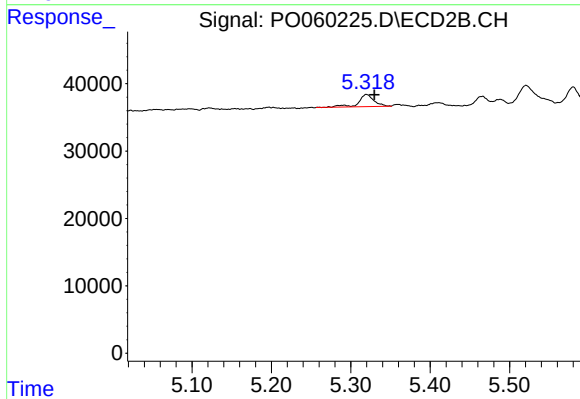

#20 AR-1242-5


R.T.: 5.320 min
Delta R.T.: -0.010 min
Response: 23785
Conc: 21.26 ng/ml

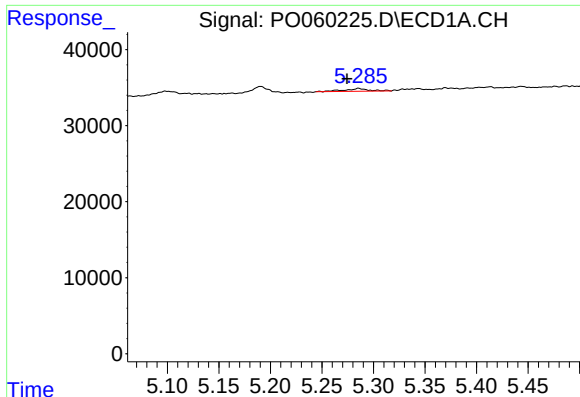

#21 AR-1248-1


R.T.: 5.286 min
Delta R.T.: 0.012 min
Response: 5986
Conc: 5.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

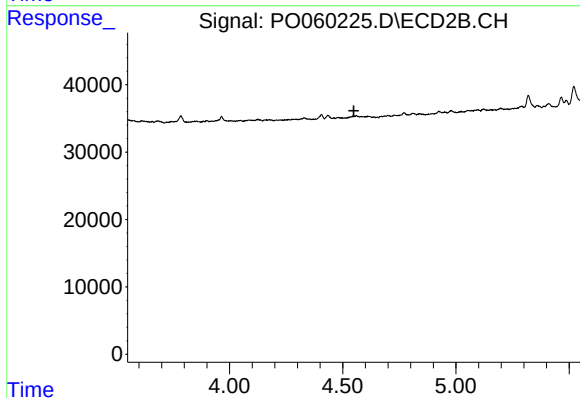


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

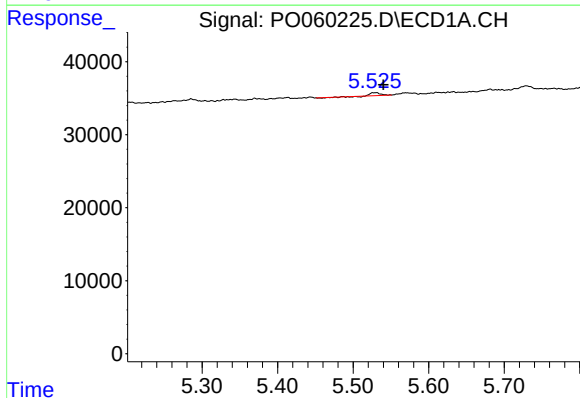


#22 AR-1248-2

R.T.: 5.529 min
Delta R.T.: -0.011 min
Response: 2474
Conc: 1.71 ng/ml

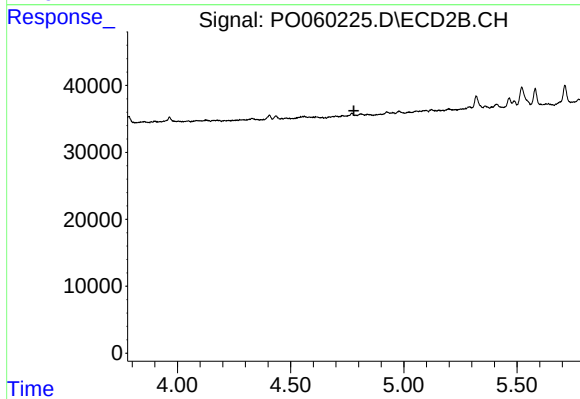

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

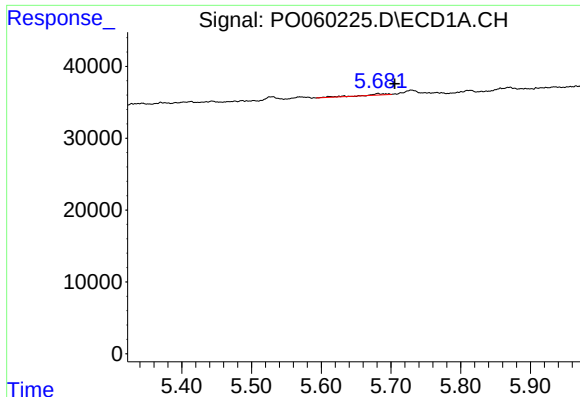

#23 AR-1248-3


R.T.: 5.682 min
Delta R.T.: -0.024 min
Response: 3759
Conc: 2.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

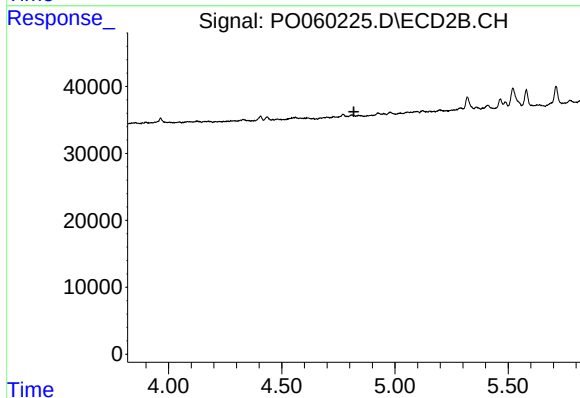


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.819 min
Response: 0
Conc: N.D.

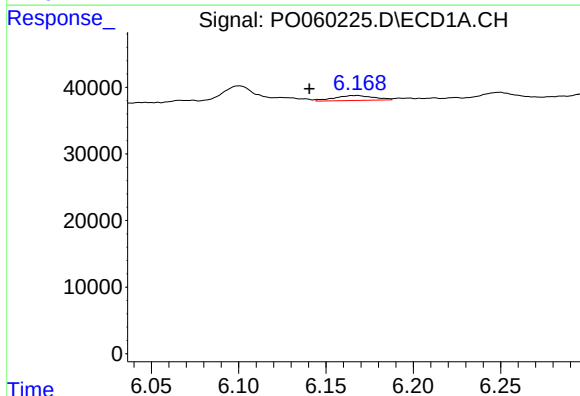


#24 AR-1248-4

R.T.: 6.167 min
Delta R.T.: 0.026 min
Response: 11705
Conc: 5.73 ng/ml

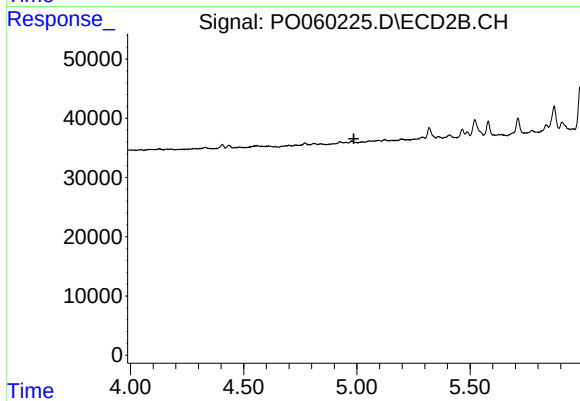

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.987 min
Response: 0
Conc: N.D.

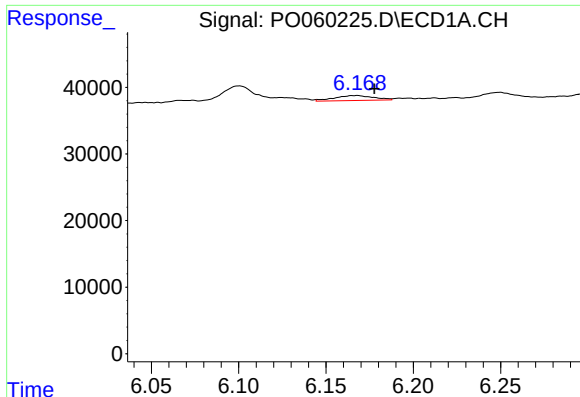

#25 AR-1248-5


R.T.: 6.167 min
Delta R.T.: -0.011 min
Response: 11705
Conc: 5.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

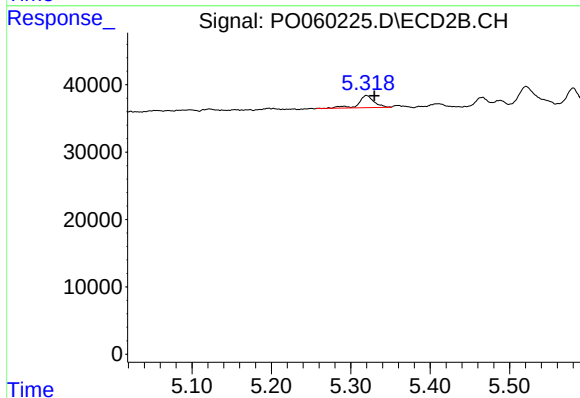


#25 AR-1248-5

R.T.: 5.320 min
Delta R.T.: -0.010 min
Response: 23785
Conc: 16.62 ng/ml

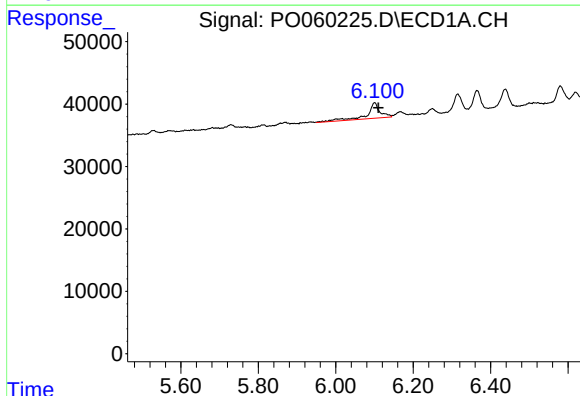


#26 AR-1254-1

R.T.: 6.100 min
Delta R.T.: -0.010 min
Response: 59270
Conc: 28.41 ng/ml

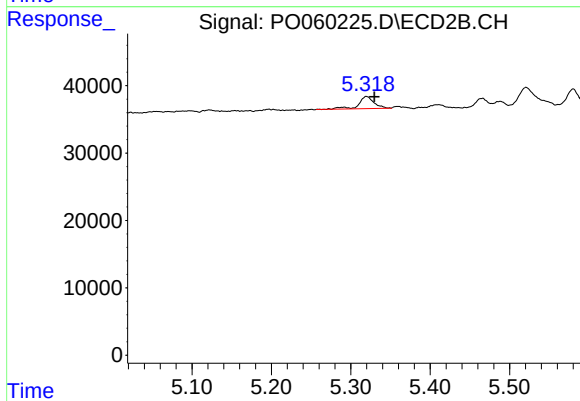

#26 AR-1254-1


R.T.: 5.320 min
Delta R.T.: -0.010 min
Response: 23785
Conc: 10.03 ng/ml

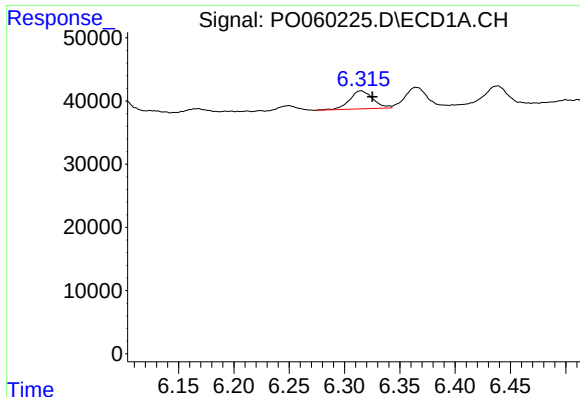

#27 AR-1254-2


R.T.: 6.315 min
Delta R.T.: -0.010 min
Response: 41908
Conc: 12.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

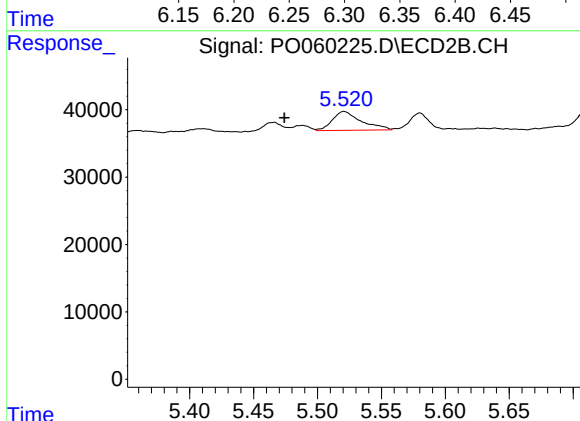


#27 AR-1254-2

R.T.: 5.521 min
Delta R.T.: 0.047 min
Response: 43922
Conc: 20.93 ng/ml

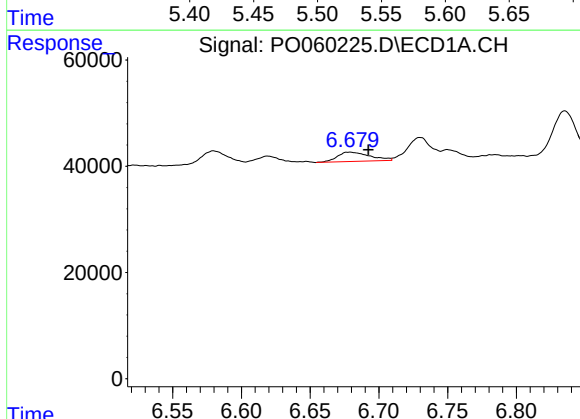


#28 AR-1254-3

R.T.: 6.679 min
Delta R.T.: -0.013 min
Response: 28988
Conc: 8.17 ng/ml

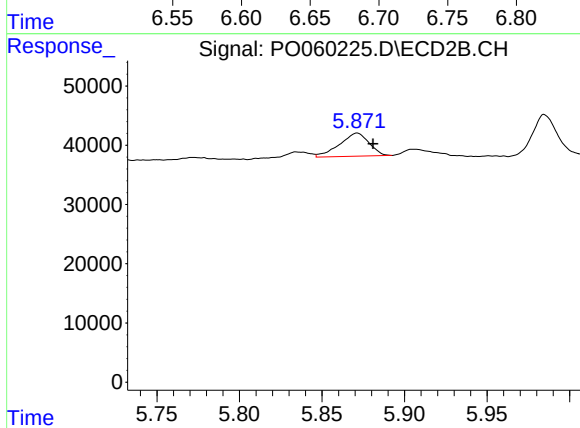

#28 AR-1254-3


R.T.: 5.871 min
Delta R.T.: -0.010 min
Response: 48481
Conc: 14.42 ng/ml

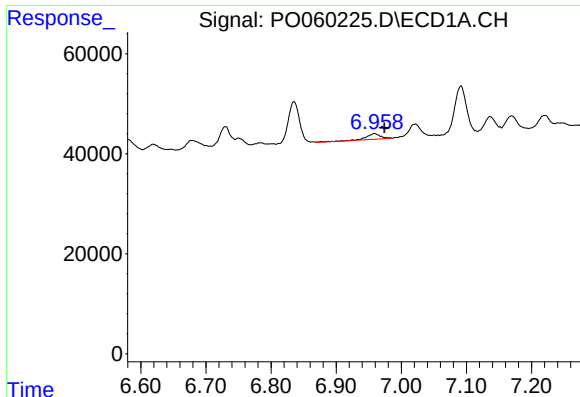

#29 AR-1254-4


R.T.: 6.959 min
Delta R.T.: -0.015 min
Response: 16601
Conc: 5.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

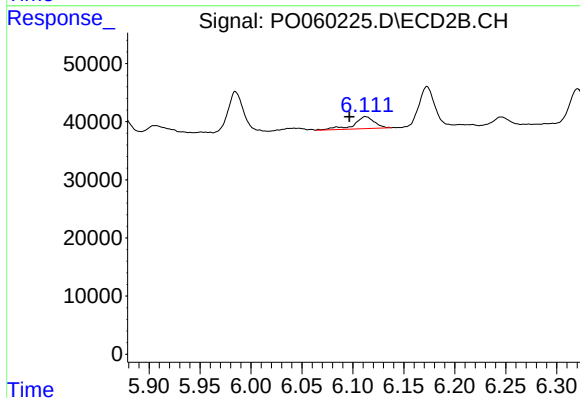


#29 AR-1254-4

R.T.: 6.113 min
Delta R.T.: 0.016 min
Response: 28930
Conc: 14.03 ng/ml

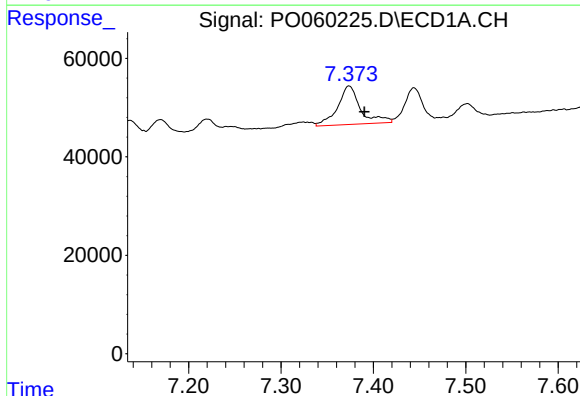


#30 AR-1254-5

R.T.: 7.374 min
Delta R.T.: -0.016 min
Response: 134846
Conc: 43.61 ng/ml

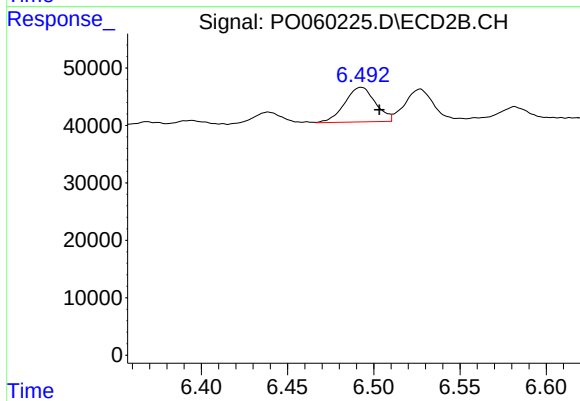

#30 AR-1254-5


R.T.: 6.493 min
Delta R.T.: -0.010 min
Response: 74446
Conc: 23.98 ng/ml

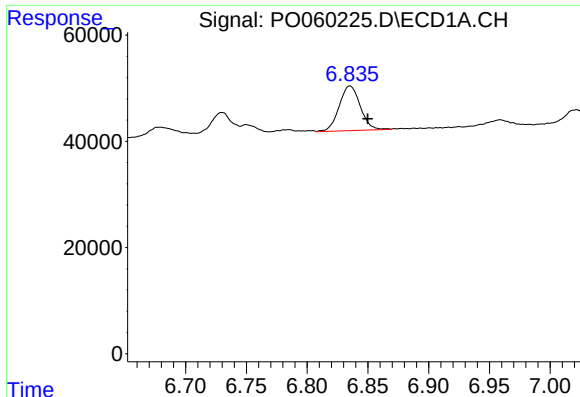

#31 AR-1260-1


R.T.: 6.835 min
Delta R.T.: -0.014 min
Response: 101398
Conc: 37.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

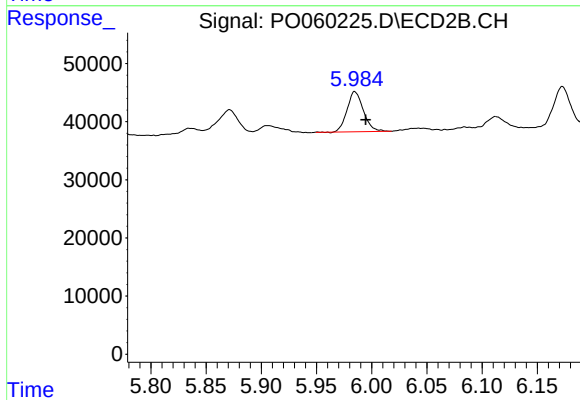


#31 AR-1260-1

R.T.: 5.985 min
Delta R.T.: -0.010 min
Response: 71094
Conc: 31.20 ng/ml

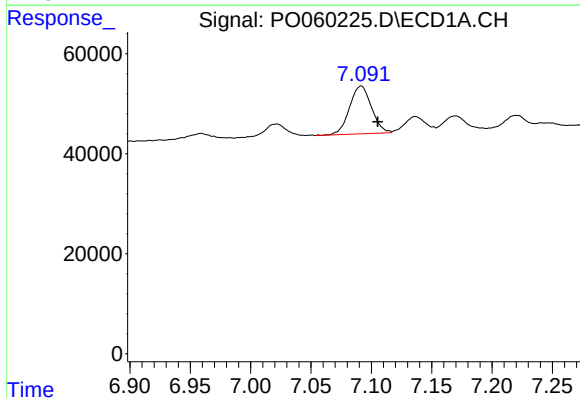


#32 AR-1260-2

R.T.: 7.091 min
Delta R.T.: -0.014 min
Response: 120943
Conc: 32.59 ng/ml

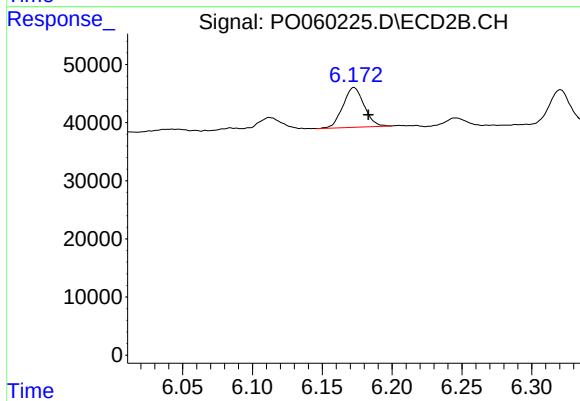

#32 AR-1260-2


R.T.: 6.173 min
Delta R.T.: -0.010 min
Response: 72448
Conc: 24.73 ng/ml

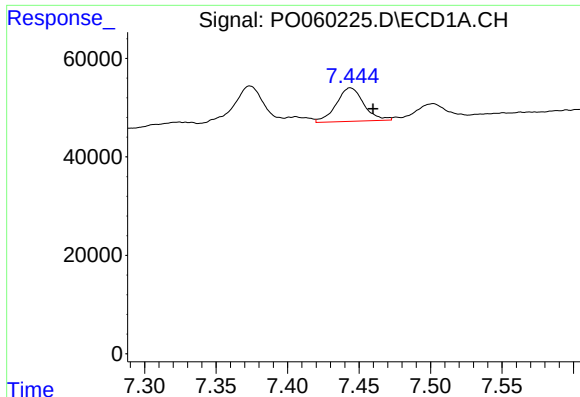

#33 AR-1260-3


R.T.: 7.444 min
Delta R.T.: -0.016 min
Response: 91283
Conc: 27.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

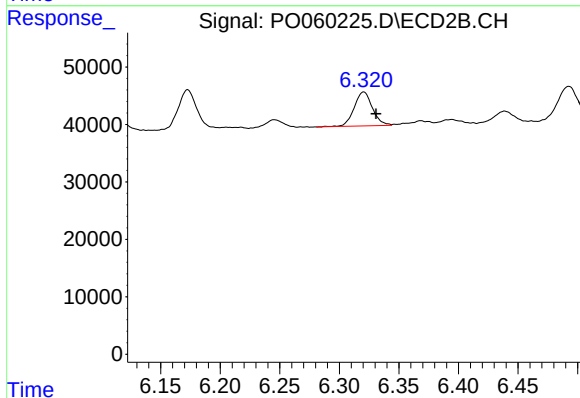


#33 AR-1260-3

R.T.: 6.321 min
Delta R.T.: -0.010 min
Response: 62476
Conc: 23.58 ng/ml

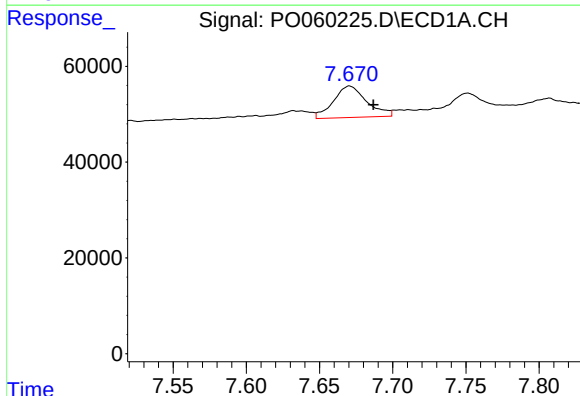


#34 AR-1260-4

R.T.: 7.671 min
Delta R.T.: -0.016 min
Response: 104026
Conc: 33.87 ng/ml

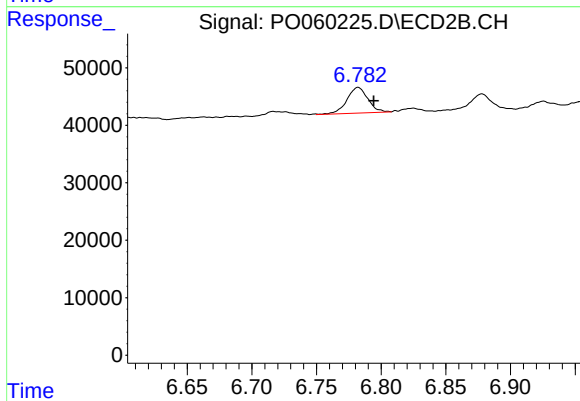

#34 AR-1260-4


R.T.: 6.782 min
Delta R.T.: -0.012 min
Response: 50280
Conc: 22.22 ng/ml

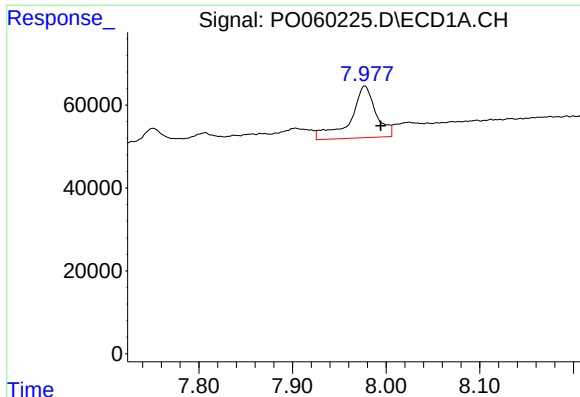

#35 AR-1260-5


R.T.: 7.977 min
Delta R.T.: -0.017 min
Response: 237337
Conc: 33.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

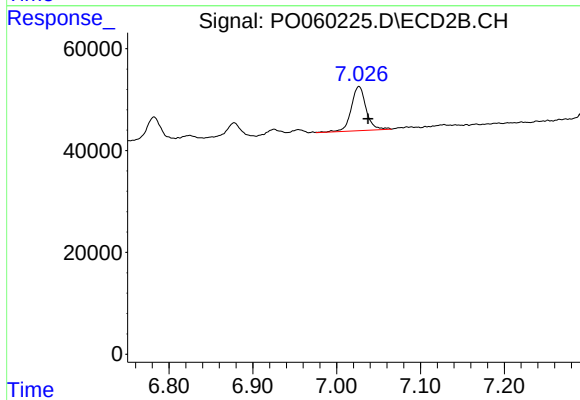


#35 AR-1260-5

R.T.: 7.027 min
Delta R.T.: -0.011 min
Response: 107440
Conc: 19.52 ng/ml

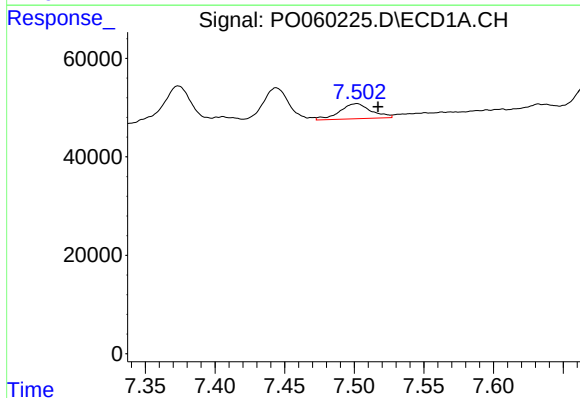


#36 AR-1262-1

R.T.: 7.501 min
Delta R.T.: -0.016 min
Response: 48122
Conc: 9.92 ng/ml

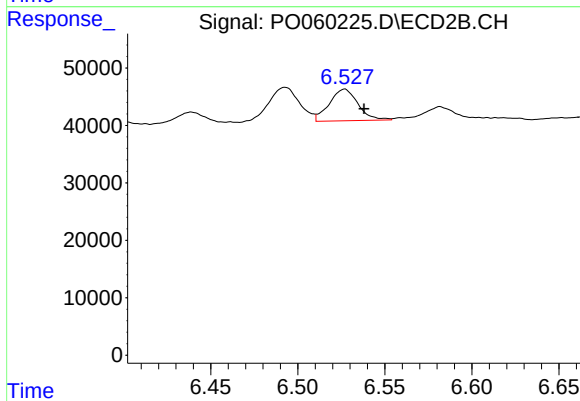

#36 AR-1262-1


R.T.: 6.527 min
Delta R.T.: -0.011 min
Response: 63143
Conc: 16.94 ng/ml

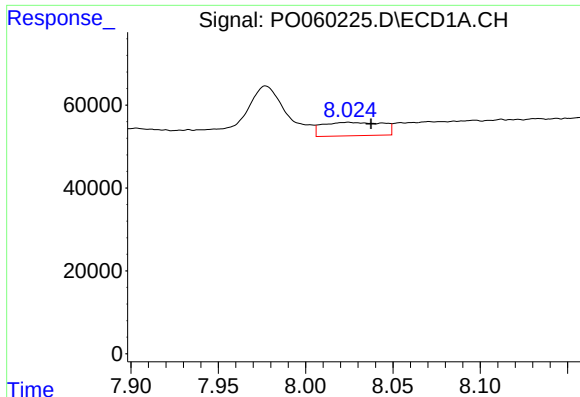

#37 AR-1262-2


R.T.: 8.024 min
Delta R.T.: -0.013 min
Response: 78011
Conc: 10.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

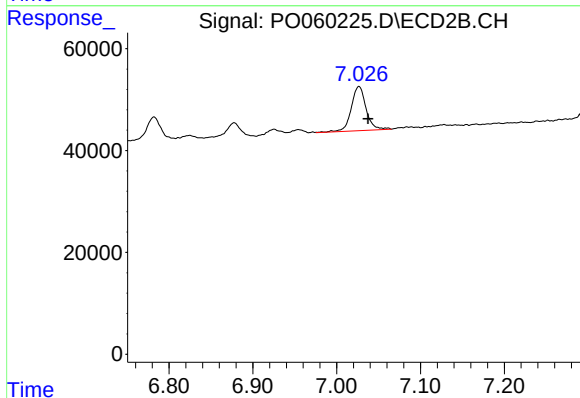


#37 AR-1262-2

R.T.: 7.027 min
Delta R.T.: -0.011 min
Response: 107440
Conc: 18.28 ng/ml

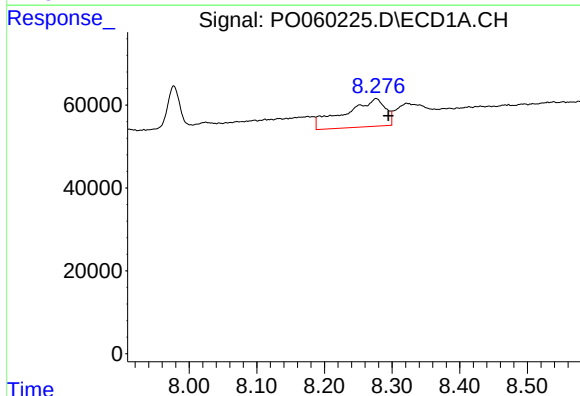


#38 AR-1262-3

R.T.: 8.276 min
Delta R.T.: -0.018 min
Response: 283197
Conc: 55.50 ng/ml

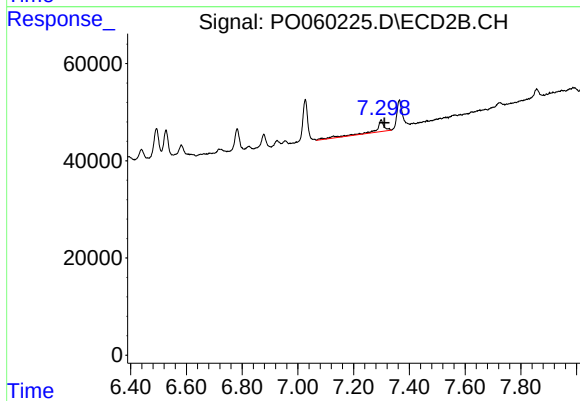

#38 AR-1262-3


R.T.: 7.299 min
Delta R.T.: -0.012 min
Response: 54929
Conc: 21.62 ng/ml

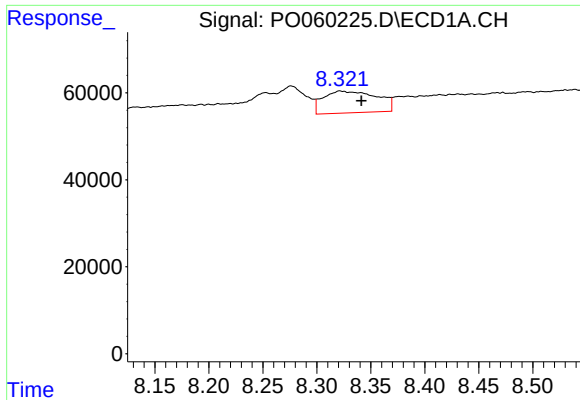

#39 AR-1262-4


R.T.: 8.322 min
Delta R.T.: -0.019 min
Response: 174035
Conc: 45.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

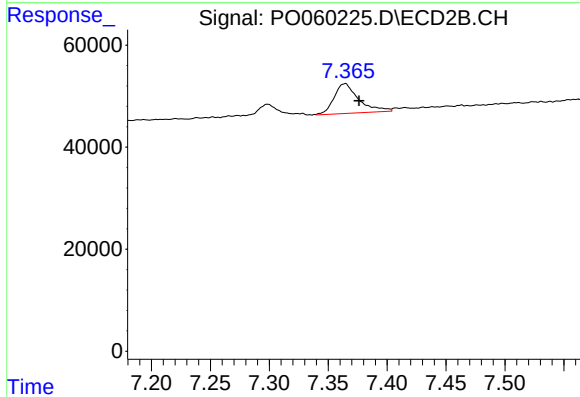


#39 AR-1262-4

R.T.: 7.364 min
Delta R.T.: -0.012 min
Response: 85450
Conc: 19.34 ng/ml

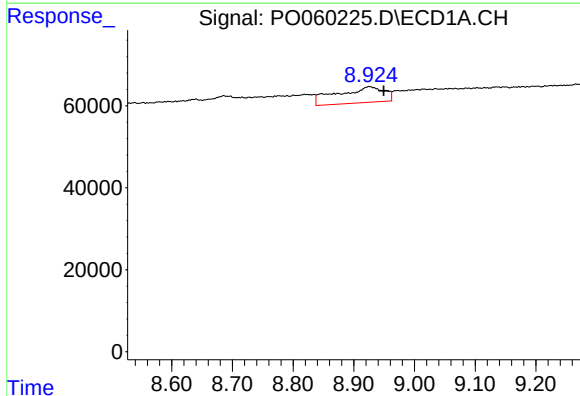


#40 AR-1262-5

R.T.: 8.925 min
Delta R.T.: -0.024 min
Response: 208973
Conc: 81.42 ng/ml

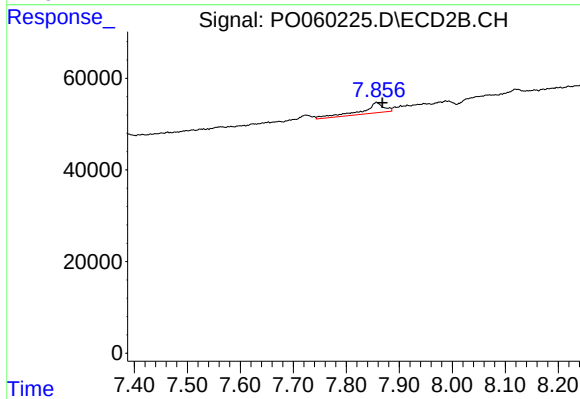

#40 AR-1262-5


R.T.: 7.857 min
Delta R.T.: -0.011 min
Response: 65247
Conc: 36.14 ng/ml

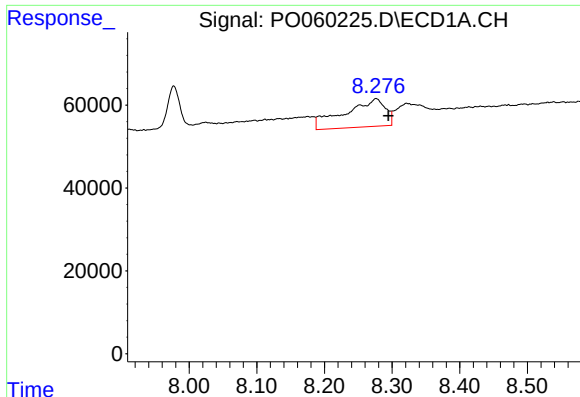

#41 AR-1268-1


R.T.: 8.276 min
Delta R.T.: -0.018 min
Response: 283197
Conc: 30.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

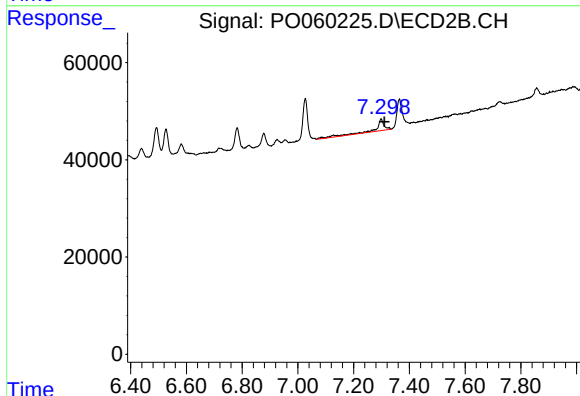


#41 AR-1268-1

R.T.: 7.299 min
Delta R.T.: -0.012 min
Response: 54929
Conc: 7.71 ng/ml

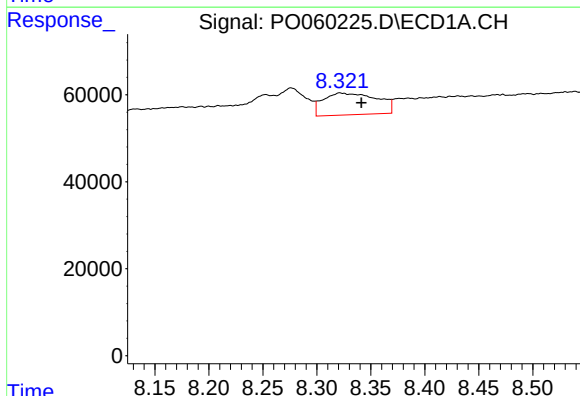


#42 AR-1268-2

R.T.: 8.322 min
Delta R.T.: -0.019 min
Response: 174035
Conc: 22.08 ng/ml

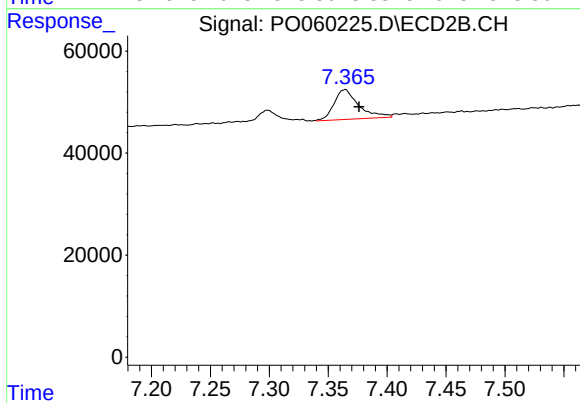

#42 AR-1268-2


R.T.: 7.364 min
Delta R.T.: -0.012 min
Response: 85450
Conc: 13.25 ng/ml

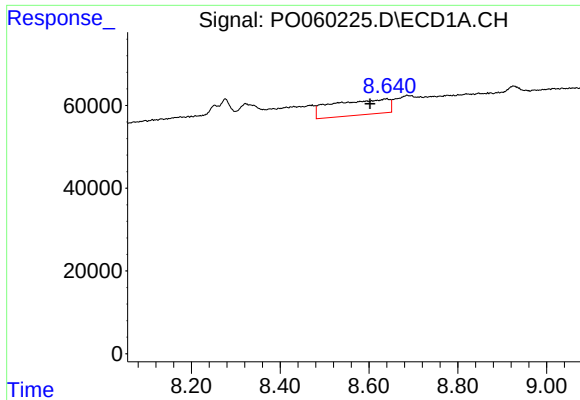

#43 AR-1268-3


R.T.: 8.639 min
Delta R.T.: 0.036 min
Response: 330049
Conc: 46.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

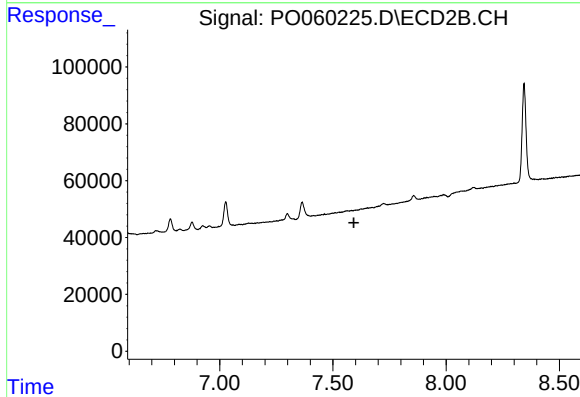


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

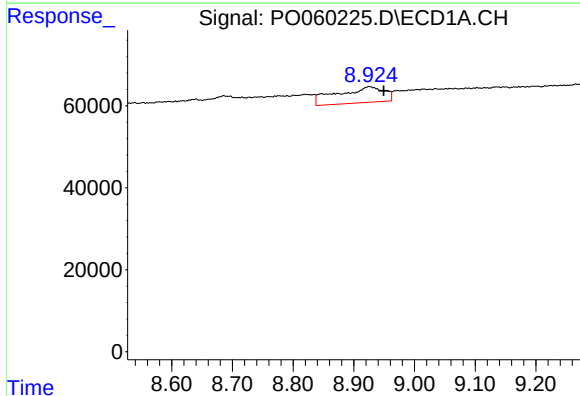


#44 AR-1268-4

R.T.: 8.925 min
Delta R.T.: -0.024 min
Response: 208973
Conc: 75.17 ng/ml

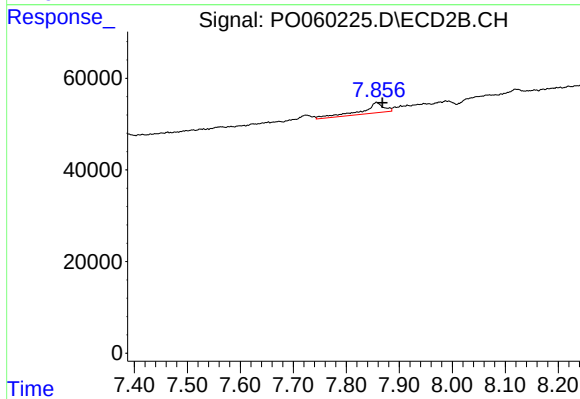

#44 AR-1268-4


R.T.: 7.857 min
Delta R.T.: -0.011 min
Response: 65247
Conc: 31.96 ng/ml

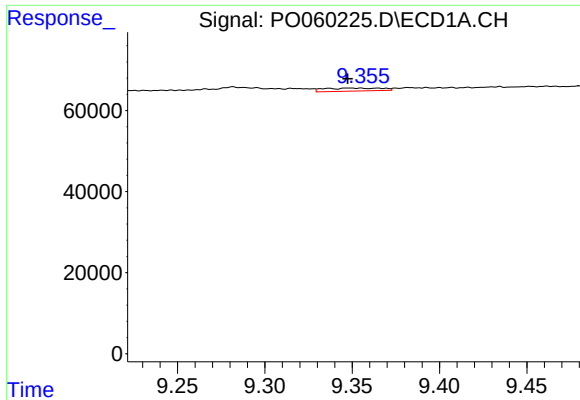

#45 AR-1268-5

R.T.: 9.350 min
Delta R.T.: 0.002 min
Response: 17222
Conc: 0.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

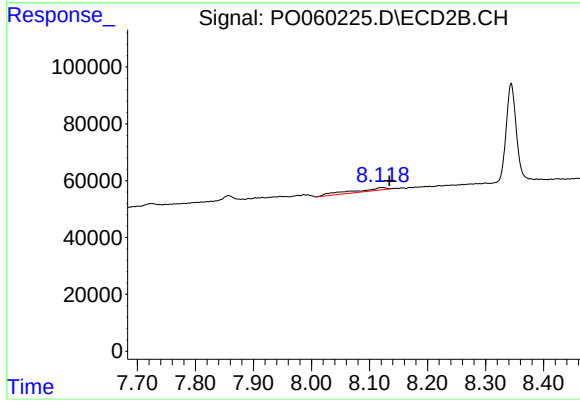

#45 AR-1268-5

R.T.: 8.119 min
Delta R.T.: -0.016 min
Response: 43560
Conc: 3.00 ng/ml