

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 10:24
 Operator : SM/AJ
 Sample : K4479-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU19-FLDDCAP1

Manual Integrations
 APPROVED

Ankita
 9/4/2019 4:55:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:13:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.117	3.493	763551	675547	21.808	18.767
2) SA Decachlor...	9.569	8.344	534114	420528	10.040	10.429
Target Compounds						
31) L7 AR-1260-1	6.835	5.985	98514	70182	36.543	30.796
32) L7 AR-1260-2	7.091	6.173	117698	72324	31.720	24.685
33) L7 AR-1260-3	7.445	6.320	90682	61002	27.678	23.027
34) L7 AR-1260-4	7.670	6.783	72515	50302	23.610m	22.232
35) L7 AR-1260-5	7.977	7.025	123881	101707	17.495m	18.481

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090319\
Data File : PO060222.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2019 10:24
Operator : SM/AJ
Sample : K4479-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:13:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

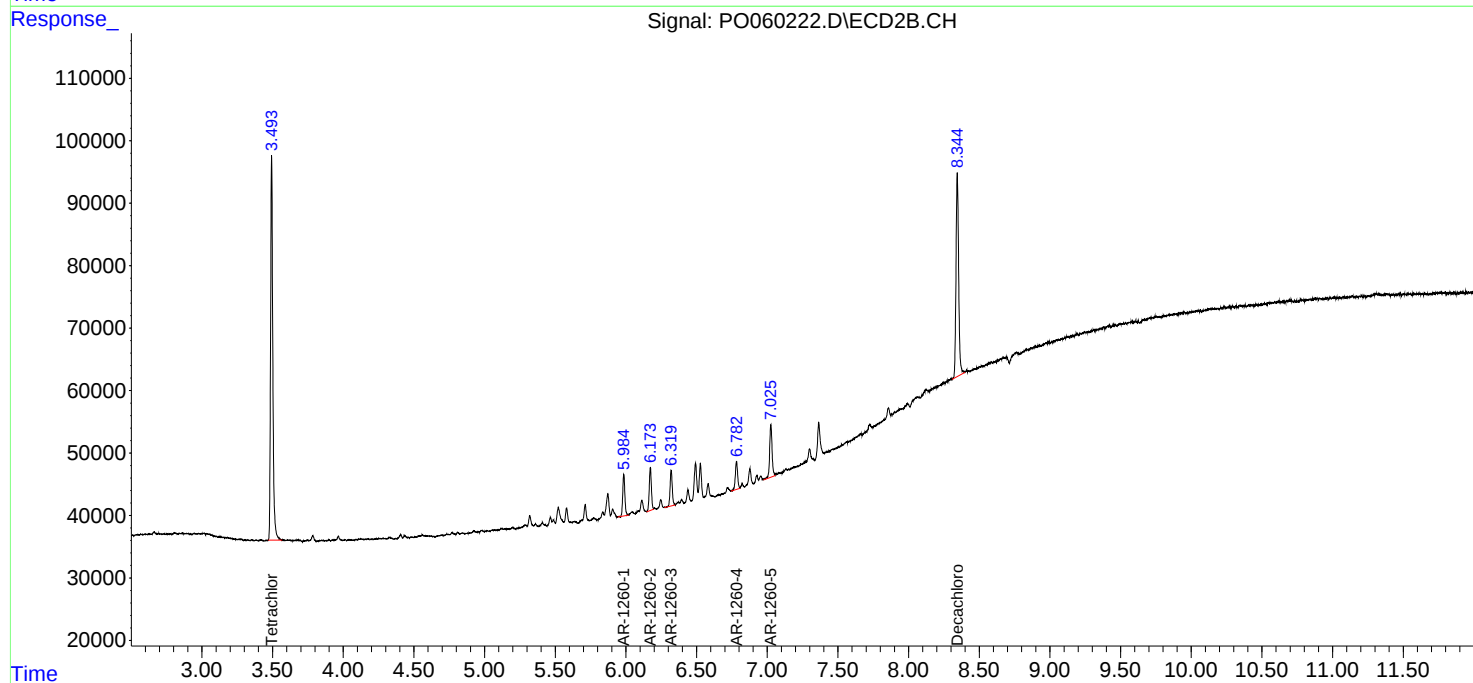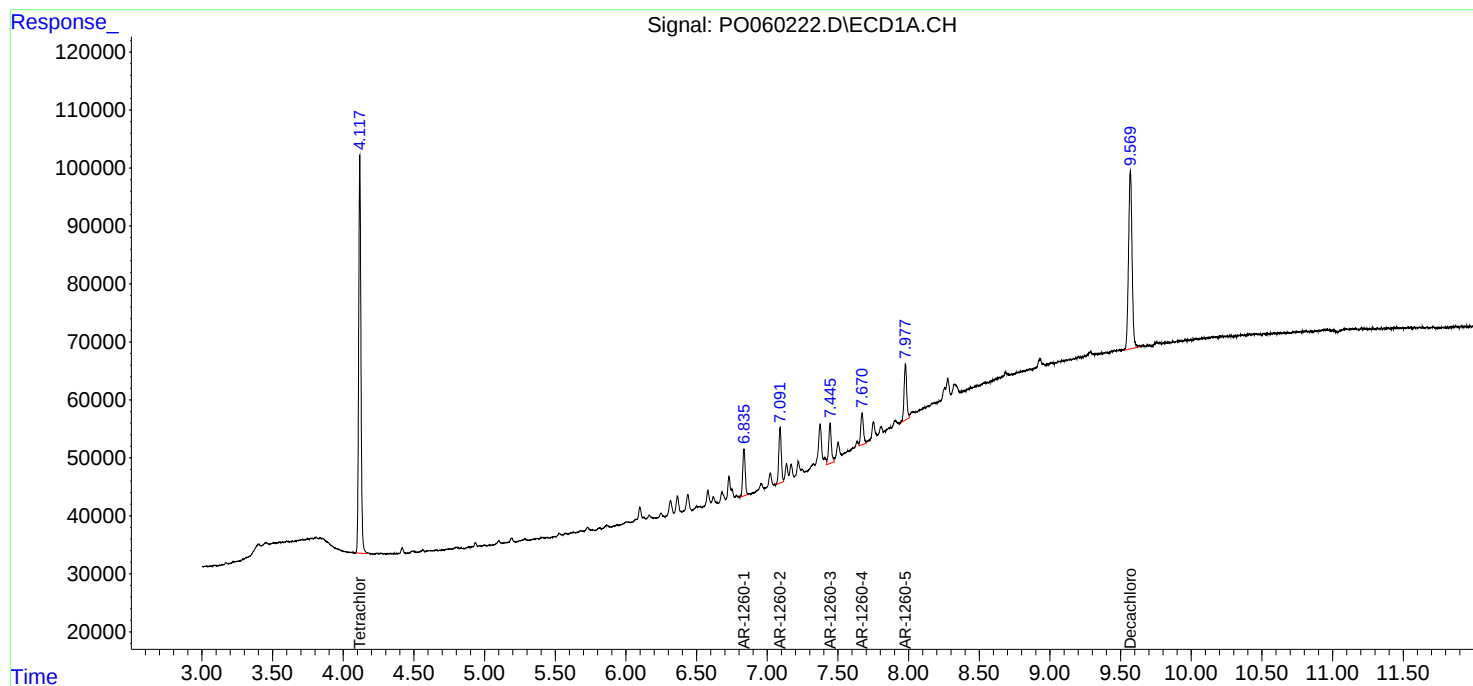

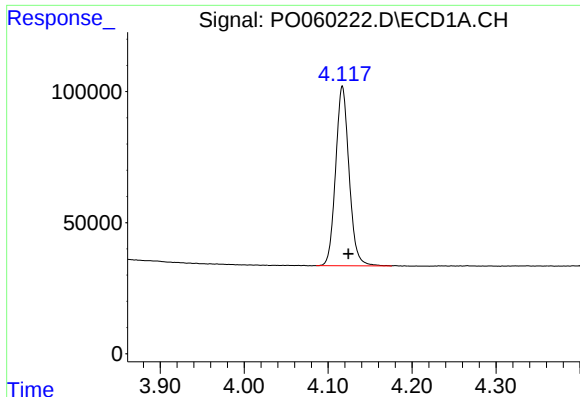


#1 Tetrachloro-m-xylene

R.T.: 4.117 min
Delta R.T.: -0.007 min
Response: 763551
Conc: 21.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:31 PM

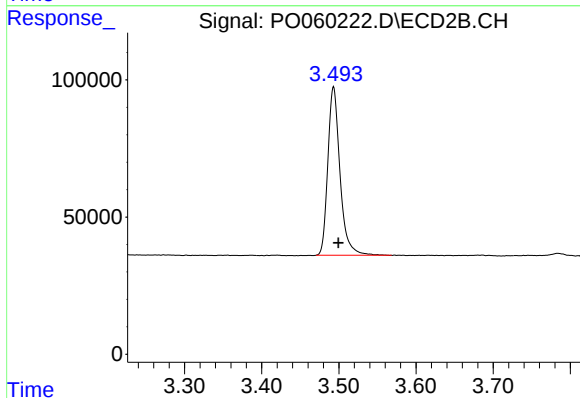


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: -0.006 min
Response: 675547
Conc: 18.77 ng/ml

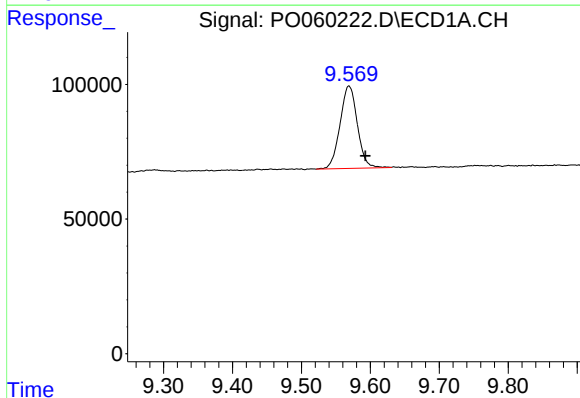


#2 Decachlorobiphenyl

R.T.: 9.569 min
Delta R.T.: -0.024 min
Response: 534114
Conc: 10.04 ng/ml

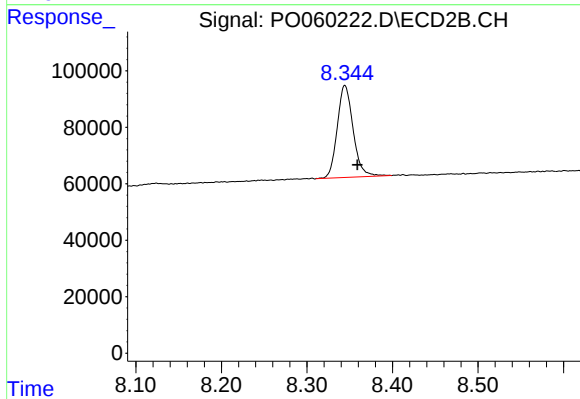

#2 Decachlorobiphenyl

R.T.: 8.344 min
Delta R.T.: -0.015 min
Response: 420528
Conc: 10.43 ng/ml

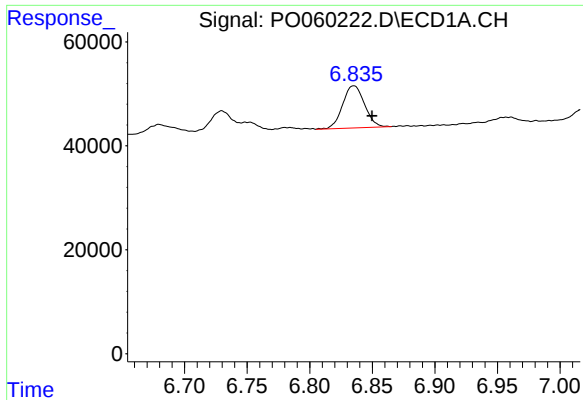


#31 AR-1260-1

R.T.: 6.835 min
Delta R.T.: -0.015 min
Response: 98514
Conc: 36.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:31 PM

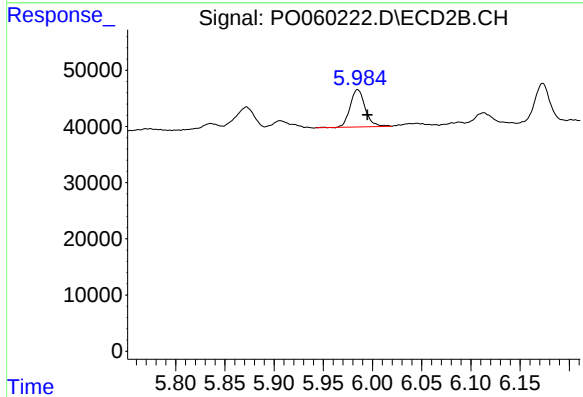


#31 AR-1260-1

R.T.: 5.985 min
Delta R.T.: -0.010 min
Response: 70182
Conc: 30.80 ng/ml

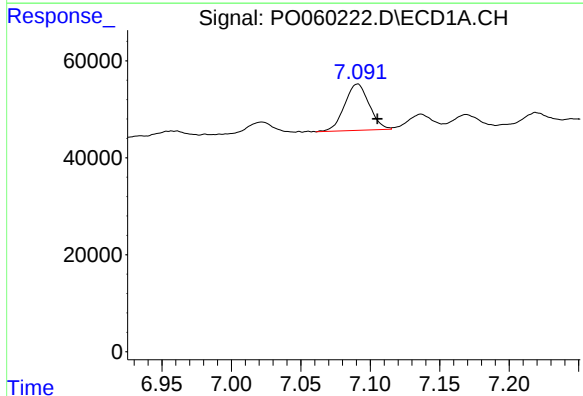


#32 AR-1260-2

R.T.: 7.091 min
Delta R.T.: -0.014 min
Response: 117698
Conc: 31.72 ng/ml

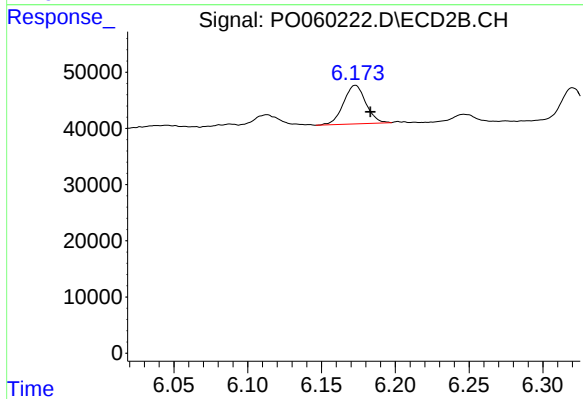

#32 AR-1260-2

R.T.: 6.173 min
Delta R.T.: -0.010 min
Response: 72324
Conc: 24.69 ng/ml

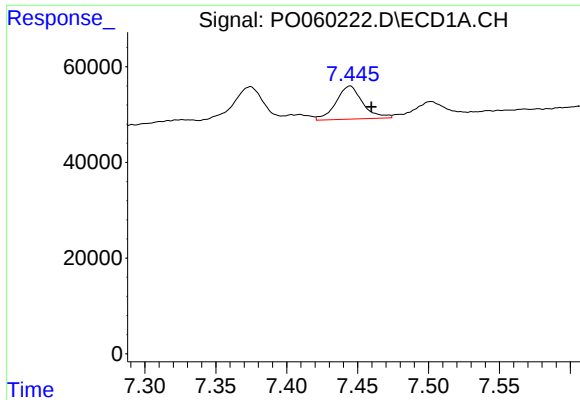


#33 AR-1260-3

R.T.: 7.445 min
Delta R.T.: -0.015 min
Response: 90682
Conc: 27.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:31 PM

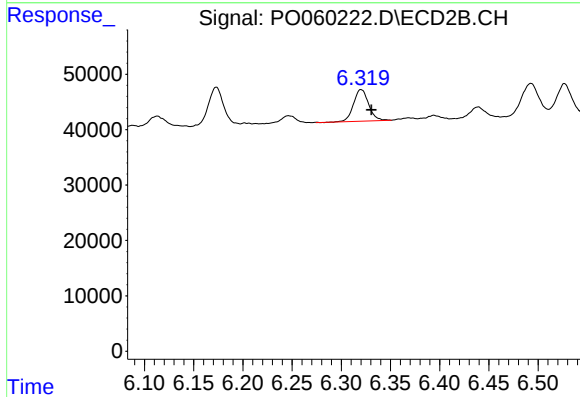


#33 AR-1260-3

R.T.: 6.320 min
Delta R.T.: -0.011 min
Response: 61002
Conc: 23.03 ng/ml

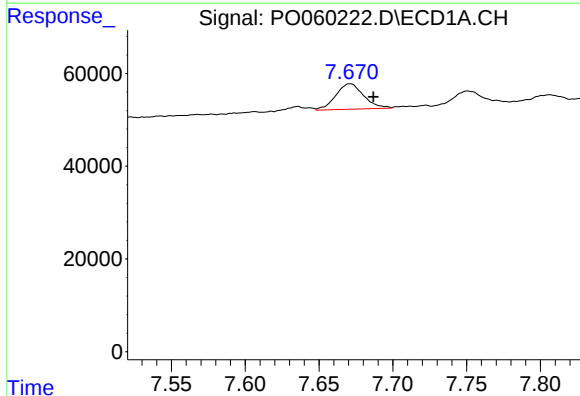


#34 AR-1260-4

R.T.: 7.670 min
Delta R.T.: -0.017 min
Response: 72515
Conc: 23.61 ng/ml m

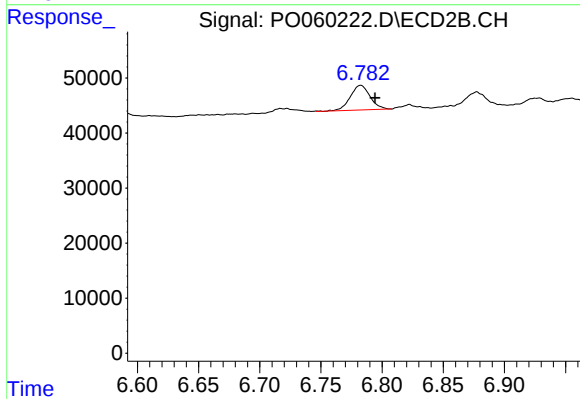

#34 AR-1260-4

R.T.: 6.783 min
Delta R.T.: -0.012 min
Response: 50302
Conc: 22.23 ng/ml

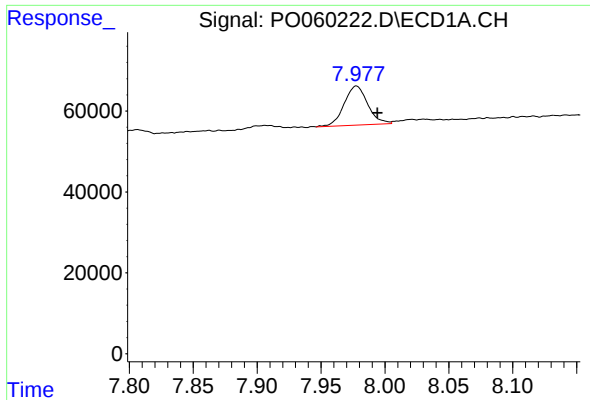


#35 AR-1260-5

R.T.: 7.977 min
Delta R.T.: -0.017 min
Response: 123881
Conc: 17.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1

Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:31 PM

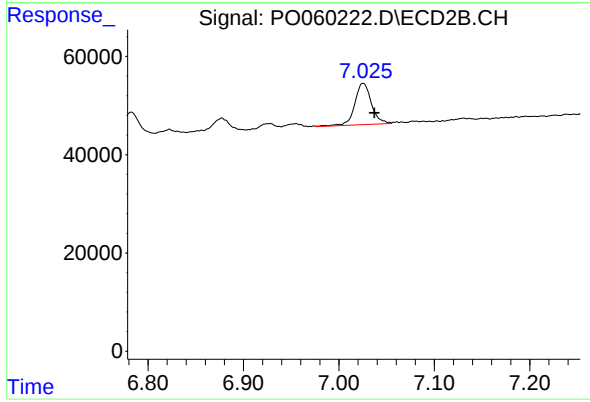

#35 AR-1260-5

R.T.: 7.025 min
Delta R.T.: -0.012 min
Response: 101707
Conc: 18.48 ng/ml