

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090319\
 Data File : P0060225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 11:16
 Operator : SM/AJ
 Sample : K4479-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SU19-FLDDCAP1RE

Manual Integrations
 APPROVED

Ankita
 9/4/2019 4:55:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:14:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.117	3.493	759319	673752	21.687	18.718
2) SA Decachlor...	9.566	8.344	548561	427735	10.311	10.608
Target Compounds						
31) L7 AR-1260-1	6.835	5.985	101398	71094	37.613	31.196
32) L7 AR-1260-2	7.091	6.173	120943	72448	32.595	24.727
33) L7 AR-1260-3	7.444	6.321	91283	62476	27.861	23.584
34) L7 AR-1260-4	7.670	6.782	72632	50280	23.648m	22.223
35) L7 AR-1260-5	7.977	7.027	124047	107440	17.518m	19.523

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090319\
Data File : PO060225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2019 11:16
Operator : SM/AJ
Sample : K4479-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:14:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

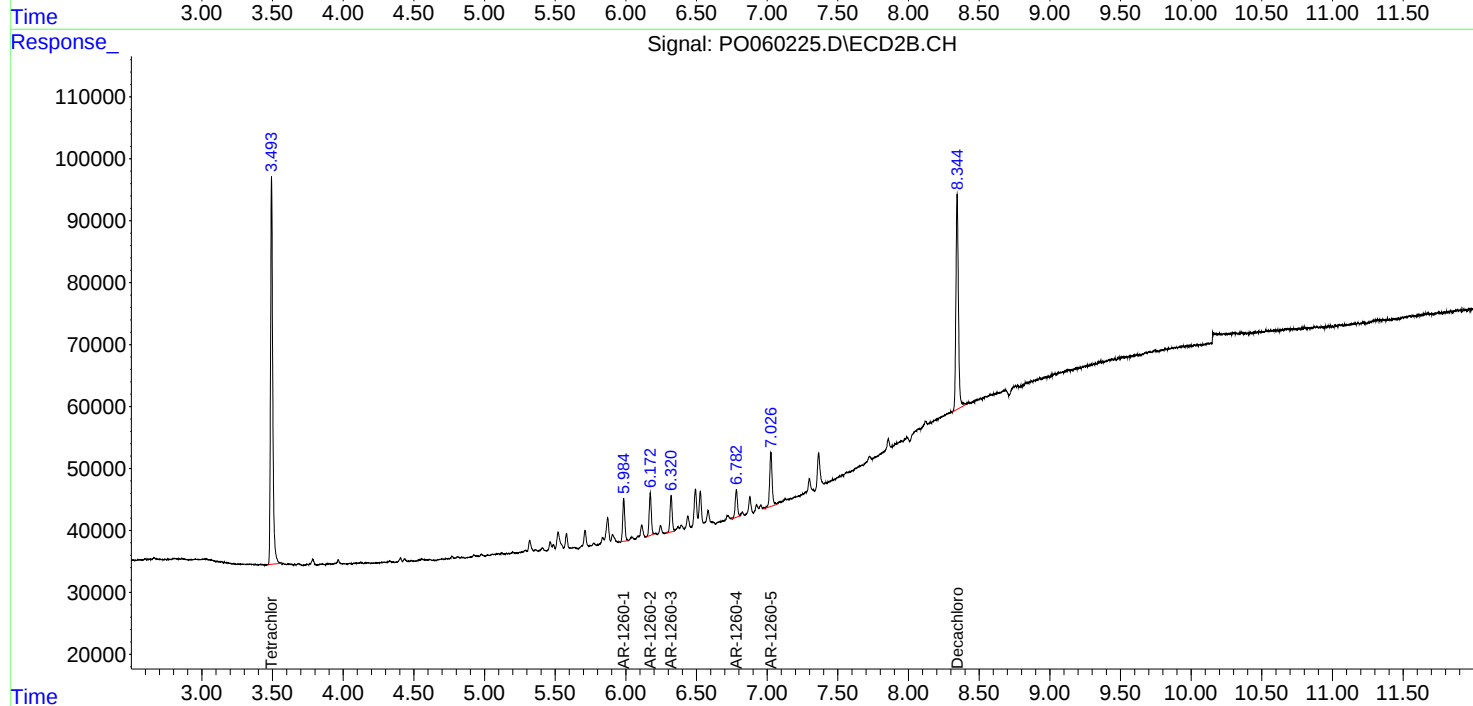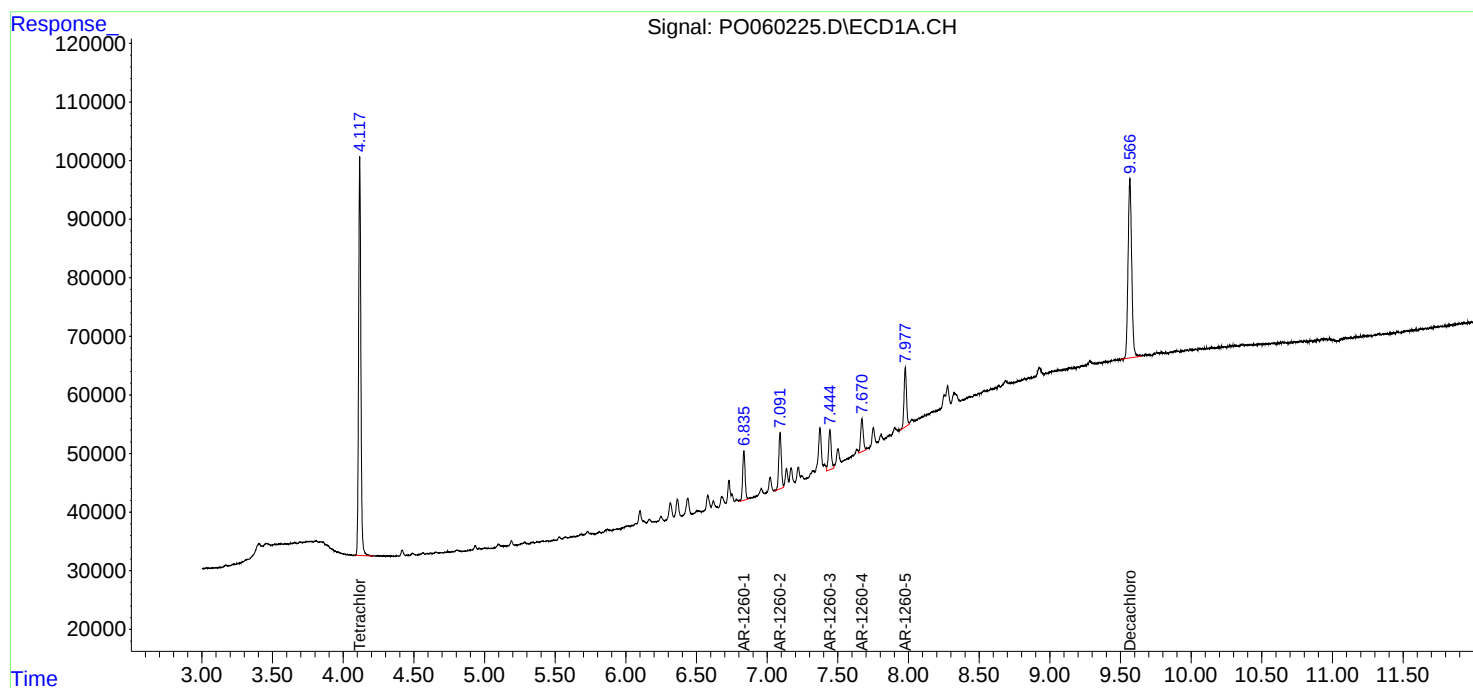

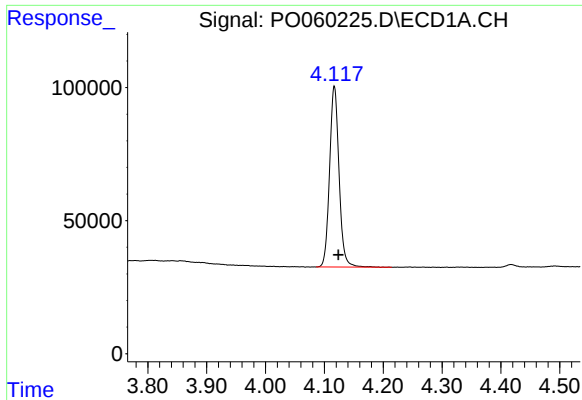


#1 Tetrachloro-m-xylene

R.T.: 4.117 min
Delta R.T.: -0.007 min
Response: 759319
Conc: 21.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:37 PM

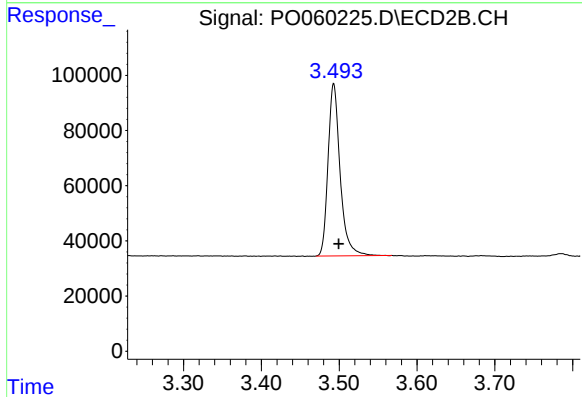


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: -0.006 min
Response: 673752
Conc: 18.72 ng/ml

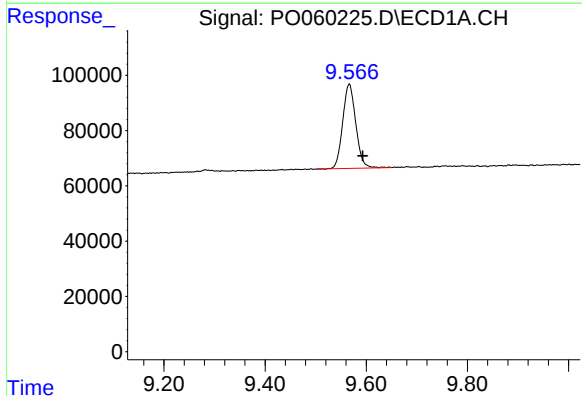


#2 Decachlorobiphenyl

R.T.: 9.566 min
Delta R.T.: -0.027 min
Response: 548561
Conc: 10.31 ng/ml

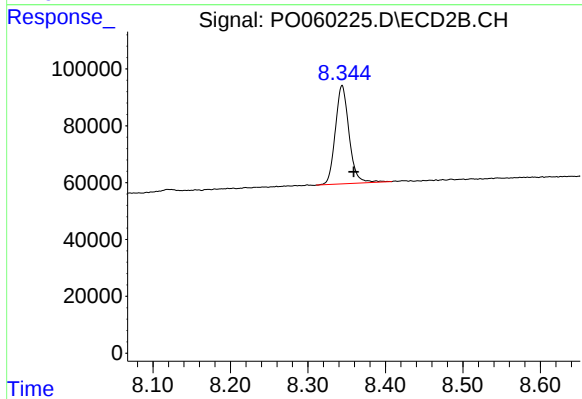

#2 Decachlorobiphenyl

R.T.: 8.344 min
Delta R.T.: -0.015 min
Response: 427735
Conc: 10.61 ng/ml

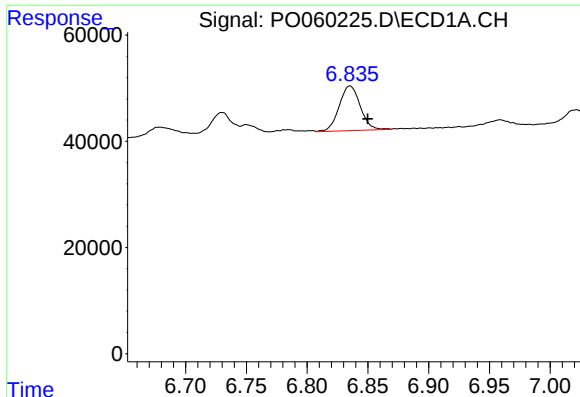


#31 AR-1260-1

R.T.: 6.835 min
Delta R.T.: -0.014 min
Response: 101398
Conc: 37.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:37 PM

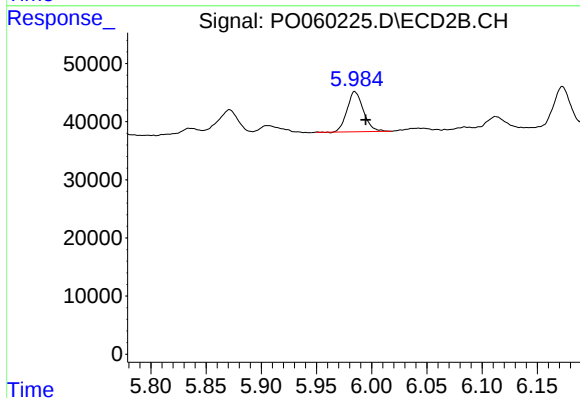


#31 AR-1260-1

R.T.: 5.985 min
Delta R.T.: -0.010 min
Response: 71094
Conc: 31.20 ng/ml

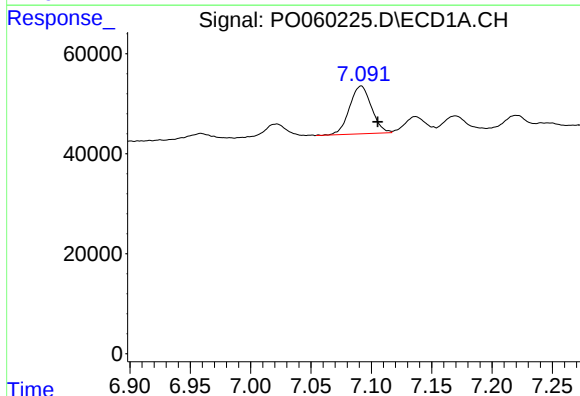


#32 AR-1260-2

R.T.: 7.091 min
Delta R.T.: -0.014 min
Response: 120943
Conc: 32.59 ng/ml

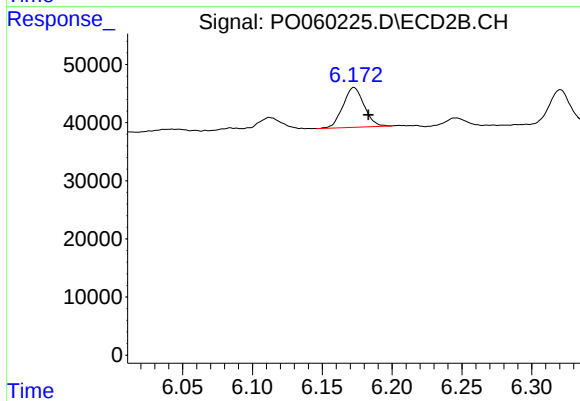

#32 AR-1260-2

R.T.: 6.173 min
Delta R.T.: -0.010 min
Response: 72448
Conc: 24.73 ng/ml

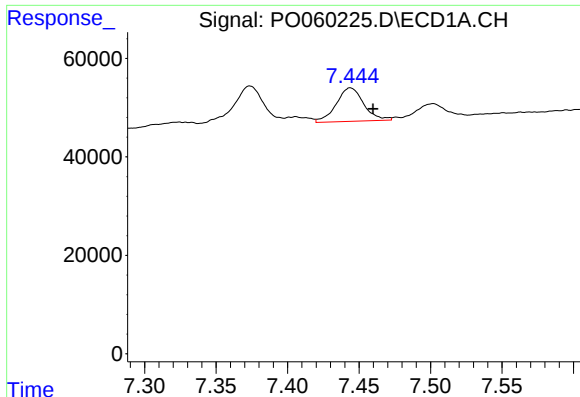


#33 AR-1260-3

R.T.: 7.444 min
Delta R.T.: -0.016 min
Response: 91283
Conc: 27.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:37 PM

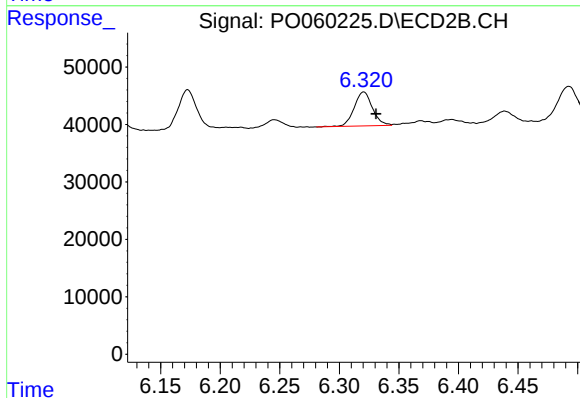


#33 AR-1260-3

R.T.: 6.321 min
Delta R.T.: -0.010 min
Response: 62476
Conc: 23.58 ng/ml

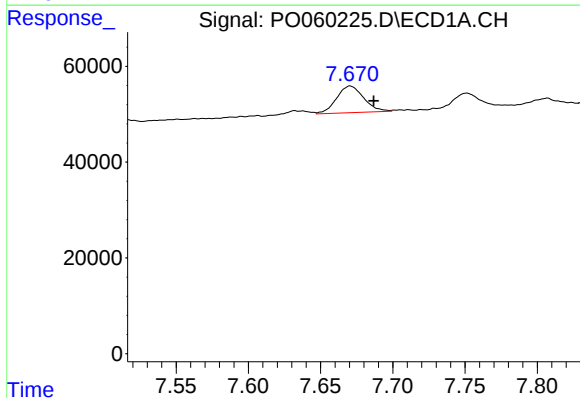


#34 AR-1260-4

R.T.: 7.670 min
Delta R.T.: -0.017 min
Response: 72632
Conc: 23.65 ng/ml m

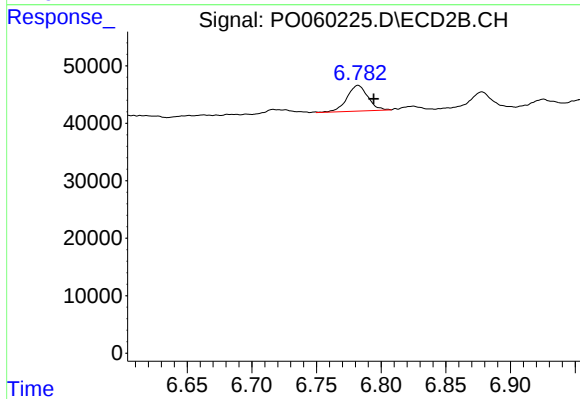

#34 AR-1260-4

R.T.: 6.782 min
Delta R.T.: -0.012 min
Response: 50280
Conc: 22.22 ng/ml

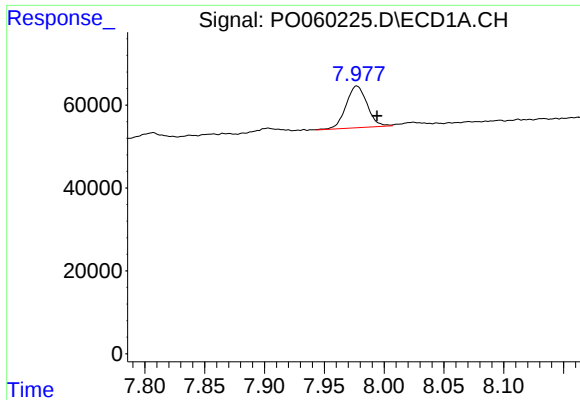


#35 AR-1260-5

R.T.: 7.977 min
Delta R.T.: -0.017 min
Response: 124047
Conc: 17.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

Manual Integrations
APPROVED

Ankita
9/4/2019 4:55:37 PM

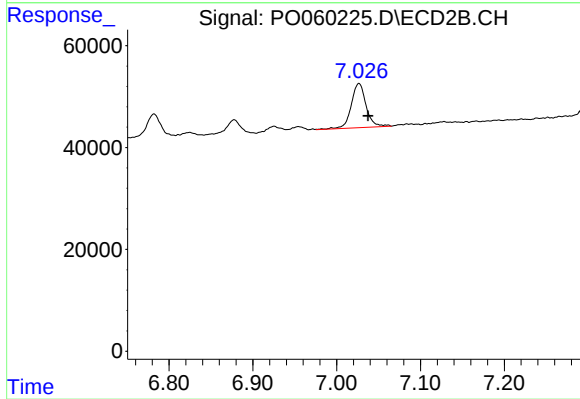

#35 AR-1260-5

R.T.: 7.027 min
Delta R.T.: -0.011 min
Response: 107440
Conc: 19.52 ng/ml