

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060231.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 13:15
 Operator : SM/AJ
 Sample : K4618-07RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-4-20-22RE

Manual Integrations
 APPROVED

Ankita
 9/4/2019 4:56:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:17:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.117	3.493	756365	623279	21.603	17.315
2)	SA Decachlor...	9.568	8.345	329236	276172	6.189m	6.849

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090319\
Data File : PO060231.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2019 13:15
Operator : SM/AJ
Sample : K4618-07RE
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-4-20-22RE


Manual Integrations
APPROVED

Ankita
9/4/2019 4:56:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:17:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

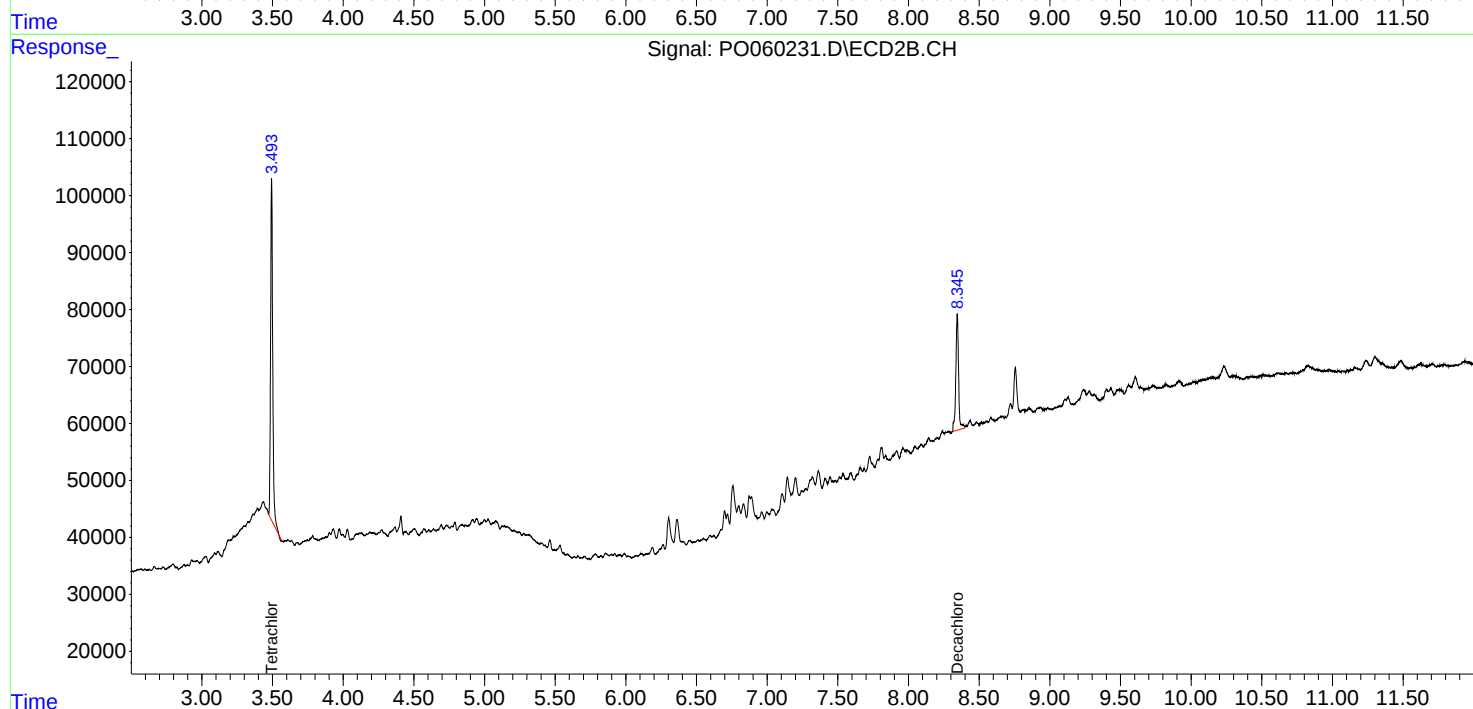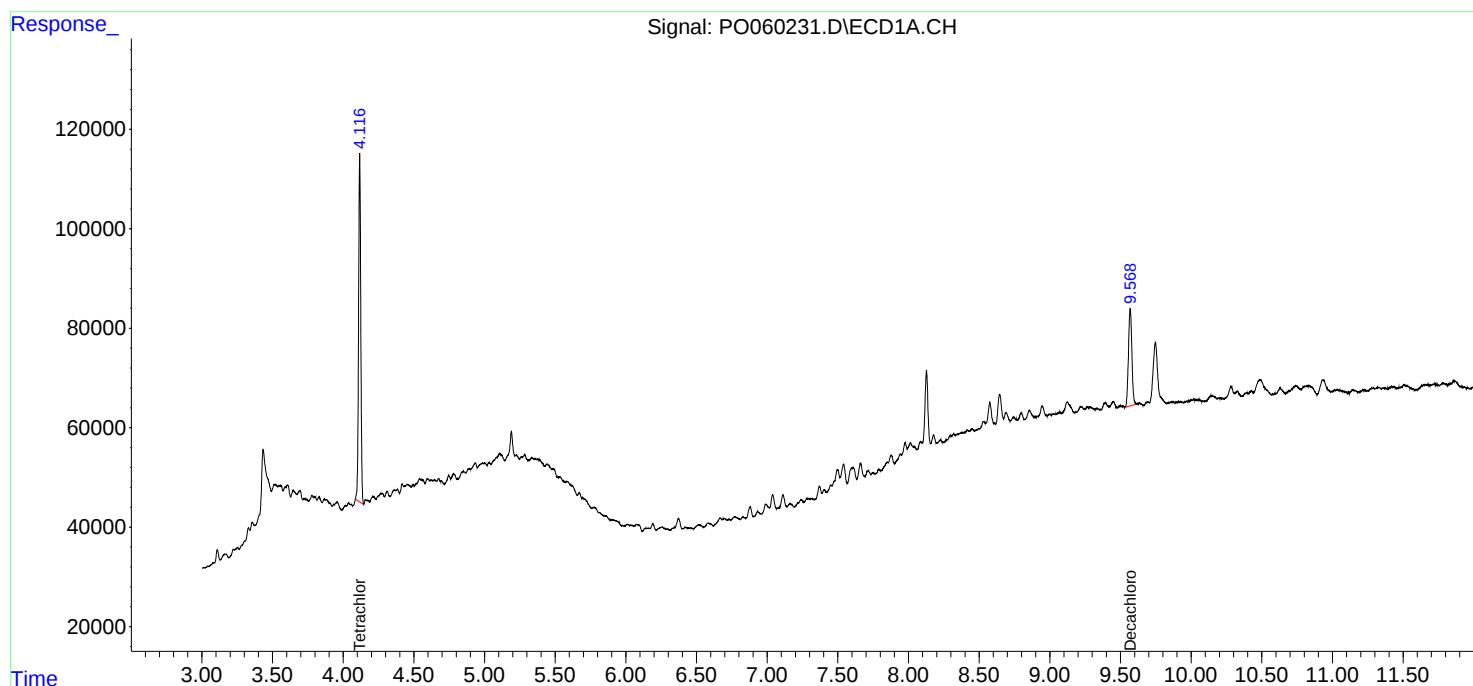

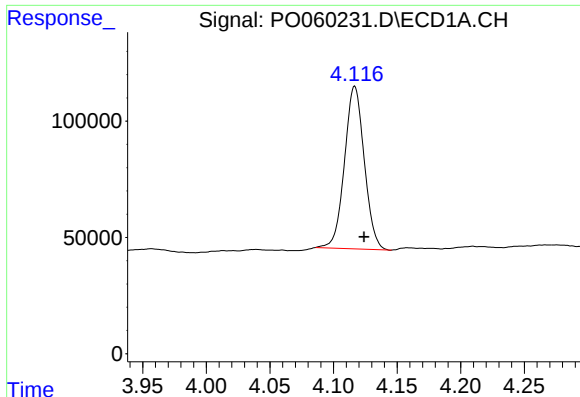


#1 Tetrachloro-m-xylene

R.T.: 4.117 min
Delta R.T.: -0.007 min
Response: 756365
Conc: 21.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-4-20-22RE


Manual Integrations
APPROVED

Ankita
9/4/2019 4:56:02 PM

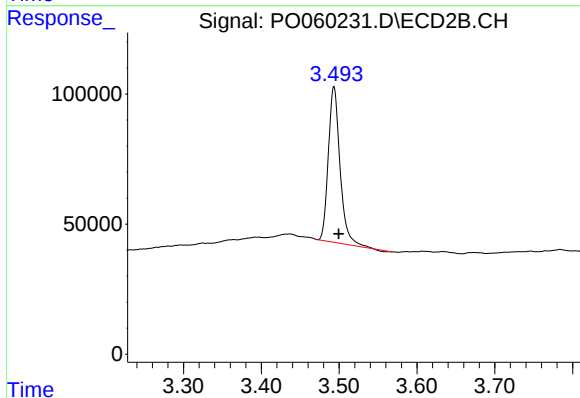


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: -0.006 min
Response: 623279
Conc: 17.32 ng/ml

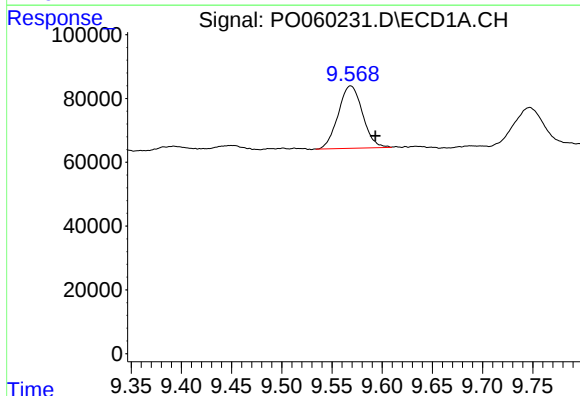

#2 Decachlorobiphenyl

R.T.: 9.568 min
Delta R.T.: -0.025 min
Response: 329236
Conc: 6.19 ng/ml m

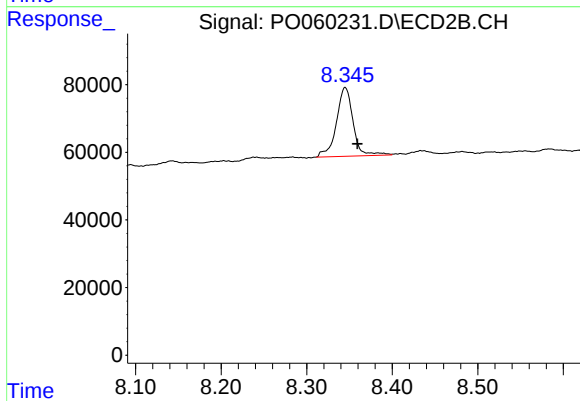

#2 Decachlorobiphenyl

R.T.: 8.345 min
Delta R.T.: -0.014 min
Response: 276172
Conc: 6.85 ng/ml