

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060254.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 19:41
 Operator : SM/AJ
 Sample : K4554-43
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-4-(0-2)

Manual Integrations
 APPROVED

Ankita
 9/4/2019 4:56:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 03:39:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.112	3.493	892062	745984	25.478	20.724
2) SA Decachlor...	9.563	8.343	790614	630533	14.861m	15.638

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090319\
Data File : PO060254.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2019 19:41
Operator : SM/AJ
Sample : K4554-43
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-4-(0-2)


Manual Integrations
APPROVED

Ankita
9/4/2019 4:56:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 03:39:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

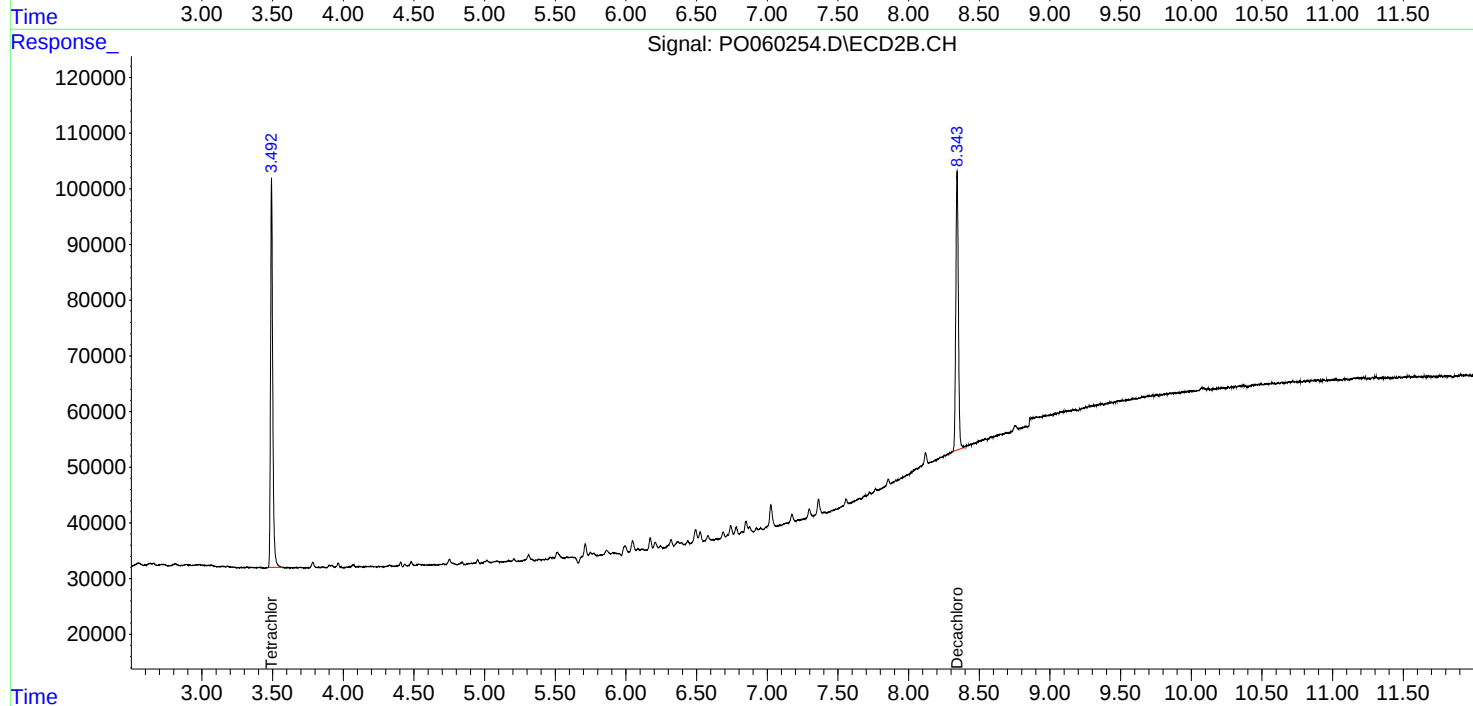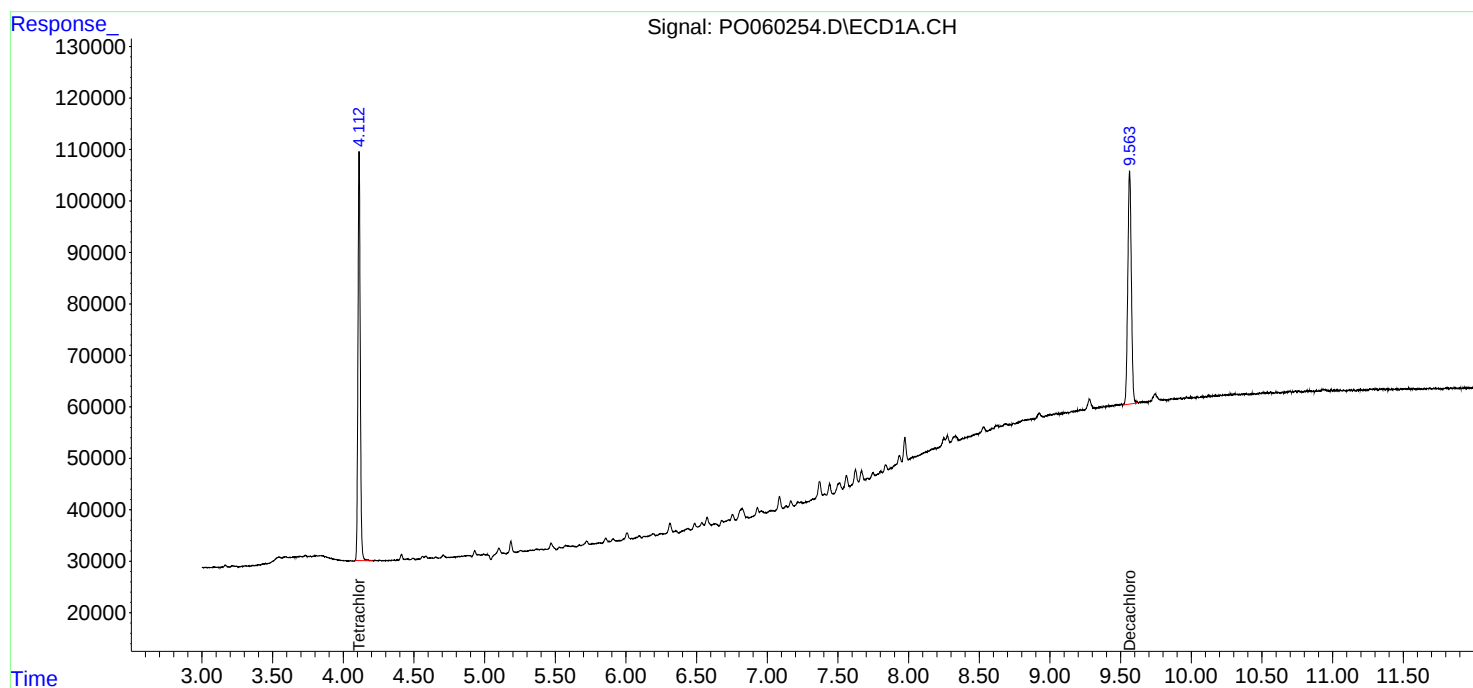

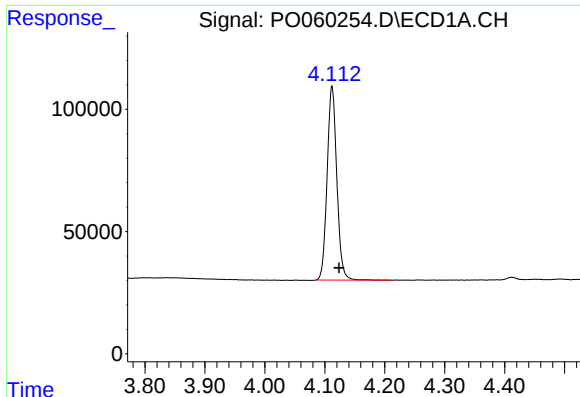


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: -0.012 min
Response: 892062
Conc: 25.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-4-(0-2)


Manual Integrations
APPROVED

Ankita
9/4/2019 4:56:38 PM

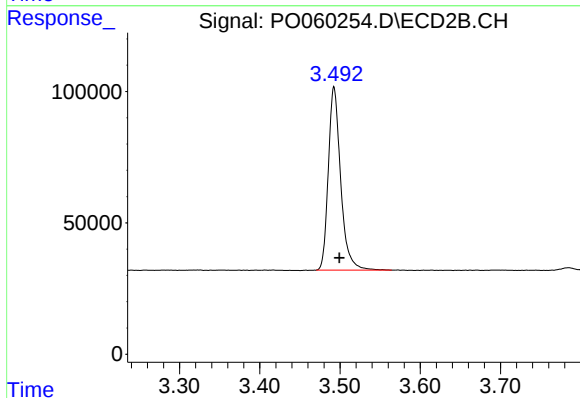


#1 Tetrachloro-m-xylene

R.T.: 3.493 min
Delta R.T.: -0.007 min
Response: 745984
Conc: 20.72 ng/ml

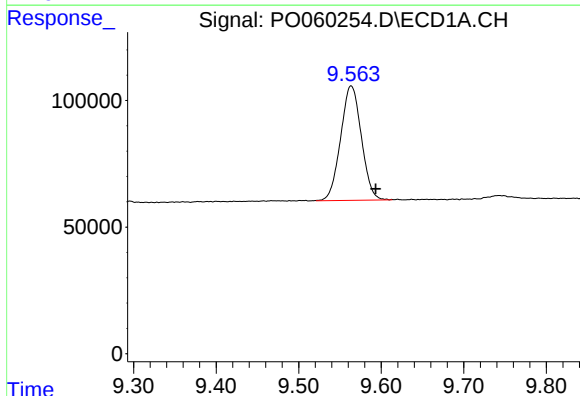

#2 Decachlorobiphenyl

R.T.: 9.563 min
Delta R.T.: -0.030 min
Response: 790614
Conc: 14.86 ng/ml m

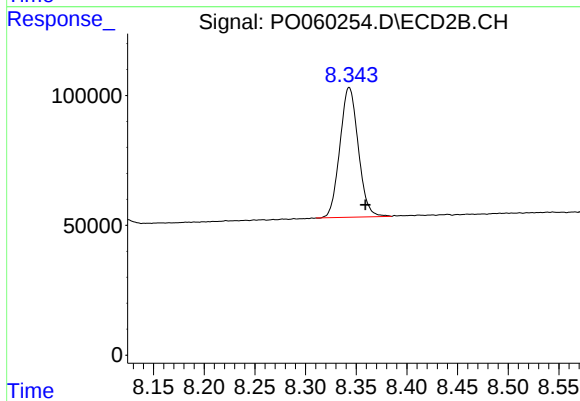

#2 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.016 min
Response: 630533
Conc: 15.64 ng/ml