

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060256.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2019 20:13
 Operator : SM/AJ
 Sample : K4554-45
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-2-(0-2)

Manual Integrations
 APPROVED

Ankita
 9/4/2019 4:56:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 03:40:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.112	3.492	1055174	879516	30.137	24.434
2) SA Decachlor...	9.562	8.343	1069275	855213	20.099m	21.210

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
Data File : P0060256.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2019 20:13
Operator : SM/AJ
Sample : K4554-45
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-2-(0-2)


Manual Integrations
APPROVED

Ankita
9/4/2019 4:56:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 03:40:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

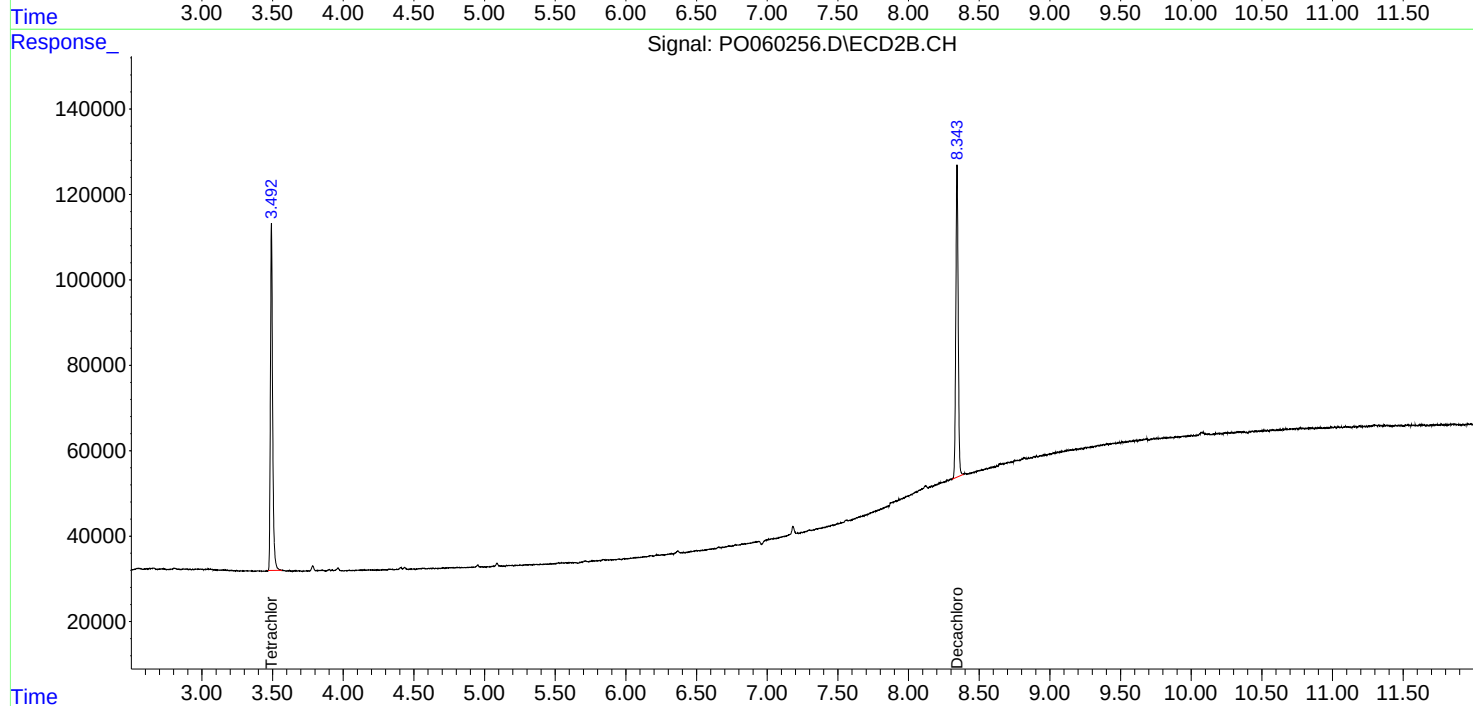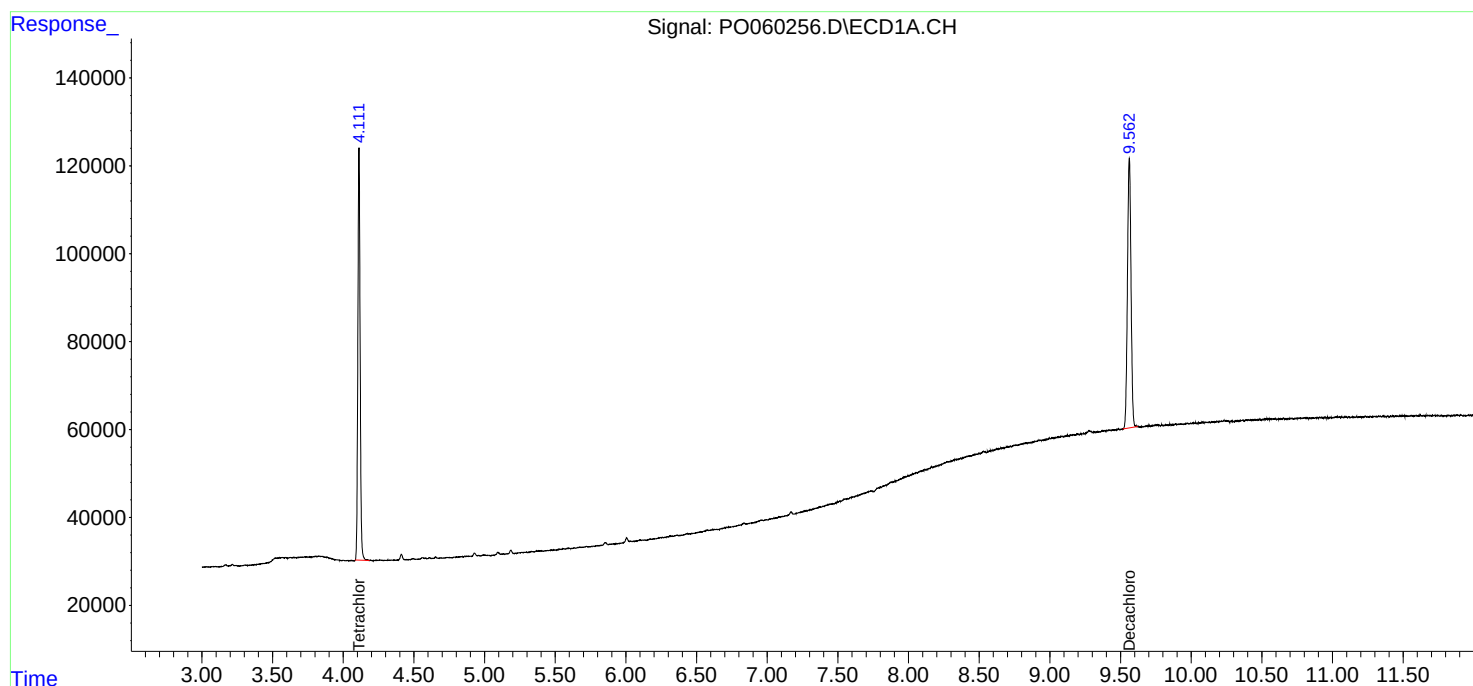

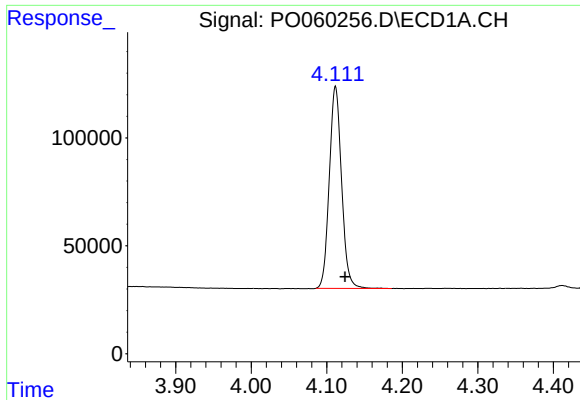


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: -0.012 min
Response: 1055174
Conc: 30.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-2-(0-2)


Manual Integrations
APPROVED

Ankita
9/4/2019 4:56:40 PM

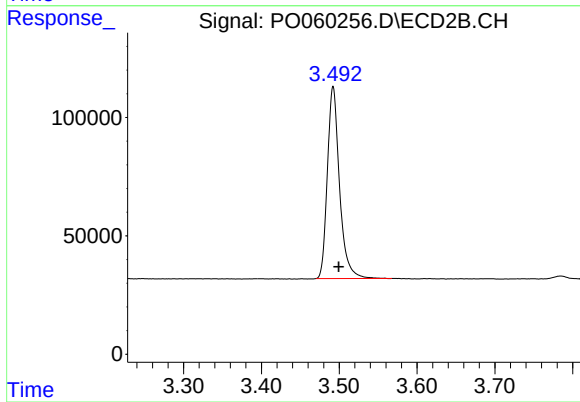


#1 Tetrachloro-m-xylene

R.T.: 3.492 min
Delta R.T.: -0.007 min
Response: 879516
Conc: 24.43 ng/ml

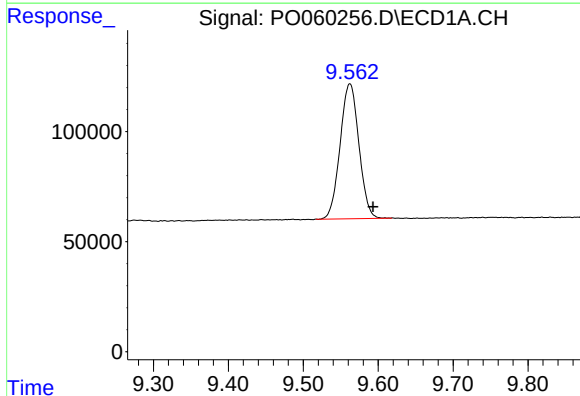

#2 Decachlorobiphenyl

R.T.: 9.562 min
Delta R.T.: -0.031 min
Response: 1069275
Conc: 20.10 ng/ml m

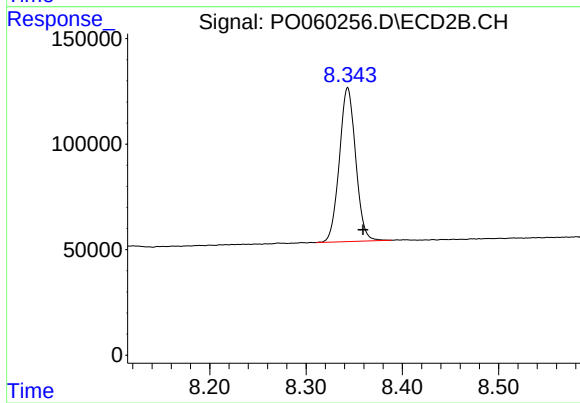

#2 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.016 min
Response: 855213
Conc: 21.21 ng/ml