

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060282.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2019 4:34
 Operator : SM/AJ
 Sample : K4626-01 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1-2-EWC-1

Manual Integrations
 APPROVED

Ankita
 9/4/2019 4:57:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 07:14:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.110	3.492	226025	176014	6.456m	4.890m
2) SA Decachlor...	9.562	8.343	299475	195044	5.629	4.837

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
Data File : P0060282.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2019 4:34
Operator : SM/AJ
Sample : K4626-01 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1-2-EWC-1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:57:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 07:14:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

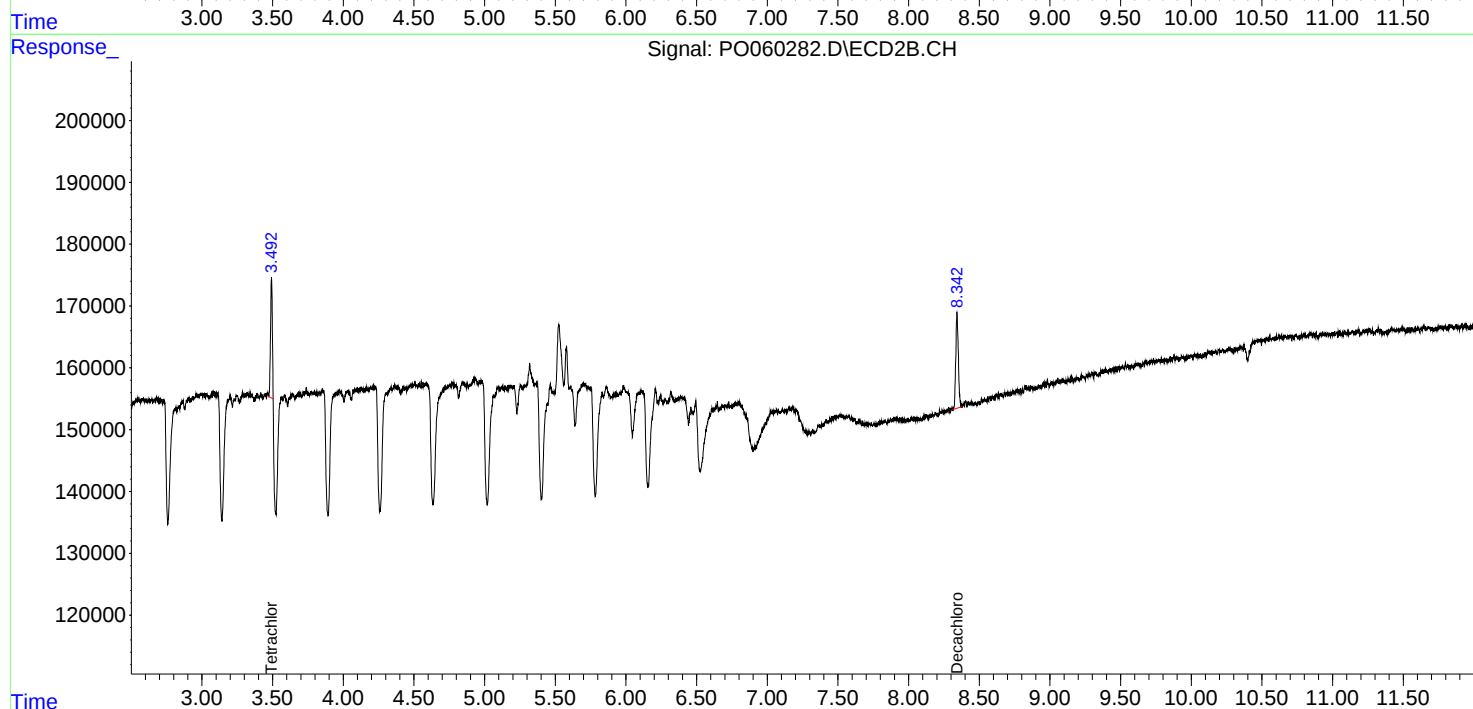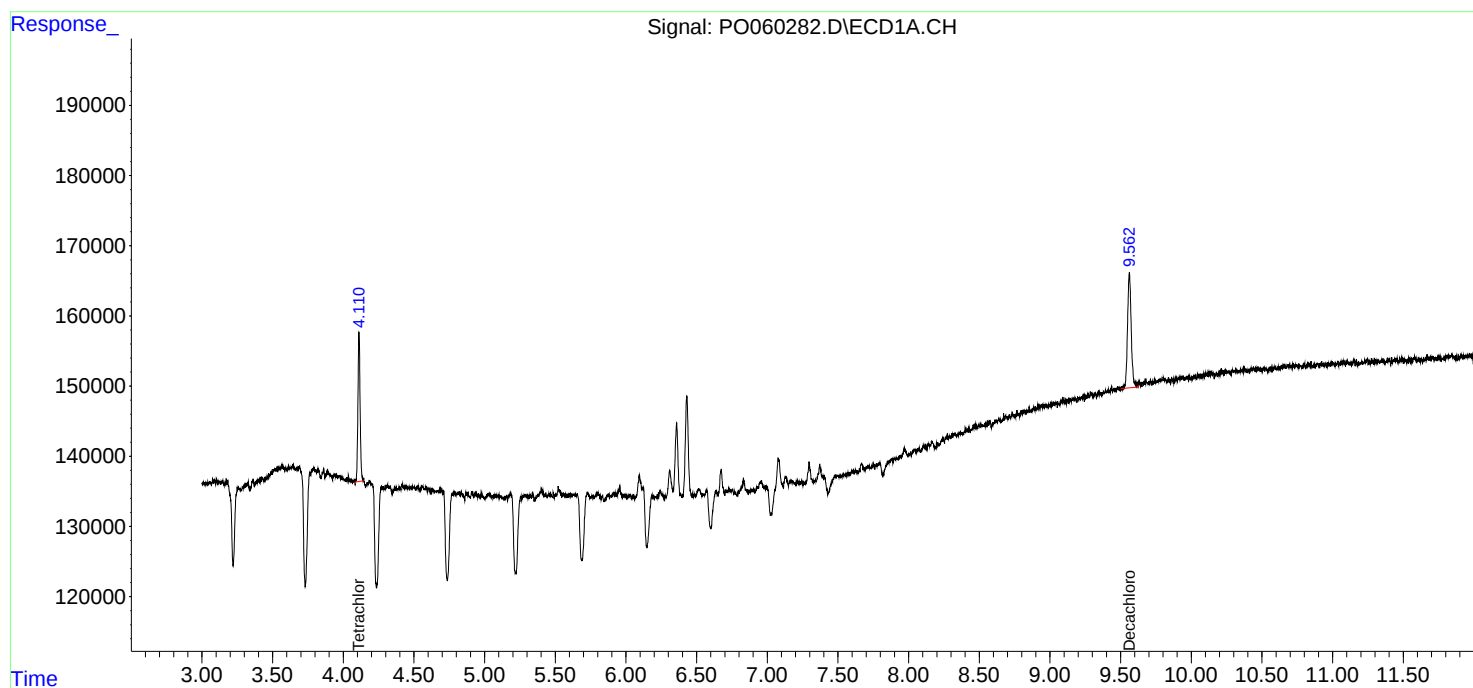

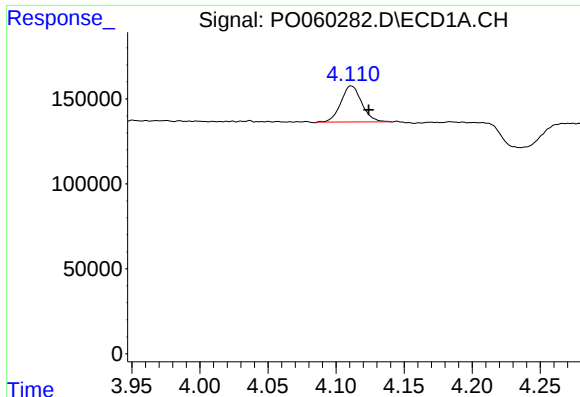


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.014 min
Response: 226025
Conc: 6.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1-2-EWC-1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:57:33 PM

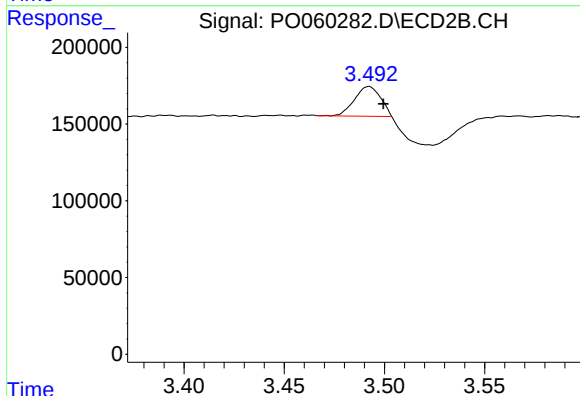


#1 Tetrachloro-m-xylene

R.T.: 3.492 min
Delta R.T.: -0.007 min
Response: 176014
Conc: 4.89 ng/ml m

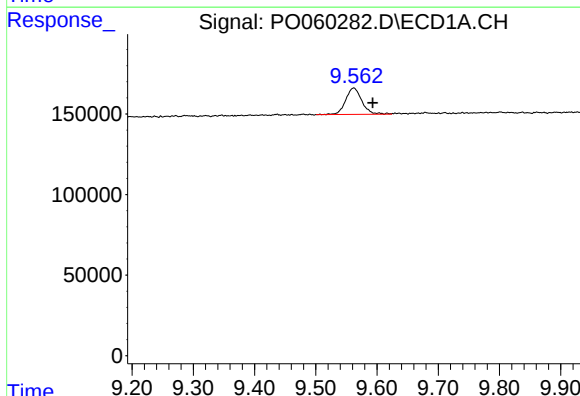

#2 Decachlorobiphenyl

R.T.: 9.562 min
Delta R.T.: -0.031 min
Response: 299475
Conc: 5.63 ng/ml

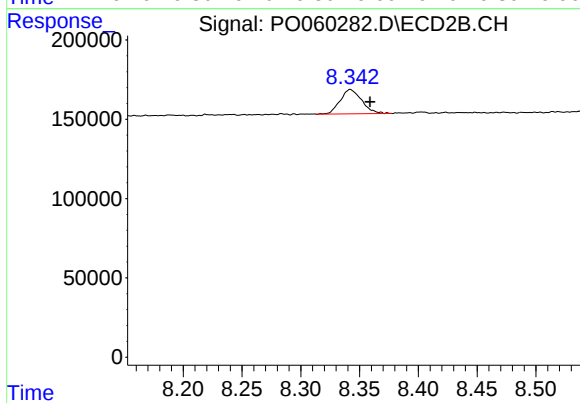

#2 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.017 min
Response: 195044
Conc: 4.84 ng/ml