

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060287.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2019 5:56
 Operator : SM/AJ
 Sample : K4626-06 5X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1-2-EXFC-1

Manual Integrations
 APPROVED

Ankita
 9/4/2019 4:58:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 07:16:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.111	3.492	278391	225508	7.951	6.265m
2) SA Decachlor...	9.561	8.341	278860	185328	5.242	4.596

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
Data File : P0060287.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2019 5:56
Operator : SM/AJ
Sample : K4626-06 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1-2-EXFC-1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:58:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 07:16:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

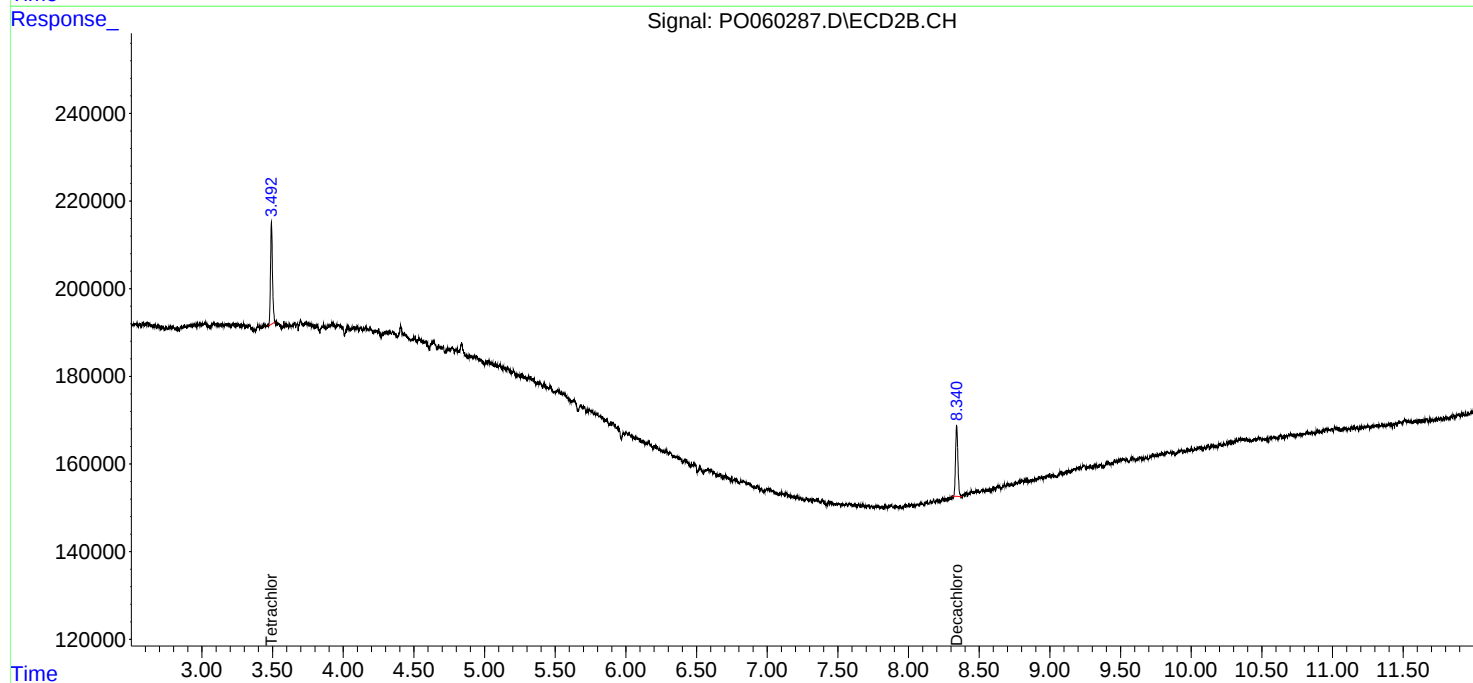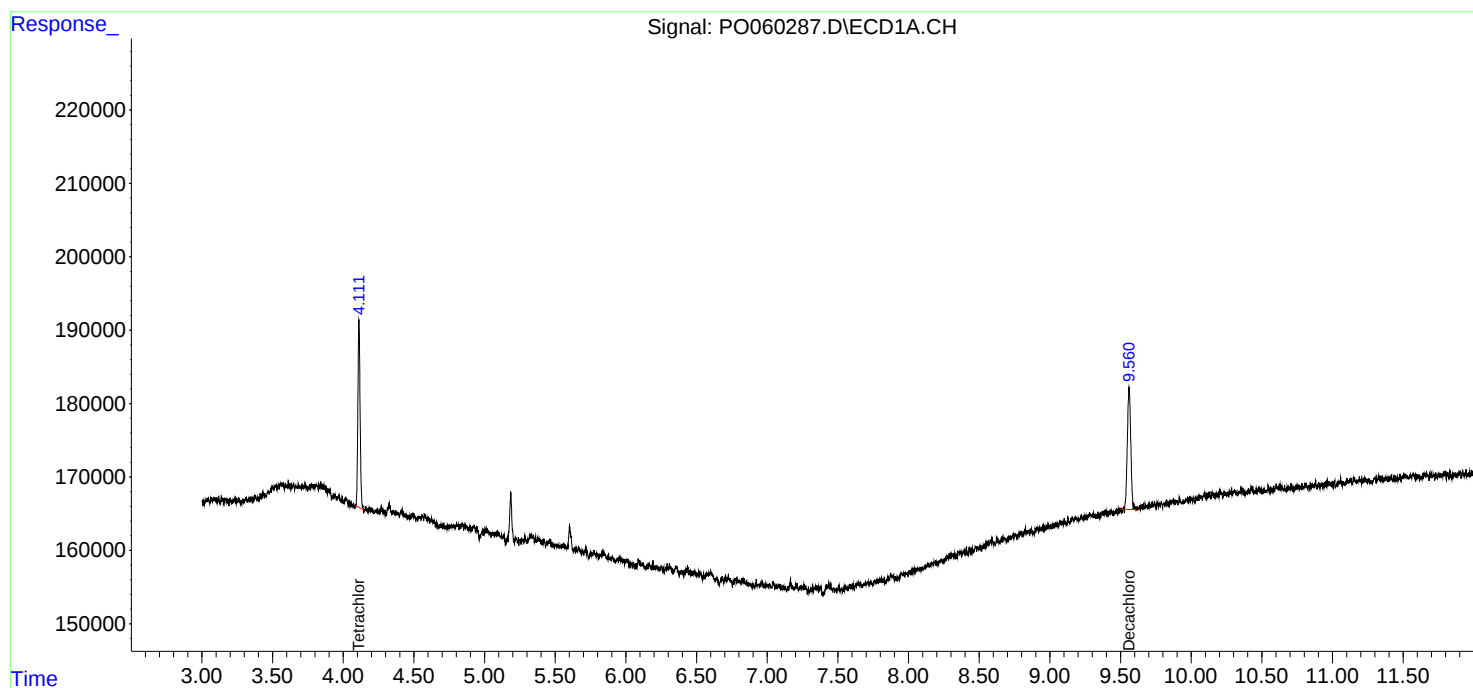

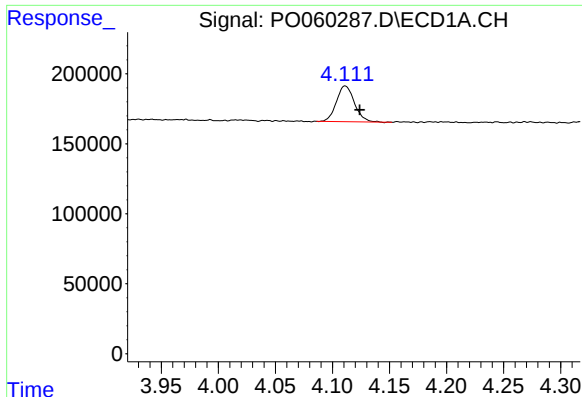


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.013 min
Response: 278391
Conc: 7.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
1-2-EXFC-1


Manual Integrations
APPROVED

Ankita
9/4/2019 4:58:17 PM

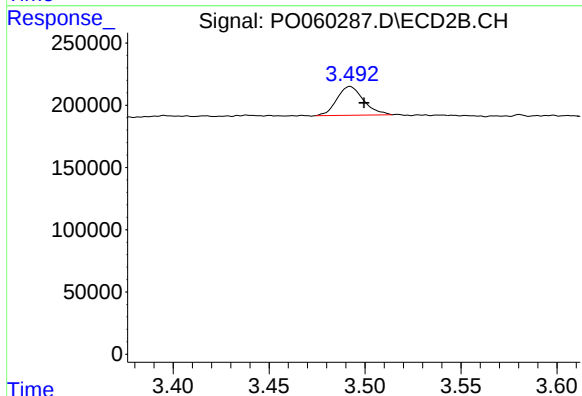


#1 Tetrachloro-m-xylene

R.T.: 3.492 min
Delta R.T.: -0.008 min
Response: 225508
Conc: 6.26 ng/ml m

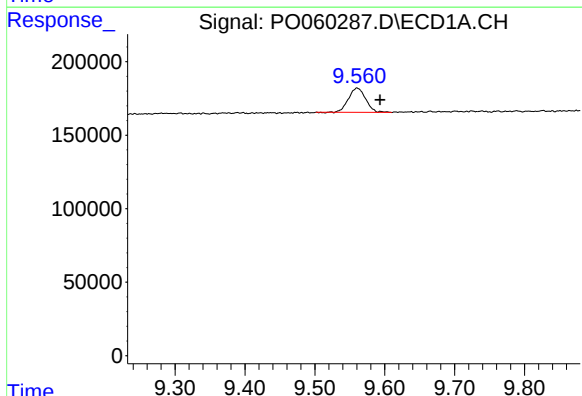

#2 Decachlorobiphenyl

R.T.: 9.561 min
Delta R.T.: -0.033 min
Response: 278860
Conc: 5.24 ng/ml

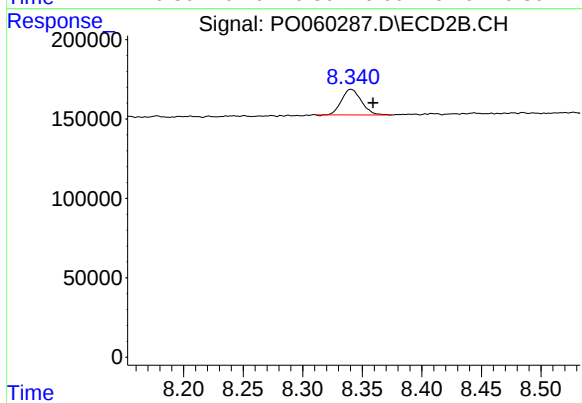

#2 Decachlorobiphenyl

R.T.: 8.341 min
Delta R.T.: -0.018 min
Response: 185328
Conc: 4.60 ng/ml