

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
 Data File : P0060300.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2019 9:29
 Operator : SM/AJ
 Sample : K4627-13DL 5X
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 7-6-FSC-1DL

Manual Integrations
 APPROVED

Ankita
 9/6/2019 9:03:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 12:10:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.116	3.492	204210	190220	5.832m	5.285
2) SA Decachlor...	9.571	8.342	290017	157639	5.451m	3.910m#
Target Compounds						
26) L6 AR-1254-1	6.097	5.318	1039286	915298	498.120m	385.908m
27) L6 AR-1254-2	6.311	5.464	1591954	893958	477.169	426.039m
28) L6 AR-1254-3	6.678	5.865	1568991	1546752	442.161	459.999m
29) L6 AR-1254-4	6.959	6.085	759066	355939	257.700	172.633m#
30) L6 AR-1254-5	7.374	6.493	1914967	1505697	619.250m	484.931

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090319\
Data File : P0060300.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2019 9:29
Operator : SM/AJ
Sample : K4627-13DL 5X
Misc :
ALS Vial : 75 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
7-6-FSC-1DL


Manual Integrations
APPROVED

Ankita
9/6/2019 9:03:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 12:10:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

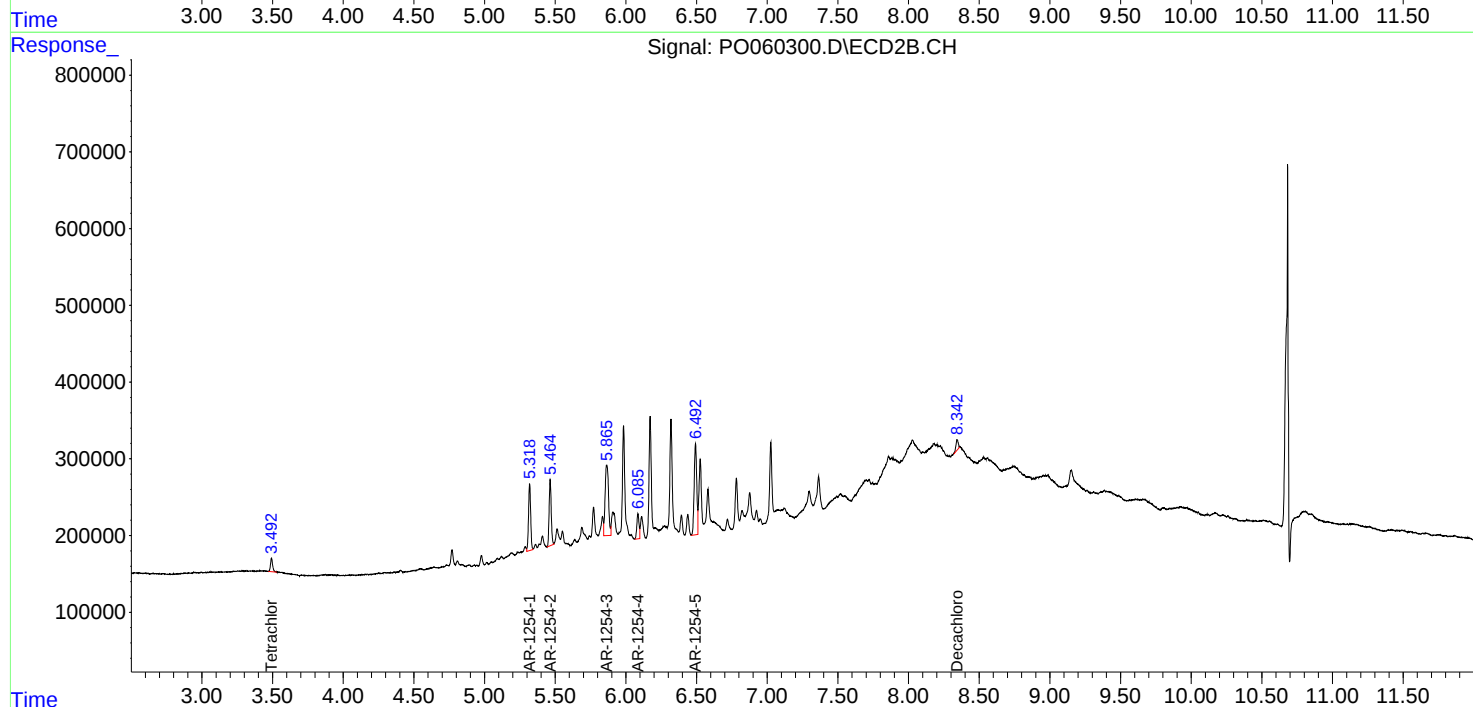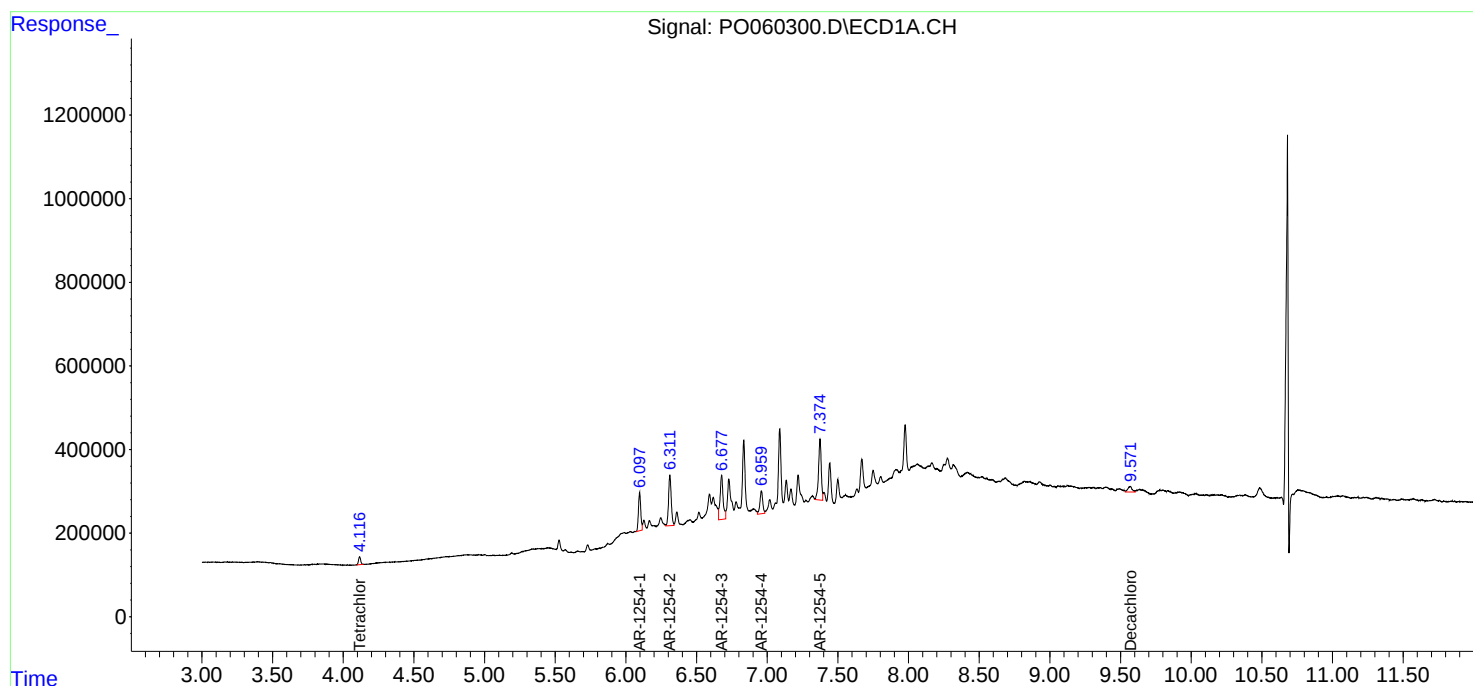

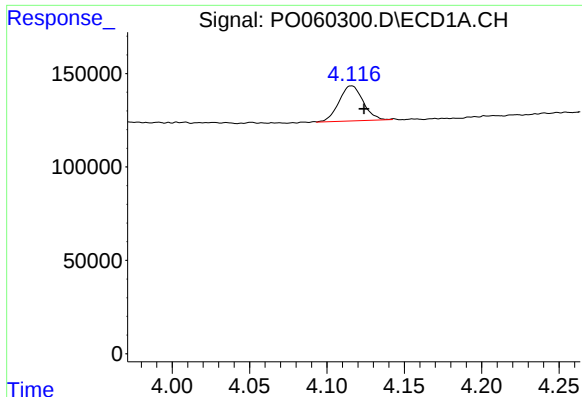


#1 Tetrachloro-m-xylene

R.T.: 4.116 min
Delta R.T.: -0.008 min
Response: 204210
Conc: 5.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
7-6-FSC-1DL


Manual Integrations
APPROVED

Ankita
9/6/2019 9:03:47 AM

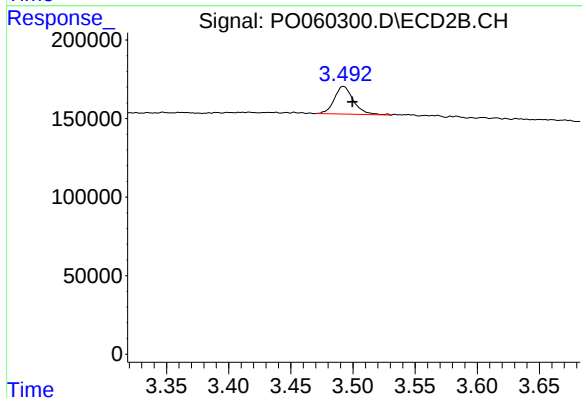


#1 Tetrachloro-m-xylene

R.T.: 3.492 min
Delta R.T.: -0.007 min
Response: 190220
Conc: 5.28 ng/ml

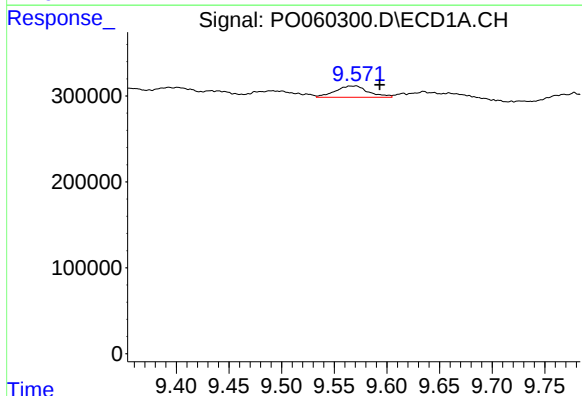


#2 Decachlorobiphenyl

R.T.: 9.571 min
Delta R.T.: -0.022 min
Response: 290017
Conc: 5.45 ng/ml m

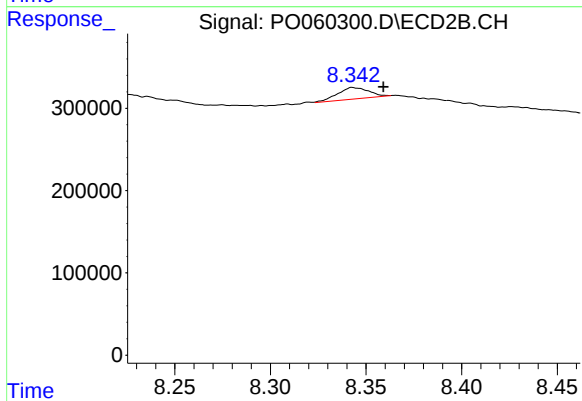

#2 Decachlorobiphenyl

R.T.: 8.342 min
Delta R.T.: -0.017 min
Response: 157639
Conc: 3.91 ng/ml m

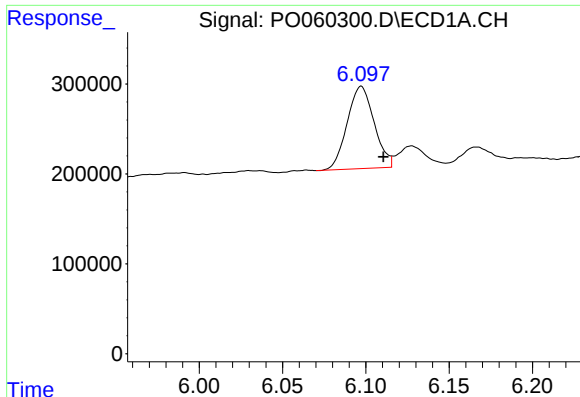


#26 AR-1254-1

R.T.: 6.097 min
Delta R.T.: -0.014 min
Response: 1039286
Conc: 498.12 ng/ml m

Instrument :
ECD_O
ClientSampleId :
7-6-FSC-1DL


Manual Integrations
APPROVED

Ankita
9/6/2019 9:03:47 AM

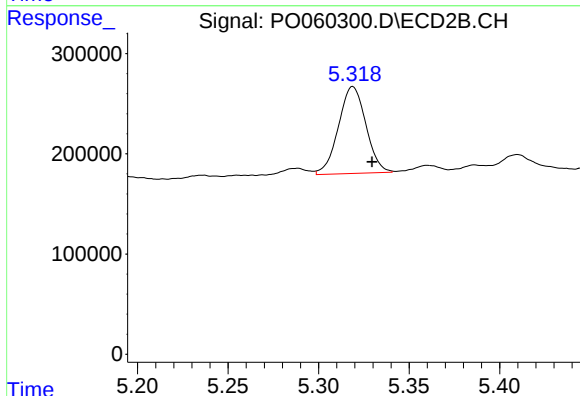


#26 AR-1254-1

R.T.: 5.318 min
Delta R.T.: -0.011 min
Response: 915298
Conc: 385.91 ng/ml m

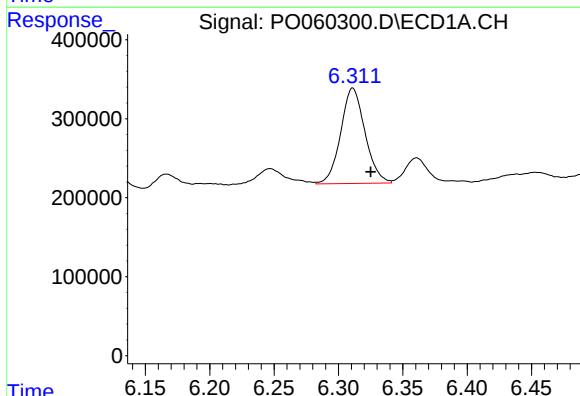


#27 AR-1254-2

R.T.: 6.311 min
Delta R.T.: -0.014 min
Response: 1591954
Conc: 477.17 ng/ml

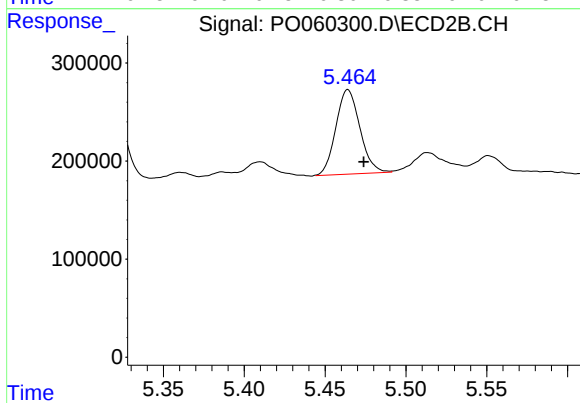

#27 AR-1254-2

R.T.: 5.464 min
Delta R.T.: -0.010 min
Response: 893958
Conc: 426.04 ng/ml m

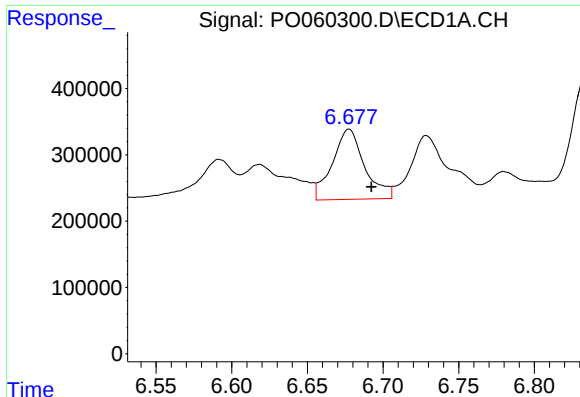


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: -0.015 min
Response: 1568991
Conc: 442.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
7-6-FSC-1DL


Manual Integrations
APPROVED

Ankita
9/6/2019 9:03:47 AM

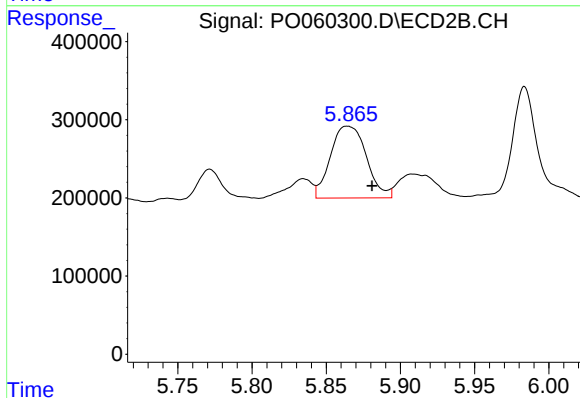


#28 AR-1254-3

R.T.: 5.865 min
Delta R.T.: -0.016 min
Response: 1546752
Conc: 460.00 ng/ml m

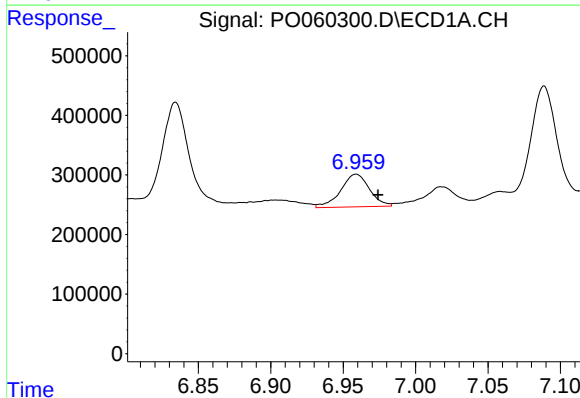


#29 AR-1254-4

R.T.: 6.959 min
Delta R.T.: -0.015 min
Response: 759066
Conc: 257.70 ng/ml

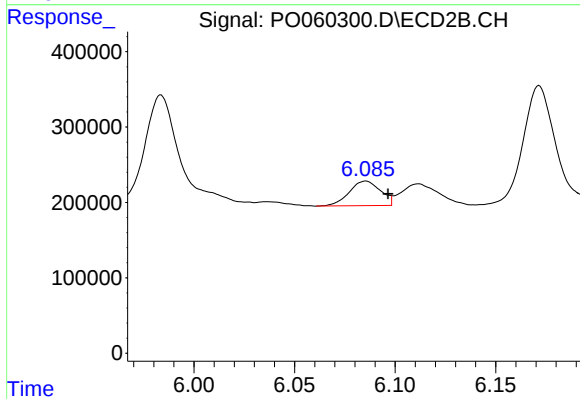

#29 AR-1254-4

R.T.: 6.085 min
Delta R.T.: -0.011 min
Response: 355939
Conc: 172.63 ng/ml m

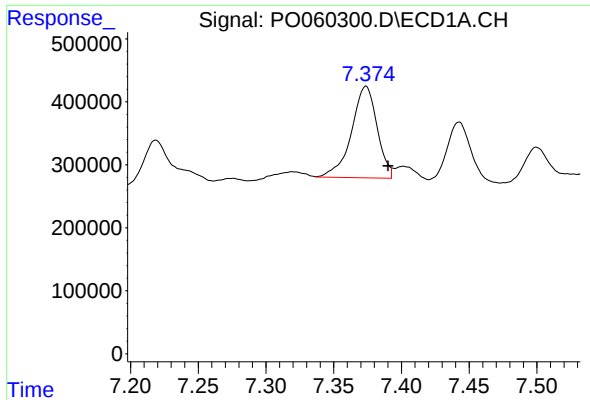


#30 AR-1254-5

R.T.: 7.374 min
Delta R.T.: -0.017 min
Response: 1914967
Conc: 619.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
7-6-FSC-1DL

Manual Integrations
APPROVED

Ankita
9/6/2019 9:03:47 AM

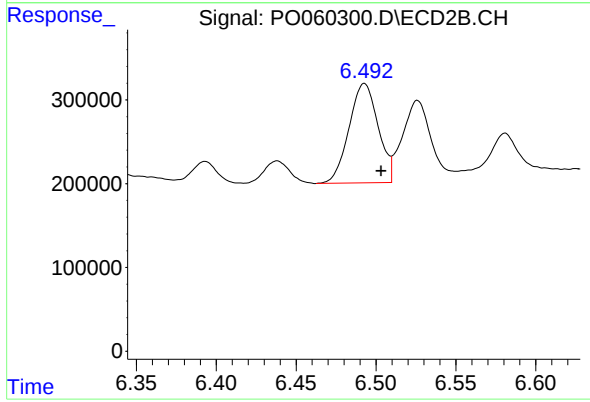

#30 AR-1254-5

R.T.: 6.493 min
Delta R.T.: -0.011 min
Response: 1505697
Conc: 484.93 ng/ml