

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090320\
 Data File : P0071137.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2020 10:40
 Operator : DD\AJ
 Sample : L3875-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DIELETRIC-FLUID-TOTE-F7RE

Manual Integrations
 APPROVED

Ankita
 9/4/2020 2:44:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 17:45:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.365	3.543	15995106	1703631	207.115	38.430 #
2) SA Decachlor...	9.972	8.721	1695242	904135	18.527	15.741m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090320\
Data File : PO071137.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2020 10:40
Operator : DD\AJ
Sample : L3875-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DIELETRIC-FLUID-TOTE-F7RE


Manual Integrations
APPROVED

Ankita
9/4/2020 2:44:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 17:45:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

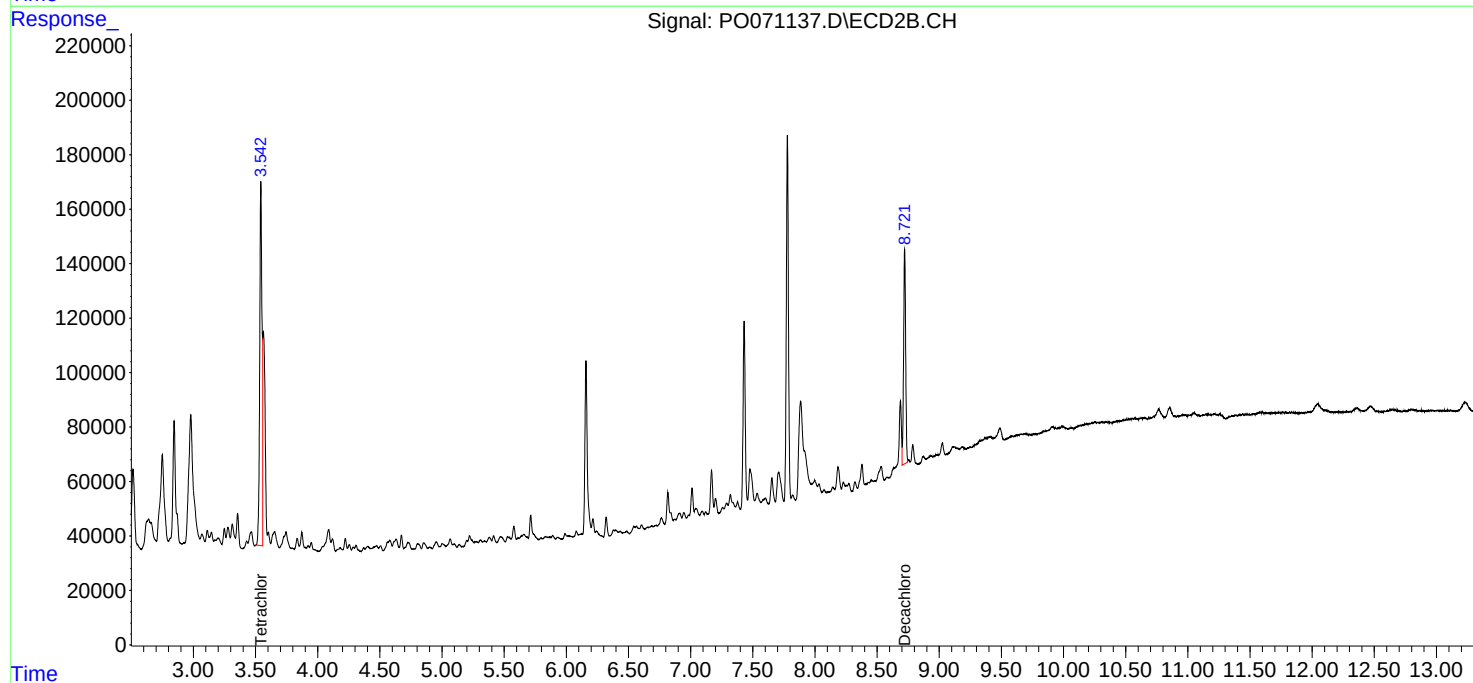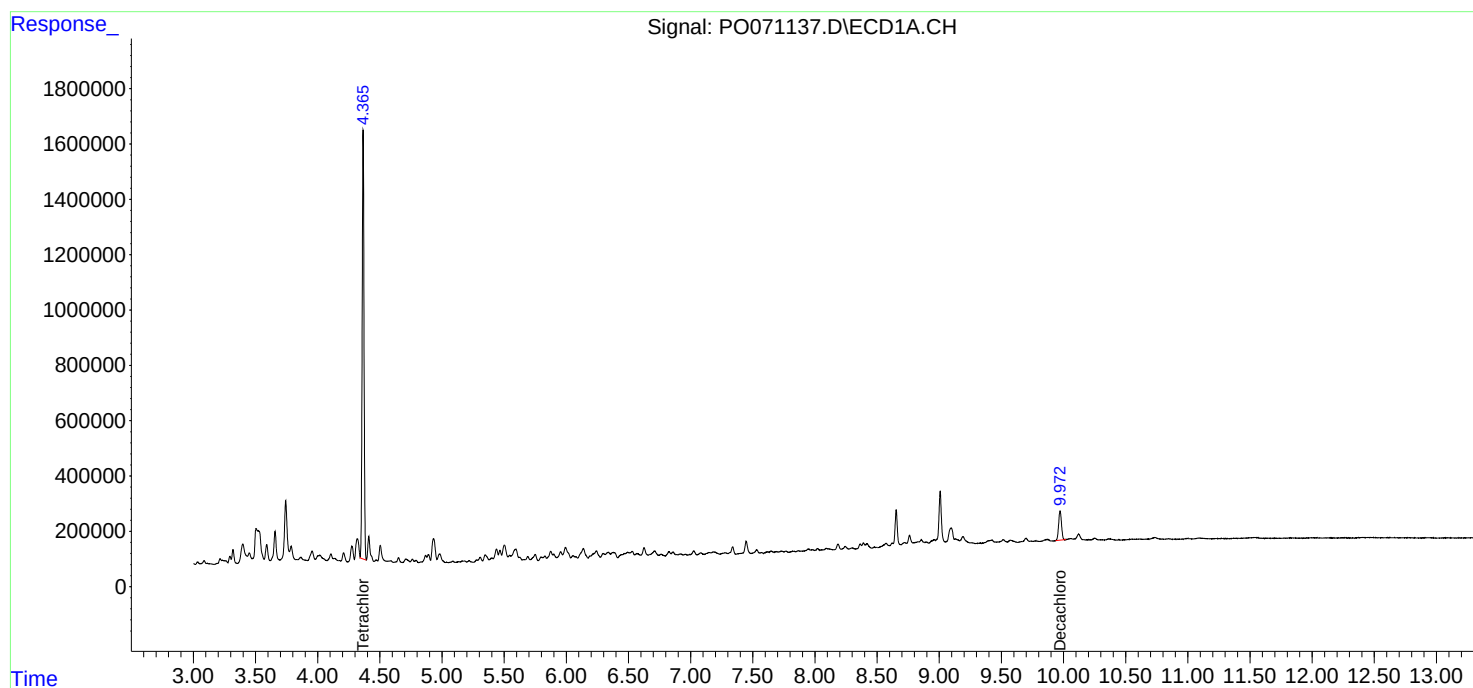

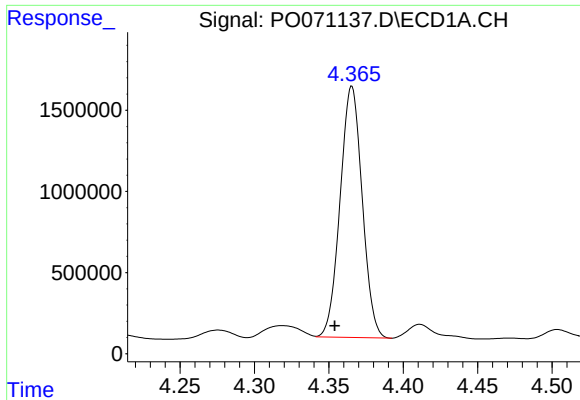


#1 Tetrachloro-m-xylene

R.T.: 4.365 min
Delta R.T.: 0.011 min
Response: 15995106
Conc: 207.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
DIELETRIC-FLUID-TOTE-F7RE


Manual Integrations
APPROVED

Ankita
9/4/2020 2:44:43 PM

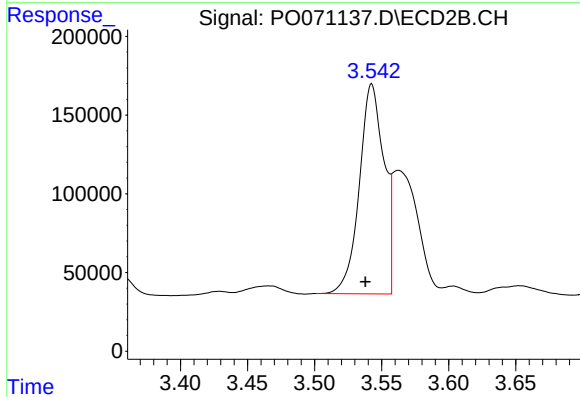


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.005 min
Response: 1703631
Conc: 38.43 ng/ml

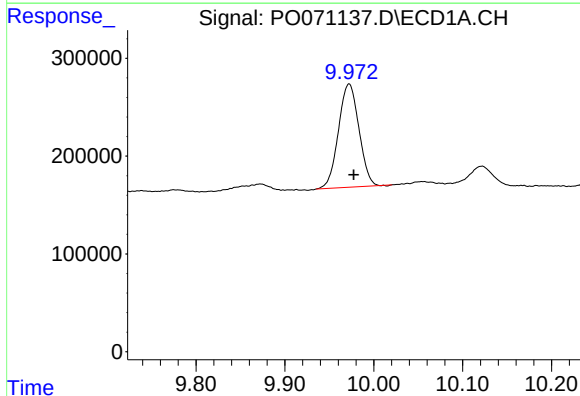

#2 Decachlorobiphenyl

R.T.: 9.972 min
Delta R.T.: -0.005 min
Response: 1695242
Conc: 18.53 ng/ml

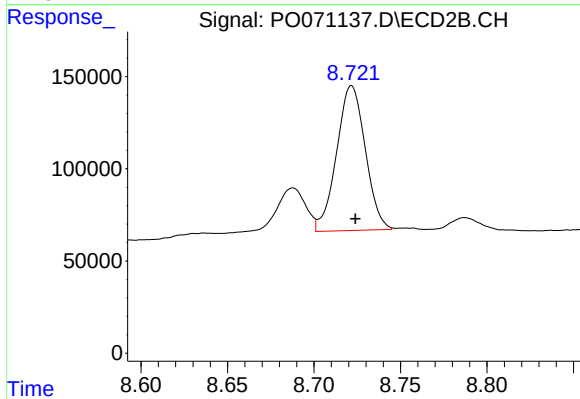

#2 Decachlorobiphenyl

R.T.: 8.721 min
Delta R.T.: -0.003 min
Response: 904135
Conc: 15.74 ng/ml m