

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090320\
 Data File : P0071146.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2020 13:55
 Operator : DD\AJ
 Sample : L3877-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

Ankita
 9/4/2020 2:44:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 17:49:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.539	2056353	1496927	26.627m	33.767 #
2) SA Decachlor...	9.971	8.720	1734603	964574	18.957	16.793

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090320\
Data File : P0071146.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2020 13:55
Operator : DD\AJ
Sample : L3877-17
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
9/4/2020 2:44:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 17:49:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

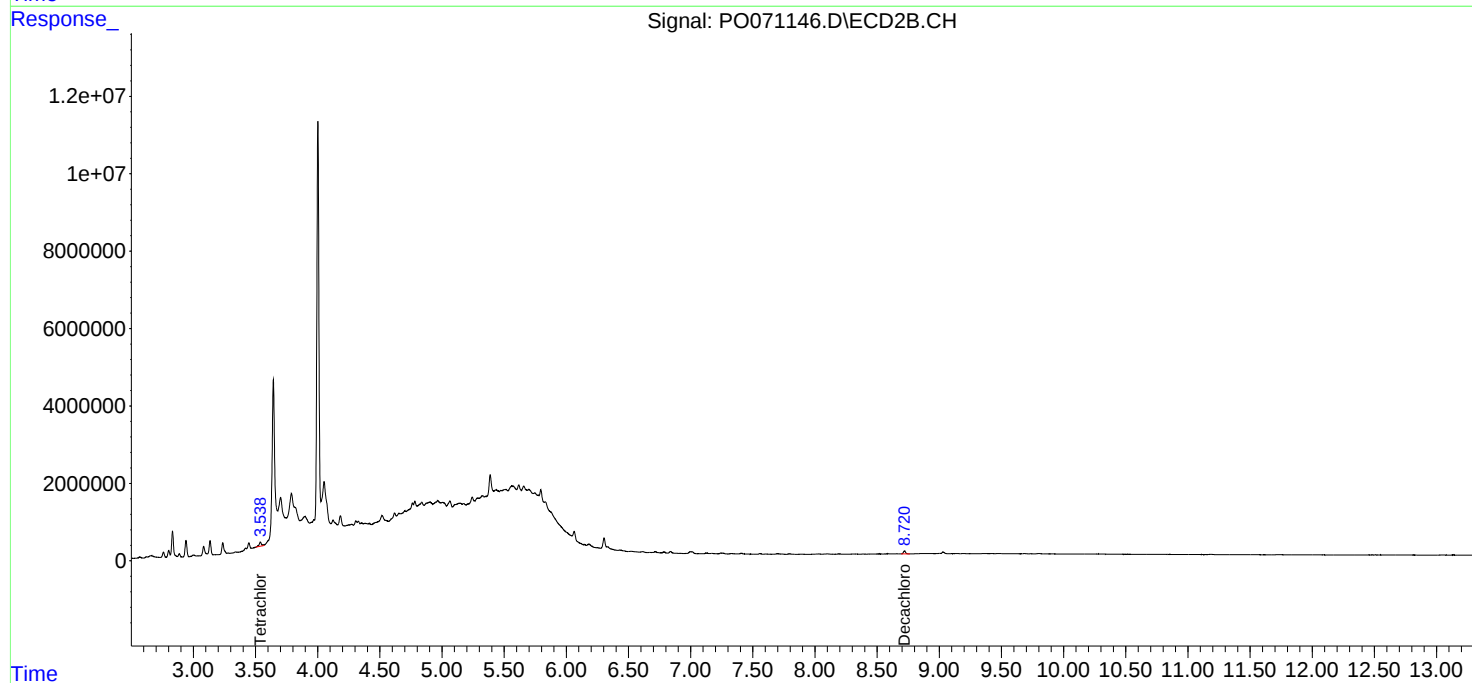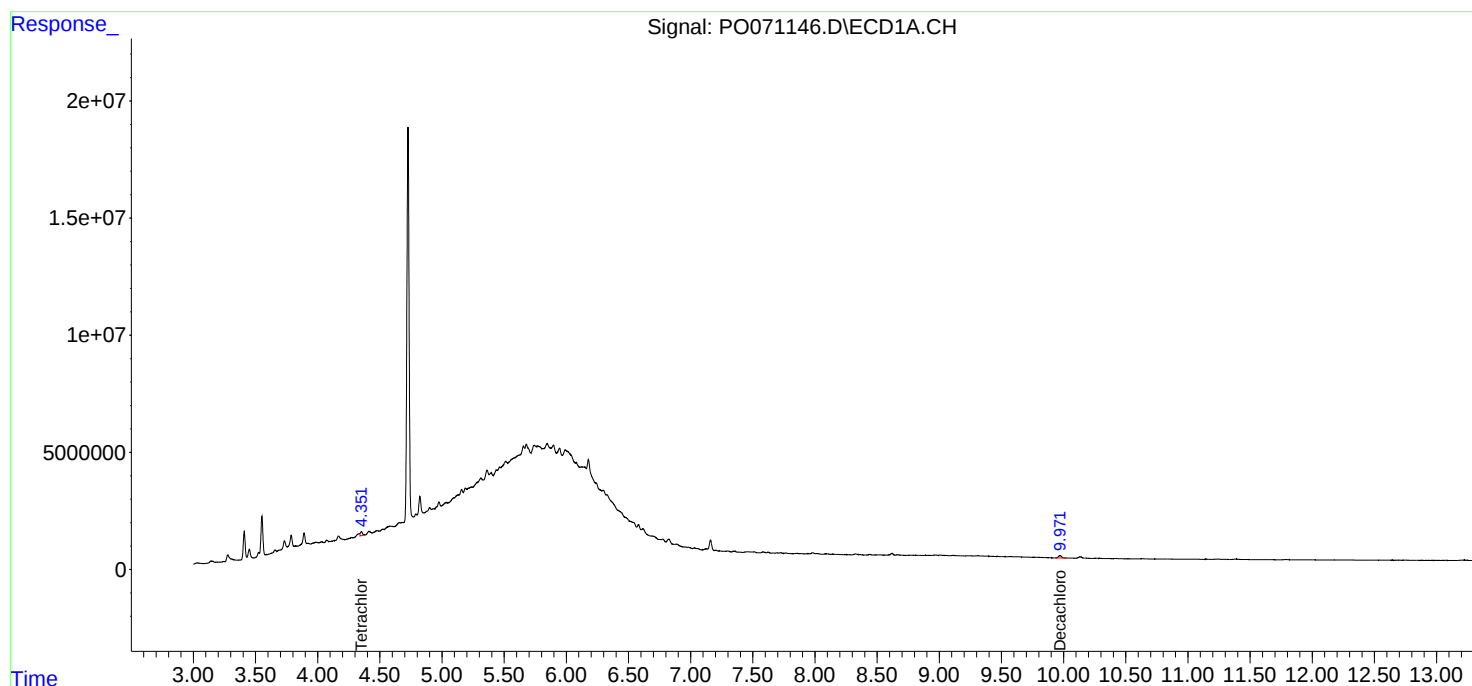

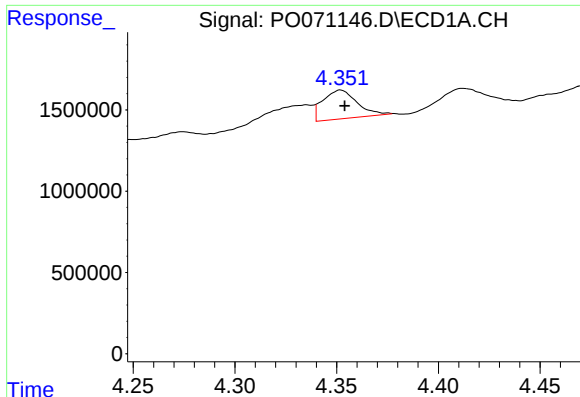


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.003 min
Response: 2056353
Conc: 26.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
9/4/2020 2:44:52 PM

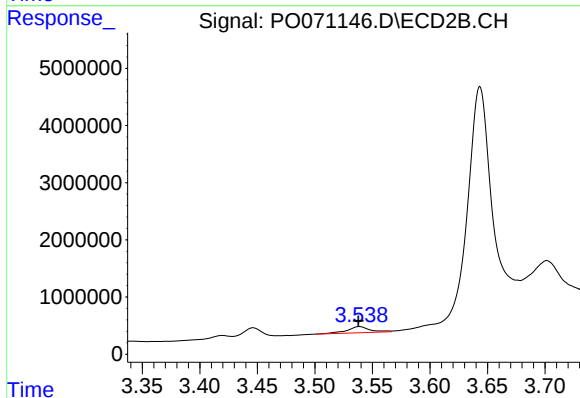


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 1496927
Conc: 33.77 ng/ml

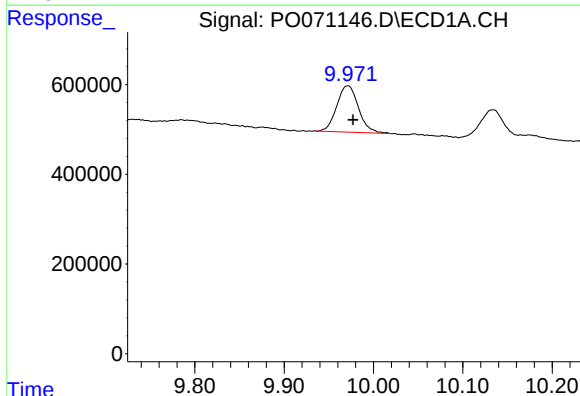

#2 Decachlorobiphenyl

R.T.: 9.971 min
Delta R.T.: -0.006 min
Response: 1734603
Conc: 18.96 ng/ml

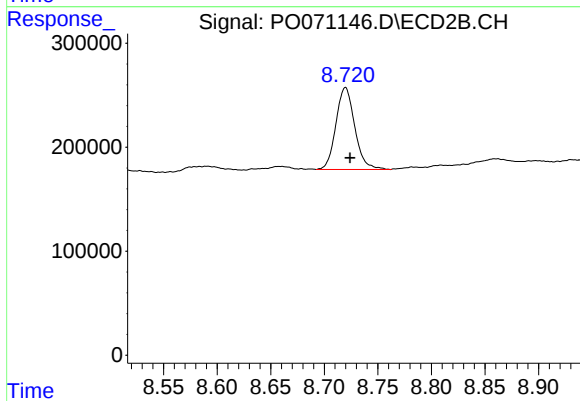

#2 Decachlorobiphenyl

R.T.: 8.720 min
Delta R.T.: -0.004 min
Response: 964574
Conc: 16.79 ng/ml