

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090321\
 Data File : P0080933.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Sep 2021 16:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 04:07:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.927	4.054	1729610	546650	21.910	22.121
2)	SA Decachlor...	10.994	9.417	1577747	594024	26.572	25.446
Target Compounds							
9)	L2 AR-1221-2	5.283	0.000	20053	0	27.279	N.D. #
21)	L5 AR-1248-1	0.000	5.287f	0	11369	N.D.	19.203 #
24)	L5 AR-1248-4	7.178f	0.000	23278	0	8.082	N.D. #
26)	L6 AR-1254-1	7.178	0.000	23278	0	7.203	N.D. #
28)	L6 AR-1254-3	7.807f	0.000	25415	0	5.026	N.D. #
32)	L7 AR-1260-2	8.198f	0.000	185855	0	41.702	N.D. #
33)	L7 AR-1260-3	0.000	7.296	0	61195	N.D.	33.427 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090321\
Data File : P0080933.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2021 16:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 04:07:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

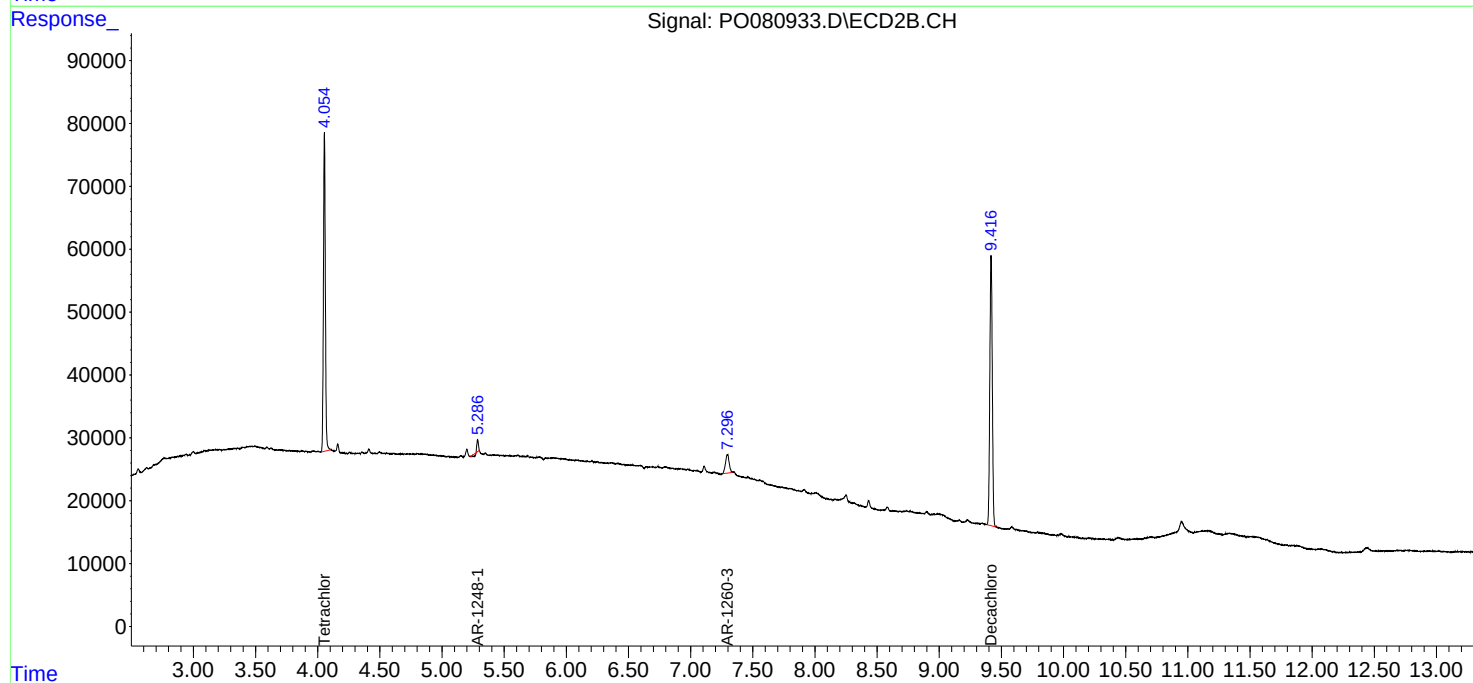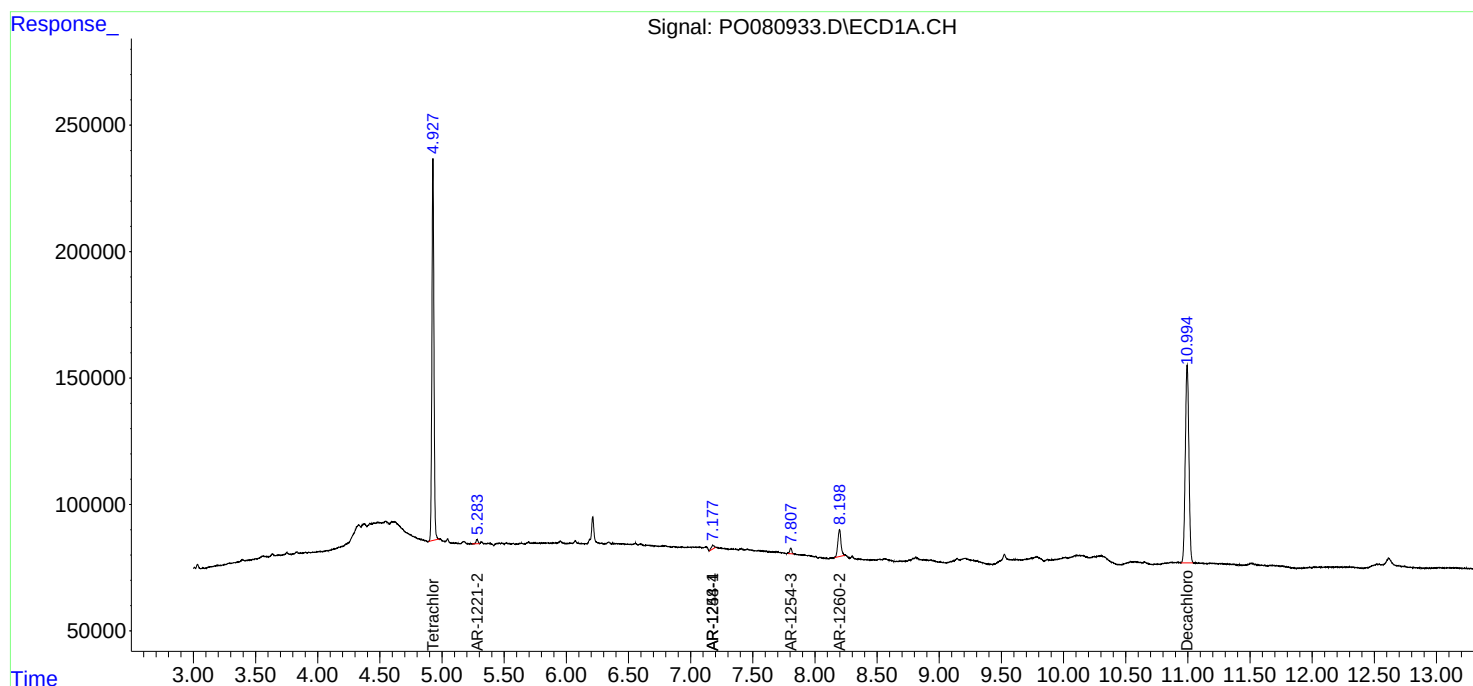


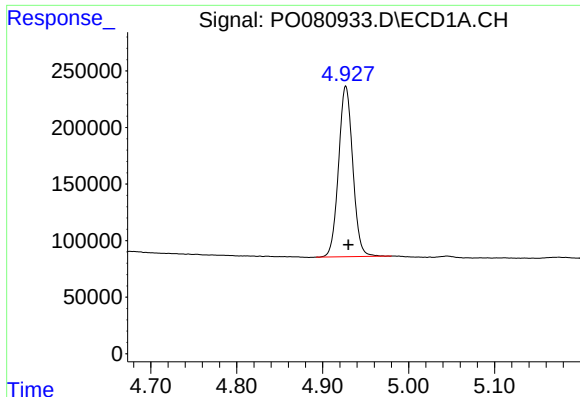

#1 Tetrachloro-m-xylene


R.T.: 4.927 min
Delta R.T.: -0.003 min
Response: 1729610
Conc: 21.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

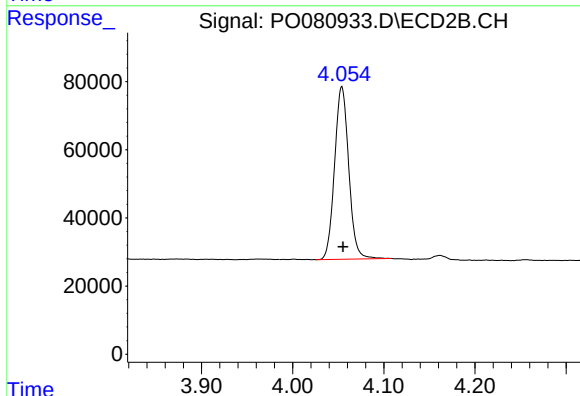


#1 Tetrachloro-m-xylene

R.T.: 4.054 min
Delta R.T.: -0.001 min
Response: 546650
Conc: 22.12 ng/ml

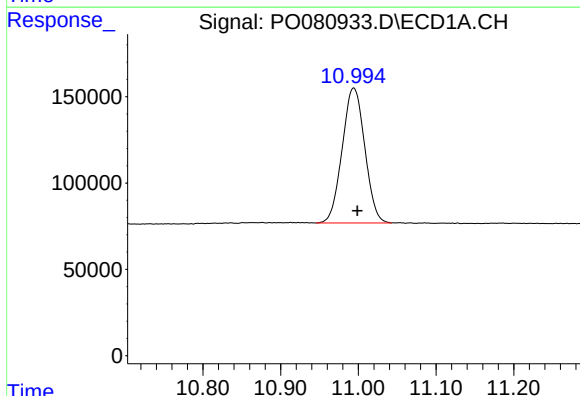


#2 Decachlorobiphenyl

R.T.: 10.994 min
Delta R.T.: -0.005 min
Response: 1577747
Conc: 26.57 ng/ml

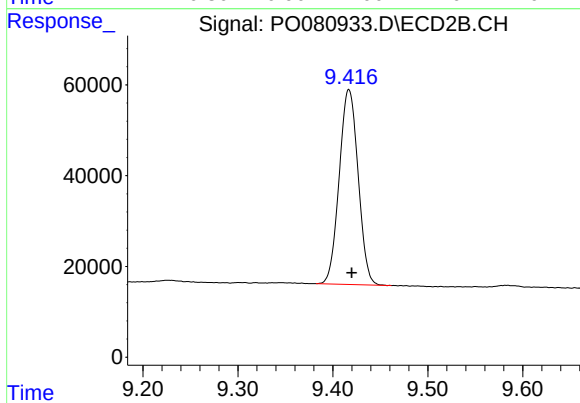

#2 Decachlorobiphenyl


R.T.: 9.417 min
Delta R.T.: -0.003 min
Response: 594024
Conc: 25.45 ng/ml

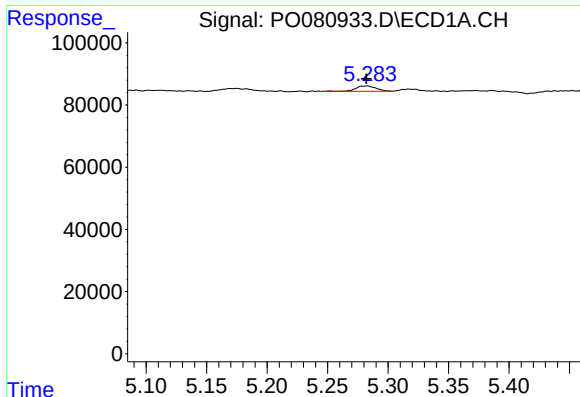

#9 AR-1221-2


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 20053
Conc: 27.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

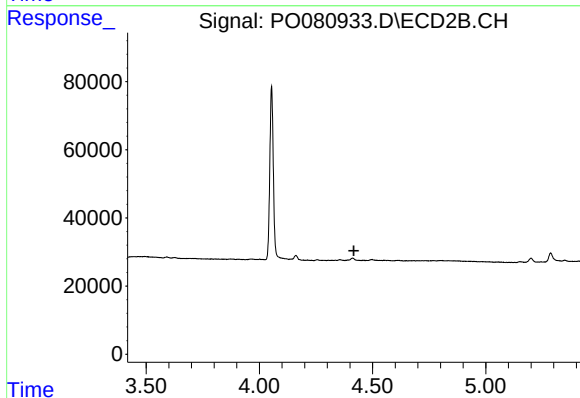


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.418 min
Response: 0
Conc: N.D.

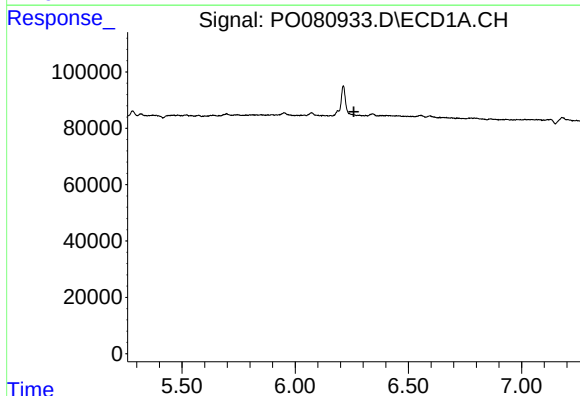


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 6.260 min
Response: 0
Conc: N.D.

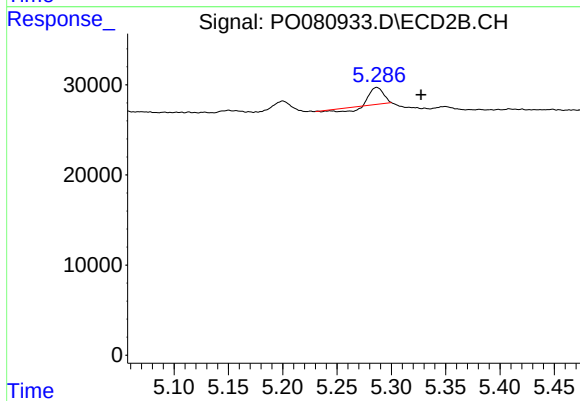

#21 AR-1248-1


R.T.: 5.287 min
Delta R.T.: -0.041 min
Response: 11369
Conc: 19.20 ng/ml

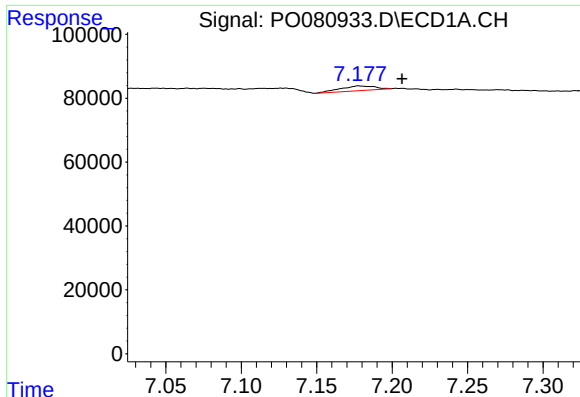

#24 AR-1248-4


R.T.: 7.178 min
Delta R.T.: -0.029 min
Response: 23278
Conc: 8.08 ng/ml

Instrument :
ECD_O
ClientSampleId :

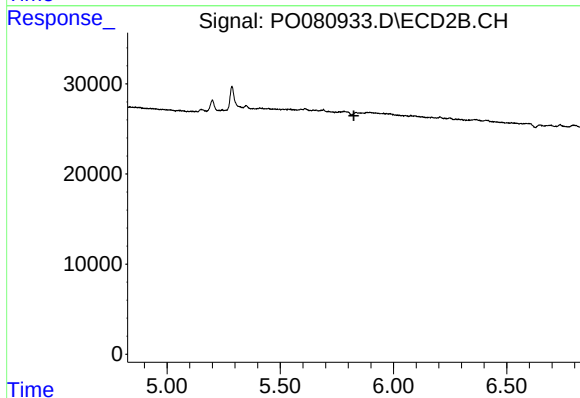


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.825 min
Response: 0
Conc: N.D.

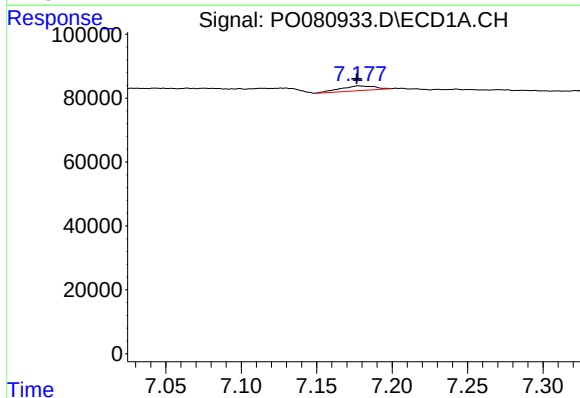


#26 AR-1254-1

R.T.: 7.178 min
Delta R.T.: 0.001 min
Response: 23278
Conc: 7.20 ng/ml

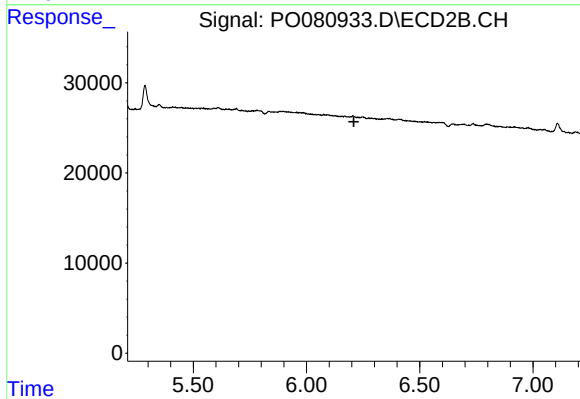

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

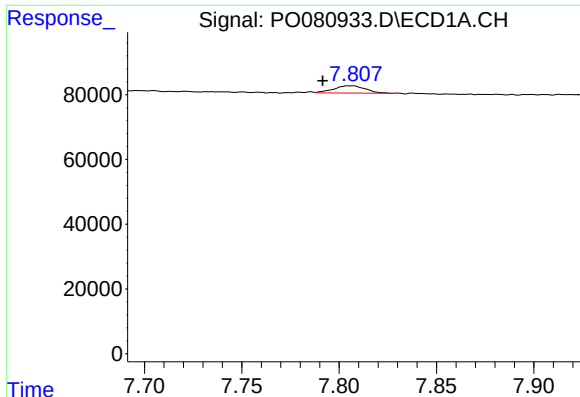

#28 AR-1254-3


R.T.: 7.807 min
Delta R.T.: 0.016 min
Response: 25415
Conc: 5.03 ng/ml

Instrument :
ECD_O
ClientSampleId :

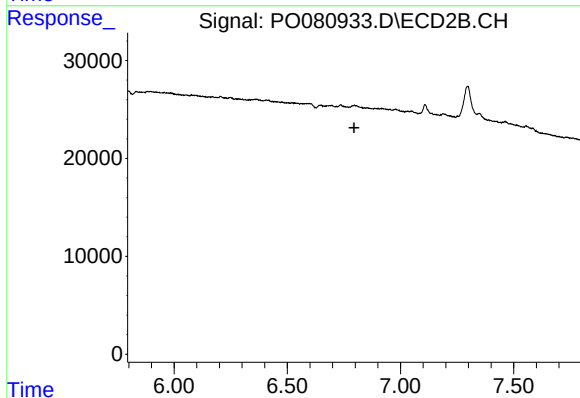


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.795 min
Response: 0
Conc: N.D.

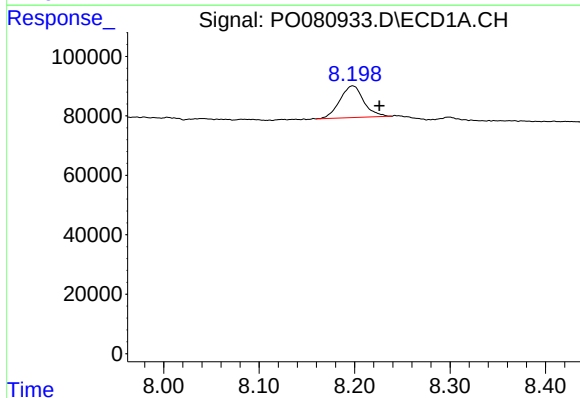


#32 AR-1260-2

R.T.: 8.198 min
Delta R.T.: -0.028 min
Response: 185855
Conc: 41.70 ng/ml

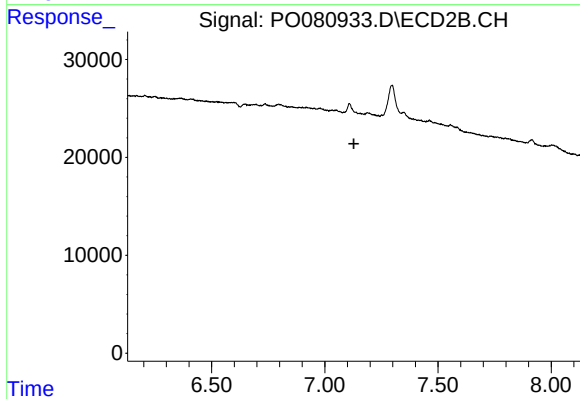

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.128 min
Response: 0
Conc: N.D.

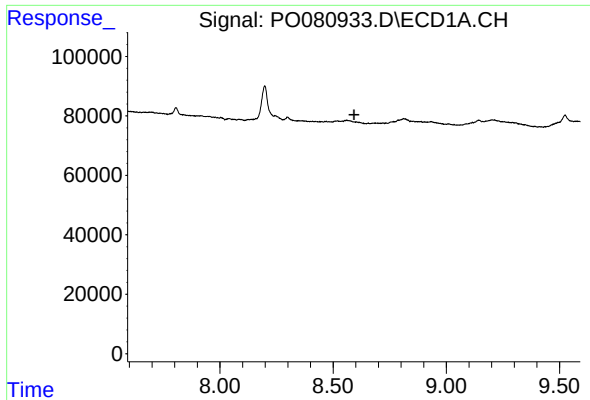

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

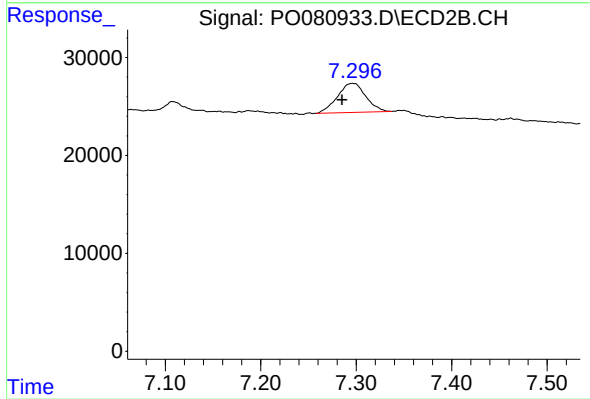

#33 AR-1260-3

R.T.: 7.296 min
Delta R.T.: 0.011 min
Response: 61195
Conc: 33.43 ng/ml