

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0090321\  
 Data File : P0080971.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 04 Sep 2021 3:38  
 Operator : DD\AJ  
 Sample : M3611-01 10X  
 Misc :  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 ECD\_0  
 ClientSampleId :  
 NWB-1528

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 04 04:29:49 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0090221.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Sep 03 07:15:29 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
-----						
System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.053	119964	35877	1.520	1.452
2) SA Decachlor...	10.991	9.415	109666	32201	1.847	1.379 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO090321\  
 Data File : PO080971.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 04 Sep 2021 3:38  
 Operator : DD\AJ  
 Sample : M3611-01 10X  
 Misc :  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 NWB-1528

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 04 04:29:49 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO090221.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Sep 03 07:15:29 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

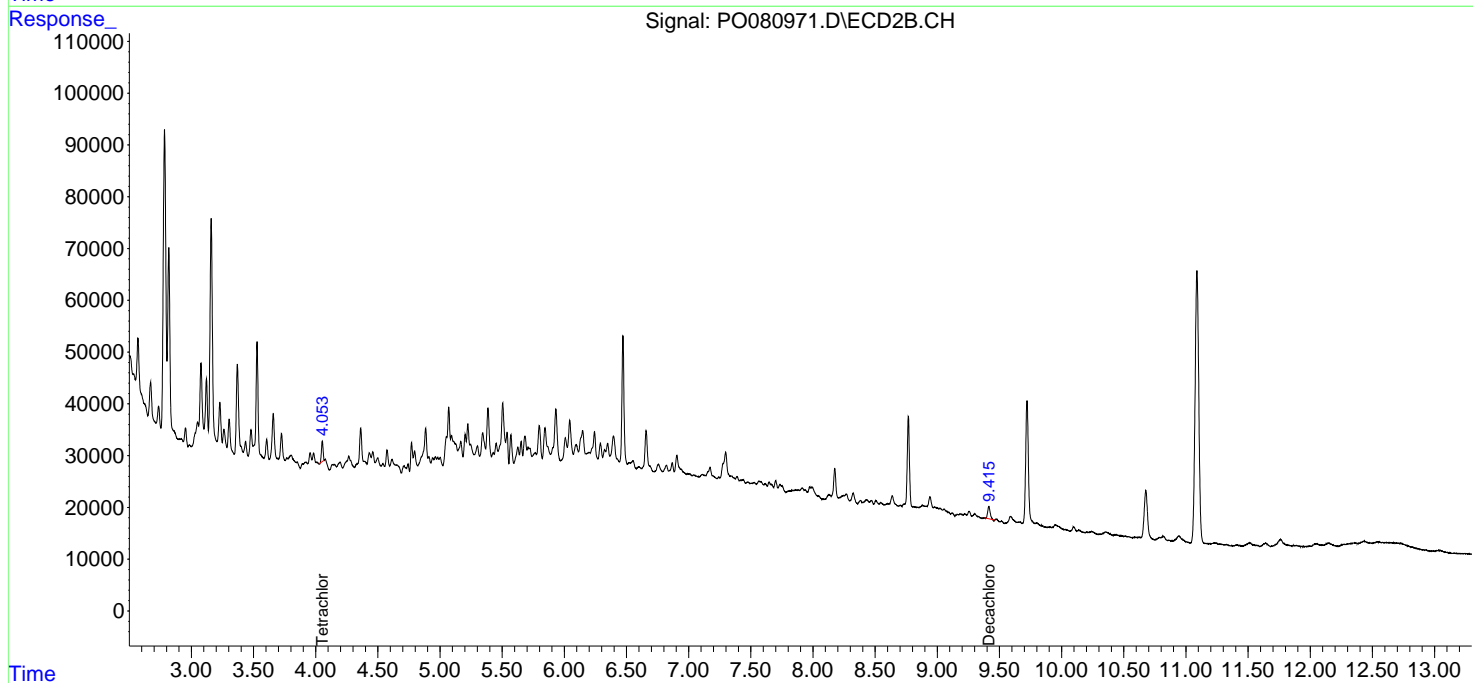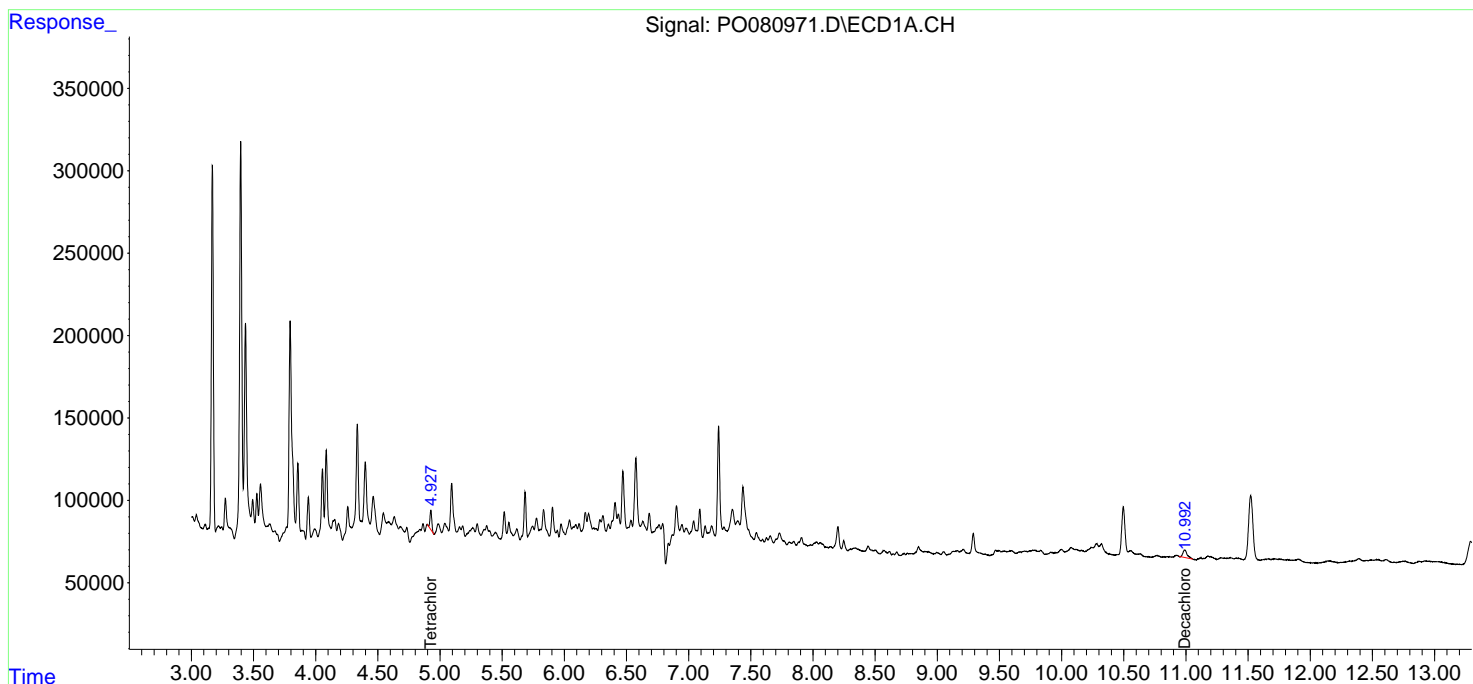

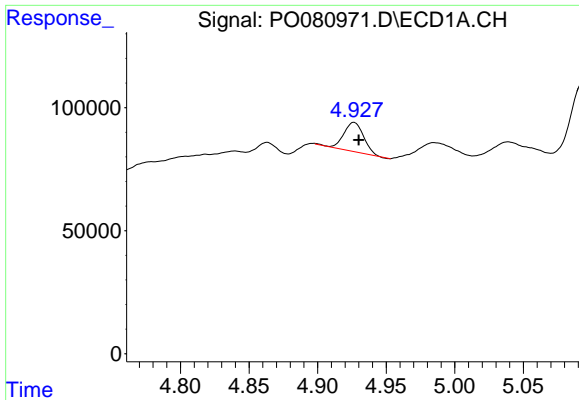


#1 Tetrachloro-m-xylene  
 R.T.: 4.927 min  
 Delta R.T.: -0.003 min  
 Response: 119964  
 Conc: 1.52 ng/ml


Instrument :  
 ECD\_O  
 ClientSampleId :  
 NWB-1528

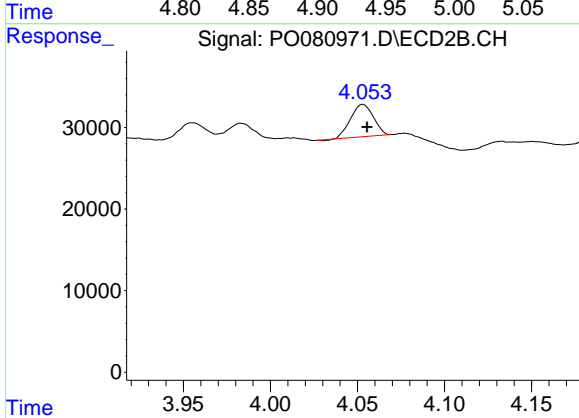

#1 Tetrachloro-m-xylene  
 R.T.: 4.053 min  
 Delta R.T.: -0.002 min  
 Response: 35877  
 Conc: 1.45 ng/ml

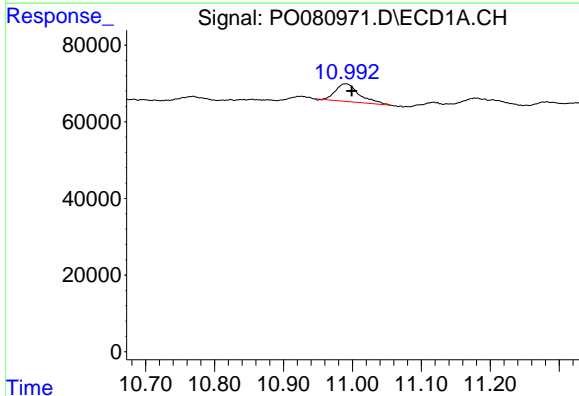

#2 Decachlorobiphenyl  
 R.T.: 10.991 min  
 Delta R.T.: -0.008 min  
 Response: 109666  
 Conc: 1.85 ng/ml

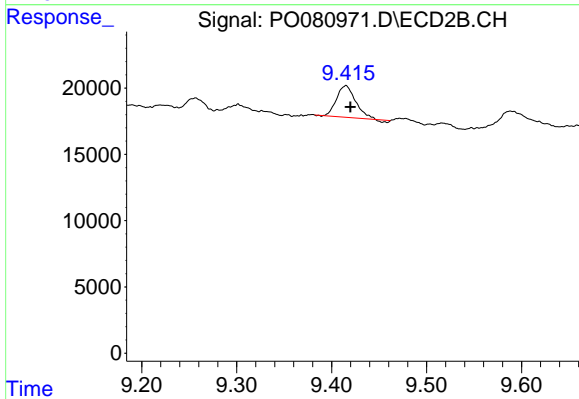

#2 Decachlorobiphenyl  
 R.T.: 9.415 min  
 Delta R.T.: -0.005 min  
 Response: 32201  
 Conc: 1.38 ng/ml