

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090324\
 Data File : P0106091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 12:27
 Operator : YP/AJ
 Sample : P3798-01 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2308-0008-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/04/2024
 Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 12:47:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.453	3.718	11106290	4046509	1.217	1.498
2) SA Decachlor...	10.192	8.749	7761816	3426649	1.430m	1.570m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090324\
Data File : PO106091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 12:27
Operator : YP/AJ
Sample : P3798-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2308-0008-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time : Sep 03 12:47:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

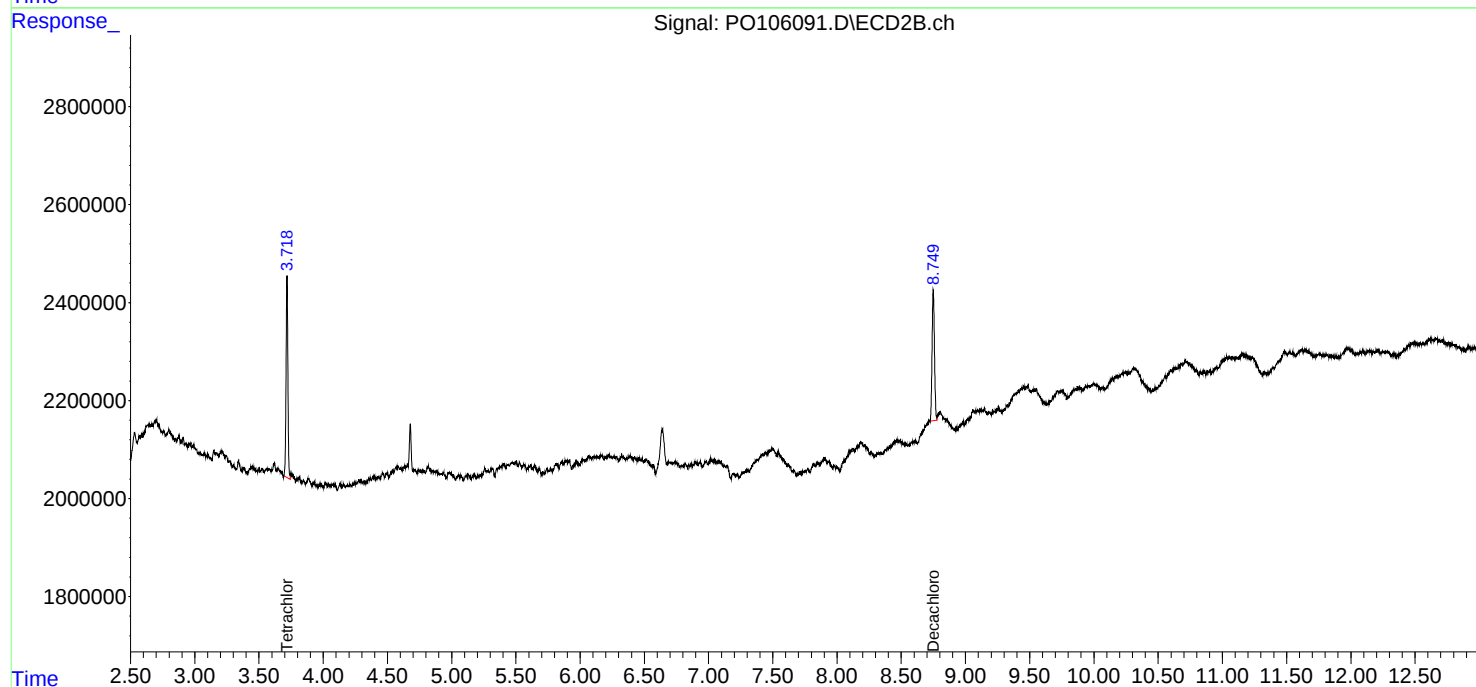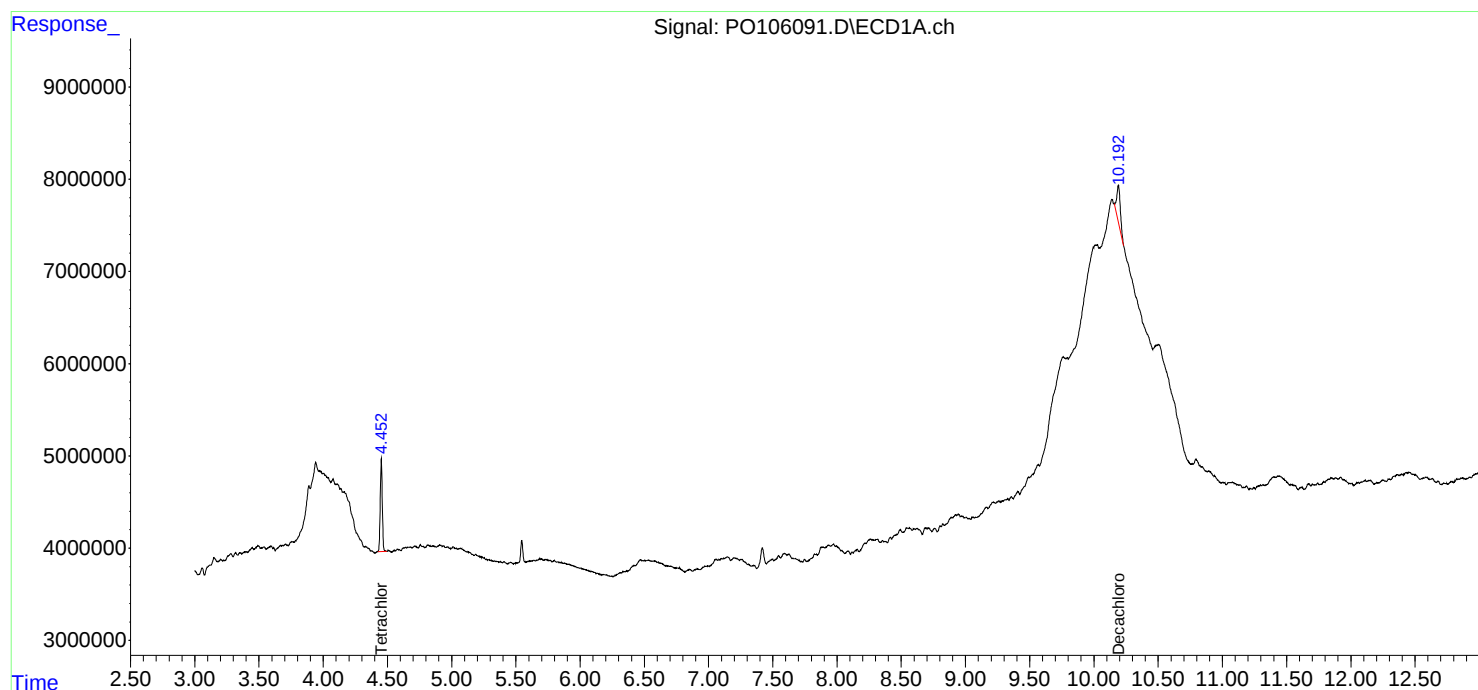

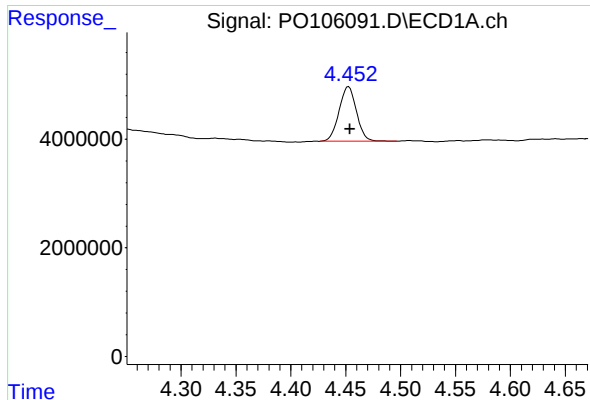


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: -0.001 min
Response: 11106290
Conc: 1.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2308-0008-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

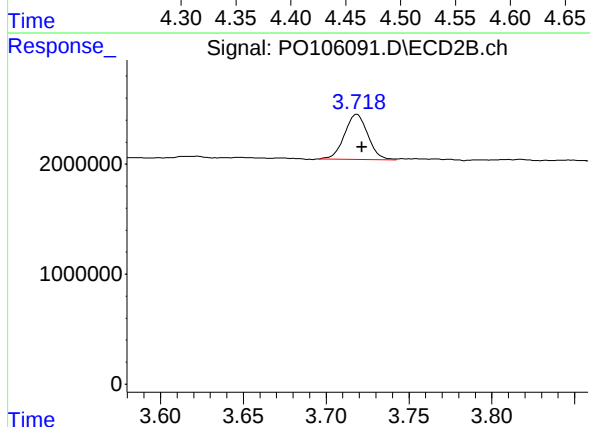


#1 Tetrachloro-m-xylene

R.T.: 3.718 min
Delta R.T.: -0.003 min
Response: 4046509
Conc: 1.50 ng/ml

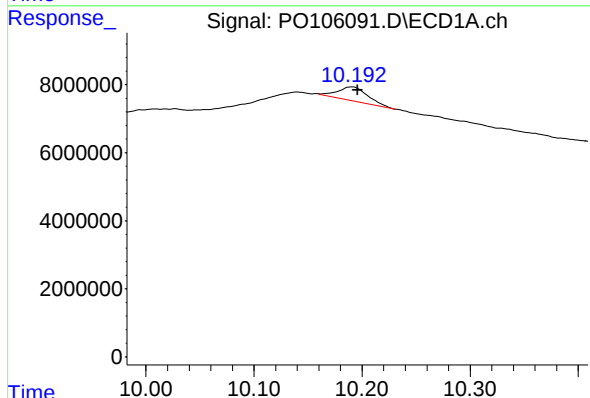

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.003 min
Response: 7761816
Conc: 1.43 ng/ml m

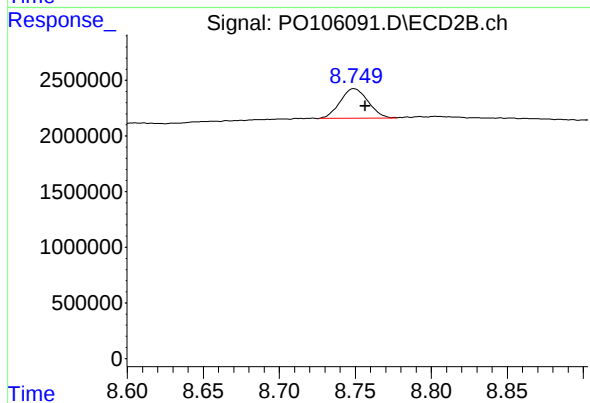

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.008 min
Response: 3426649
Conc: 1.57 ng/ml m