

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090324\
 Data File : P0106111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 21:45
 Operator : YP/AJ
 Sample : P3801-04 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-23-00274-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/04/2024
 Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 03:14:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.717	18435231	4312474	2.021m	1.596m
2) SA Decachlor...	10.189	8.749	9751307	3252431	1.797m	1.490m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090324\
Data File : PO106111.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 21:45
Operator : YP/AJ
Sample : P3801-04 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MOO-23-00274-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 03:14:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

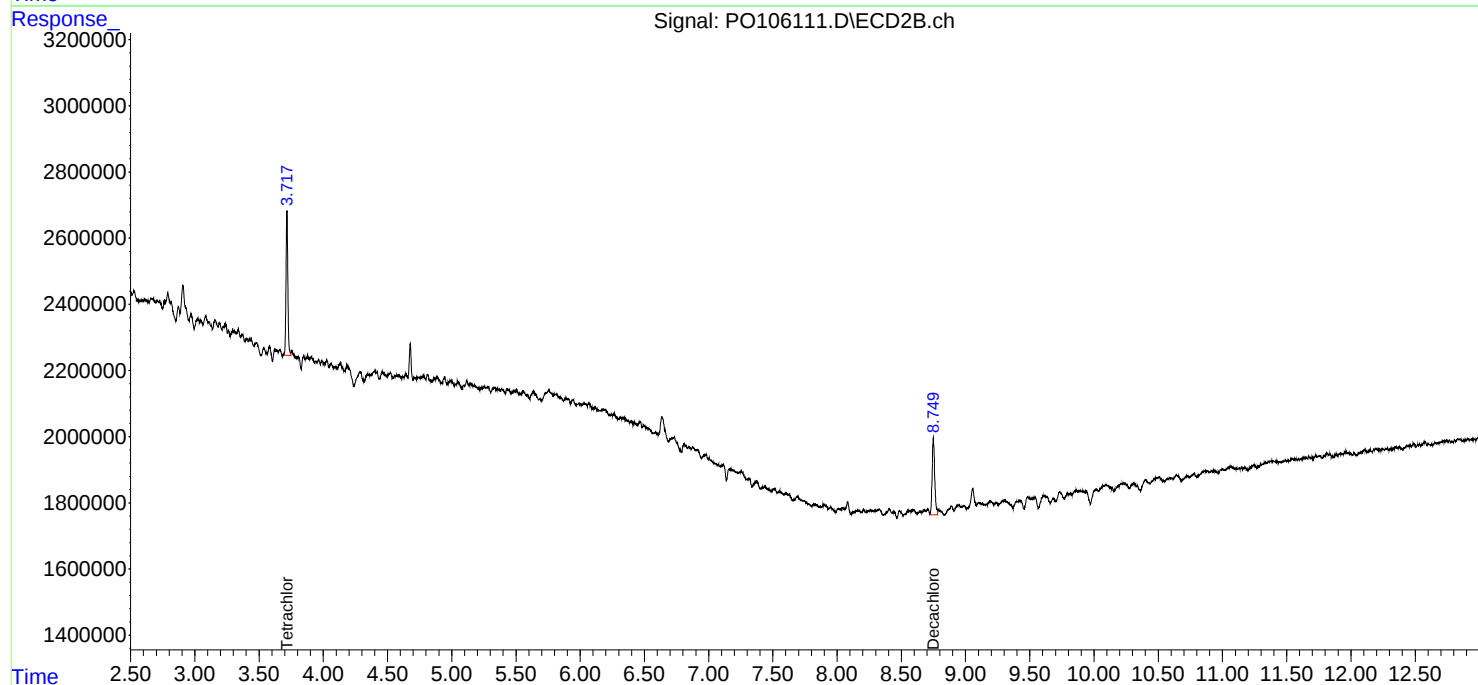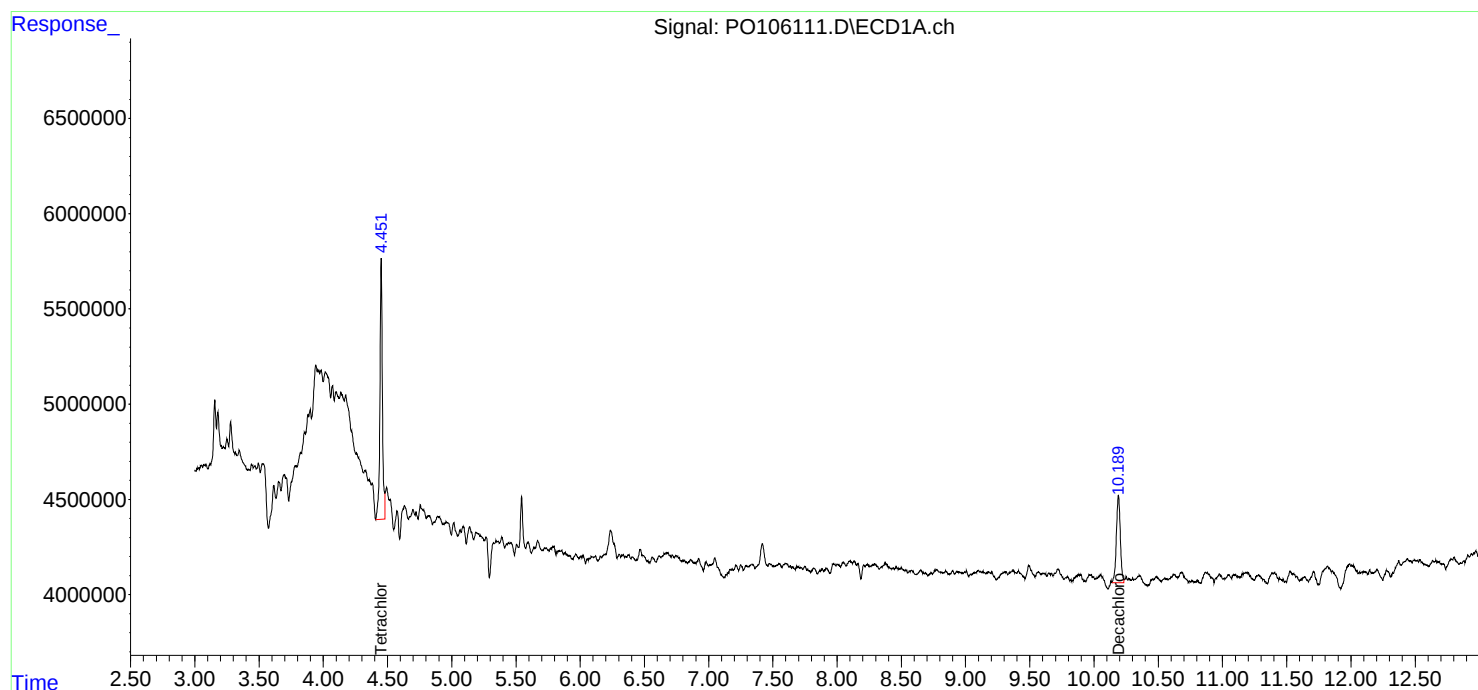

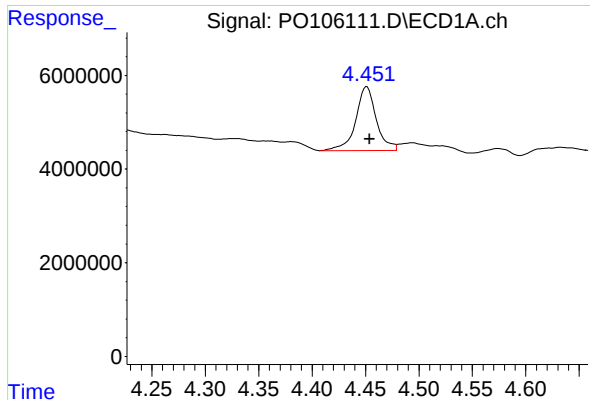


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: -0.003 min
Response: 18435231
Conc: 2.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-23-00274-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

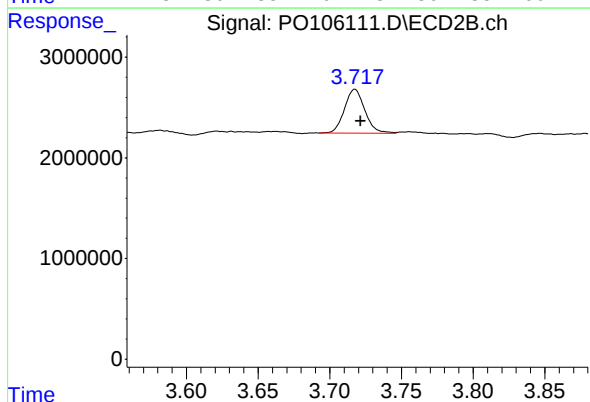


#1 Tetrachloro-m-xylene

R.T.: 3.717 min
Delta R.T.: -0.004 min
Response: 4312474
Conc: 1.60 ng/ml m

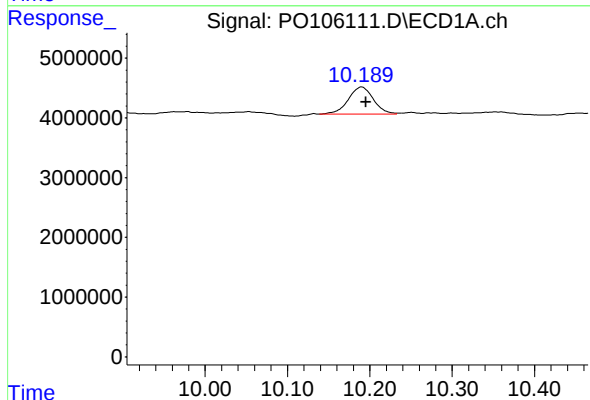

#2 Decachlorobiphenyl

R.T.: 10.189 min
Delta R.T.: -0.006 min
Response: 9751307
Conc: 1.80 ng/ml m

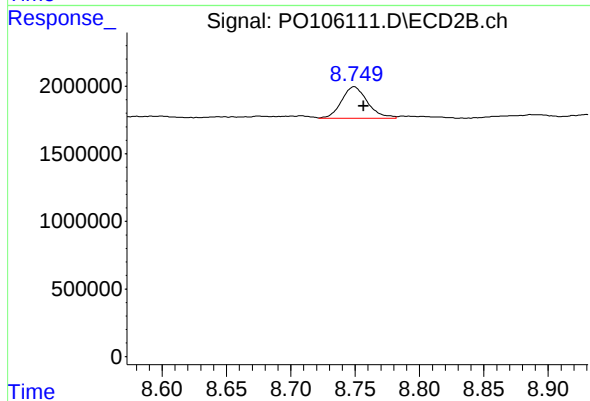

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.008 min
Response: 3252431
Conc: 1.49 ng/ml m