

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090324\
 Data File : P0106113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 22:19
 Operator : YP/AJ
 Sample : P3801-06 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RANDOM-MOO-23-00277-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/04/2024
 Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 03:15:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.717	10898825	4461633	1.195	1.651m#
2) SA Decachlor...	10.191	8.749	8560245	3350904	1.577	1.535

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090324\
Data File : PO106113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 22:19
Operator : YP/AJ
Sample : P3801-06 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RANDOM-MOO-23-00277-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 03:15:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

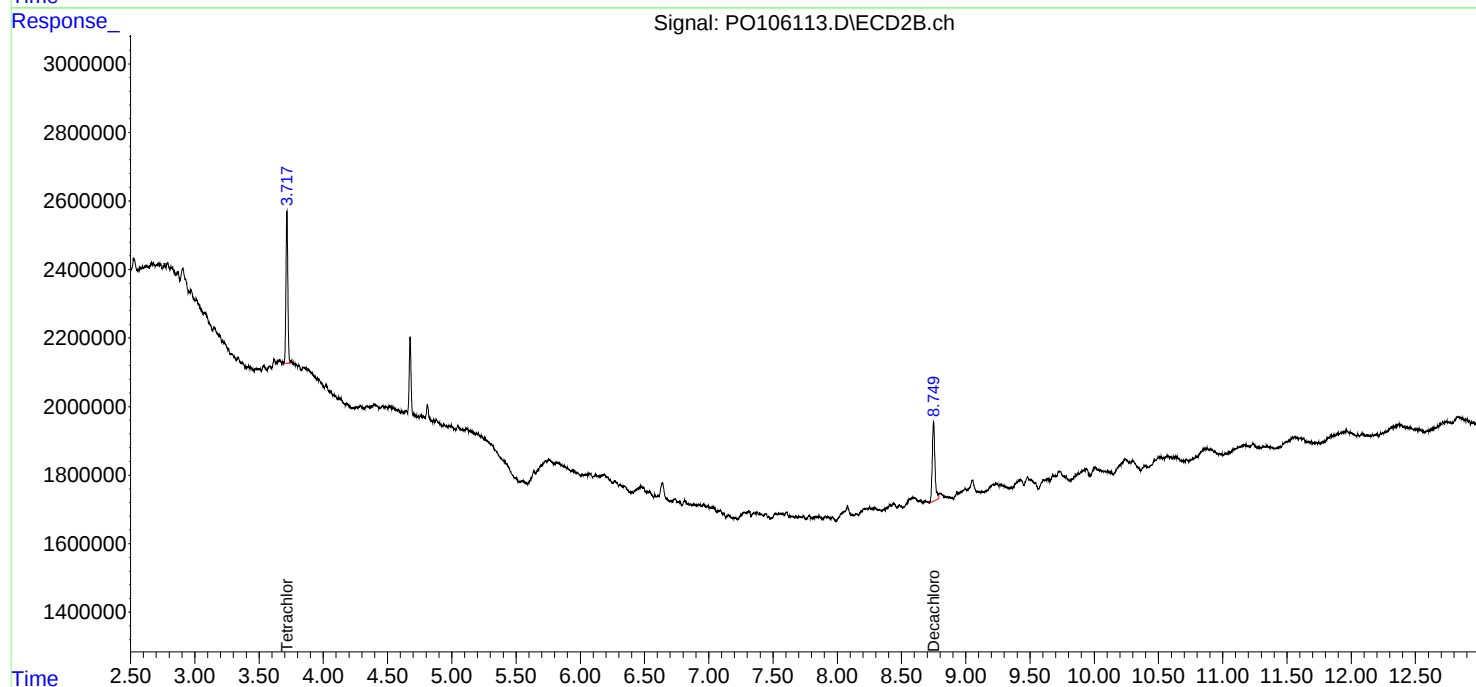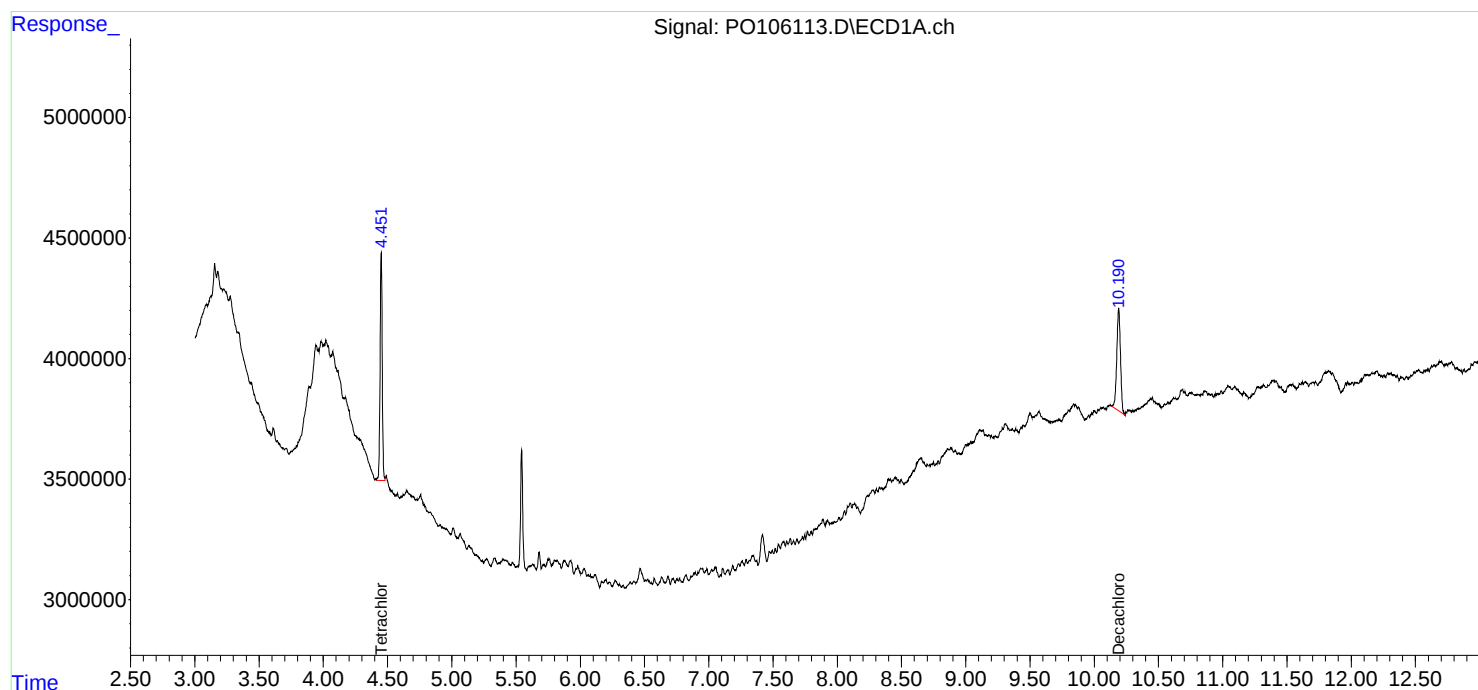

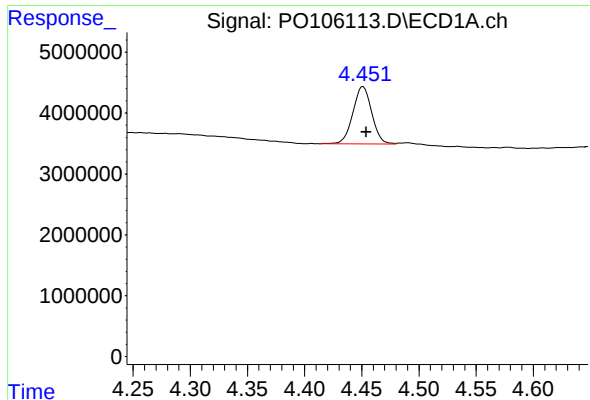

#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: -0.003 min
Response: 10898825
Conc: 1.19 ng/ml

Instrument :


ECD_O

ClientSampleId :

RANDOM-MOO-23-00277-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

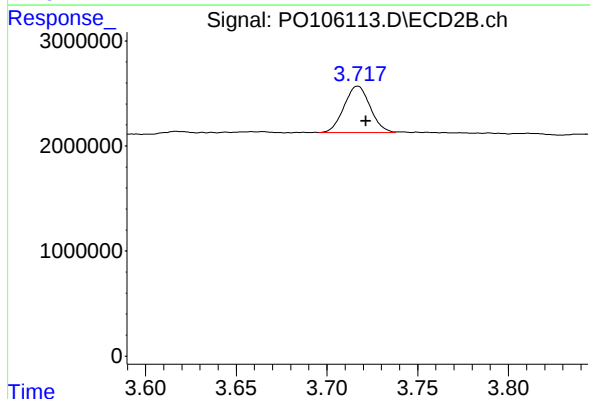


#1 Tetrachloro-m-xylene

R.T.: 3.717 min
Delta R.T.: -0.005 min
Response: 4461633
Conc: 1.65 ng/ml m

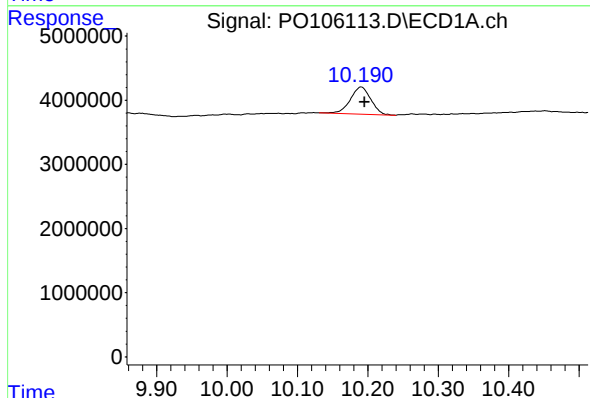

#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: -0.005 min
Response: 8560245
Conc: 1.58 ng/ml

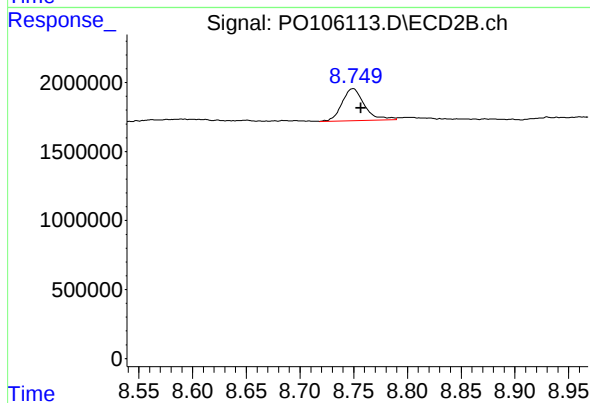

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.007 min
Response: 3350904
Conc: 1.53 ng/ml