

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090324\
 Data File : P0106127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2024 03:47
 Operator : YP/AJ
 Sample : P3812-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-02-083024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/04/2024
 Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 04:27:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.717	143.6E6	51882935	15.744m	19.203m
2) SA Decachlor...	10.187	8.746	105.8E6	37806206	19.487	17.318

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090324\
Data File : PO106127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2024 03:47
Operator : YP/AJ
Sample : P3812-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-02-083024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 04:27:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

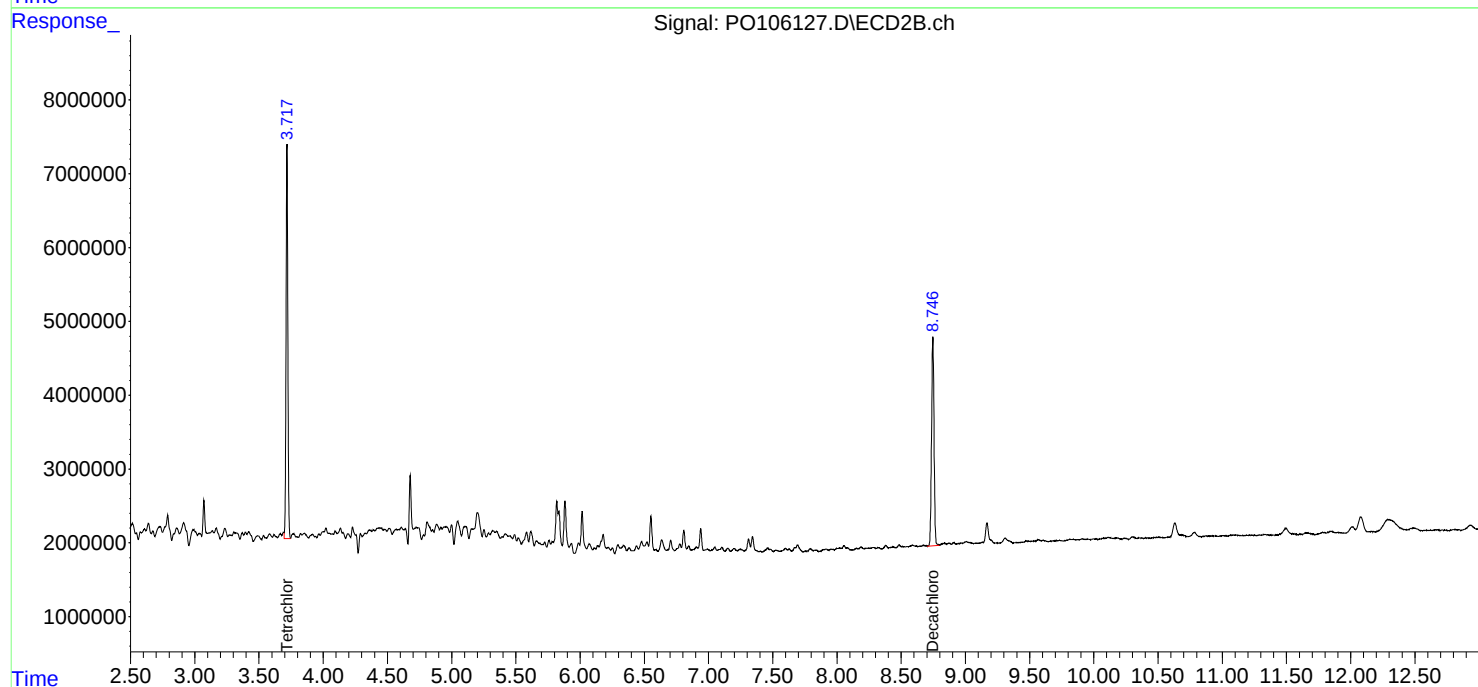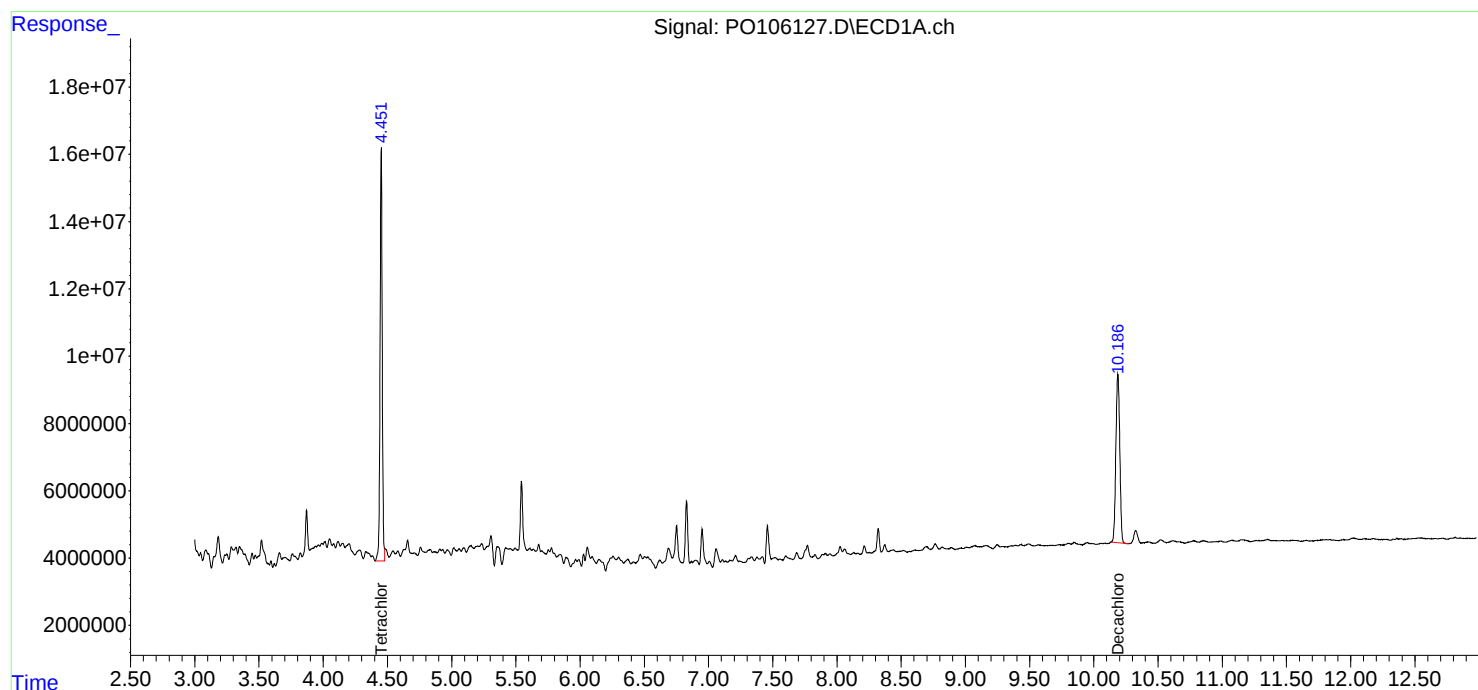

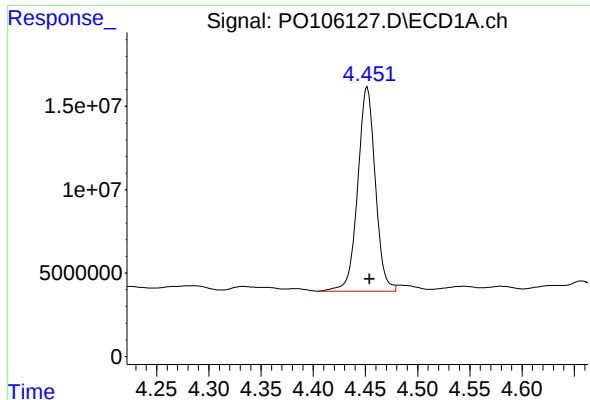


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: -0.003 min
Response: 143637761
Conc: 15.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-02-083024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

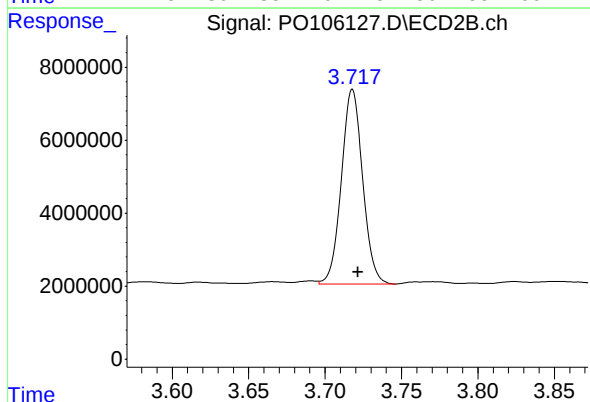


#1 Tetrachloro-m-xylene

R.T.: 3.717 min
Delta R.T.: -0.004 min
Response: 51882935
Conc: 19.20 ng/ml

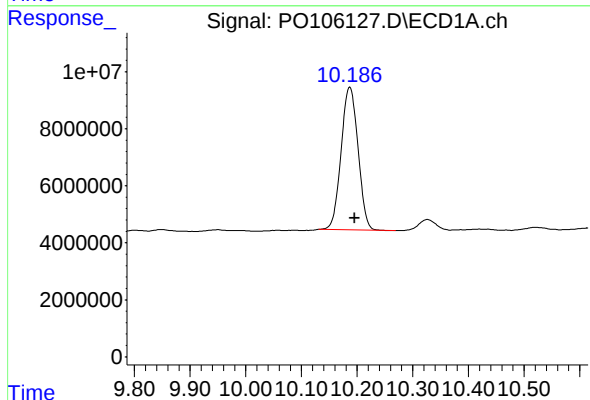

#2 Decachlorobiphenyl

R.T.: 10.187 min
Delta R.T.: -0.009 min
Response: 105751821
Conc: 19.49 ng/ml

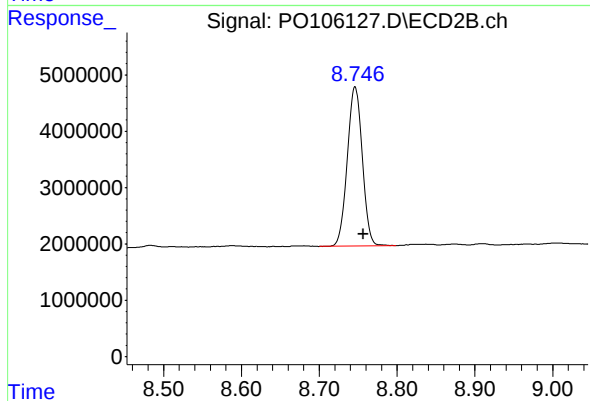

#2 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.011 min
Response: 37806206
Conc: 17.32 ng/ml