

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090325\
 Data File : P0113421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2025 11:25
 Operator : YP/AJ
 Sample : Q2999-06 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEH766W-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/03/2025
 Supervised By :mohammad ahmed 09/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 12:11:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.661	3.652	14134914	7932210	1.727	1.567m
2) SA Decachlor...	8.676	8.622	9203611	2667951	1.328m	1.408m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090325\
Data File : PO113421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2025 11:25
Operator : YP/AJ
Sample : Q2999-06 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HEH766W-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/03/2025
Supervised By :mohammad ahmed 09/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 12:11:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

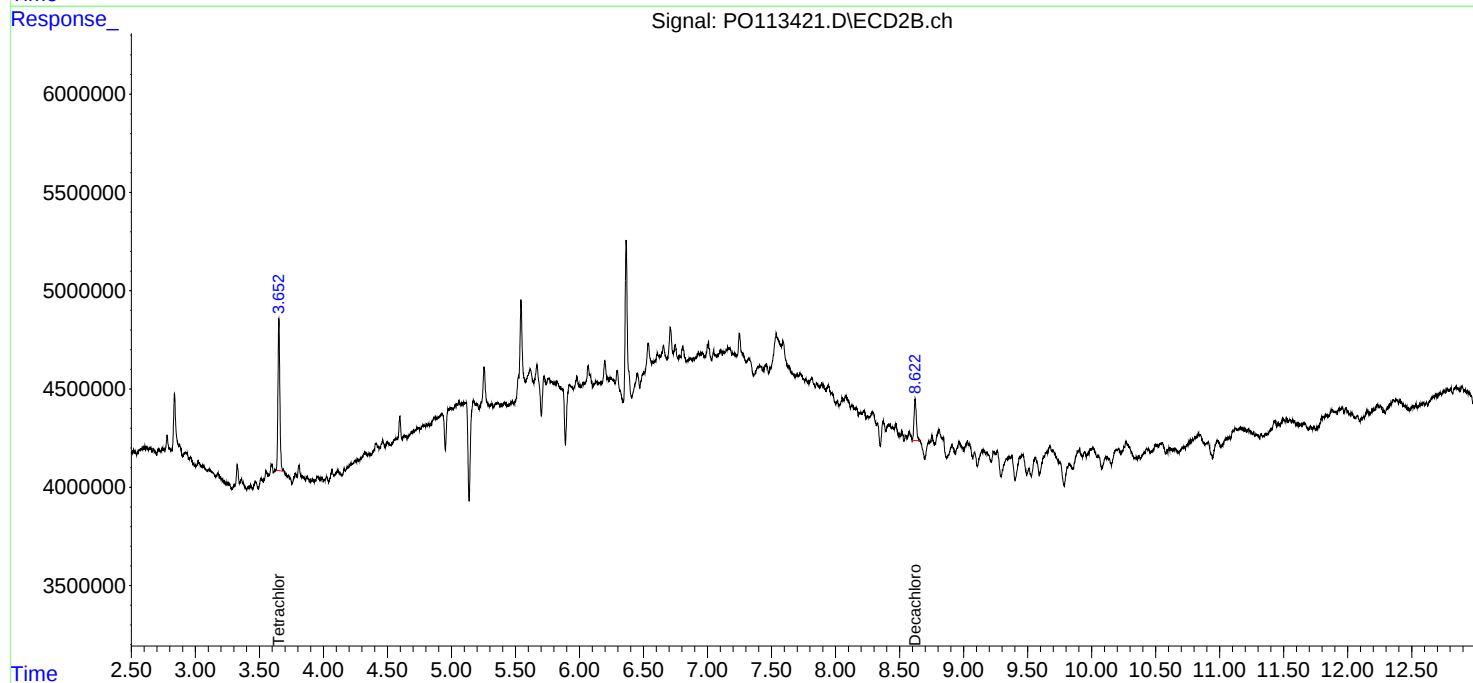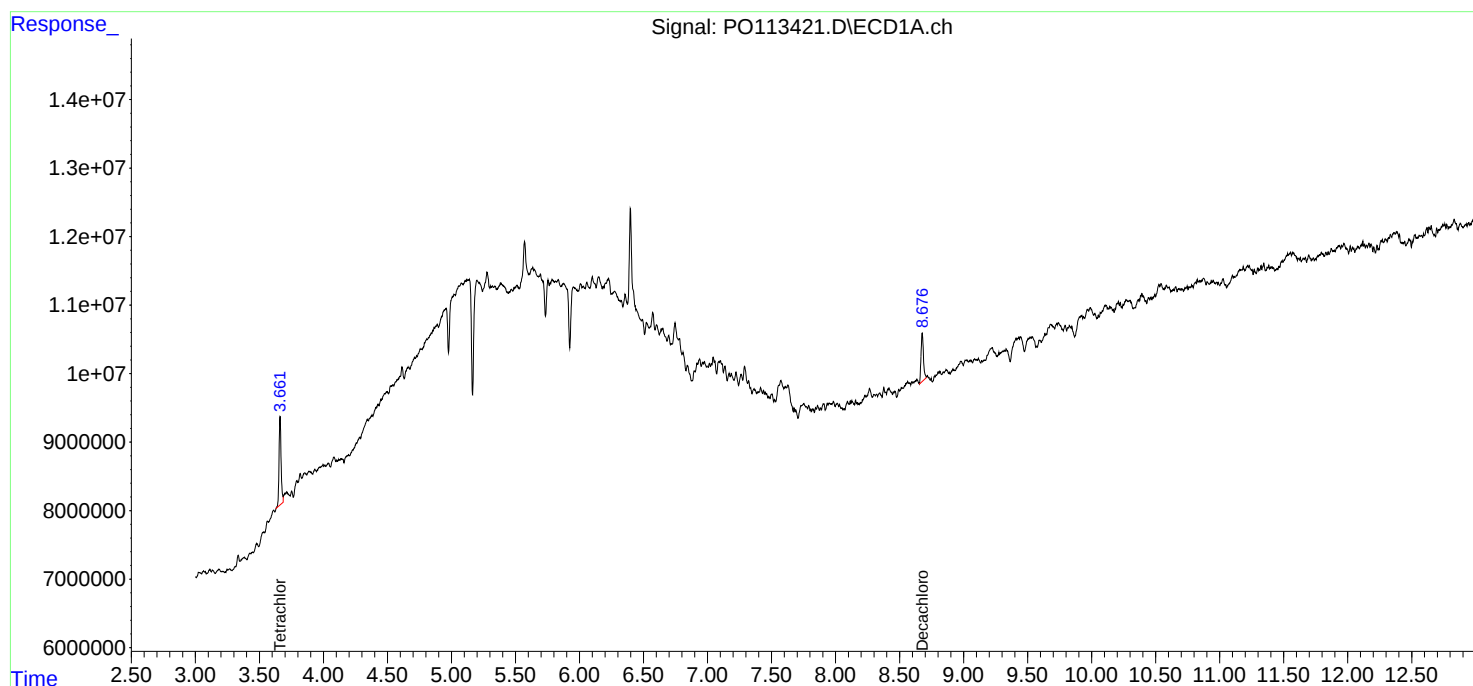

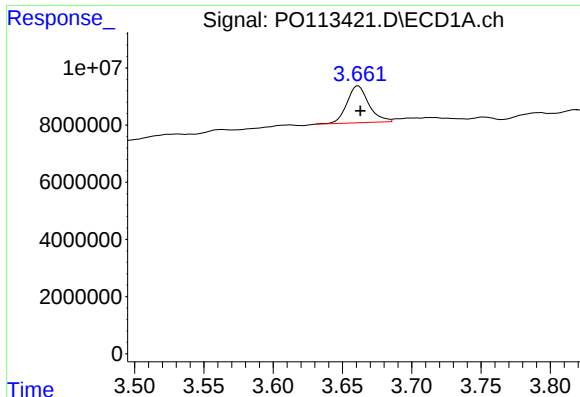


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.002 min
Response: 14134914
Conc: 1.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEH766W-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/03/2025
Supervised By :mohammad ahmed 09/05/2025

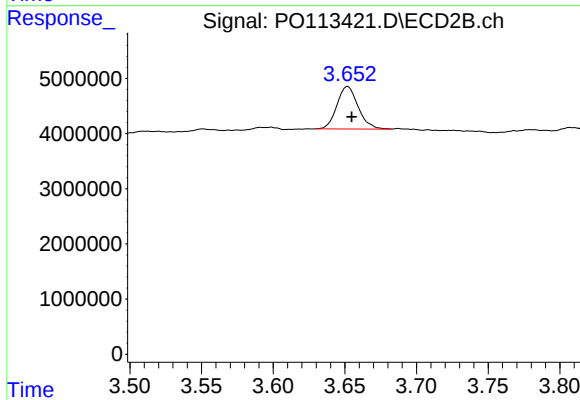


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 7932210
Conc: 1.57 ng/ml m

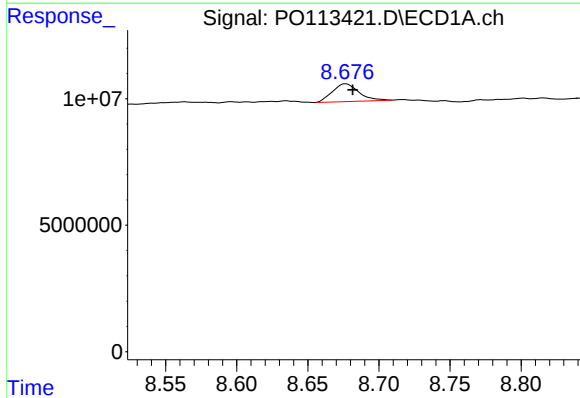

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.006 min
Response: 9203611
Conc: 1.33 ng/ml m

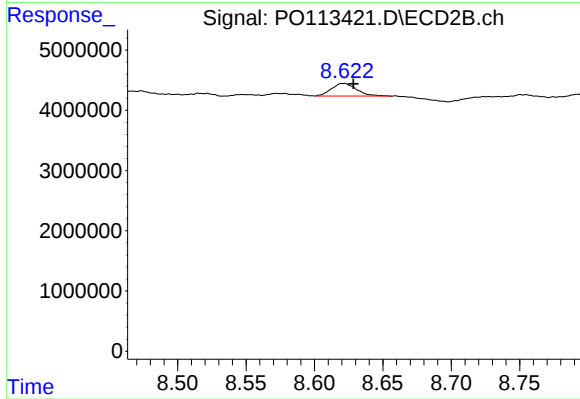

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.007 min
Response: 2667951
Conc: 1.41 ng/ml m