

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090325\
Data File : P0113434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2025 16:15
Operator : YP/AJ
Sample : Q2990-02RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
308RE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2025
Supervised By :mohammad ahmed 09/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 16:29:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	2278151	2483495	0.278m	0.491m#
2) SA Decachlor...	8.678	8.625	63062862	17572204	9.098m	9.274m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090325\
Data File : PO113434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2025 16:15
Operator : YP/AJ
Sample : Q2990-02RE
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
308RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2025
Supervised By :mohammad ahmed 09/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 16:29:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

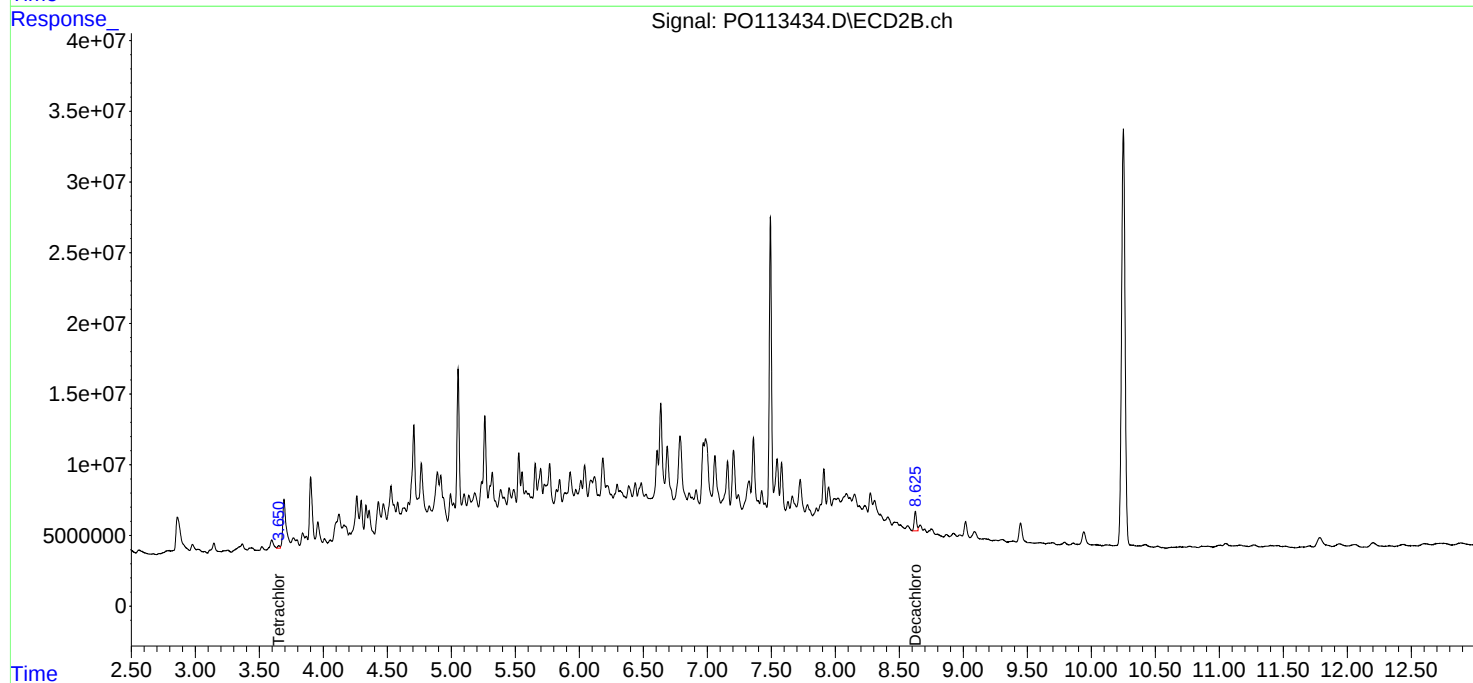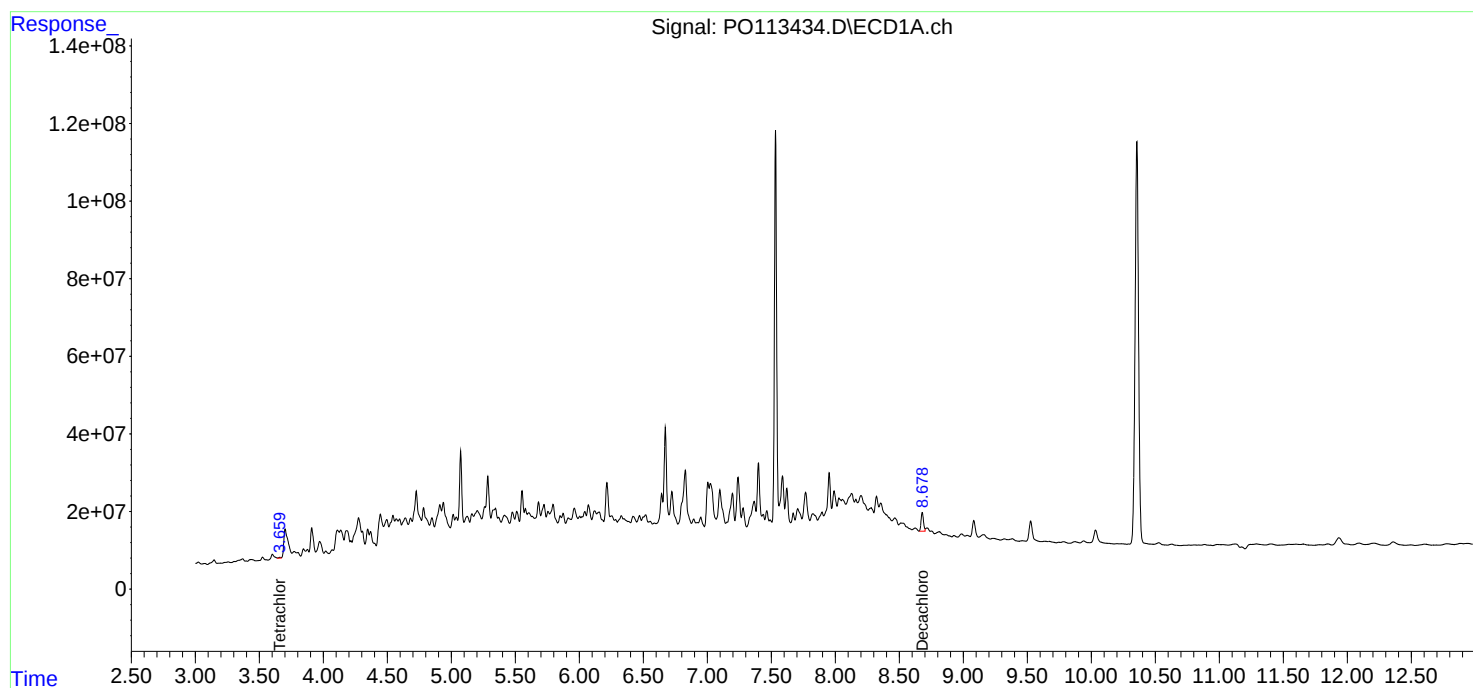

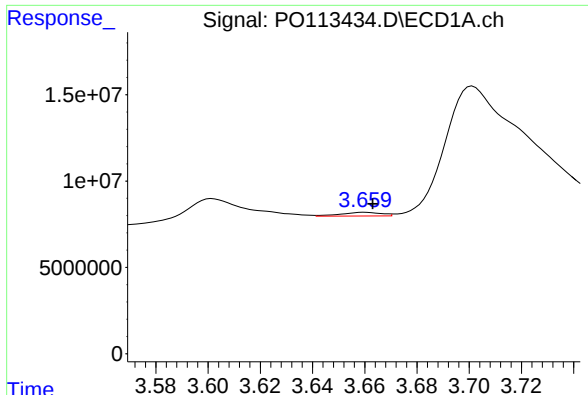


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 2278151
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
308RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/04/2025
Supervised By :mohammad ahmed 09/05/2025

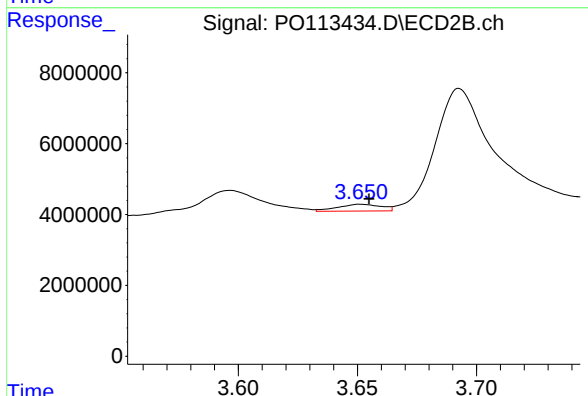


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.004 min
Response: 2483495
Conc: 0.49 ng/ml m

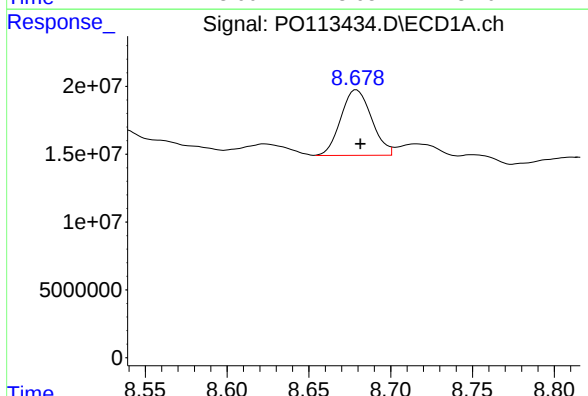

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.003 min
Response: 63062862
Conc: 9.10 ng/ml m

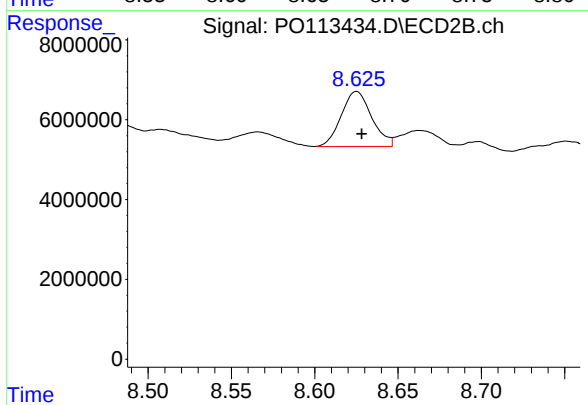

#2 Decachlorobiphenyl

R.T.: 8.625 min
Delta R.T.: -0.003 min
Response: 17572204
Conc: 9.27 ng/ml m