

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090418\
Data File : P0048693.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2018 20:18
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 07:35:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 05 03:48:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.529	2454320	3372095	20.341	21.574
2) SA Decachlor...	10.180	8.470	2837339	3203082	20.335	21.664

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090418\
Data File : P0048693.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2018 20:18
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 07:35:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 05 03:48:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

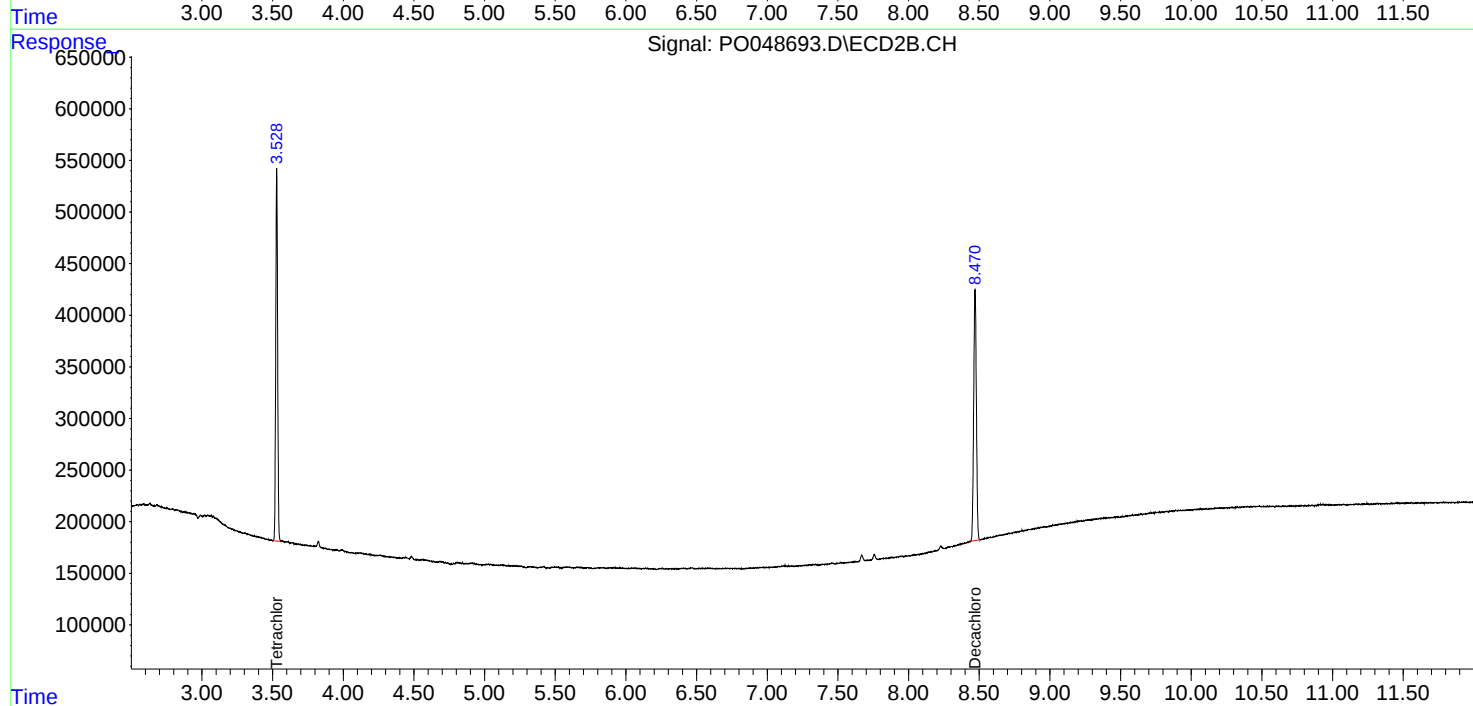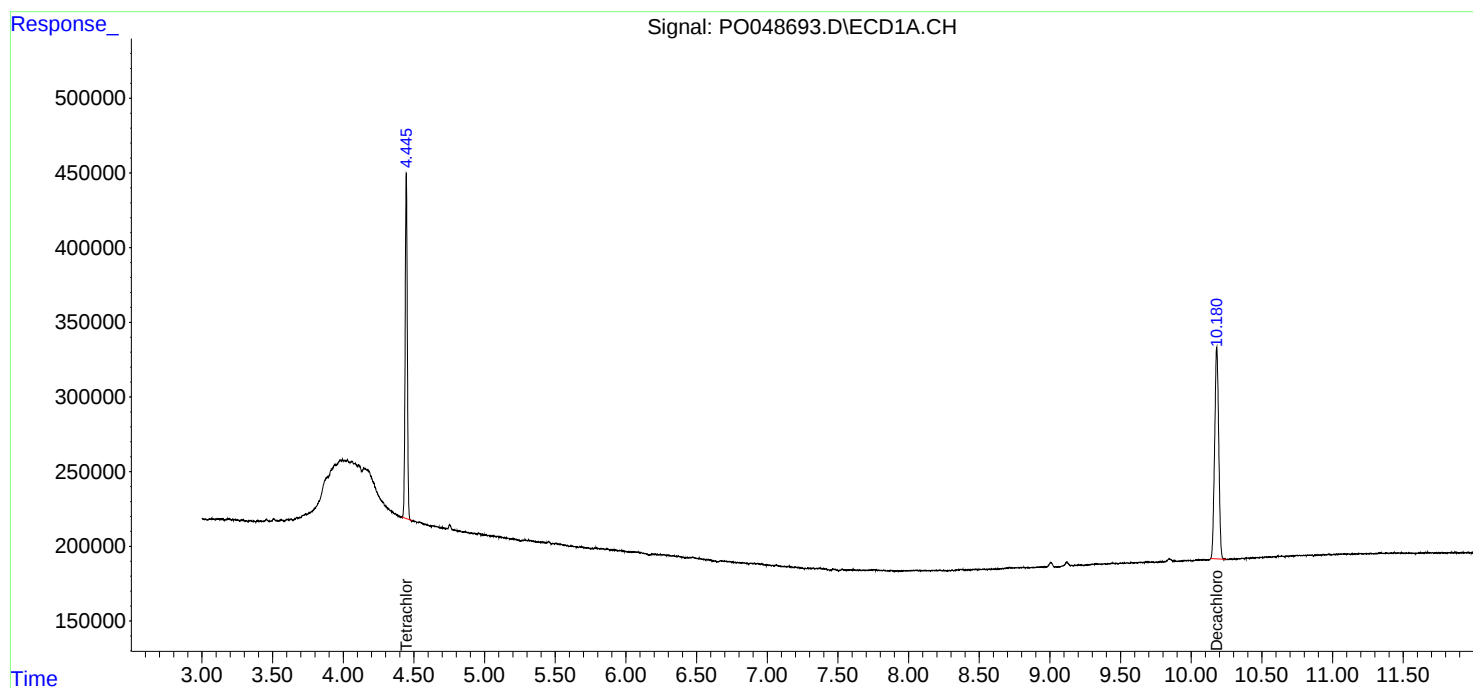


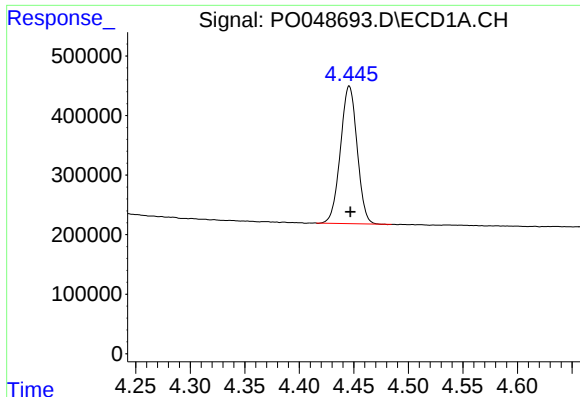

#1 Tetrachloro-m-xylene


R.T.: 4.446 min
Delta R.T.: -0.001 min
Response: 2454320
Conc: 20.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

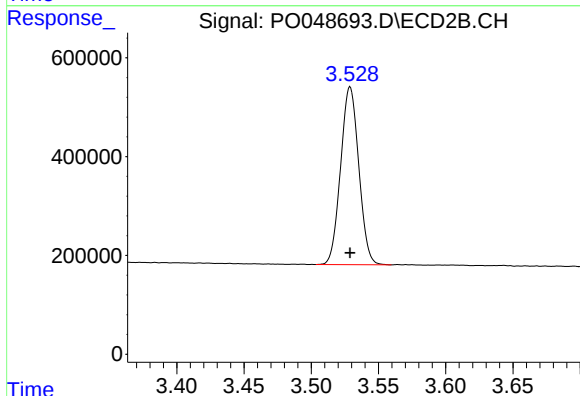


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 3372095
Conc: 21.57 ng/ml

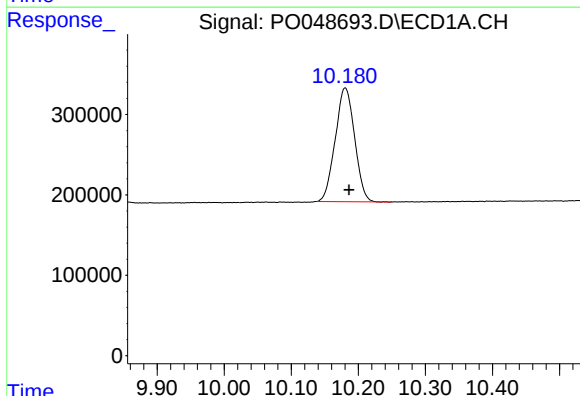

#2 Decachlorobiphenyl

R.T.: 10.180 min
Delta R.T.: -0.006 min
Response: 2837339
Conc: 20.34 ng/ml

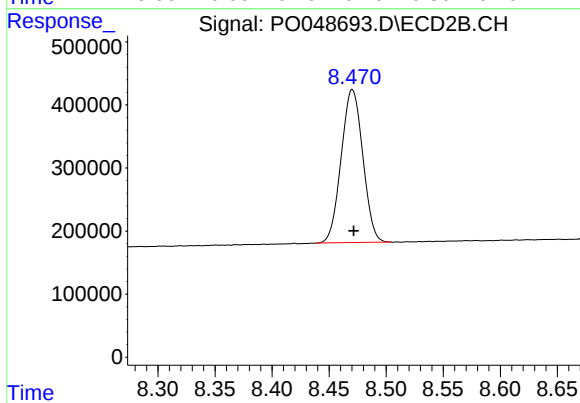

#2 Decachlorobiphenyl

R.T.: 8.470 min
Delta R.T.: -0.001 min
Response: 3203082
Conc: 21.66 ng/ml