

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090418\
 Data File : P0048713.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2018 1:37
 Operator : SM/SJ
 Sample : J4759-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 083018-SIDI-E-D-S

Manual Integrations
 APPROVED

Sohil
 9/5/2018 3:27:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 04:17:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 05 03:48:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.465	3.529	2164689	2835984	17.941m	18.144m
2)	SA Decachlor...	10.181	8.470	2300664	2467613	16.489	16.690

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090418\
Data File : PO048713.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2018 1:37
Operator : SM/SJ
Sample : J4759-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
083018-SIDI-E-D-S


Manual Integrations
APPROVED

Sohil
9/5/2018 3:27:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 04:17:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 05 03:48:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

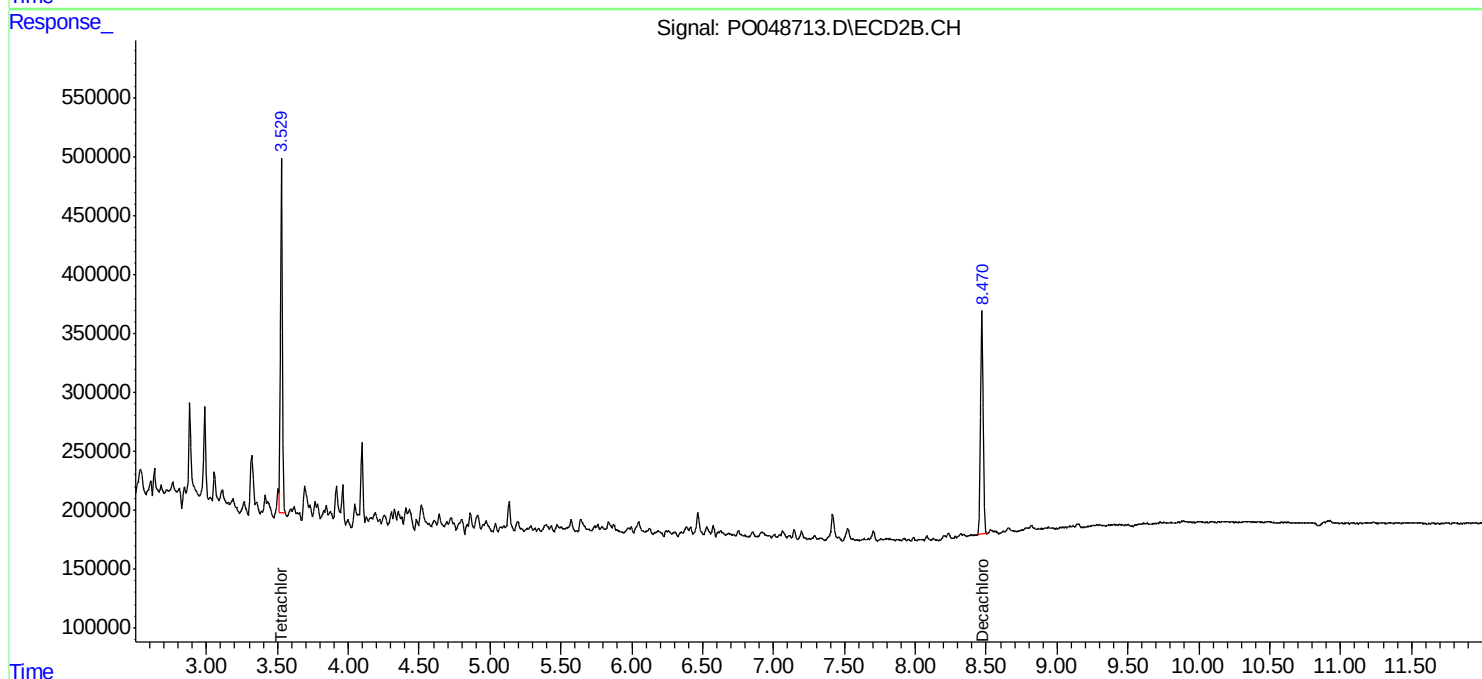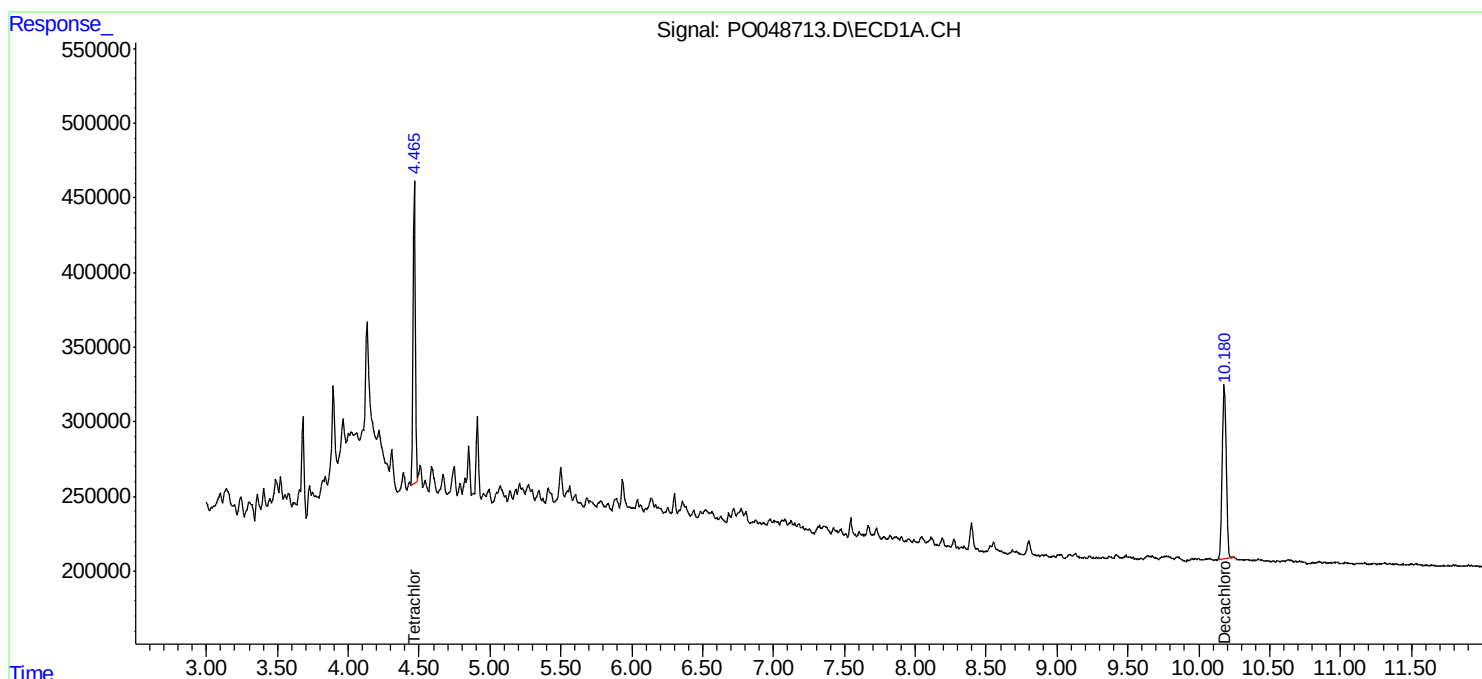

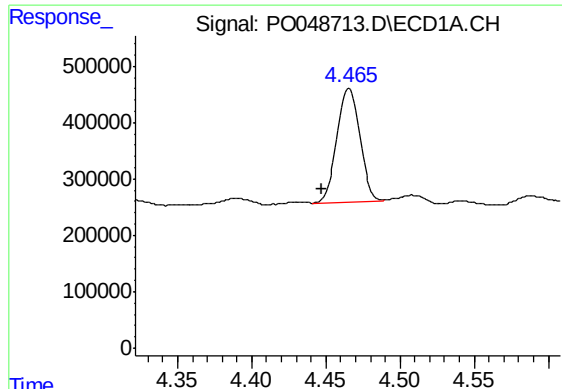


#1 Tetrachloro-m-xylene

R.T.: 4.465 min
Delta R.T.: 0.018 min
Response: 2164689
Conc: 17.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
083018-SIDI-E-D-S


Manual Integrations
APPROVED

Sohil
9/5/2018 3:27:06 PM

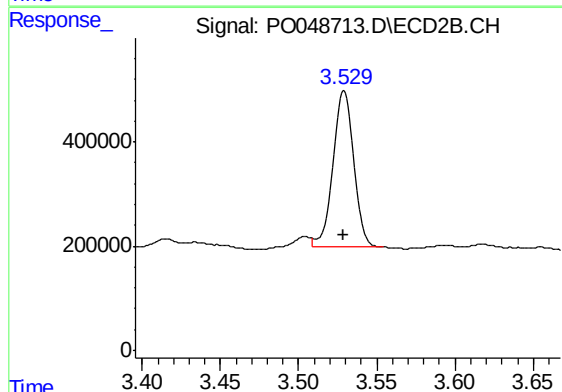


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 2835984
Conc: 18.14 ng/ml m

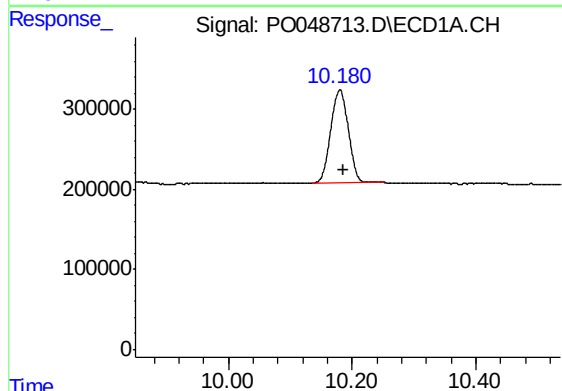

#2 Decachlorobiphenyl

R.T.: 10.181 min
Delta R.T.: -0.006 min
Response: 2300664
Conc: 16.49 ng/ml

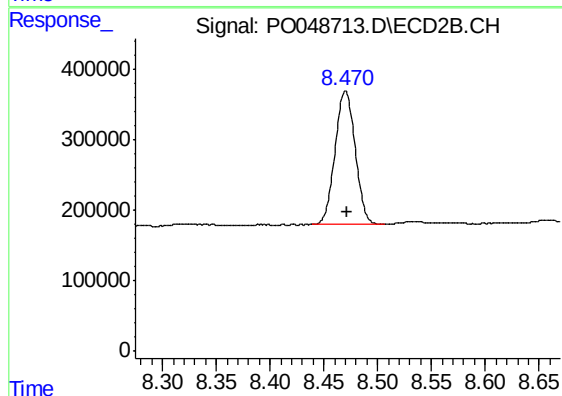

#2 Decachlorobiphenyl

R.T.: 8.470 min
Delta R.T.: -0.001 min
Response: 2467613
Conc: 16.69 ng/ml