

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090419\
 Data File : P0060341.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2019 22:34
 Operator : SM/AJ
 Sample : K4094-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-WATER

Manual Integrations
 APPROVED

Ankita
 9/6/2019 9:07:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:21:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.107	3.489	925250	746025	26.426	20.725
2) SA Decachlor...	9.555	8.338	654166	446210	12.296	11.066m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090419\
Data File : P0060341.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2019 22:34
Operator : SM/AJ
Sample : K4094-03
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Ankita
9/6/2019 9:07:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:21:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

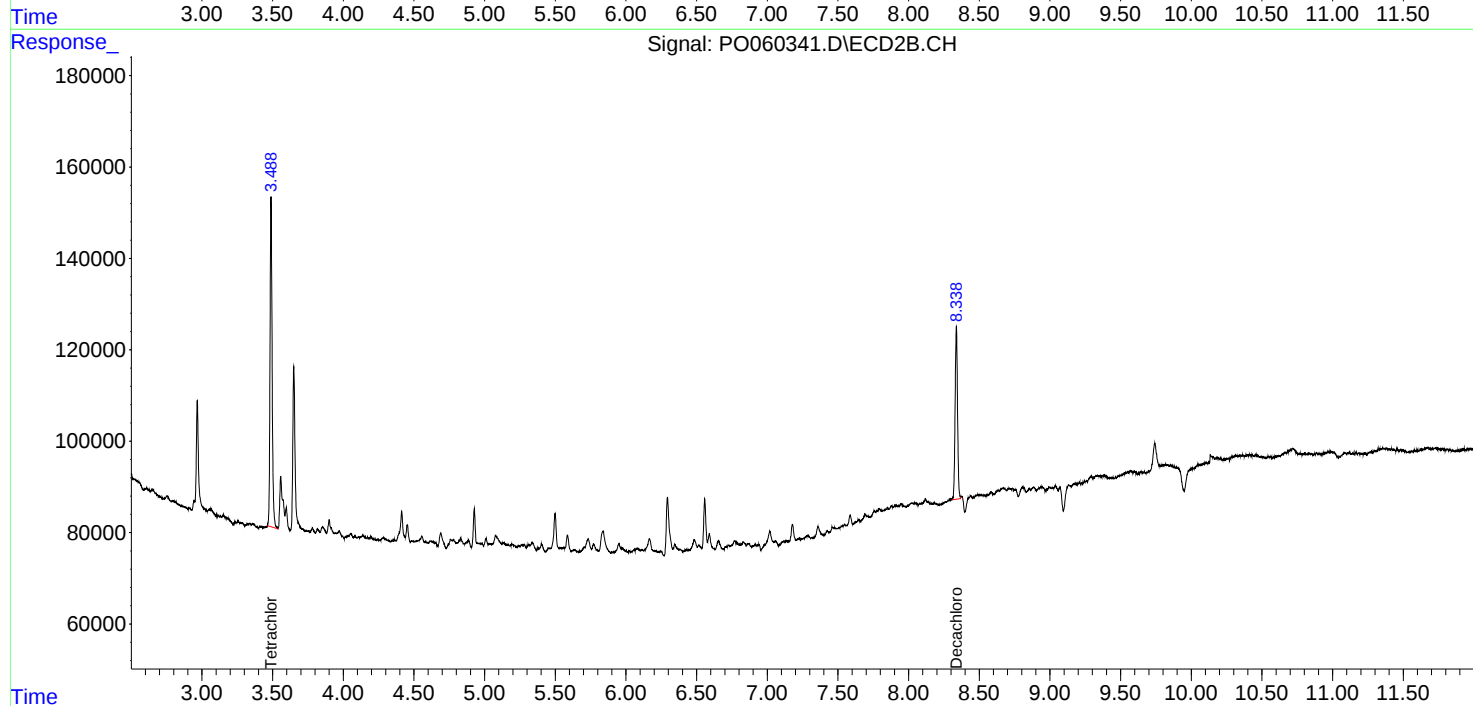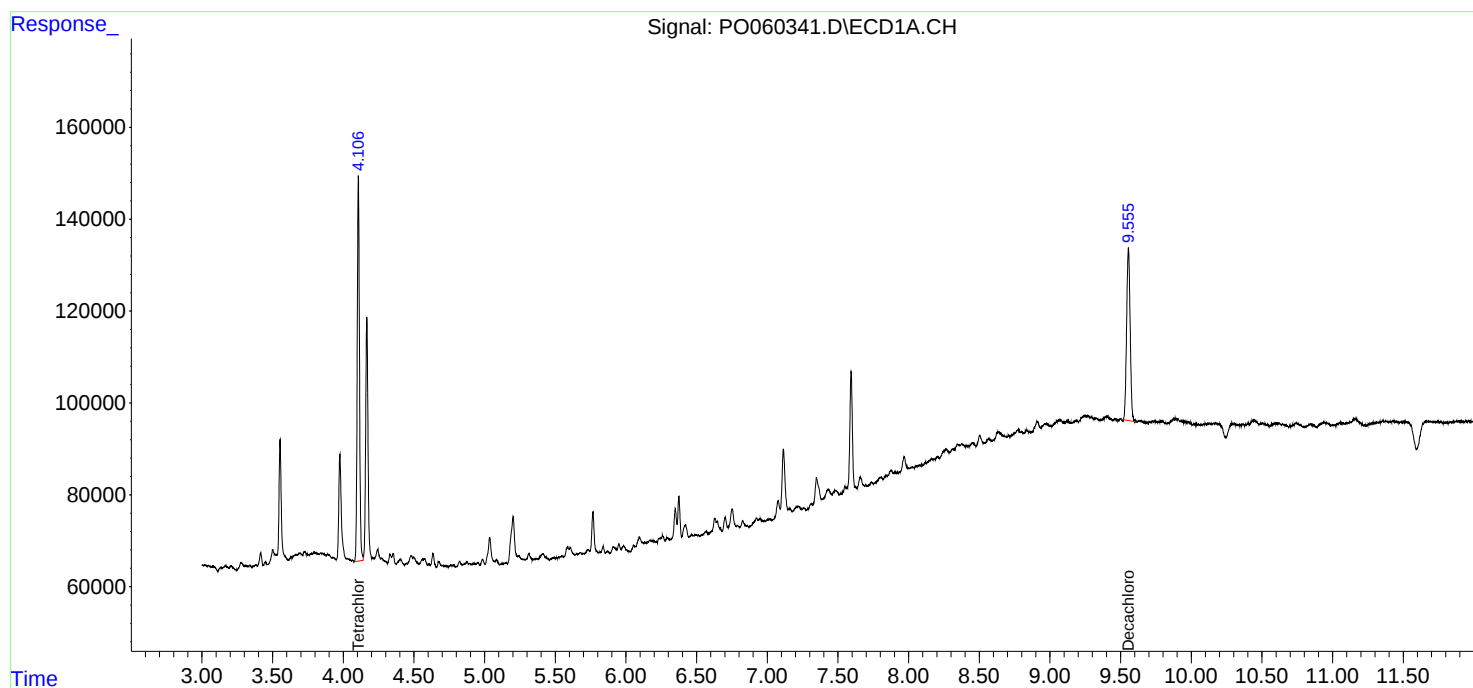

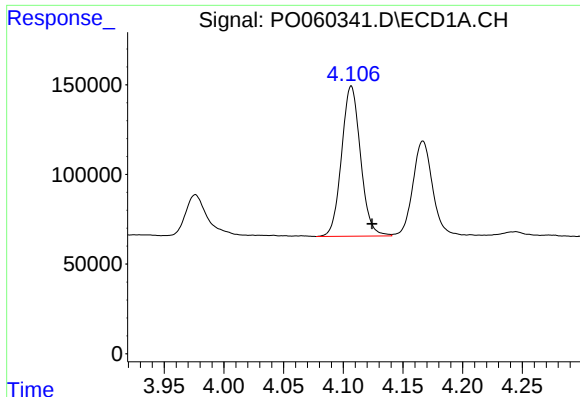


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: -0.017 min
Response: 925250
Conc: 26.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Ankita
9/6/2019 9:07:00 AM

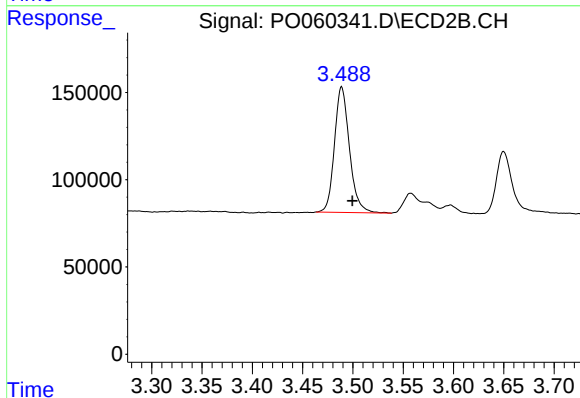


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: -0.011 min
Response: 746025
Conc: 20.73 ng/ml

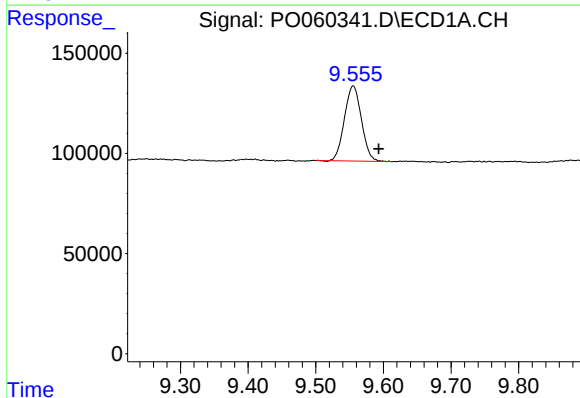

#2 Decachlorobiphenyl

R.T.: 9.555 min
Delta R.T.: -0.038 min
Response: 654166
Conc: 12.30 ng/ml

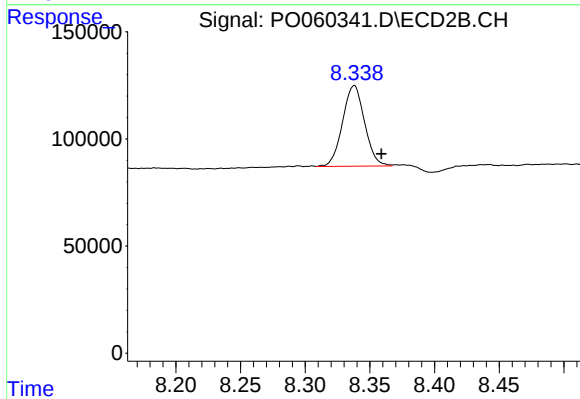

#2 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.021 min
Response: 446210
Conc: 11.07 ng/ml m