

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090419\
 Data File : P0060355.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2019 2:52
 Operator : SM/AJ
 Sample : K4670-04 5X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SDC-1

Manual Integrations
 APPROVED

Ankita
 9/6/2019 9:08:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 14:55:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 05 12:44:29 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.106	3.487	227866	223975	6.508	6.222
2) SA Decachlor...	9.554	8.336	282455	208300	5.309m	5.166
Target Compounds						
31) L7 AR-1260-1	6.822	5.977	100984	54355	37.460m	23.852 #
32) L7 AR-1260-2	7.081	6.170	197816	88409	53.313m	30.175 #
33) L7 AR-1260-3	7.429	6.312	114340	60543	34.899m	22.854m#
34) L7 AR-1260-4	7.657	6.774	53850	31041	17.533m	13.719m
35) L7 AR-1260-5	7.966	7.018	72940	72737	10.301m	13.217m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090419\
Data File : PO060355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2019 2:52
Operator : SM/AJ
Sample : K4670-04 5X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SDC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 14:55:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 05 12:44:29 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

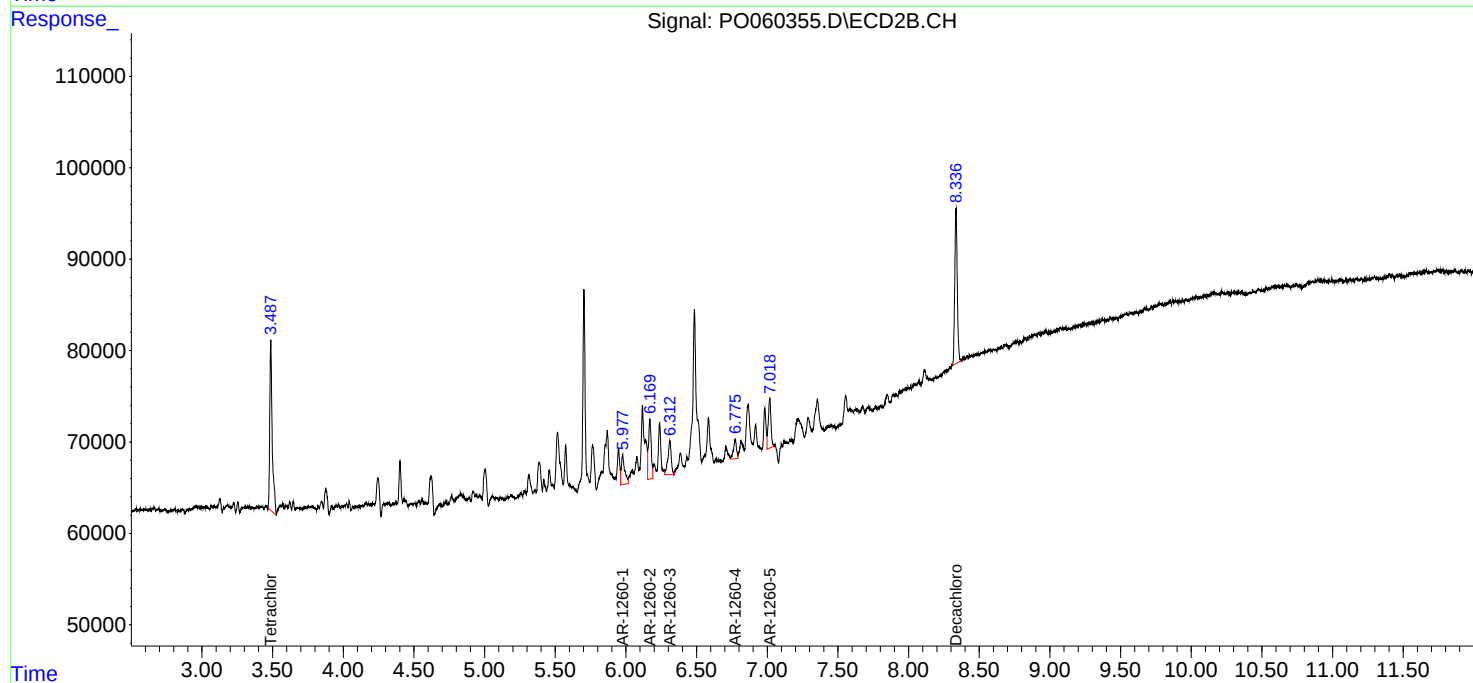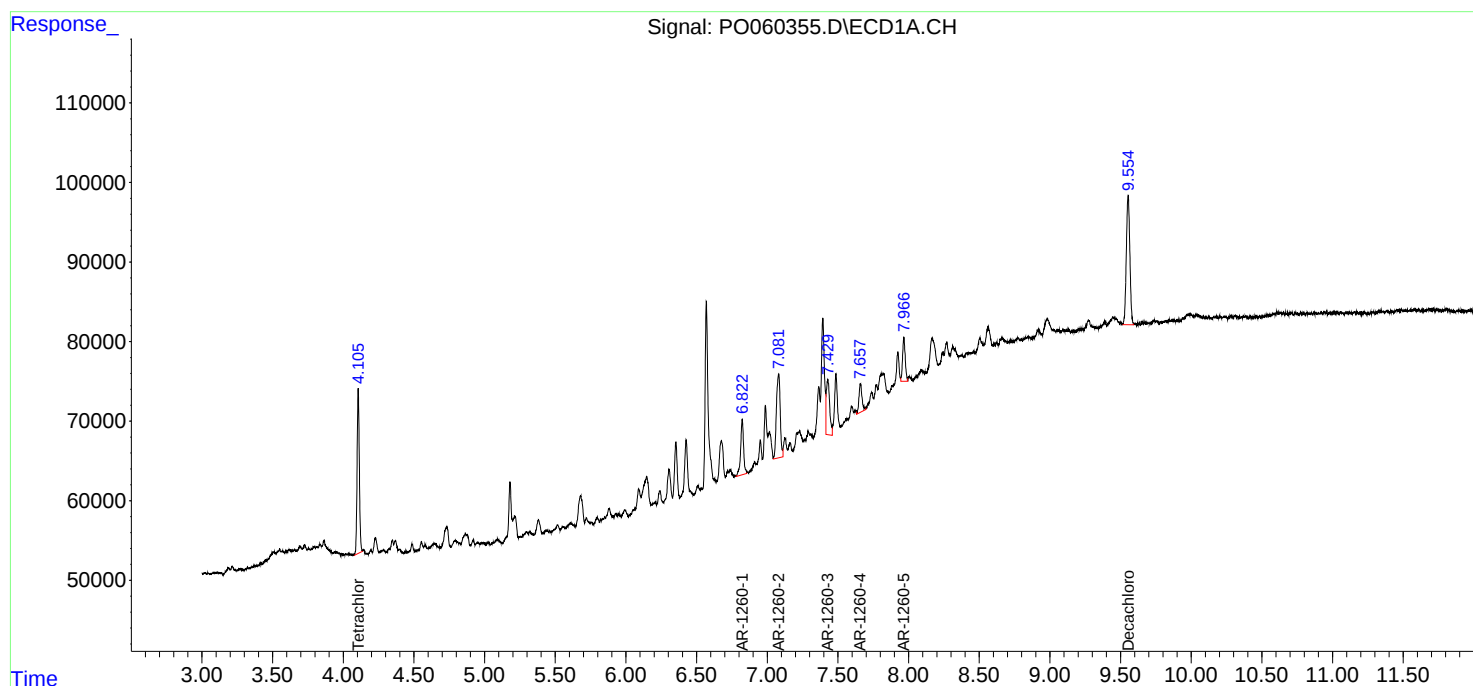

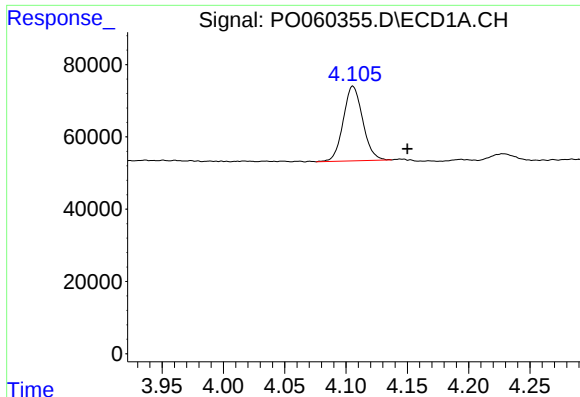


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.044 min
Response: 227866
Conc: 6.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
SDC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:05 AM

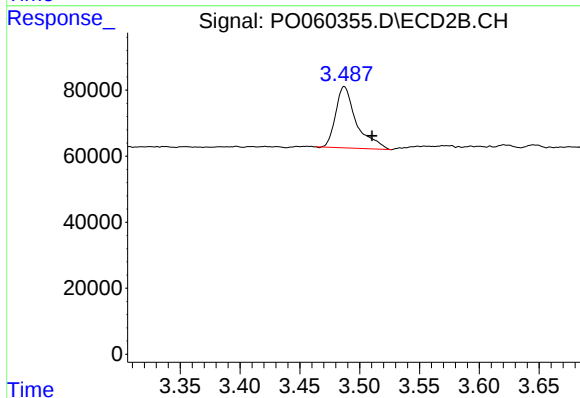


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.023 min
Response: 223975
Conc: 6.22 ng/ml

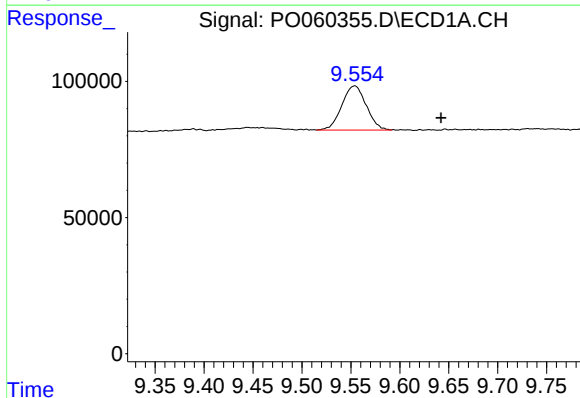


#2 Decachlorobiphenyl

R.T.: 9.554 min
Delta R.T.: -0.088 min
Response: 282455
Conc: 5.31 ng/ml m

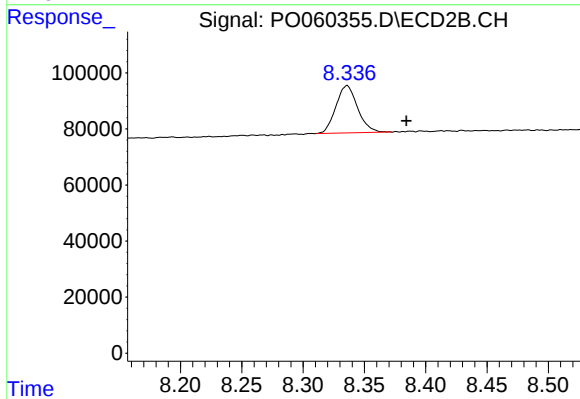

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.049 min
Response: 208300
Conc: 5.17 ng/ml

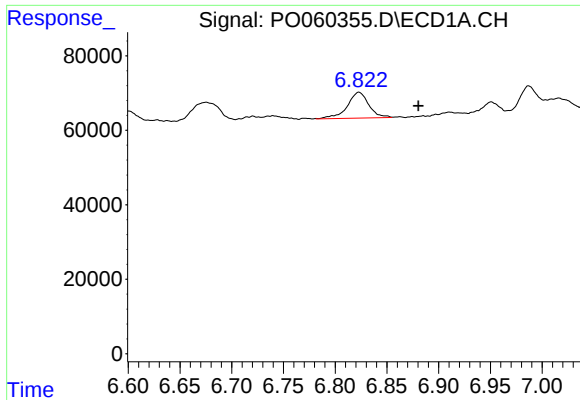


#31 AR-1260-1

R.T.: 6.822 min
Delta R.T.: -0.058 min
Response: 100984
Conc: 37.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SDC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:05 AM

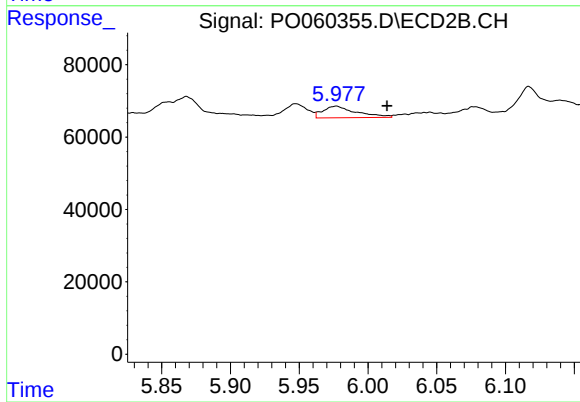


#31 AR-1260-1

R.T.: 5.977 min
Delta R.T.: -0.037 min
Response: 54355
Conc: 23.85 ng/ml

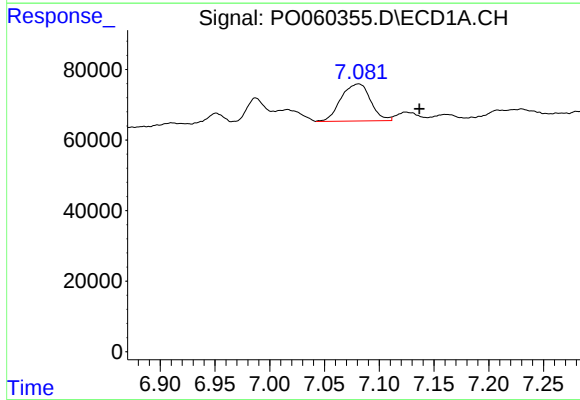


#32 AR-1260-2

R.T.: 7.081 min
Delta R.T.: -0.056 min
Response: 197816
Conc: 53.31 ng/ml m

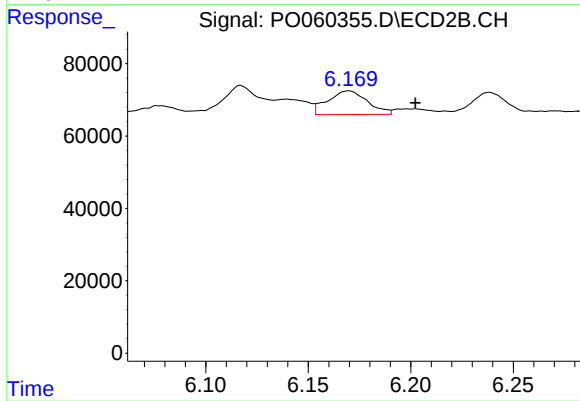

#32 AR-1260-2

R.T.: 6.170 min
Delta R.T.: -0.032 min
Response: 88409
Conc: 30.18 ng/ml

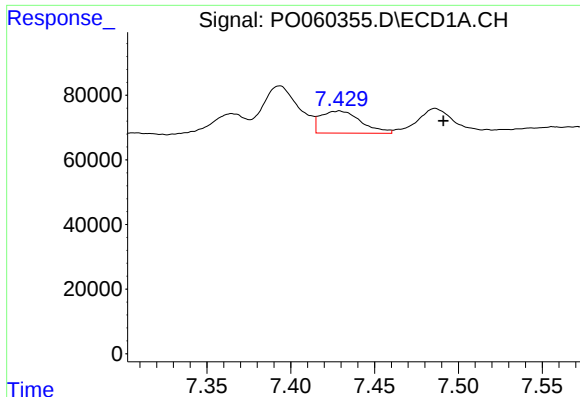


#33 AR-1260-3

R.T.: 7.429 min
Delta R.T.: -0.062 min
Response: 114340
Conc: 34.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SDC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:05 AM

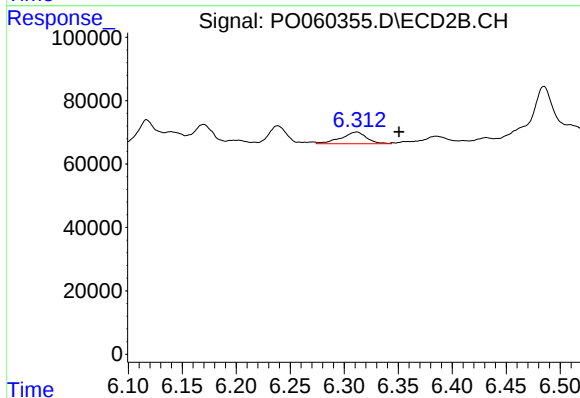


#33 AR-1260-3

R.T.: 6.312 min
Delta R.T.: -0.039 min
Response: 60543
Conc: 22.85 ng/ml m

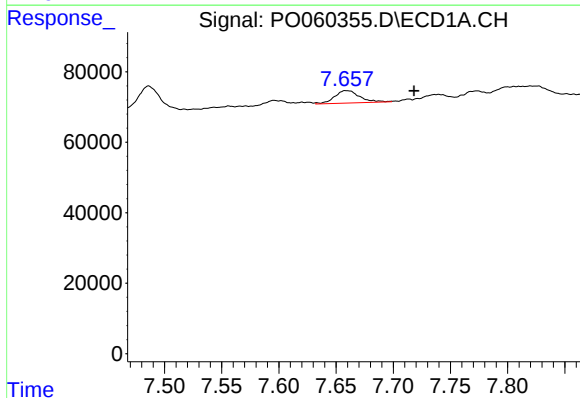


#34 AR-1260-4

R.T.: 7.657 min
Delta R.T.: -0.061 min
Response: 53850
Conc: 17.53 ng/ml m

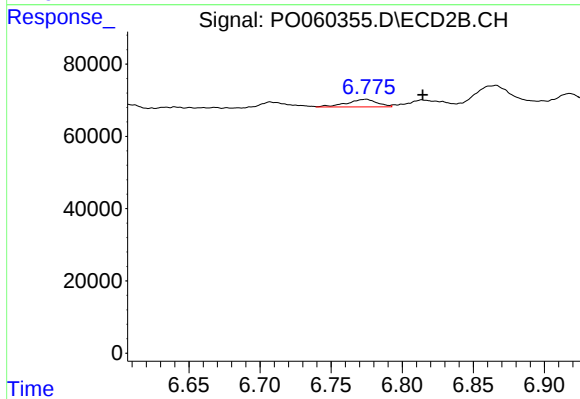

#34 AR-1260-4

R.T.: 6.774 min
Delta R.T.: -0.040 min
Response: 31041
Conc: 13.72 ng/ml m

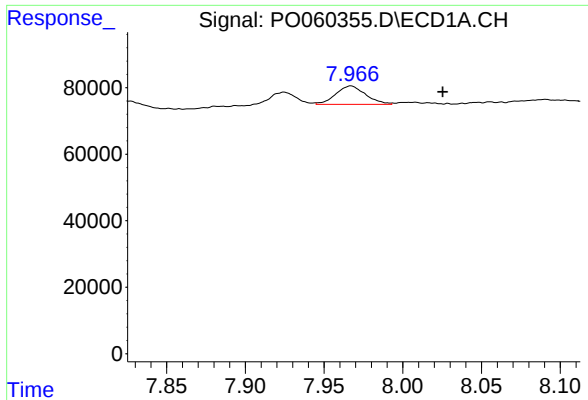


#35 AR-1260-5

R.T.: 7.966 min
Delta R.T.: -0.059 min
Response: 72940
Conc: 10.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SDC-1

Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:05 AM

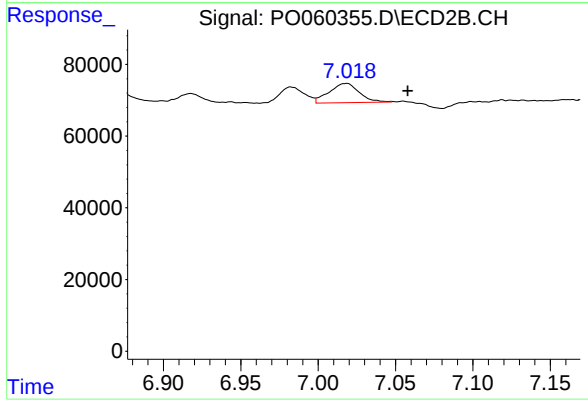

#35 AR-1260-5

R.T.: 7.018 min
Delta R.T.: -0.039 min
Response: 72737
Conc: 13.22 ng/ml m