

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090419\
 Data File : P0060357.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2019 3:24
 Operator : SM/AJ
 Sample : K4672-01 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 DC-1

Manual Integrations
 APPROVED

Ankita
 9/6/2019 9:08:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 05:07:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.105	3.487	218574	192767	6.243	5.355
2) SA Decachlor...	9.553	8.335	269915	195602	5.074	4.851
Target Compounds						
31) L7 AR-1260-1	6.821	5.977	204621	57345	75.903	25.163 #
32) L7 AR-1260-2	7.070	6.172	204444	153252	55.099	52.307
33) L7 AR-1260-3	7.432	6.311	134204	67149	40.962m	25.348 #
34) L7 AR-1260-4	7.665	6.766	111623	68693	36.344m	30.360m
35) L7 AR-1260-5	7.923	7.017	130461	144699	18.424m	26.293 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090419\
Data File : P0060357.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2019 3:24
Operator : SM/AJ
Sample : K4672-01 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
DC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 05:07:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

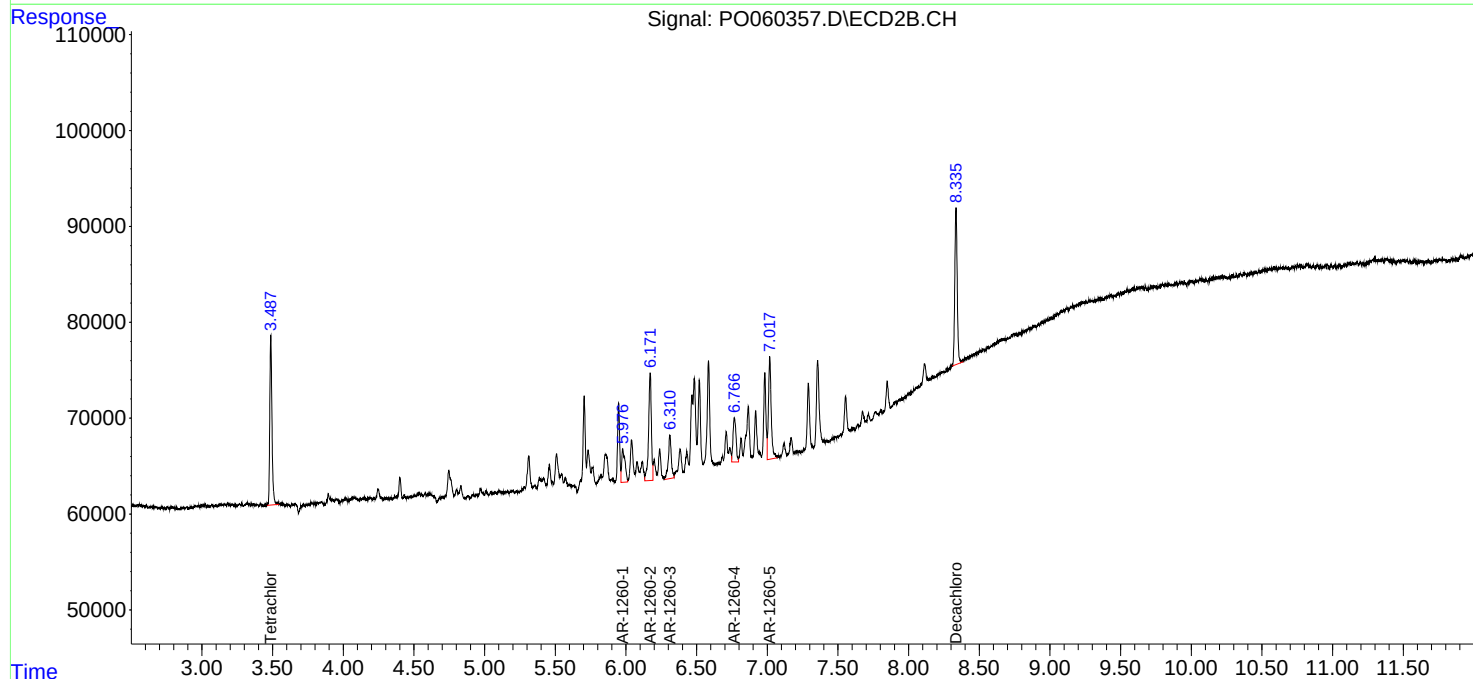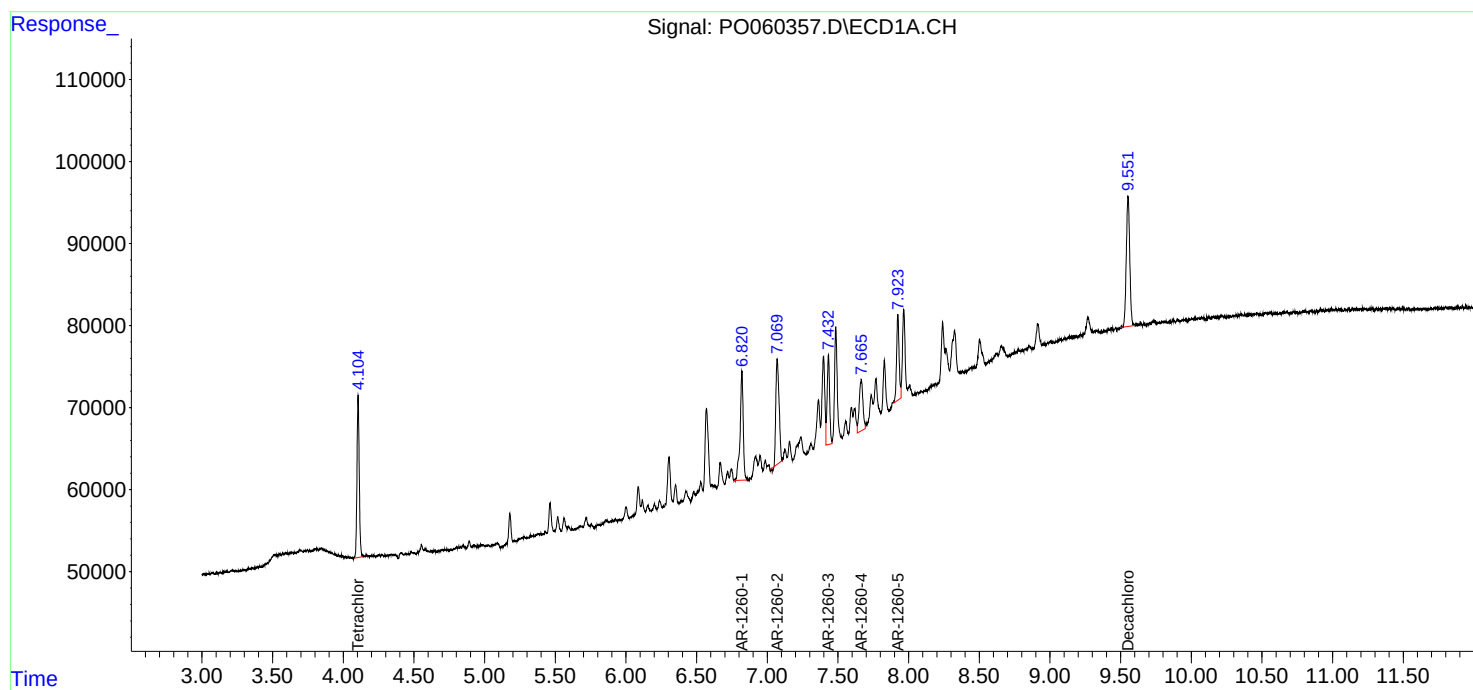

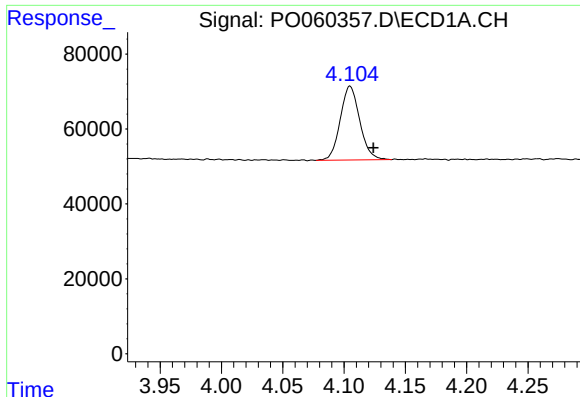


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: -0.019 min
Response: 218574
Conc: 6.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
DC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:07 AM

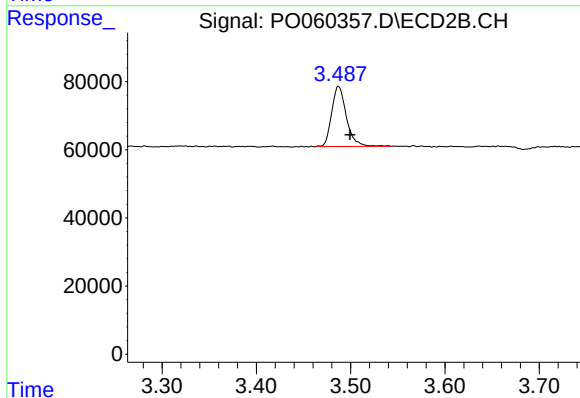


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.012 min
Response: 192767
Conc: 5.36 ng/ml

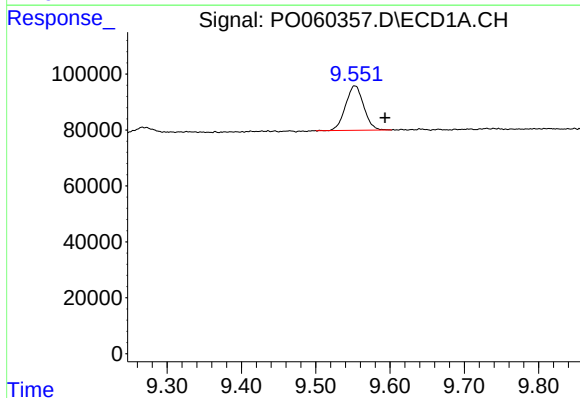


#2 Decachlorobiphenyl

R.T.: 9.553 min
Delta R.T.: -0.040 min
Response: 269915
Conc: 5.07 ng/ml

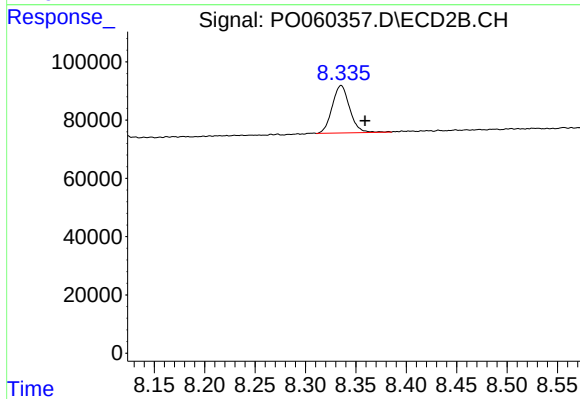

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.024 min
Response: 195602
Conc: 4.85 ng/ml

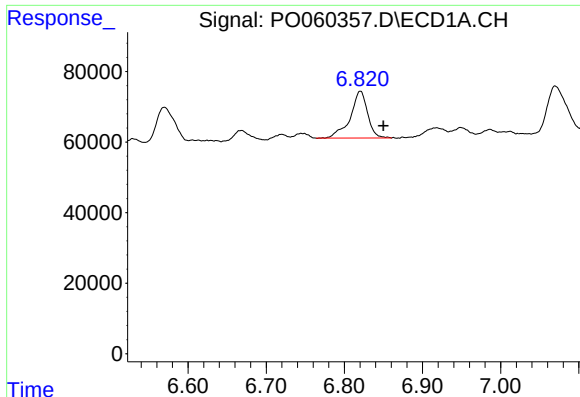


#31 AR-1260-1

R.T.: 6.821 min
Delta R.T.: -0.029 min
Response: 204621
Conc: 75.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
DC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:07 AM

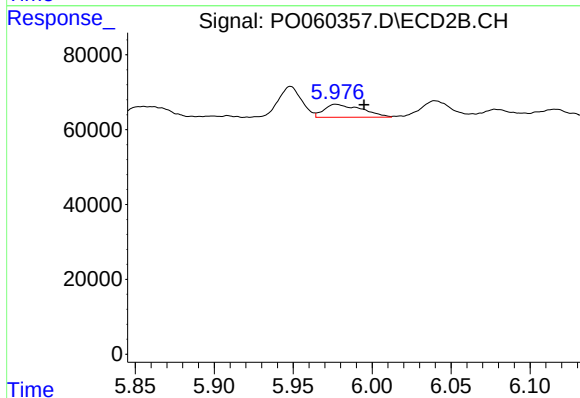


#31 AR-1260-1

R.T.: 5.977 min
Delta R.T.: -0.018 min
Response: 57345
Conc: 25.16 ng/ml

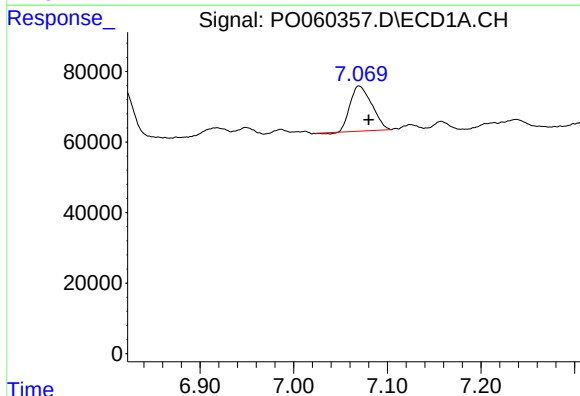


#32 AR-1260-2

R.T.: 7.070 min
Delta R.T.: -0.010 min
Response: 204444
Conc: 55.10 ng/ml

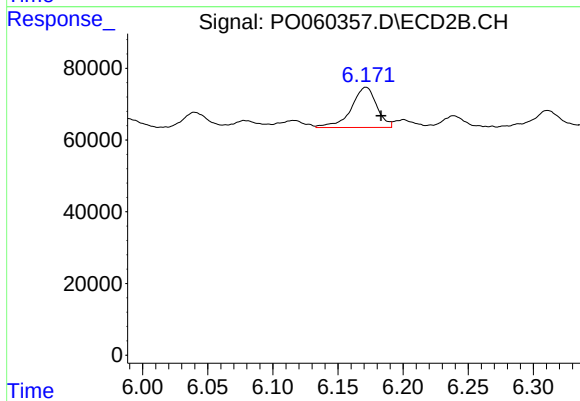

#32 AR-1260-2

R.T.: 6.172 min
Delta R.T.: -0.012 min
Response: 153252
Conc: 52.31 ng/ml

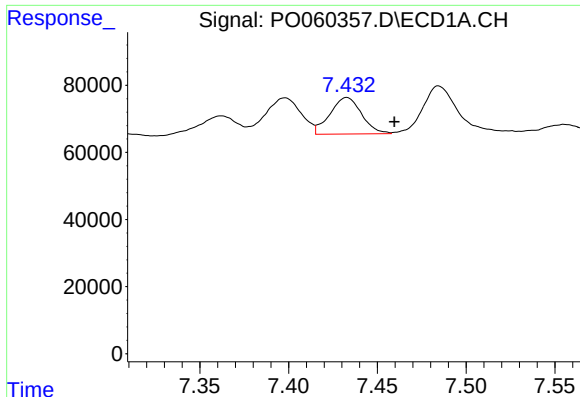


#33 AR-1260-3

R.T.: 7.432 min
Delta R.T.: -0.027 min
Response: 134204
Conc: 40.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DC-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:07 AM

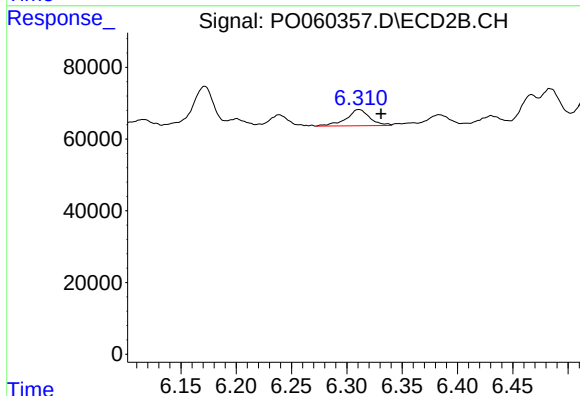


#33 AR-1260-3

R.T.: 6.311 min
Delta R.T.: -0.020 min
Response: 67149
Conc: 25.35 ng/ml

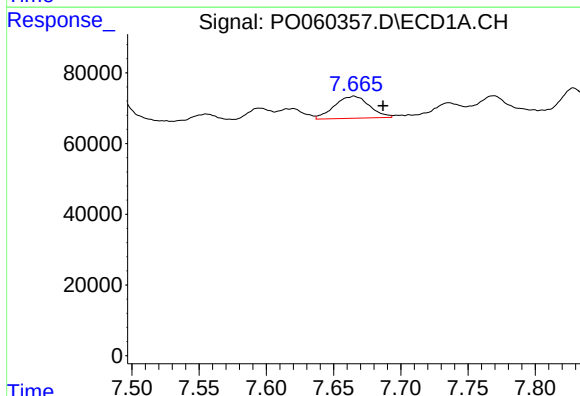


#34 AR-1260-4

R.T.: 7.665 min
Delta R.T.: -0.022 min
Response: 111623
Conc: 36.34 ng/ml m

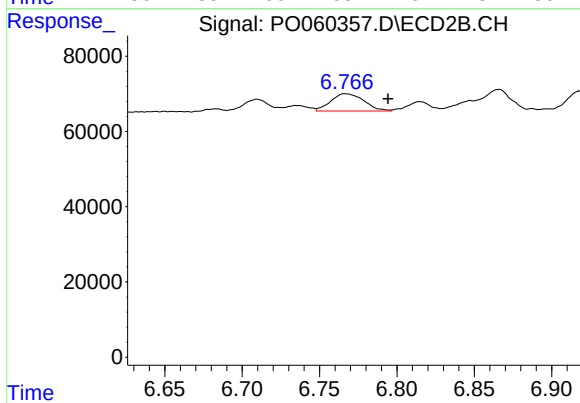

#34 AR-1260-4

R.T.: 6.766 min
Delta R.T.: -0.028 min
Response: 68693
Conc: 30.36 ng/ml m

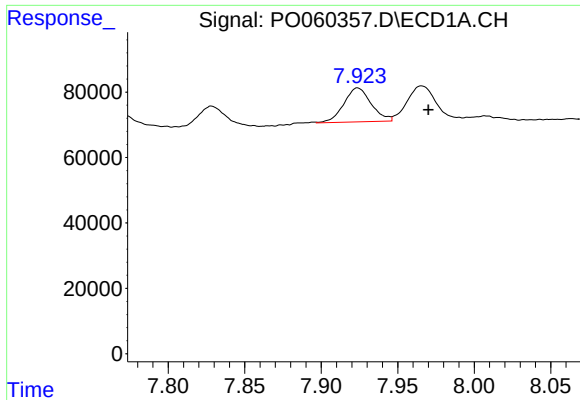


#35 AR-1260-5

R.T.: 7.923 min
Delta R.T.: -0.047 min
Response: 130461
Conc: 18.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DC-1

Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:07 AM

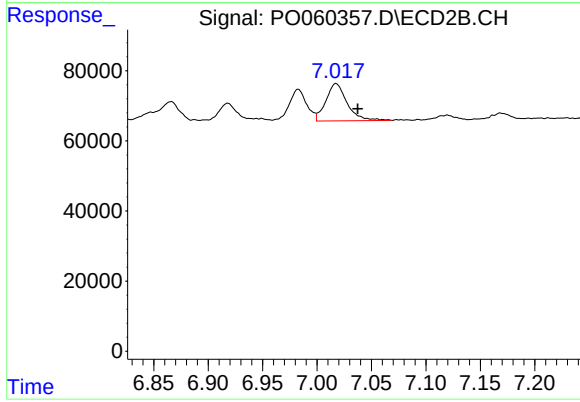

#35 AR-1260-5

R.T.: 7.017 min
Delta R.T.: -0.020 min
Response: 144699
Conc: 26.29 ng/ml