

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090419\
 Data File : P0060367.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2019 6:07
 Operator : SM/AJ
 Sample : K4676-01 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CFM-1

Manual Integrations
 APPROVED

Ankita
 9/6/2019 9:08:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 07:00:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 30 18:12:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.106	3.487	225537	203824	6.442	5.662
2)	SA Decachlor...	9.553	8.336	304430	232310	5.722	5.762
Target Compounds							
26)	L6 AR-1254-1	6.087	5.313	46099	40385	22.095m	17.027
27)	L6 AR-1254-2	6.302	5.458	88858	39945	26.634m	19.037 #
28)	L6 AR-1254-3	6.666	5.852	91828	83587	25.878m	24.858m
29)	L6 AR-1254-4	6.948	6.078	94520	48911	32.089m	23.722m#
30)	L6 AR-1254-5	7.364	6.485	148935	108747	48.162m	35.024m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090419\
Data File : PO060367.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2019 6:07
Operator : SM/AJ
Sample : K4676-01 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CFM-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 07:00:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 30 18:12:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

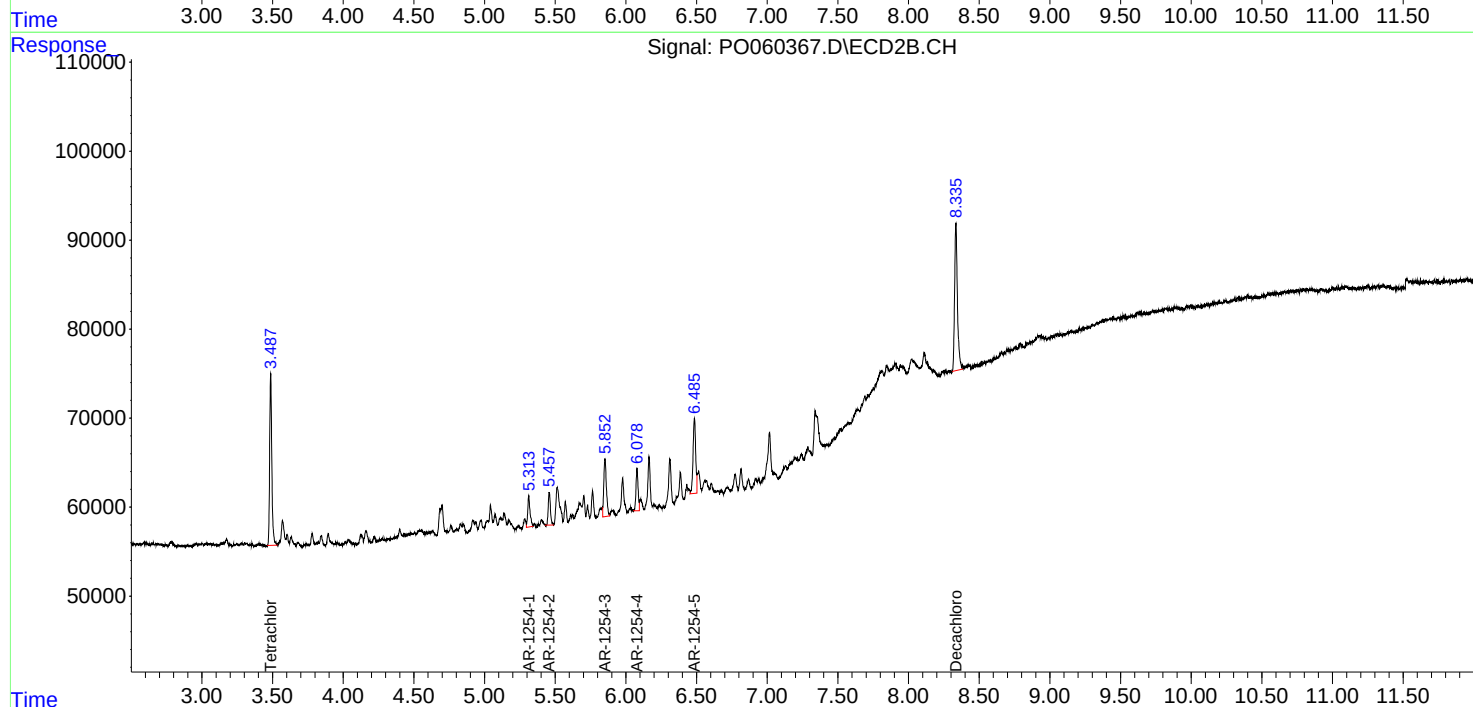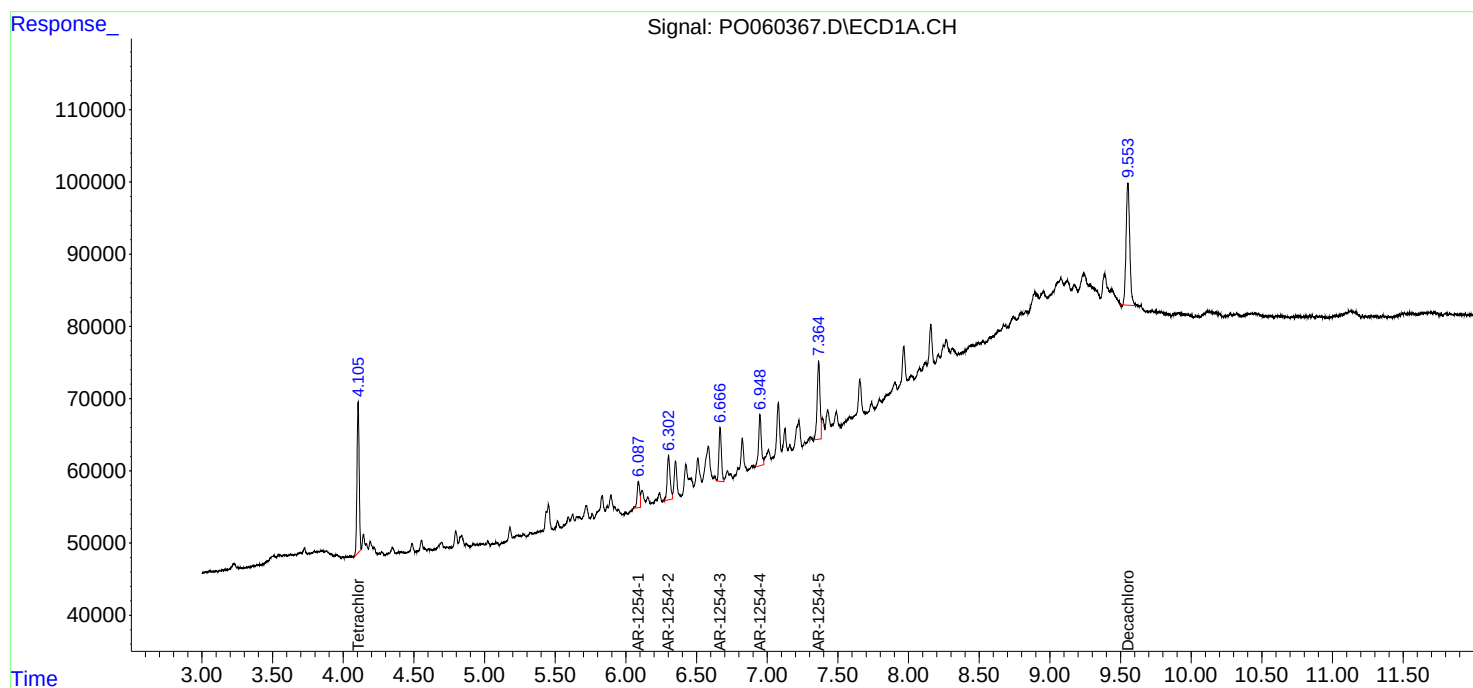

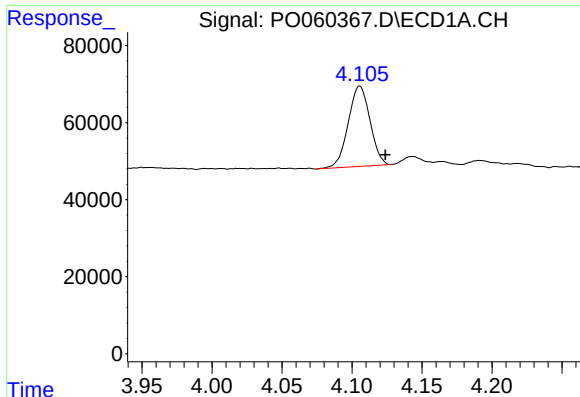


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.018 min
Response: 225537
Conc: 6.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
CFM-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:28 AM

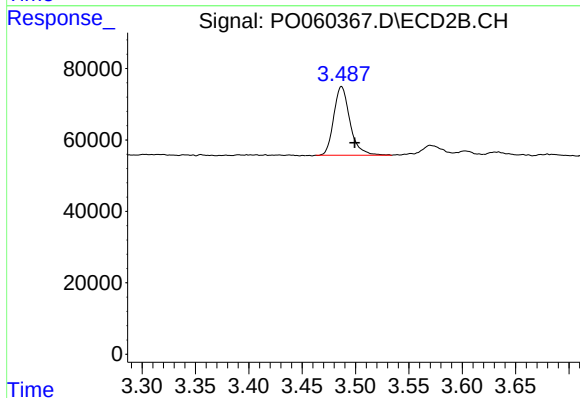


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.012 min
Response: 203824
Conc: 5.66 ng/ml

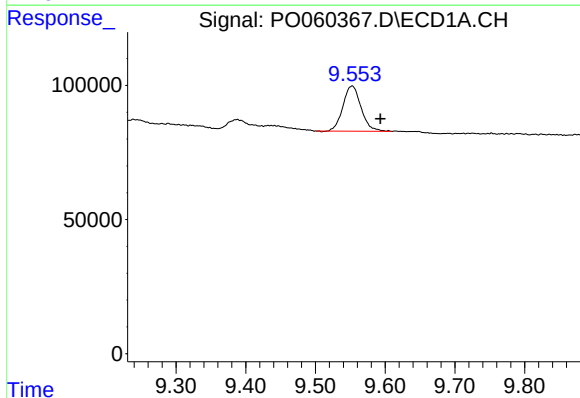


#2 Decachlorobiphenyl

R.T.: 9.553 min
Delta R.T.: -0.041 min
Response: 304430
Conc: 5.72 ng/ml

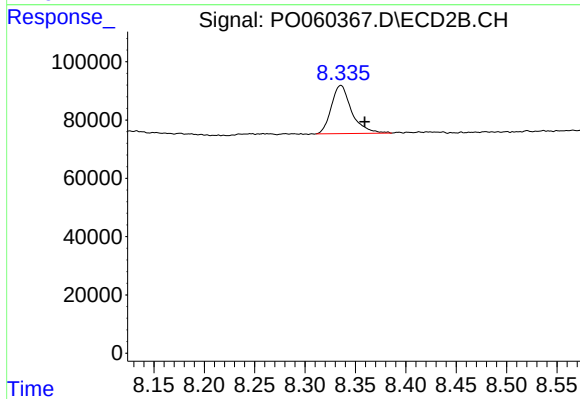

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.024 min
Response: 232310
Conc: 5.76 ng/ml

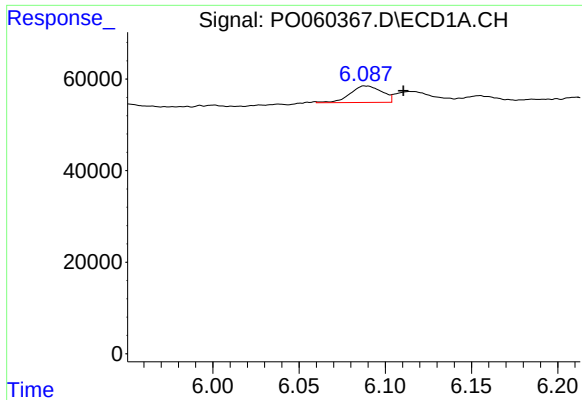


#26 AR-1254-1

R.T.: 6.087 min
Delta R.T.: -0.023 min
Response: 46099
Conc: 22.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CFM-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:28 AM

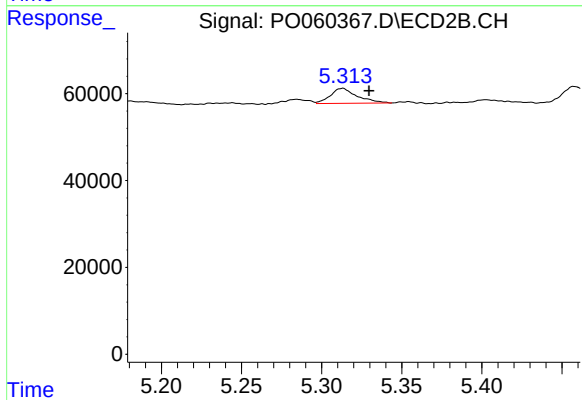


#26 AR-1254-1

R.T.: 5.313 min
Delta R.T.: -0.017 min
Response: 40385
Conc: 17.03 ng/ml

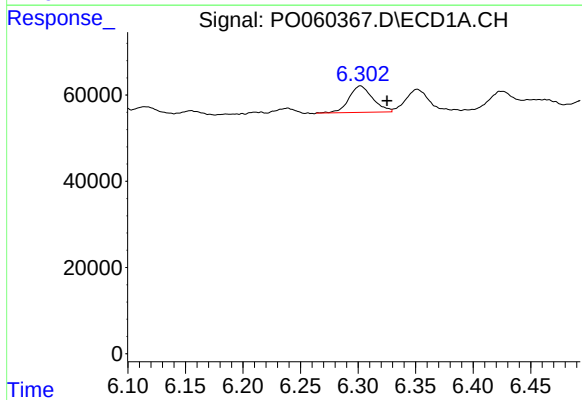


#27 AR-1254-2

R.T.: 6.302 min
Delta R.T.: -0.024 min
Response: 88858
Conc: 26.63 ng/ml m

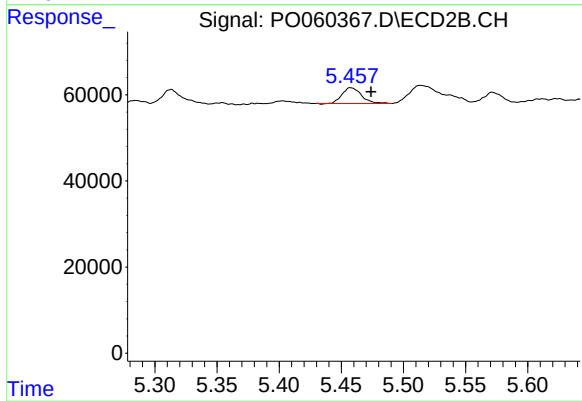

#27 AR-1254-2

R.T.: 5.458 min
Delta R.T.: -0.016 min
Response: 39945
Conc: 19.04 ng/ml

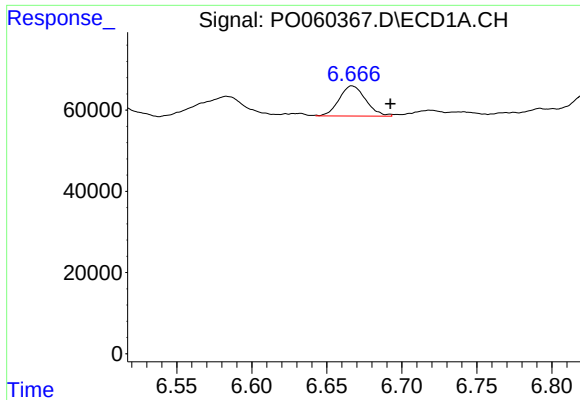


#28 AR-1254-3

R.T.: 6.666 min
Delta R.T.: -0.026 min
Response: 91828
Conc: 25.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CFM-1


Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:28 AM

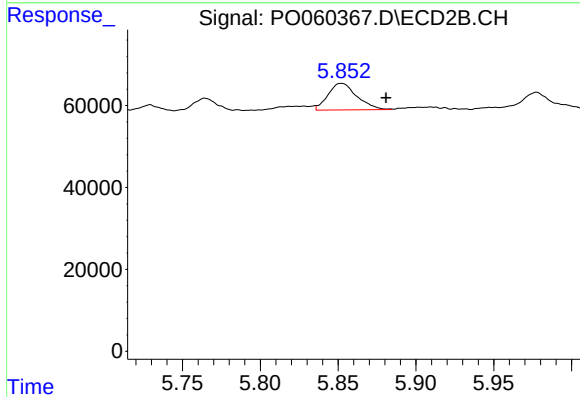


#28 AR-1254-3

R.T.: 5.852 min
Delta R.T.: -0.029 min
Response: 83587
Conc: 24.86 ng/ml m

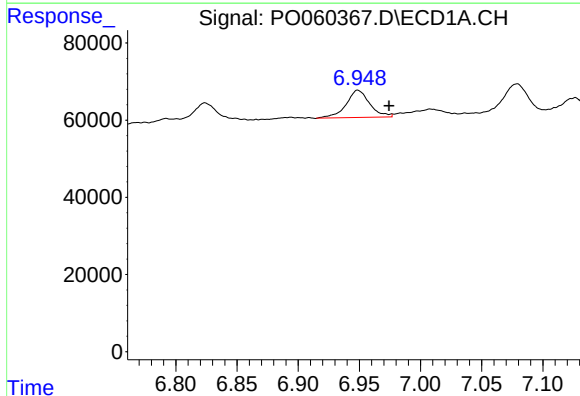


#29 AR-1254-4

R.T.: 6.948 min
Delta R.T.: -0.026 min
Response: 94520
Conc: 32.09 ng/ml m

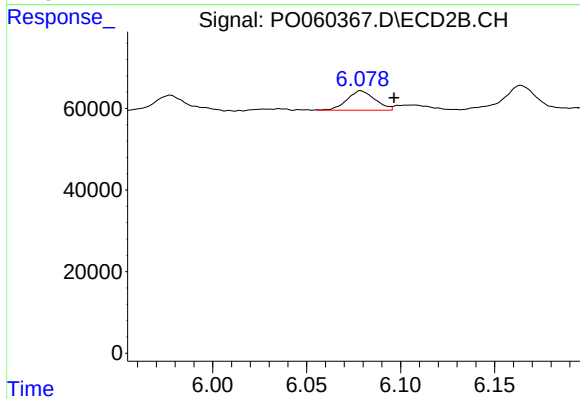

#29 AR-1254-4

R.T.: 6.078 min
Delta R.T.: -0.018 min
Response: 48911
Conc: 23.72 ng/ml m

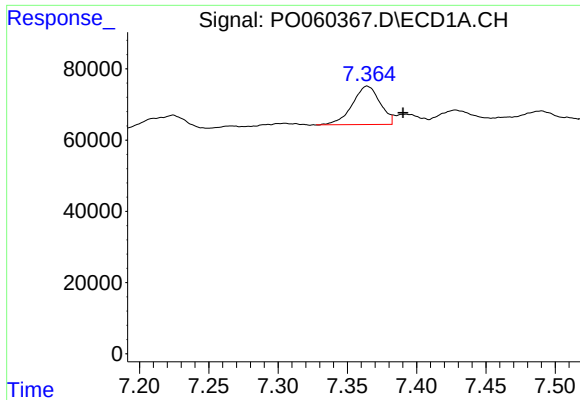


#30 AR-1254-5

R.T.: 7.364 min
Delta R.T.: -0.026 min
Response: 148935
Conc: 48.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CFM-1

Manual Integrations
APPROVED

Ankita
9/6/2019 9:08:28 AM

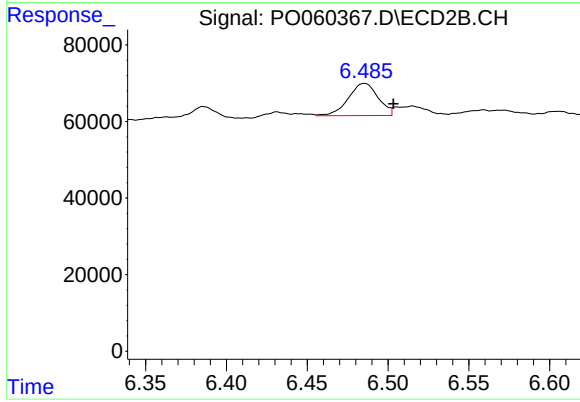

#30 AR-1254-5

R.T.: 6.485 min
Delta R.T.: -0.018 min
Response: 108747
Conc: 35.02 ng/ml m