

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
 Data File : P0071207.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2020 21:52
 Operator : DD\AJ
 Sample : L3899-06 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH3050-END-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:06:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.352	3.538	311101	233891	4.028	5.276 #
2)	SA Decachlor...	9.969	8.719	295513	171185	3.230	2.980
Target Compounds							
30)	L6 AR-1254-5	7.896f	0.000	44519	0	8.462	N.D. #
31)	L7 AR-1260-1	0.000	6.315	0	100146	N.D.	35.652 #
34)	L7 AR-1260-4	8.161	0.000	41804	0	7.890	N.D. #
35)	L7 AR-1260-5	8.458f	0.000	52938	0	4.331	N.D. #
37)	L8 AR-1262-2	8.458f	0.000	52938	0	4.008	N.D. #
39)	L8 AR-1262-4	8.856f	0.000	8988	0	2.740	N.D. #
42)	L9 AR-1268-2	8.856f	0.000	8988	0	0.667	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090420\
Data File : PO071207.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2020 21:52
Operator : DD\AJ
Sample : L3899-06 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KMH3050-END-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:06:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

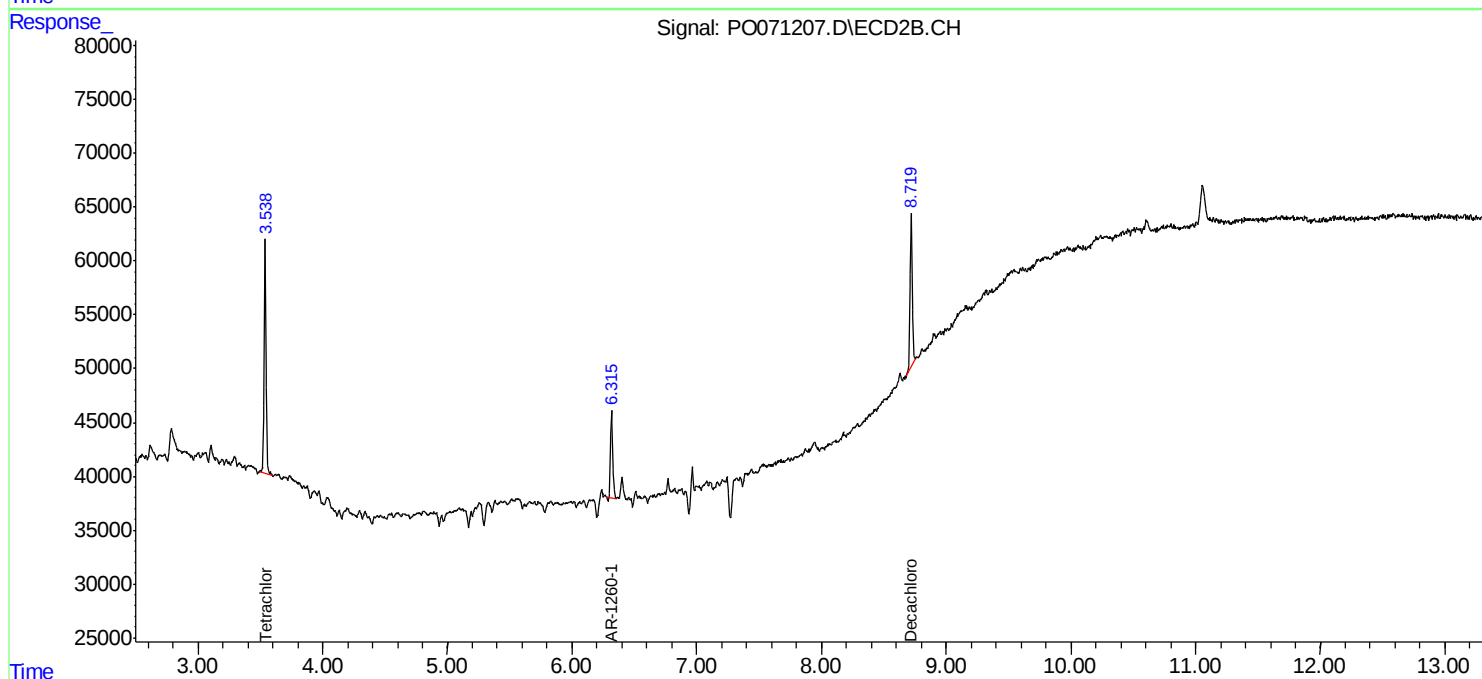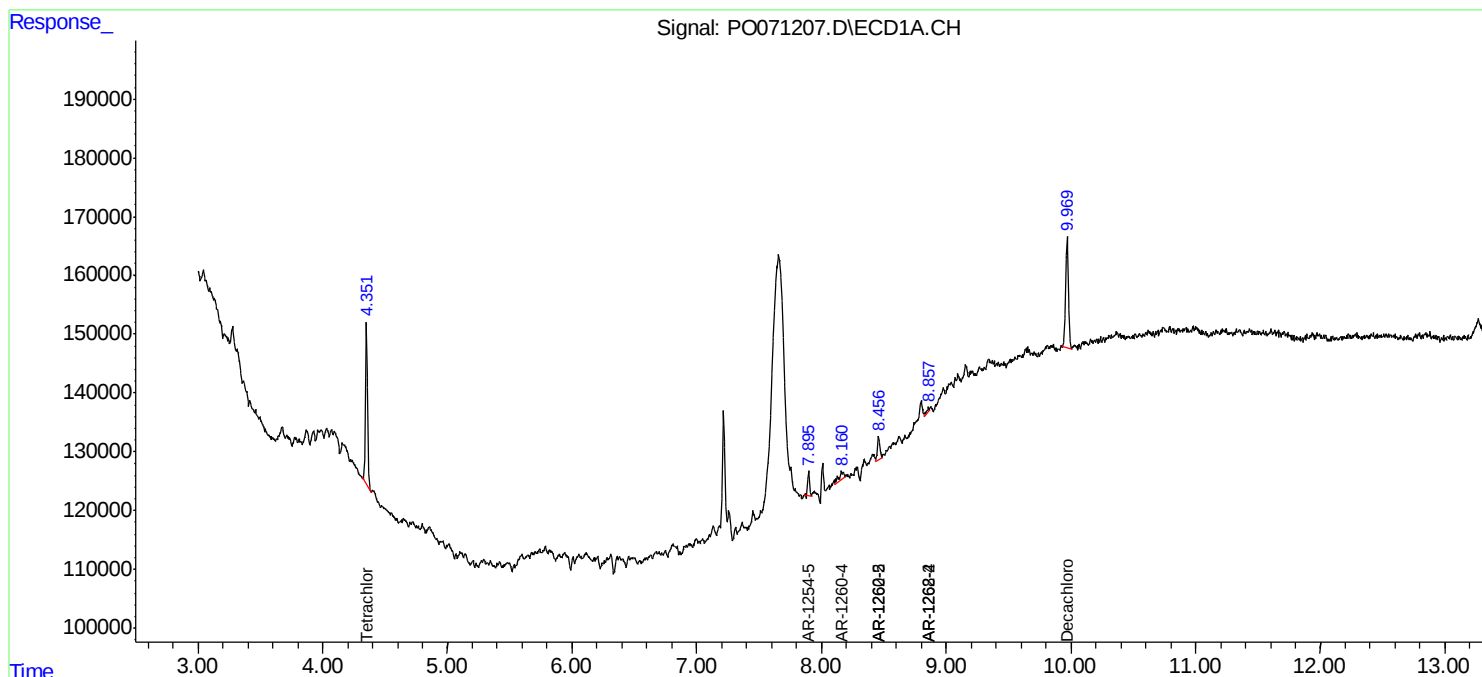


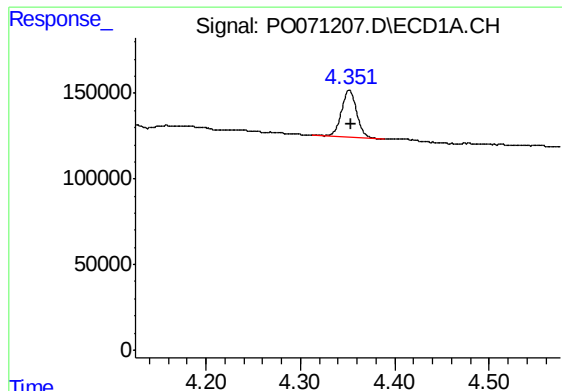

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: -0.002 min
Response: 311101
Conc: 4.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH3050-END-2

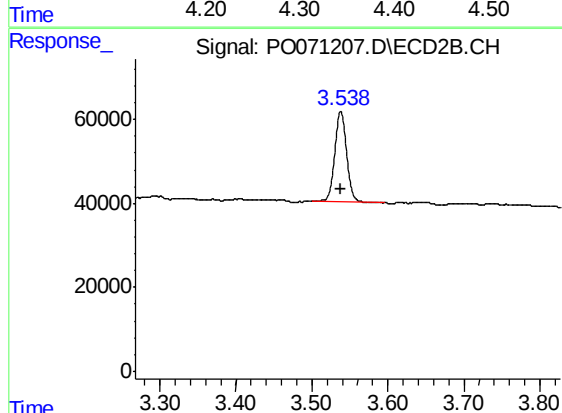


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 233891
Conc: 5.28 ng/ml

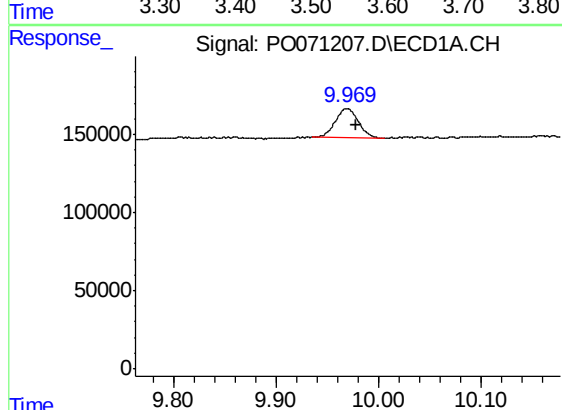


#2 Decachlorobiphenyl

R.T.: 9.969 min
Delta R.T.: -0.008 min
Response: 295513
Conc: 3.23 ng/ml

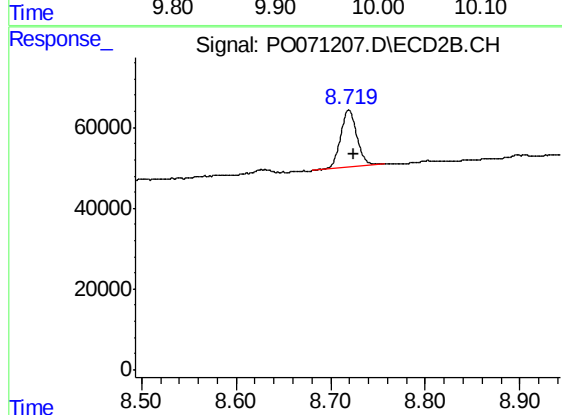

#2 Decachlorobiphenyl


R.T.: 8.719 min
Delta R.T.: -0.005 min
Response: 171185
Conc: 2.98 ng/ml

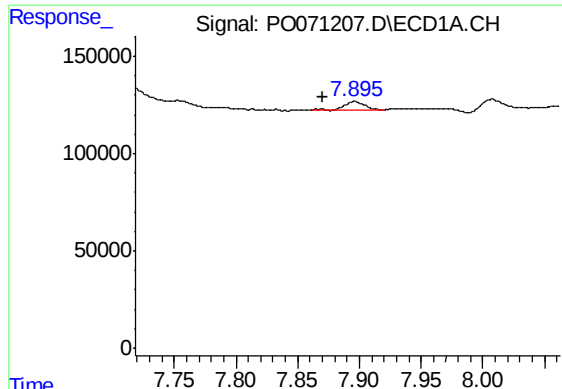

#30 AR-1254-5


R.T.: 7.896 min
Delta R.T.: 0.025 min
Response: 44519
Conc: 8.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH3050-END-2

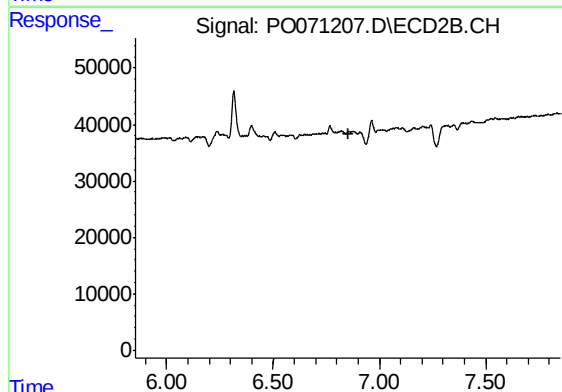


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

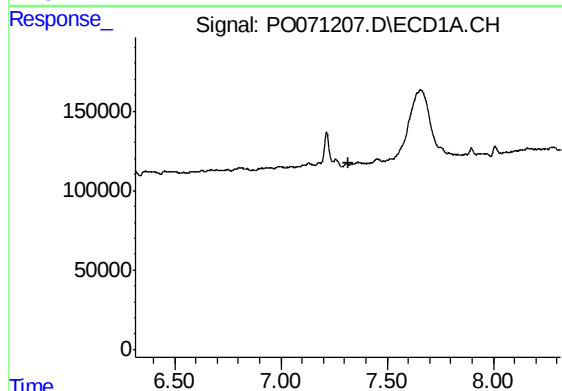


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.316 min
Response: 0
Conc: N.D.

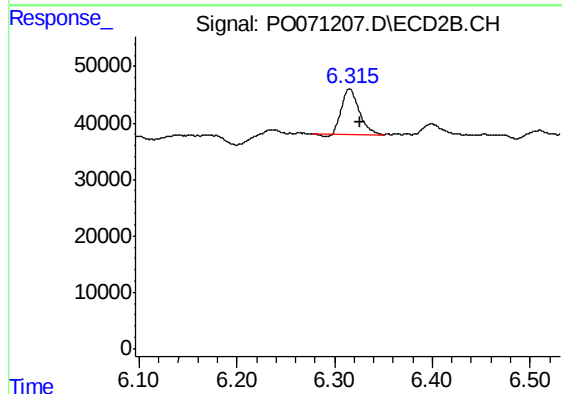

#31 AR-1260-1


R.T.: 6.315 min
Delta R.T.: -0.011 min
Response: 100146
Conc: 35.65 ng/ml

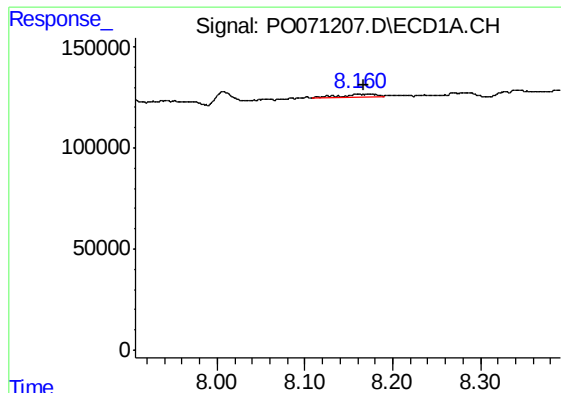

#34 AR-1260-4


R.T.: 8.161 min
Delta R.T.: -0.006 min
Response: 41804
Conc: 7.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH3050-END-2

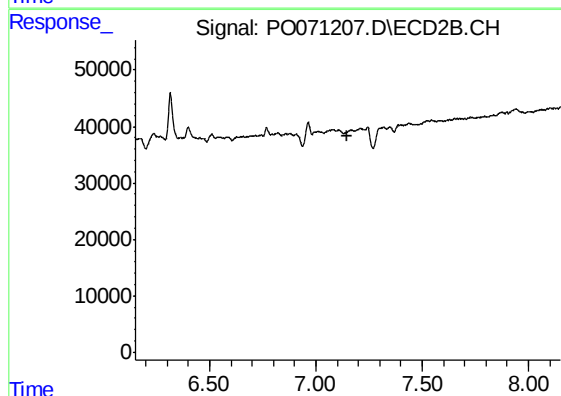


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.150 min
Response: 0
Conc: N.D.

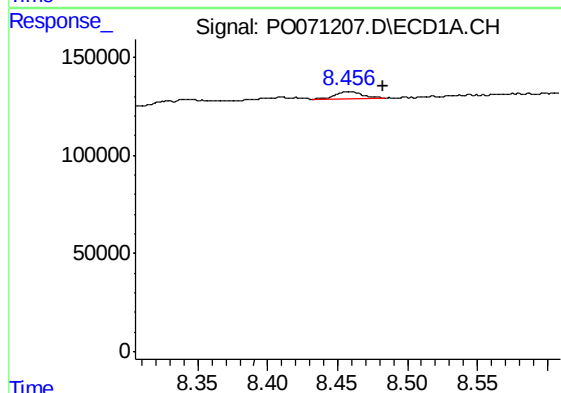


#35 AR-1260-5

R.T.: 8.458 min
Delta R.T.: -0.025 min
Response: 52938
Conc: 4.33 ng/ml

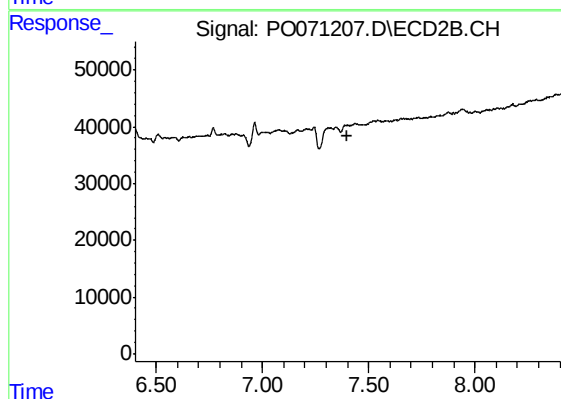

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.402 min
Response: 0
Conc: N.D.

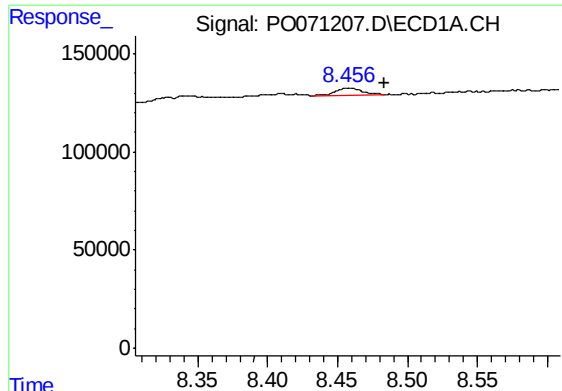

#37 AR-1262-2


R.T.: 8.458 min
Delta R.T.: -0.025 min
Response: 52938
Conc: 4.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH3050-END-2

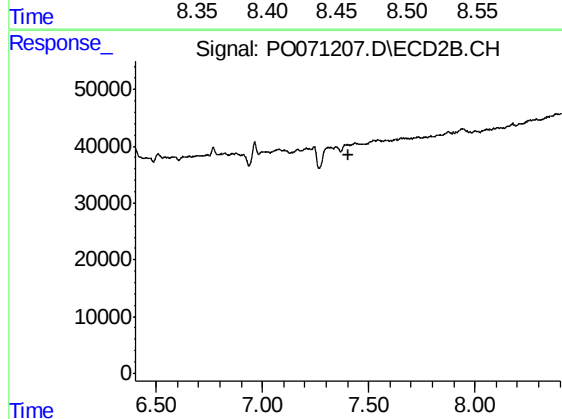


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.403 min
Response: 0
Conc: N.D.

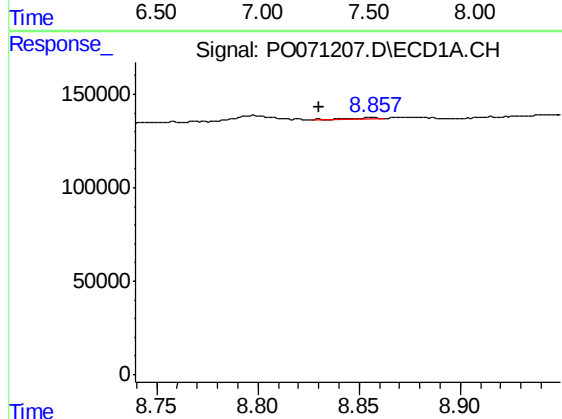


#39 AR-1262-4

R.T.: 8.856 min
Delta R.T.: 0.026 min
Response: 8988
Conc: 2.74 ng/ml

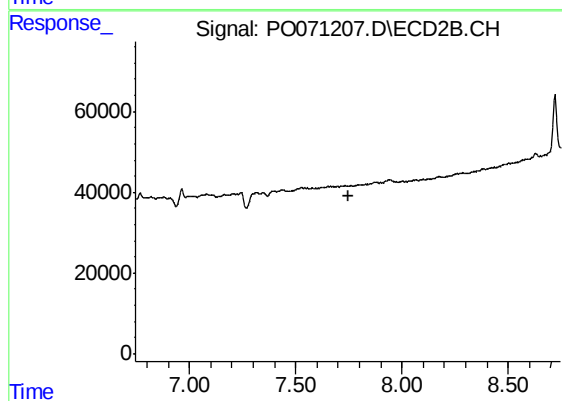

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.746 min
Response: 0
Conc: N.D.

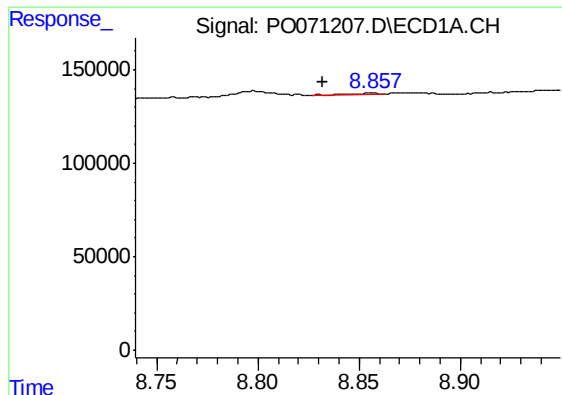

#42 AR-1268-2

R.T.: 8.856 min
Delta R.T.: 0.024 min
Response: 8988
Conc: 0.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH3050-END-2

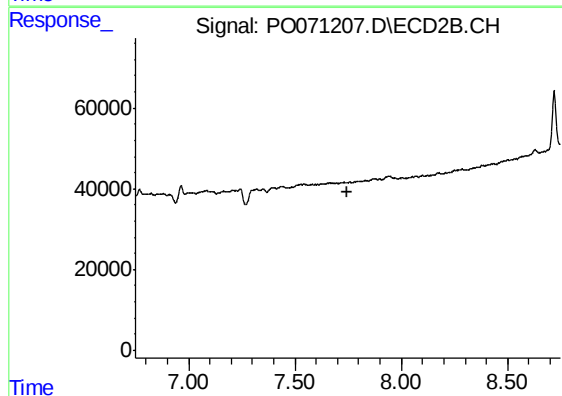

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.749 min
Response: 0
Conc: N.D.