

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
 Data File : P0071170.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2020 10:36
 Operator : DD\AJ
 Sample : L3877-17DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4DL

Manual Integrations
 APPROVED

Ankita
 9/8/2020 2:40:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 14:41:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.536	1396912	608919	18.088m	13.736
2) SA Decachlor...	9.967	8.717	1080467	559759	11.808	9.745
Target Compounds						
16) L4 AR-1242-1	5.653	4.760	1633676	912863	688.003	632.385
17) L4 AR-1242-2	5.675	4.778	2421599	1174994	708.373	582.282
18) L4 AR-1242-3	5.738	4.962	1132766	577983	556.410	533.419
19) L4 AR-1242-4	5.844	5.061	1135605	573518	651.763	585.838
20) L4 AR-1242-5	6.617	5.615	1429845	615411	690.652	466.269 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090420\
Data File : PO071170.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2020 10:36
Operator : DD\AJ
Sample : L3877-17DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-4DL


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 14:41:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

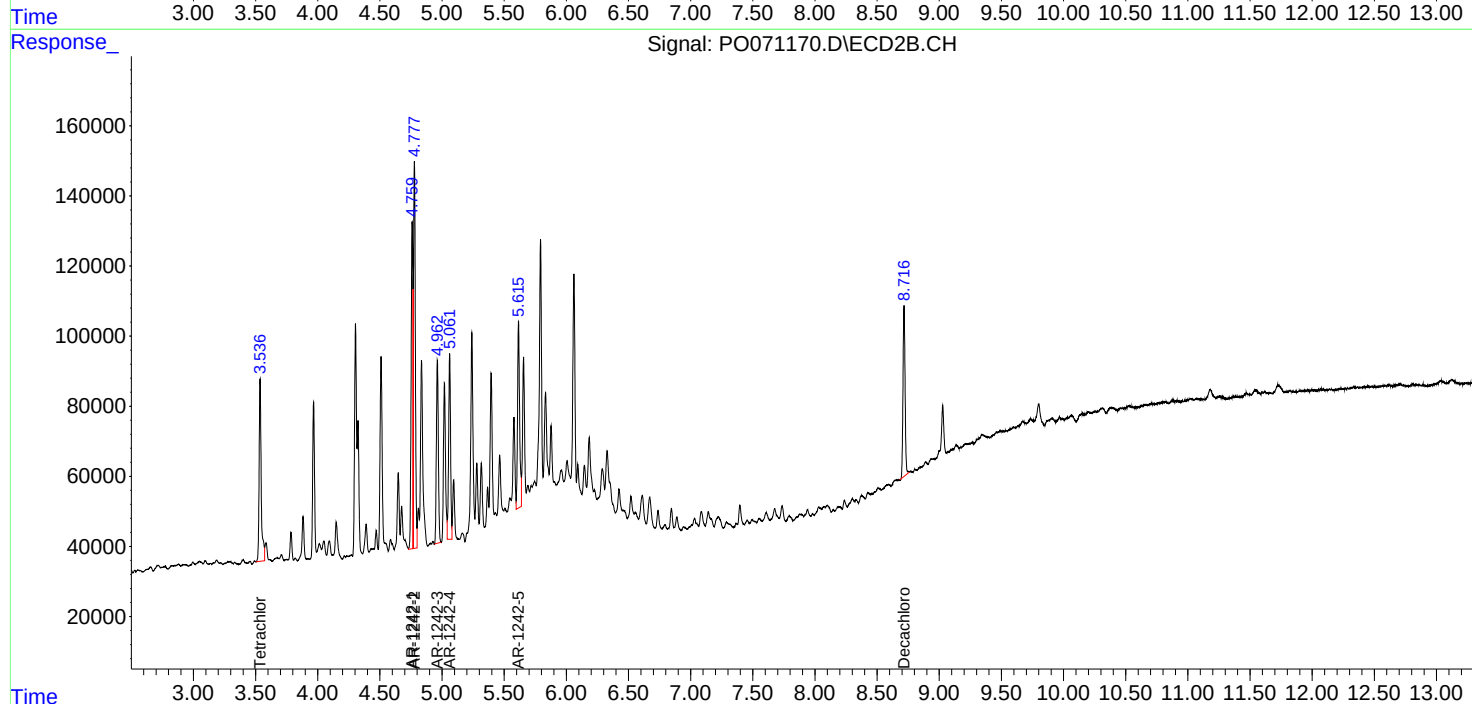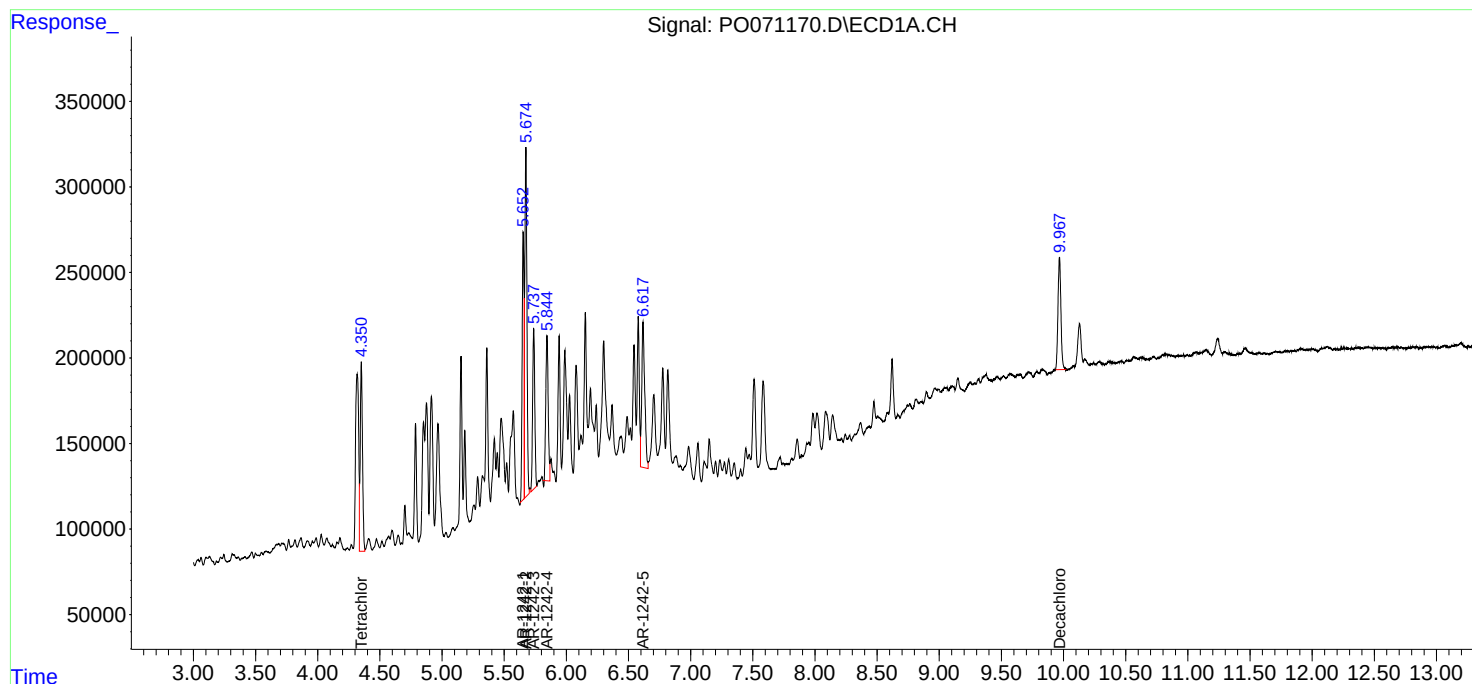

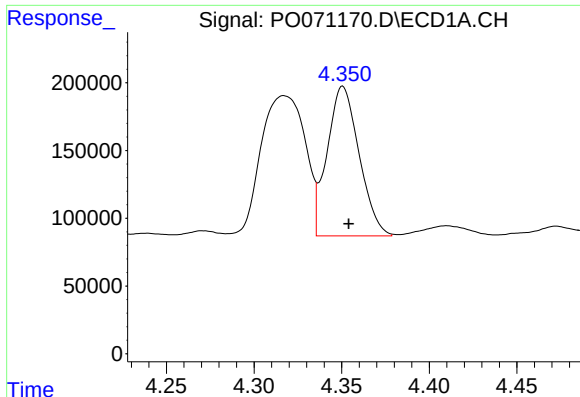


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: -0.004 min
Response: 1396912
Conc: 18.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-4DL


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:40 PM

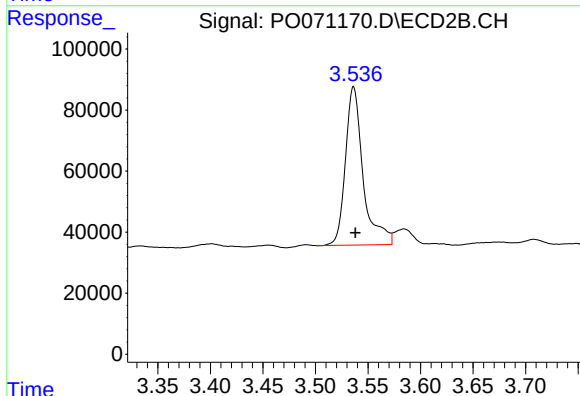


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 608919
Conc: 13.74 ng/ml

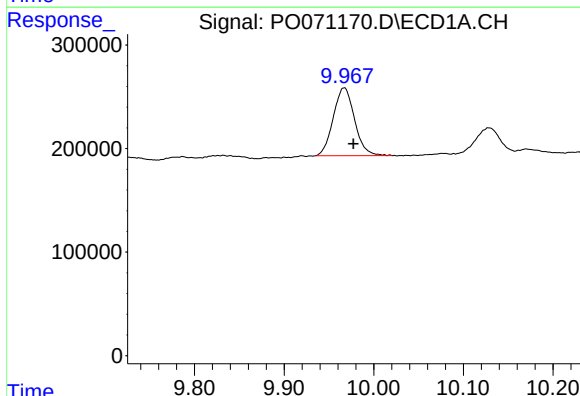


#2 Decachlorobiphenyl

R.T.: 9.967 min
Delta R.T.: -0.010 min
Response: 1080467
Conc: 11.81 ng/ml

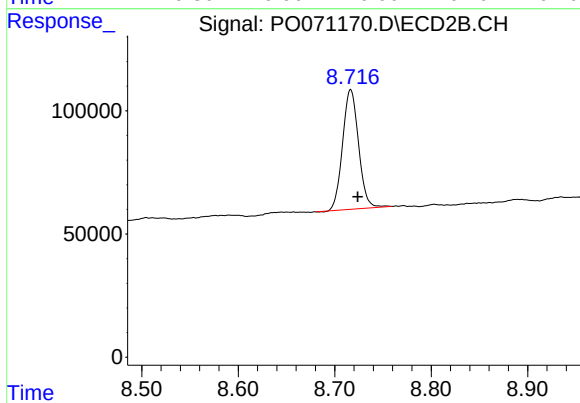

#2 Decachlorobiphenyl

R.T.: 8.717 min
Delta R.T.: -0.007 min
Response: 559759
Conc: 9.75 ng/ml

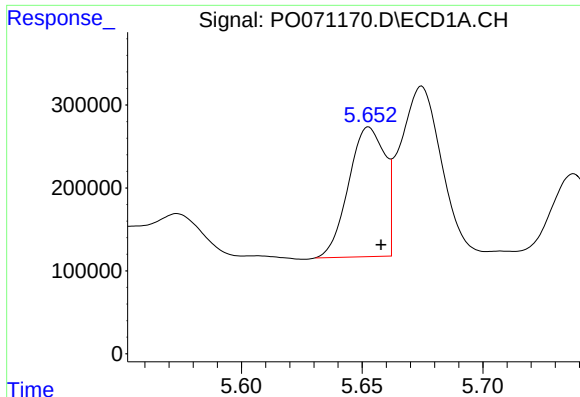


#16 AR-1242-1

R.T.: 5.653 min
Delta R.T.: -0.005 min
Response: 1633676
Conc: 688.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4DL


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:40 PM

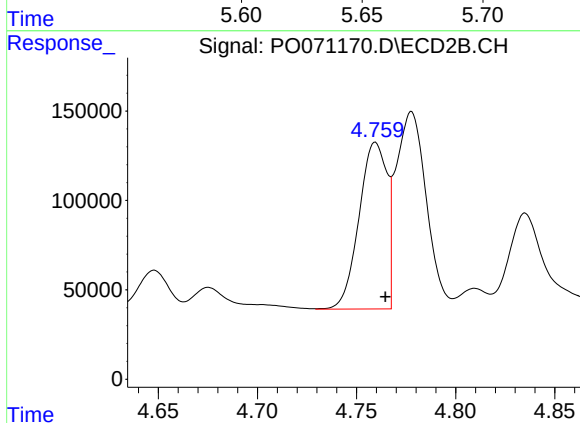


#16 AR-1242-1

R.T.: 4.760 min
Delta R.T.: -0.005 min
Response: 912863
Conc: 632.38 ng/ml

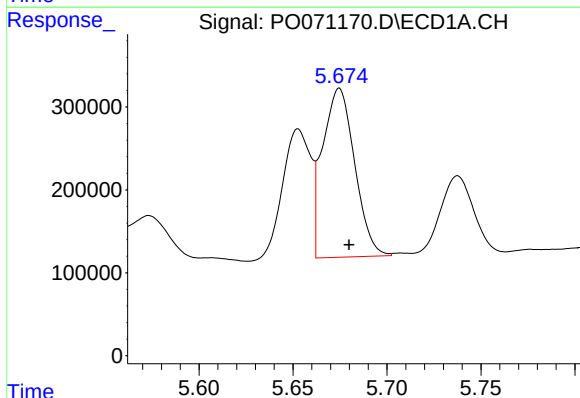


#17 AR-1242-2

R.T.: 5.675 min
Delta R.T.: -0.005 min
Response: 2421599
Conc: 708.37 ng/ml

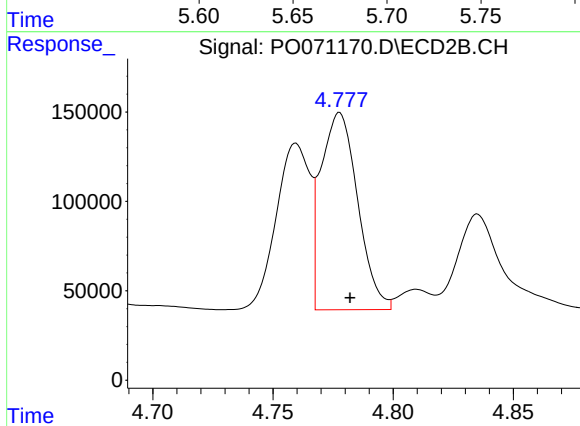

#17 AR-1242-2

R.T.: 4.778 min
Delta R.T.: -0.004 min
Response: 1174994
Conc: 582.28 ng/ml

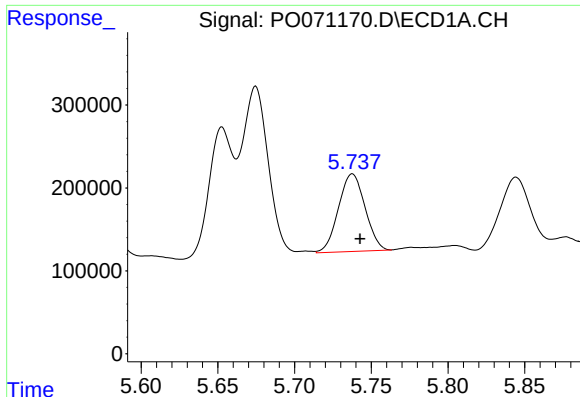


#18 AR-1242-3

R.T.: 5.738 min
Delta R.T.: -0.005 min
Response: 1132766
Conc: 556.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4DL


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:40 PM

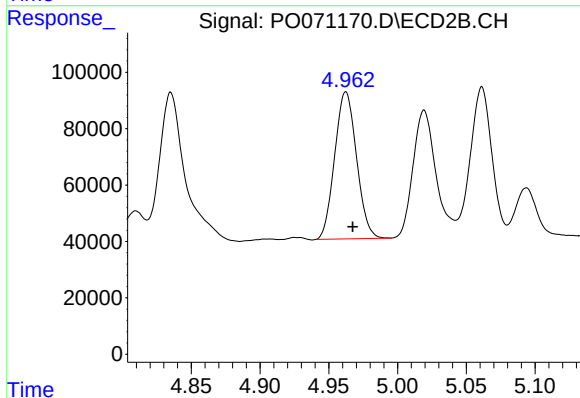


#18 AR-1242-3

R.T.: 4.962 min
Delta R.T.: -0.005 min
Response: 577983
Conc: 533.42 ng/ml

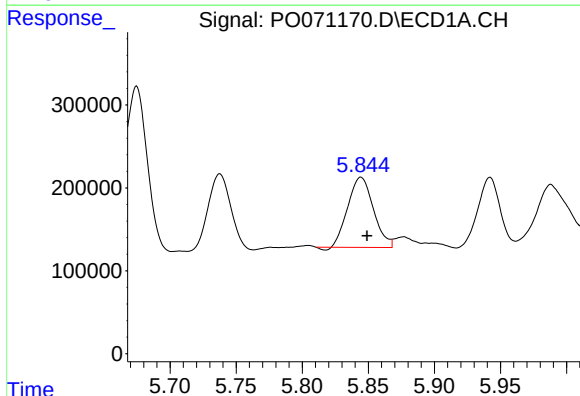


#19 AR-1242-4

R.T.: 5.844 min
Delta R.T.: -0.005 min
Response: 1135605
Conc: 651.76 ng/ml

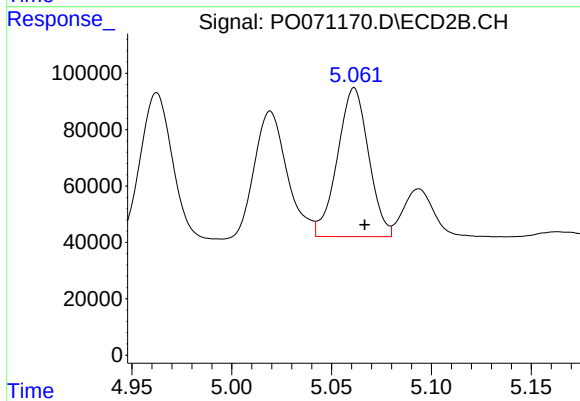

#19 AR-1242-4

R.T.: 5.061 min
Delta R.T.: -0.005 min
Response: 573518
Conc: 585.84 ng/ml

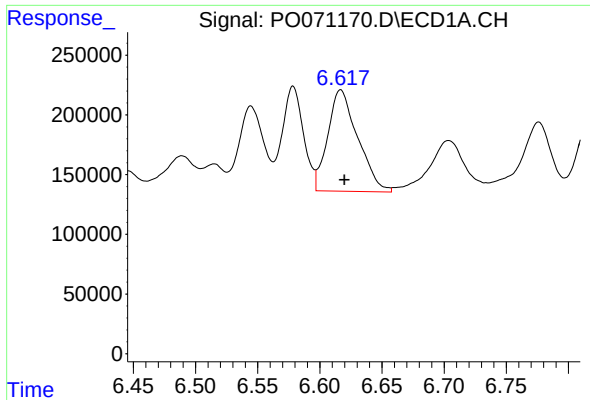


#20 AR-1242-5

R.T.: 6.617 min
Delta R.T.: -0.003 min
Response: 1429845
Conc: 690.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4DL

Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:40 PM

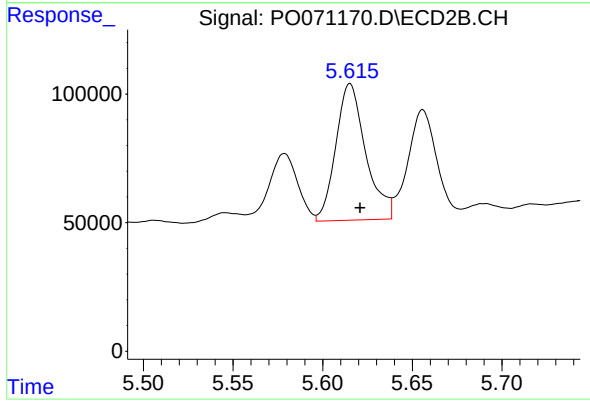

#20 AR-1242-5

R.T.: 5.615 min
Delta R.T.: -0.006 min
Response: 615411
Conc: 466.27 ng/ml