

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
 Data File : P0071176.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2020 12:27
 Operator : DD\AJ
 Sample : L3886-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-31230

Manual Integrations
 APPROVED

Ankita
 9/8/2020 2:40:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 14:43:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.538	1532863	1158541	19.849	26.134 #
2) SA Decachlor...	9.996f	8.738	2707937	1540121	29.594	26.814m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090420\
Data File : PO071176.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2020 12:27
Operator : DD\AJ
Sample : L3886-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-31230


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 14:43:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

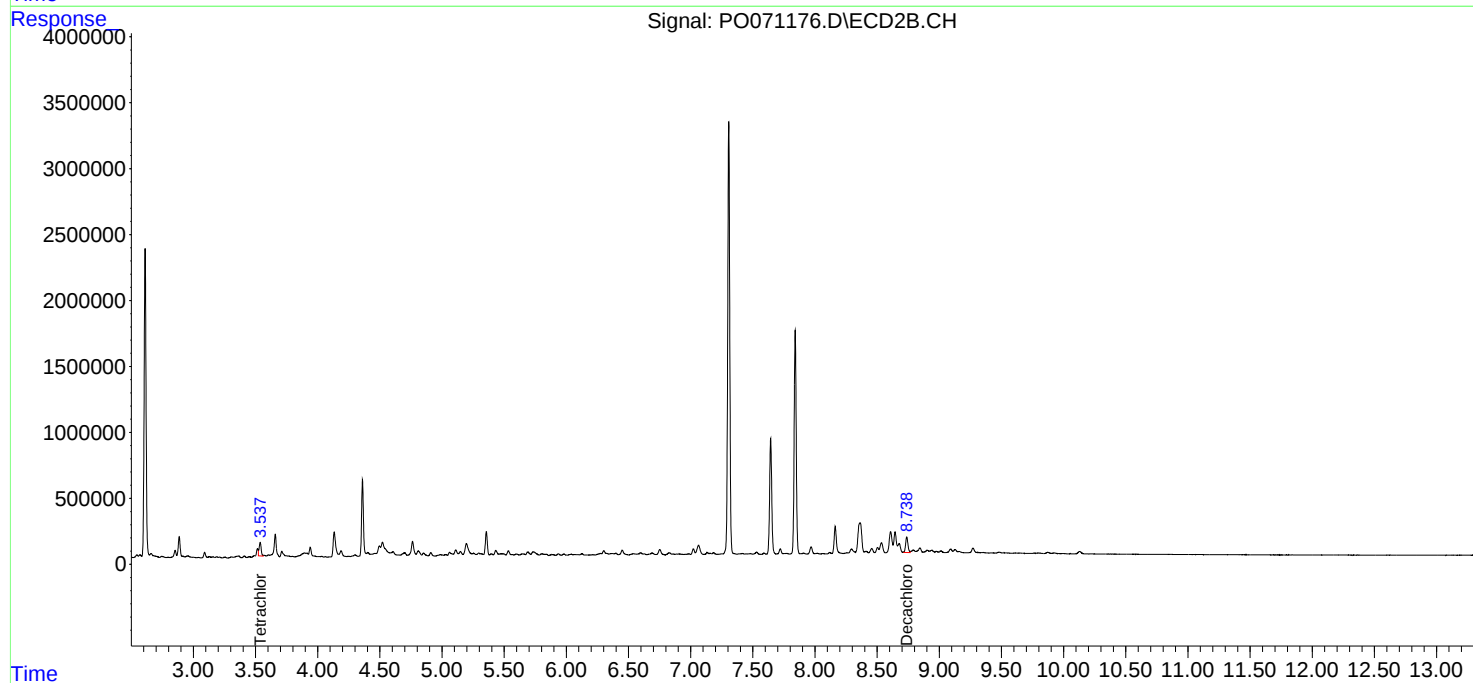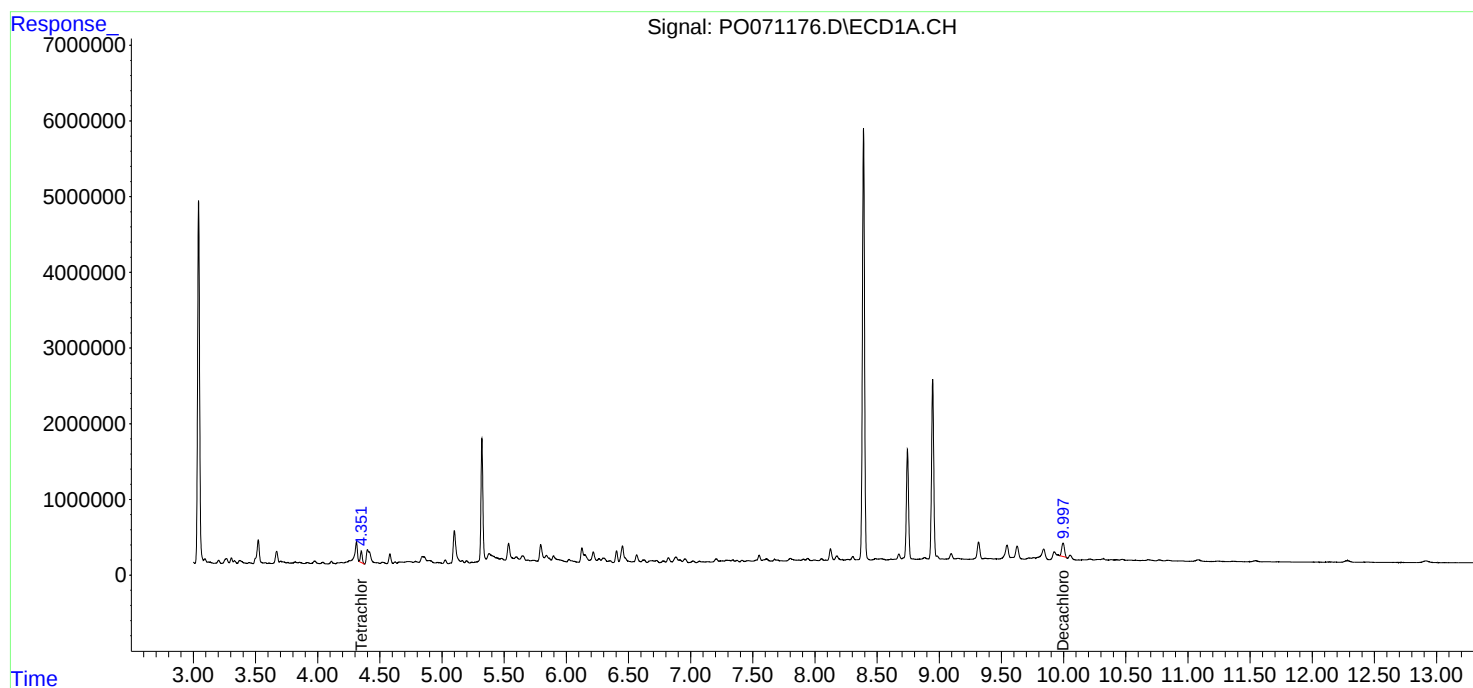

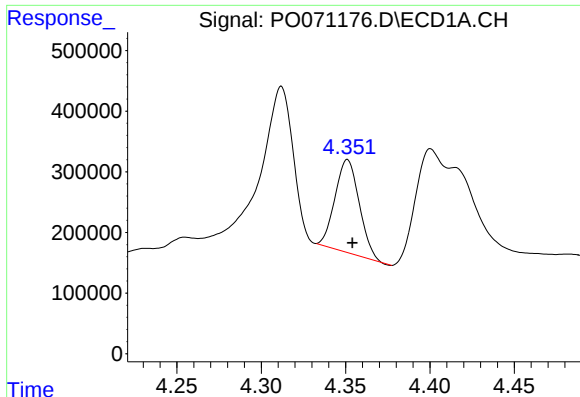


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.003 min
Response: 1532863
Conc: 19.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-31230


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:42 PM

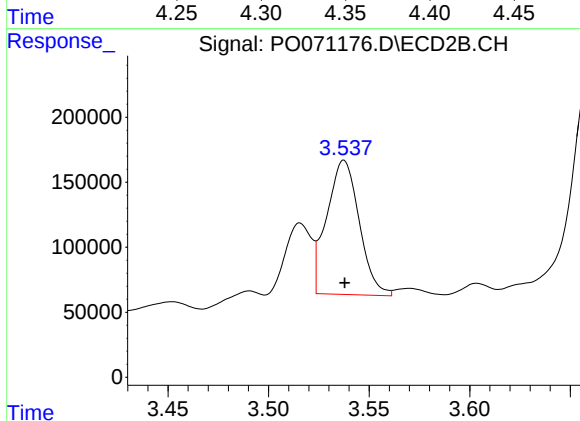


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 1158541
Conc: 26.13 ng/ml

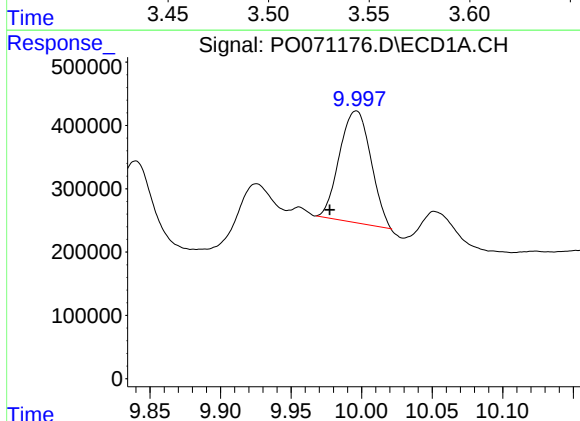

#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: 0.019 min
Response: 2707937
Conc: 29.59 ng/ml

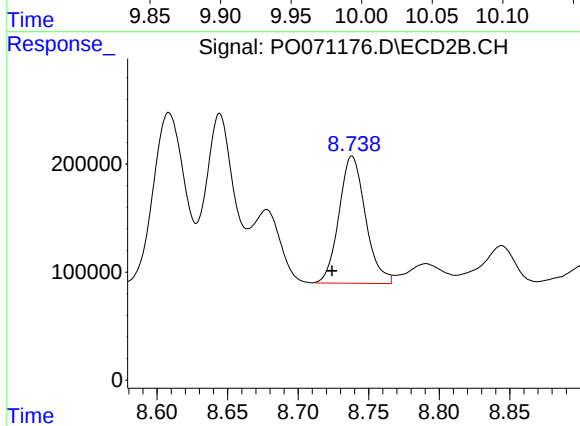

#2 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: 0.014 min
Response: 1540121
Conc: 26.81 ng/ml m