

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
 Data File : P0071186.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2020 15:18
 Operator : DD\AJ
 Sample : L3895-10RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-25A-(8.5-9)RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 18:08:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.537	1748141	925779	22.636	20.883
2) SA Decachlor...	9.970	8.718	1005941	602954	10.993	10.497

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
Data File : P0071186.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2020 15:18
Operator : DD\AJ
Sample : L3895-10RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-25A-(8.5-9)RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 18:08:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

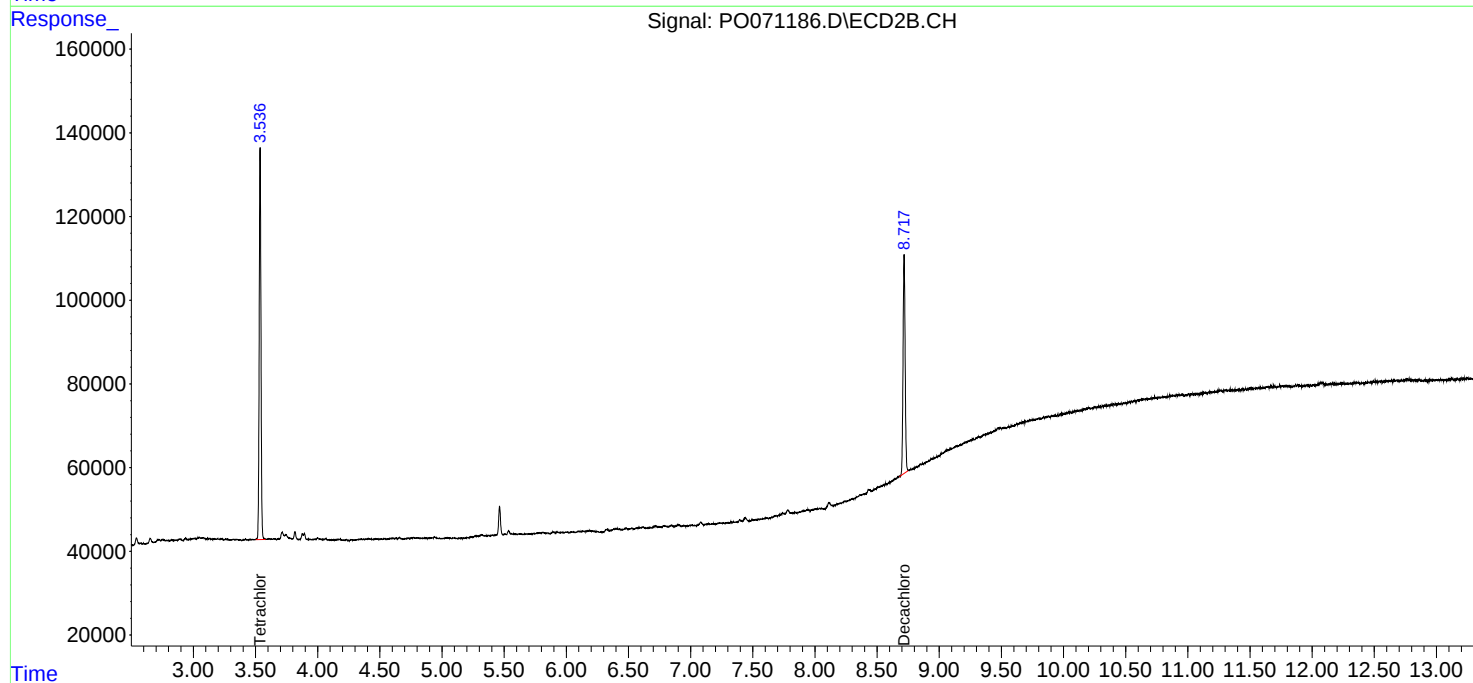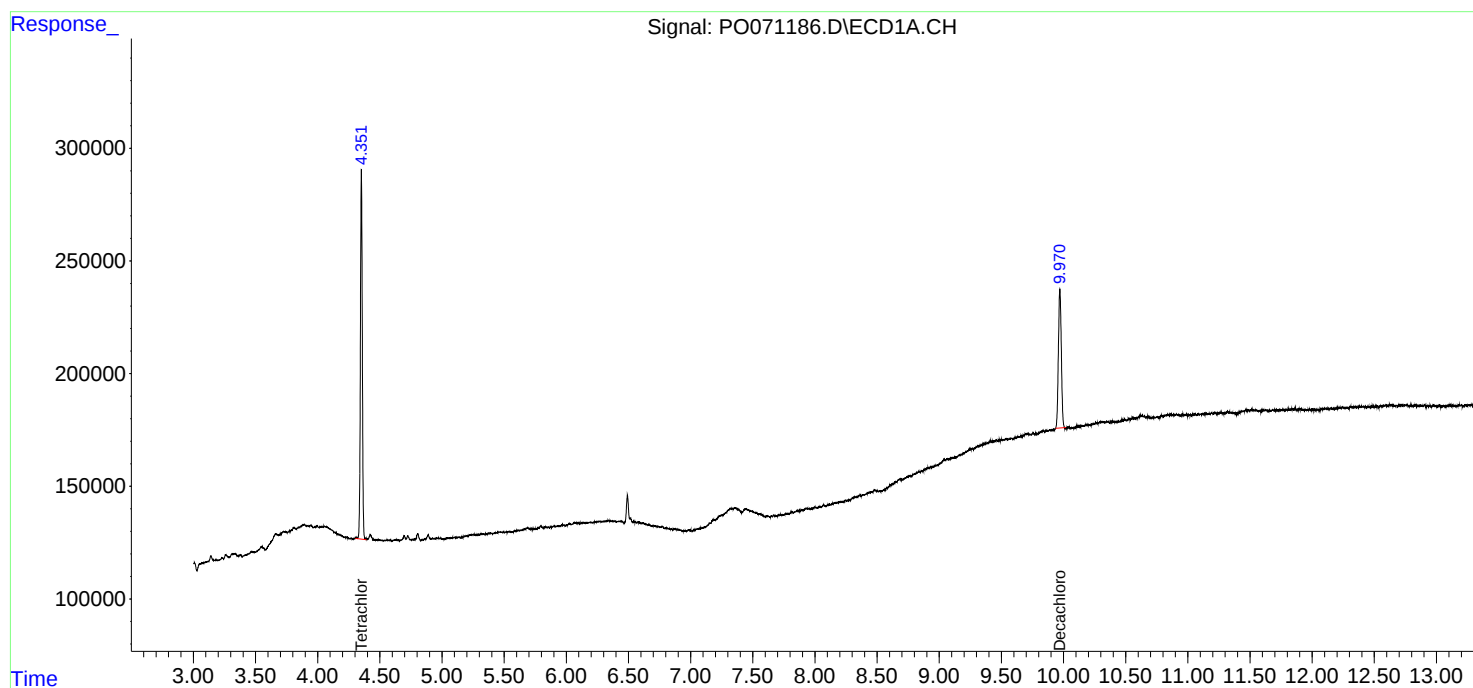


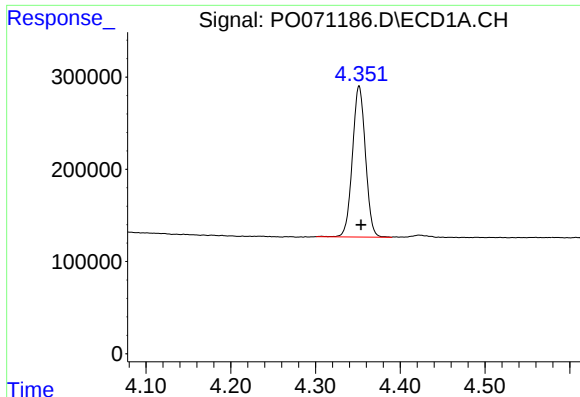

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: -0.002 min
Response: 1748141
Conc: 22.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-25A-(8.5-9)RE

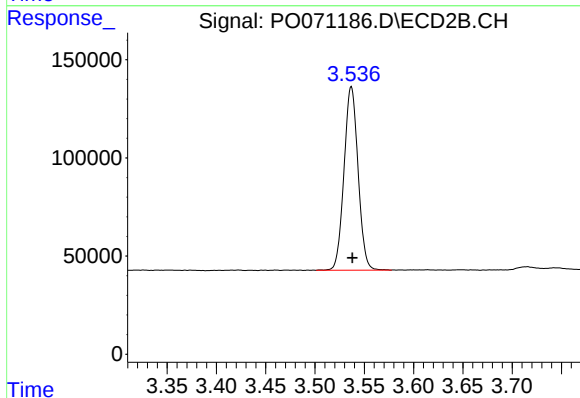


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.001 min
Response: 925779
Conc: 20.88 ng/ml

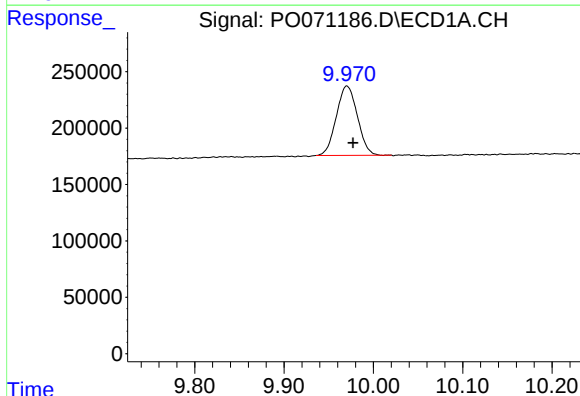

#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.007 min
Response: 1005941
Conc: 10.99 ng/ml

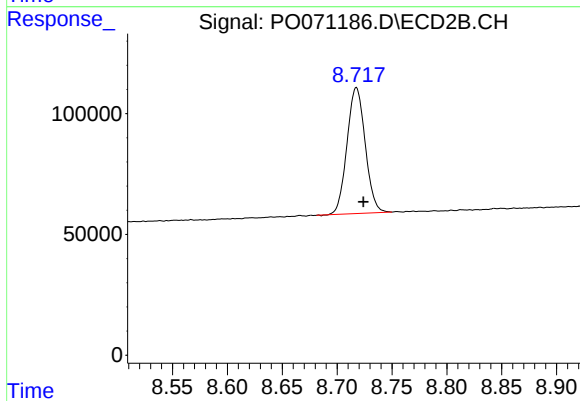

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: -0.006 min
Response: 602954
Conc: 10.50 ng/ml