

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
 Data File : P0071200.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2020 19:35
 Operator : DD\AJ
 Sample : L3886-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-31231

Manual Integrations
 APPROVED

Ankita
 9/8/2020 2:40:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:02:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330f	3.542	4597747	2733054	59.535	61.651
2) SA Decachlor...	9.996f	8.732	2152543	704177	23.524	12.260m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090420\
Data File : PO071200.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2020 19:35
Operator : DD\AJ
Sample : L3886-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-31231


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:02:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

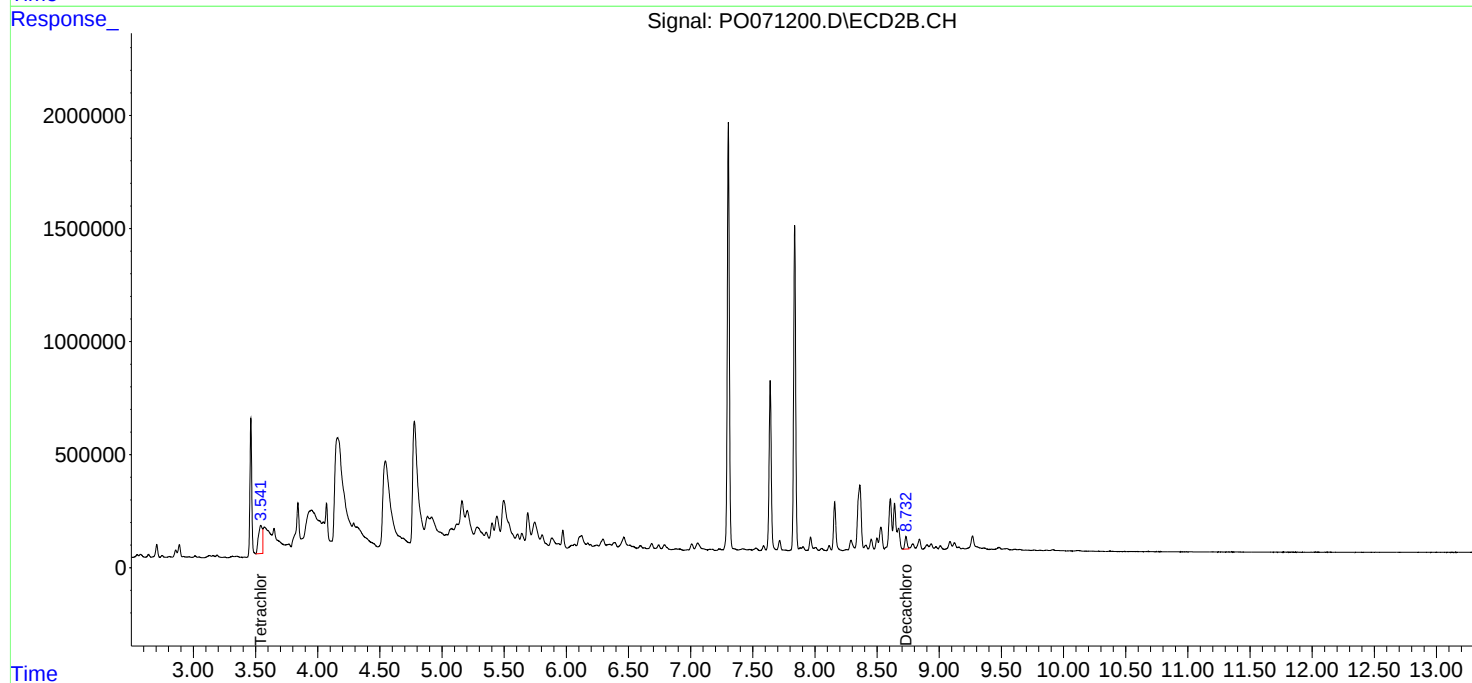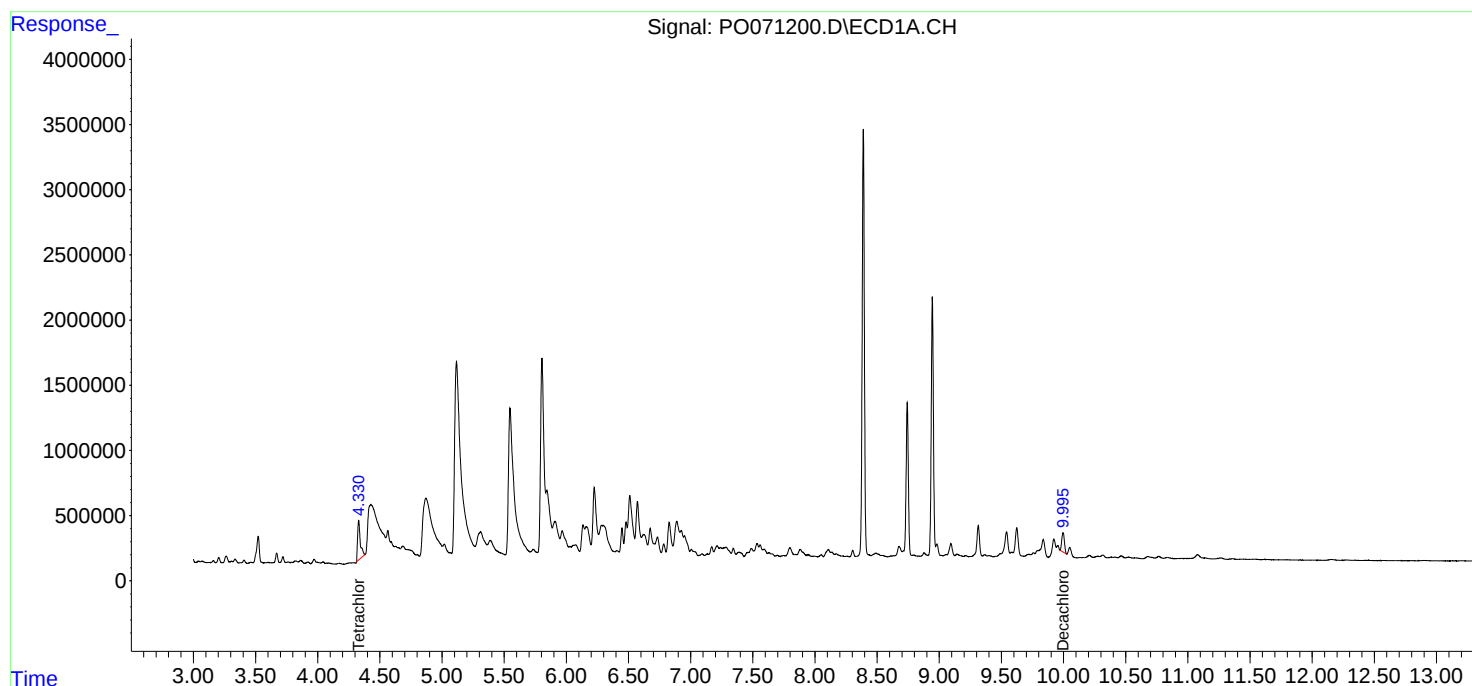

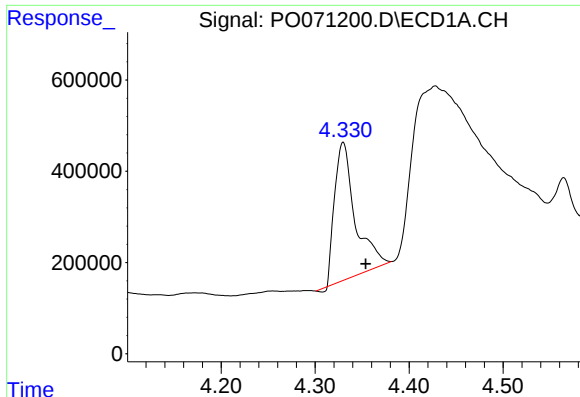


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: -0.024 min
Response: 4597747
Conc: 59.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-31231


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:49 PM

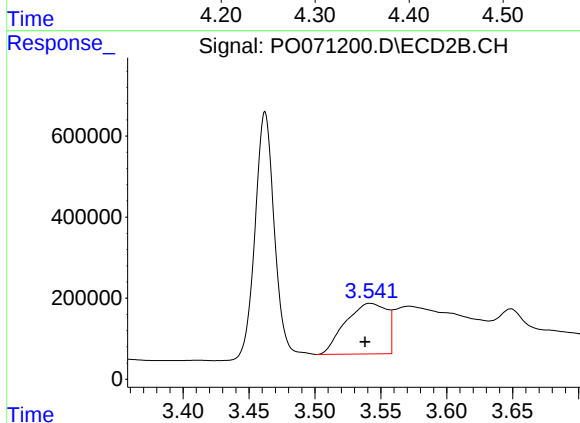


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.004 min
Response: 2733054
Conc: 61.65 ng/ml

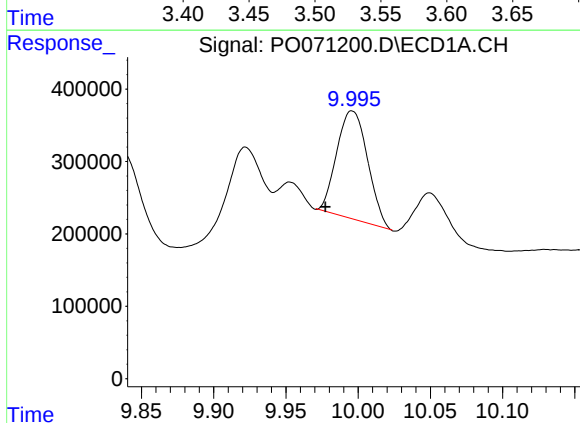

#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: 0.018 min
Response: 2152543
Conc: 23.52 ng/ml

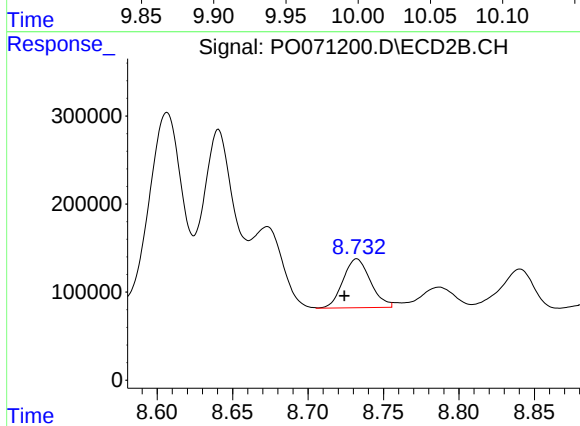

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: 0.008 min
Response: 704177
Conc: 12.26 ng/ml m