

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
 Data File : P0071201.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Sep 2020 19:52
 Operator : DD\AJ
 Sample : L3912-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LS-1-B-2-ELEVATOR-SHAFT

Manual Integrations
 APPROVED

Ankita
 9/8/2020 2:40:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:03:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.539	1172647	885029	15.184	19.964 #
2) SA Decachlor...	9.988	8.739	1328360	642986	14.517m	11.194

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090420\
Data File : P0071201.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Sep 2020 19:52
Operator : DD\AJ
Sample : L3912-02
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LS-1-B-2-ELEVATOR-SHAFT


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:03:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

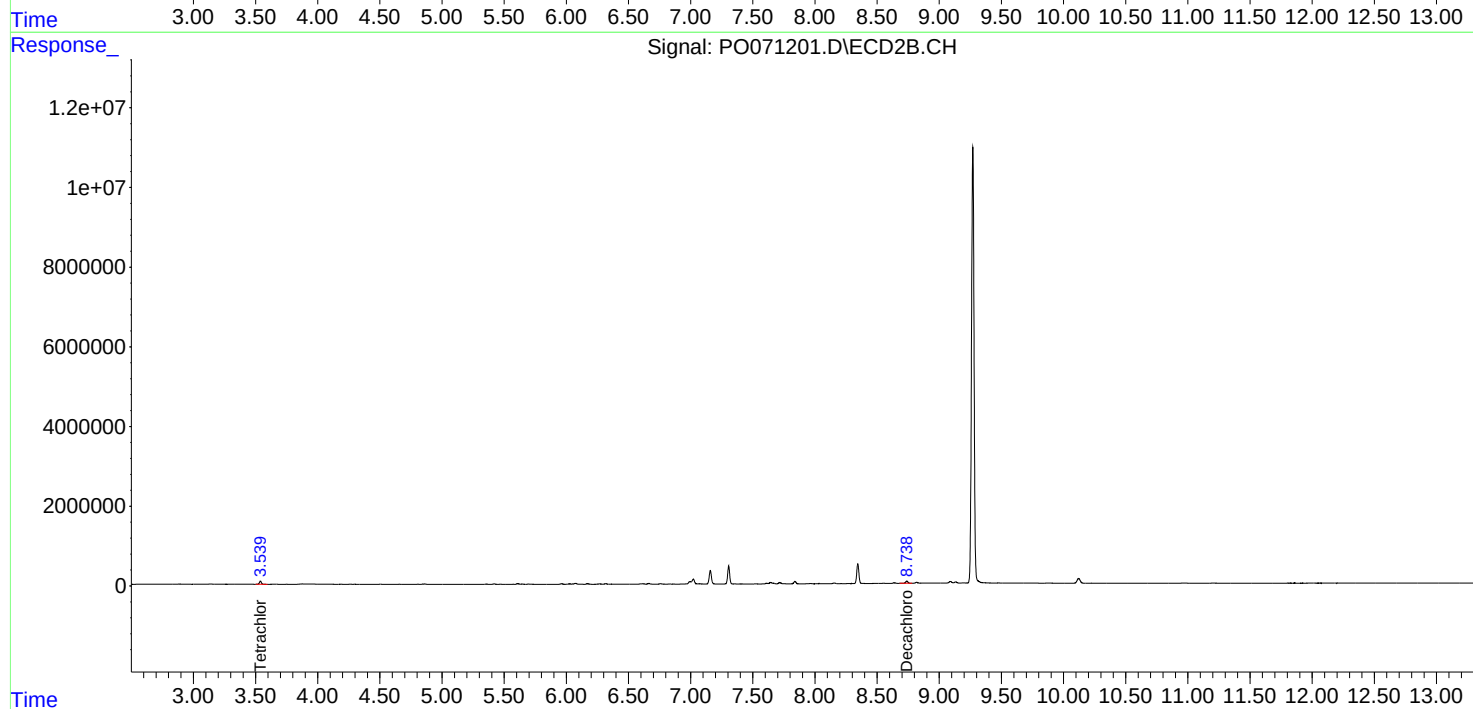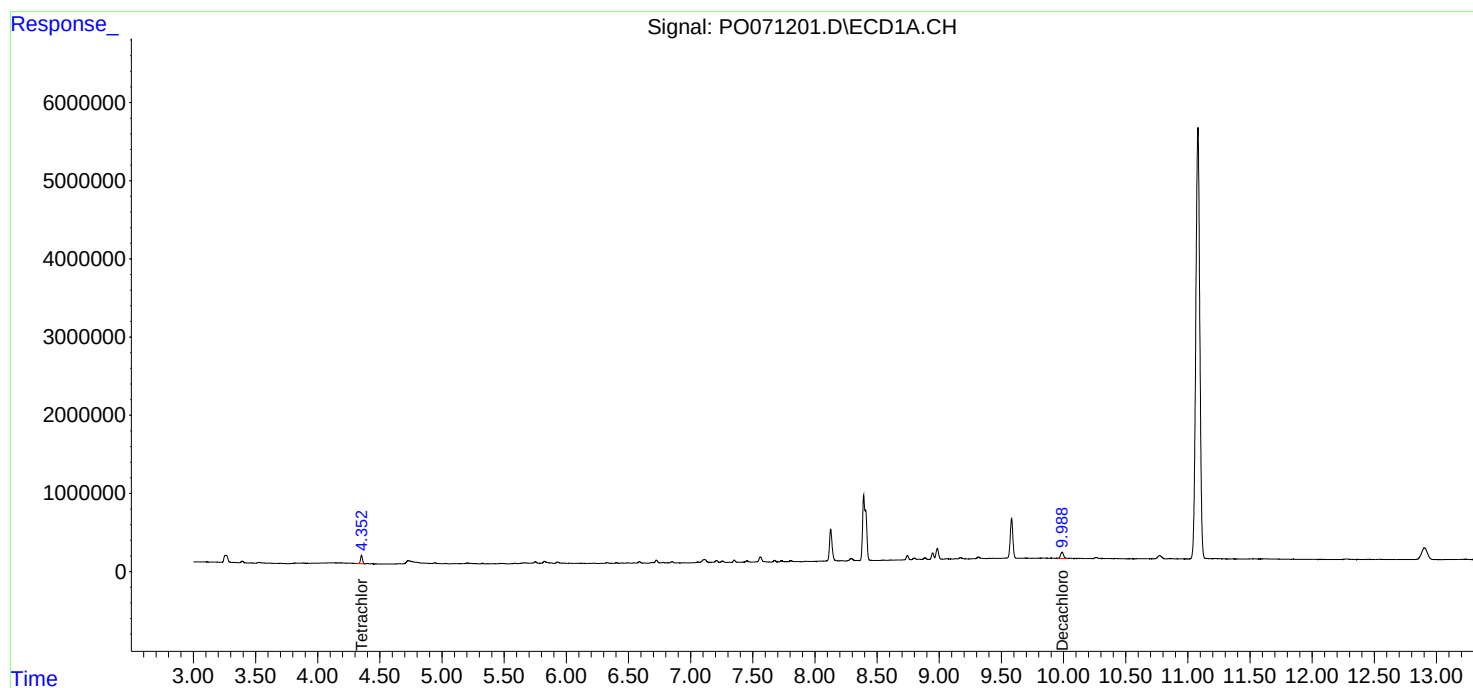

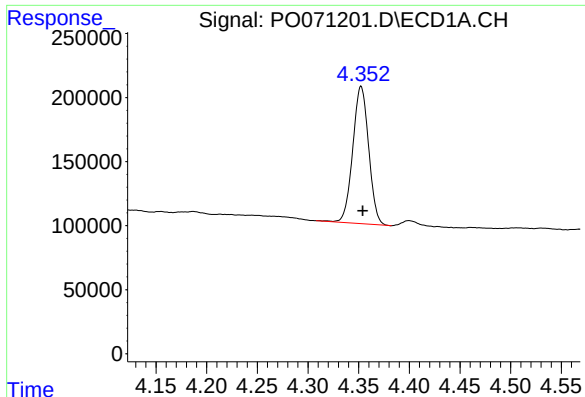


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.002 min
Response: 1172647
Conc: 15.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LS-1-B-2-ELEVATOR-SHAFT


Manual Integrations
APPROVED

Ankita
9/8/2020 2:40:51 PM

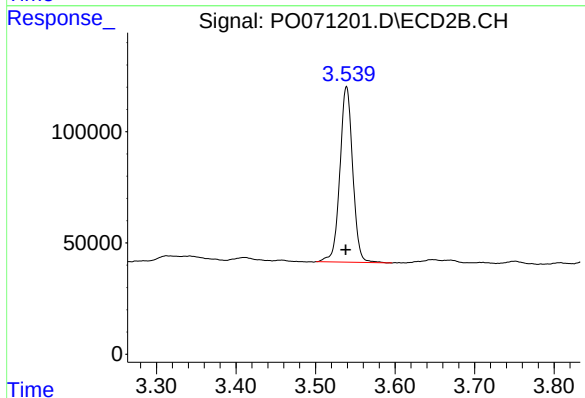


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.001 min
Response: 885029
Conc: 19.96 ng/ml

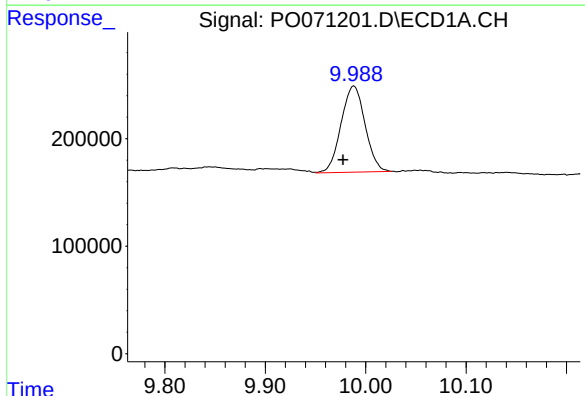

#2 Decachlorobiphenyl

R.T.: 9.988 min
Delta R.T.: 0.010 min
Response: 1328360
Conc: 14.52 ng/ml m

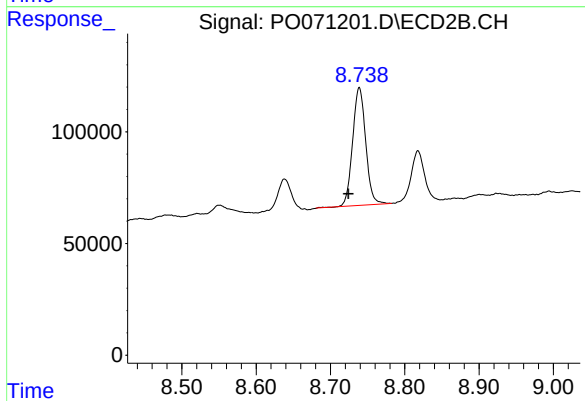

#2 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: 0.015 min
Response: 642986
Conc: 11.19 ng/ml