

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090425\
 Data File : P0113473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 16:28
 Operator : YP/AJ
 Sample : Q3004-02 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Drum Speedy Dry/RAGS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/05/2025
 Supervised By :mohammad ahmed 09/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:33:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.657	3.651	7340812	4926716	0.897m	0.974m
2) SA Decachlor...	8.673	8.620	11350613	3777333	1.638m	1.993

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090425\
Data File : PO113473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 16:28
Operator : YP/AJ
Sample : Q3004-02 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Drum Speedy Dry/RAGS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2025
Supervised By :mohammad ahmed 09/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:33:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

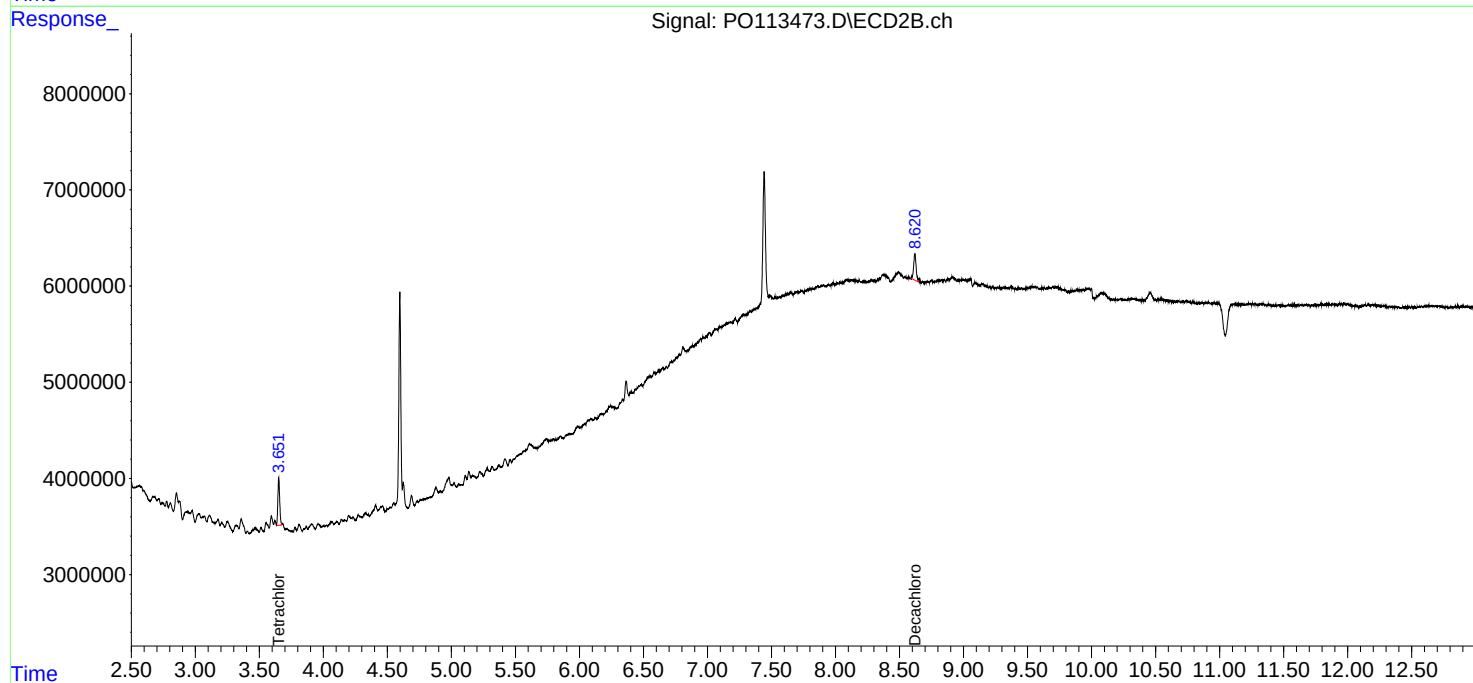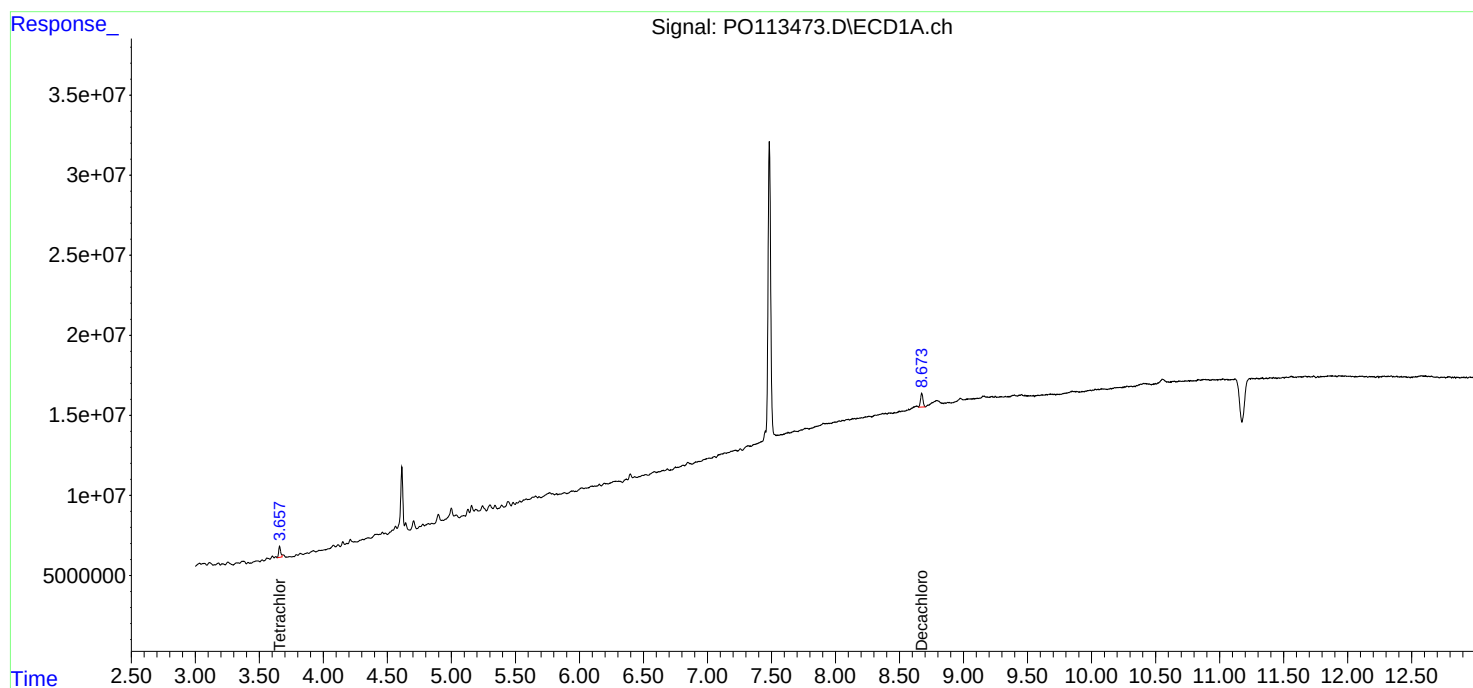

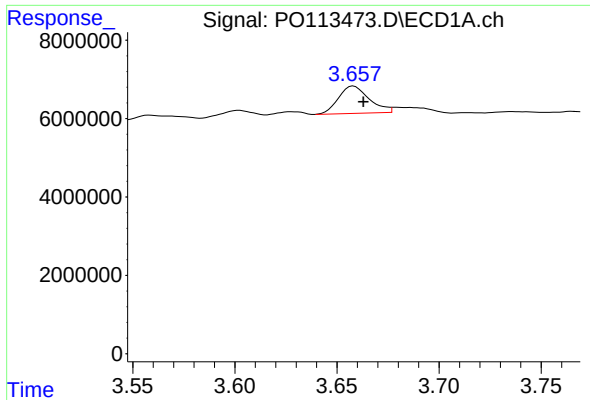


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: -0.006 min
Response: 7340812
Conc: 0.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
Drum Speedy Dry/RAGS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2025
Supervised By :mohammad ahmed 09/08/2025

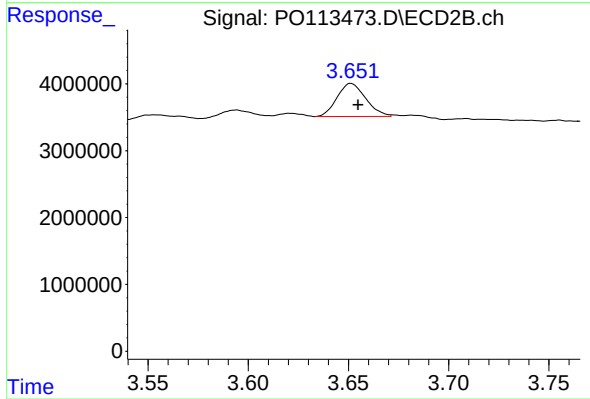


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.004 min
Response: 4926716
Conc: 0.97 ng/ml m

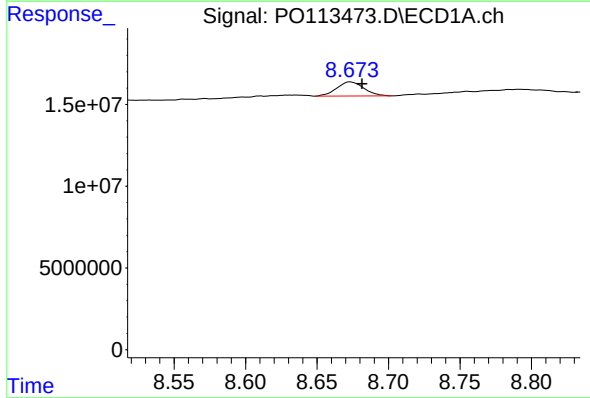

#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: -0.009 min
Response: 11350613
Conc: 1.64 ng/ml m

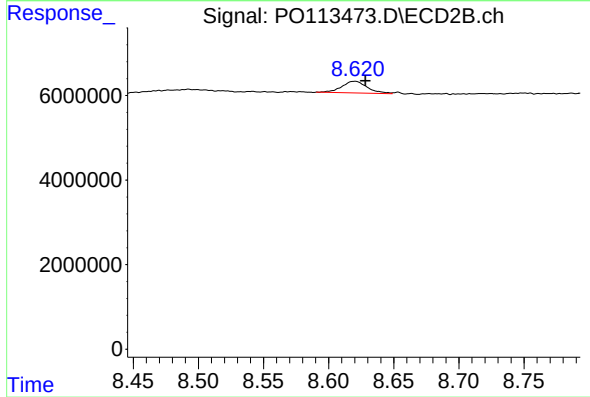

#2 Decachlorobiphenyl

R.T.: 8.620 min
Delta R.T.: -0.008 min
Response: 3777333
Conc: 1.99 ng/ml