

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090425\
 Data File : P0113474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 16:45
 Operator : YP/AJ
 Sample : Q3009-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-090325

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/05/2025
 Supervised By :mohammad ahmed 09/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:33:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.651	96639448	62782058	11.805m	12.406m
2) SA Decachlor...	8.675	8.620	86958136	26936924	12.545	14.216

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090425\
Data File : PO113474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 16:45
Operator : YP/AJ
Sample : Q3009-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-090325


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2025
Supervised By :mohammad ahmed 09/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:33:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

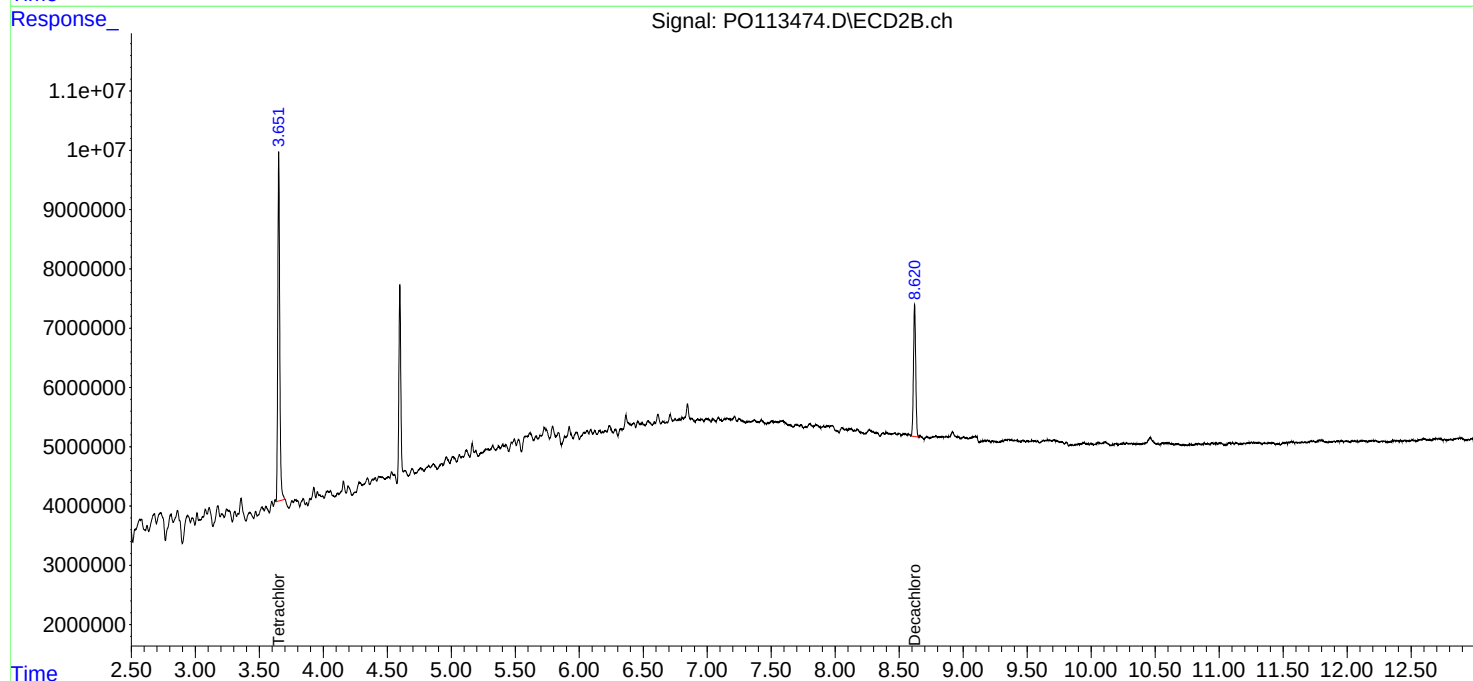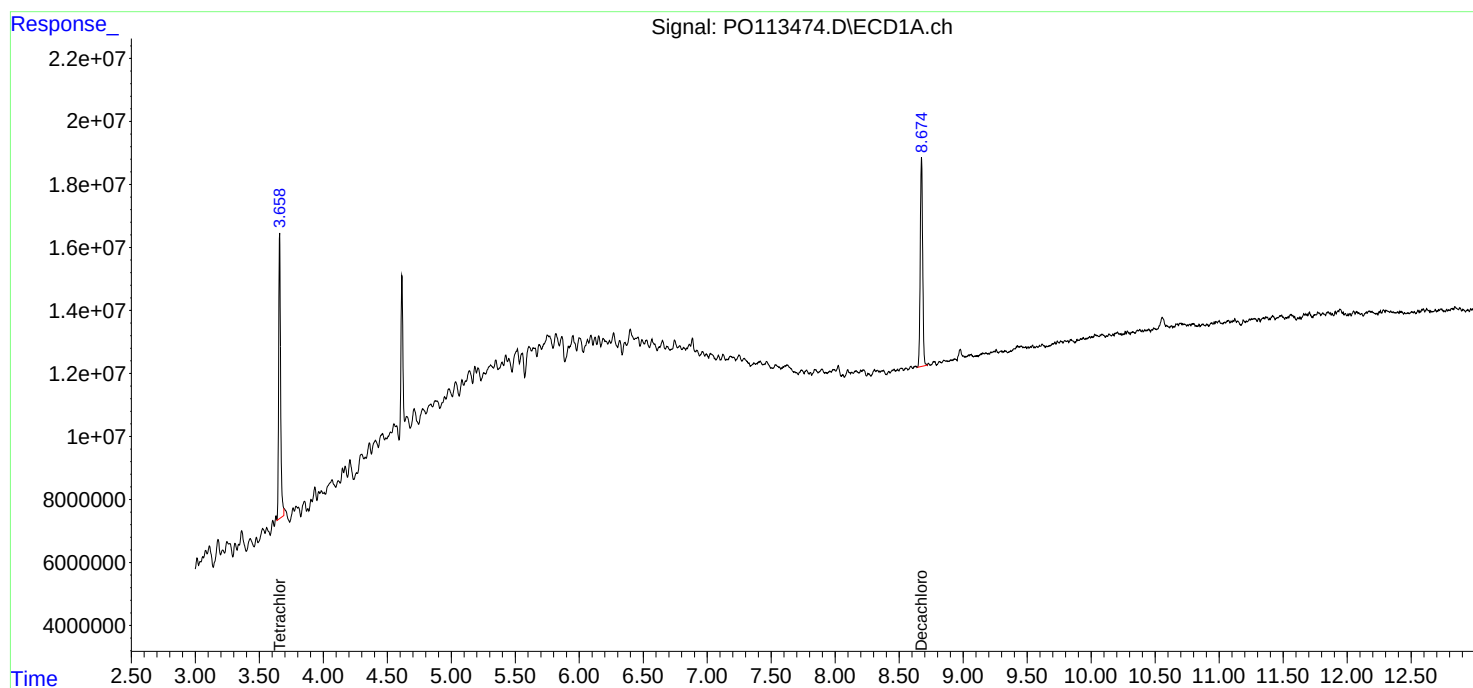

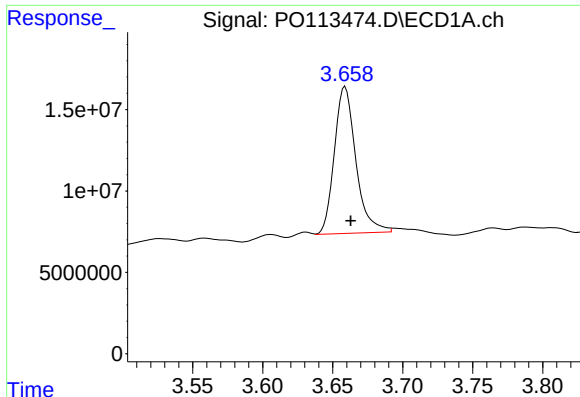


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 96639448
Conc: 11.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-090325


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2025
Supervised By :mohammad ahmed 09/08/2025

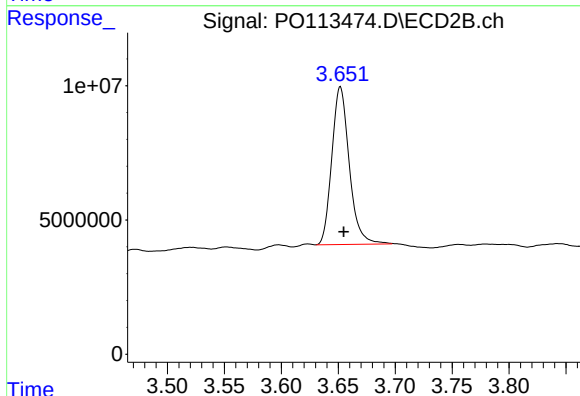


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.003 min
Response: 62782058
Conc: 12.41 ng/ml m

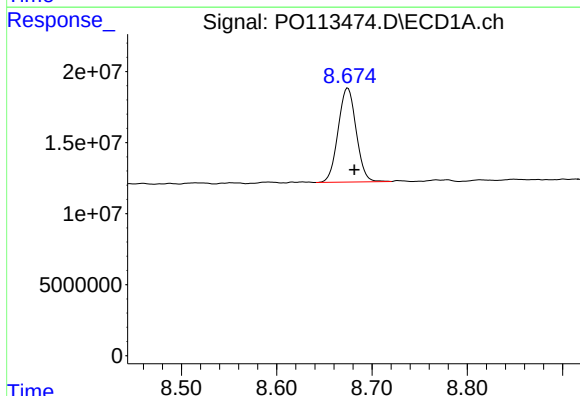

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: -0.007 min
Response: 86958136
Conc: 12.55 ng/ml

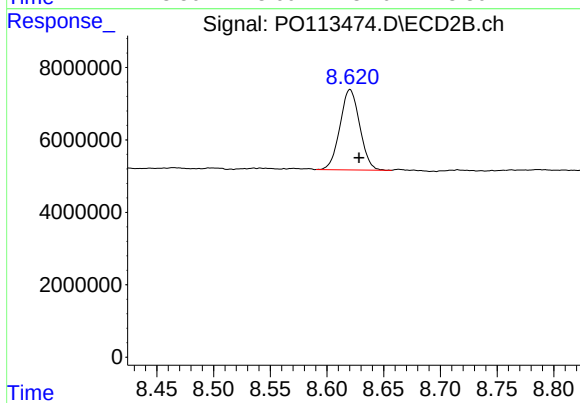

#2 Decachlorobiphenyl

R.T.: 8.620 min
Delta R.T.: -0.008 min
Response: 26936924
Conc: 14.22 ng/ml