

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090518\
 Data File : P0048762.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2018 18:38
 Operator : SM/SJ
 Sample : J4720-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BZTRANS-3

Manual Integrations
 APPROVED

Sohil
 9/6/2018 2:21:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 02:18:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 05 03:48:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.529	5500087	6147895	45.584	39.333
2) SA Decachlor...	10.191	8.468	2768825	3099291	19.844	20.962
Target Compounds						
31) L7 AR-1260-1	7.223	6.065	1308935	1347242	158.873	129.415m
32) L7 AR-1260-2	7.480	6.250	2443764	1938381	248.690	154.790m#
33) L7 AR-1260-3	7.763	6.405	2026599	1189705	169.844	100.276 #
34) L7 AR-1260-4	8.062	6.872	1214179	893381	141.464	94.427 #
35) L7 AR-1260-5	8.384	7.112	1092806	1561531	65.825	71.911

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090518\
Data File : PO048762.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2018 18:38
Operator : SM/SJ
Sample : J4720-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BZTRANS-3


Manual Integrations
APPROVED

Sohil
9/6/2018 2:21:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 02:18:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 05 03:48:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

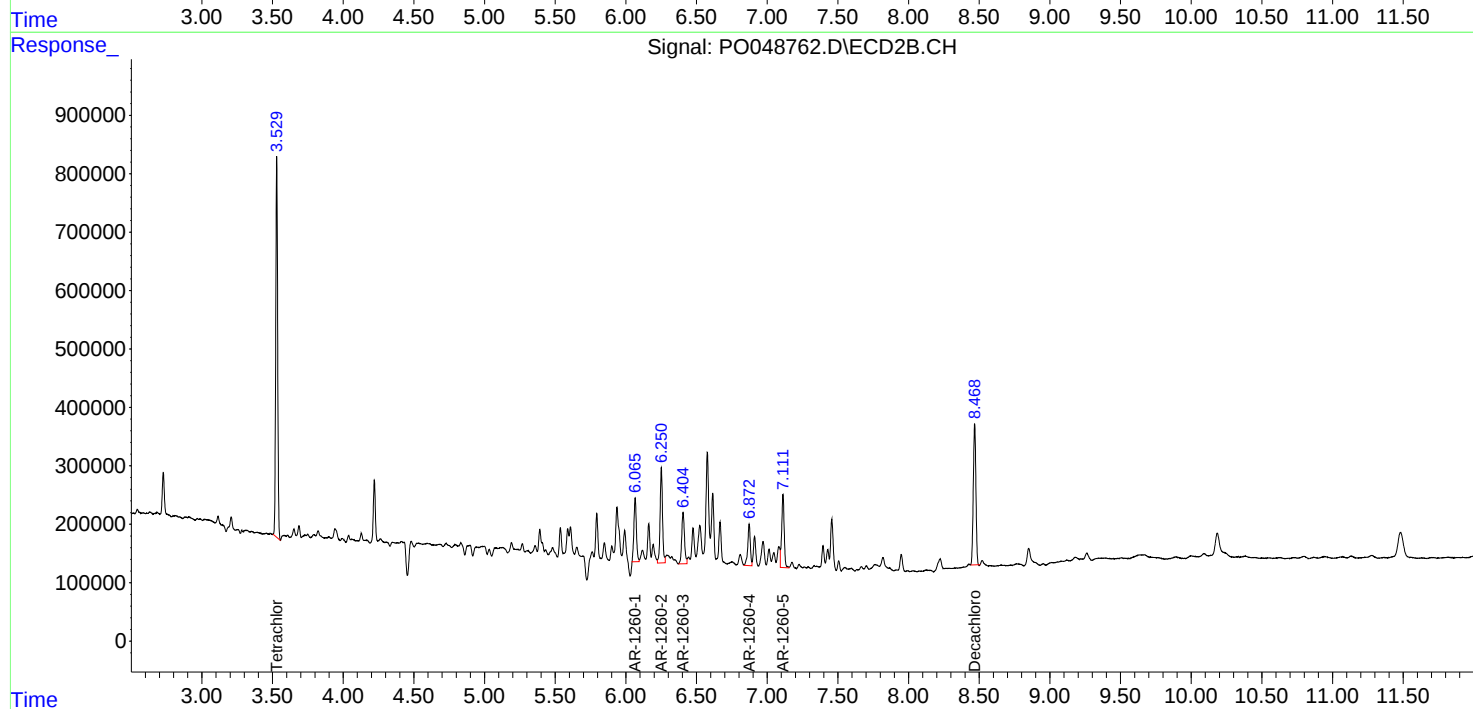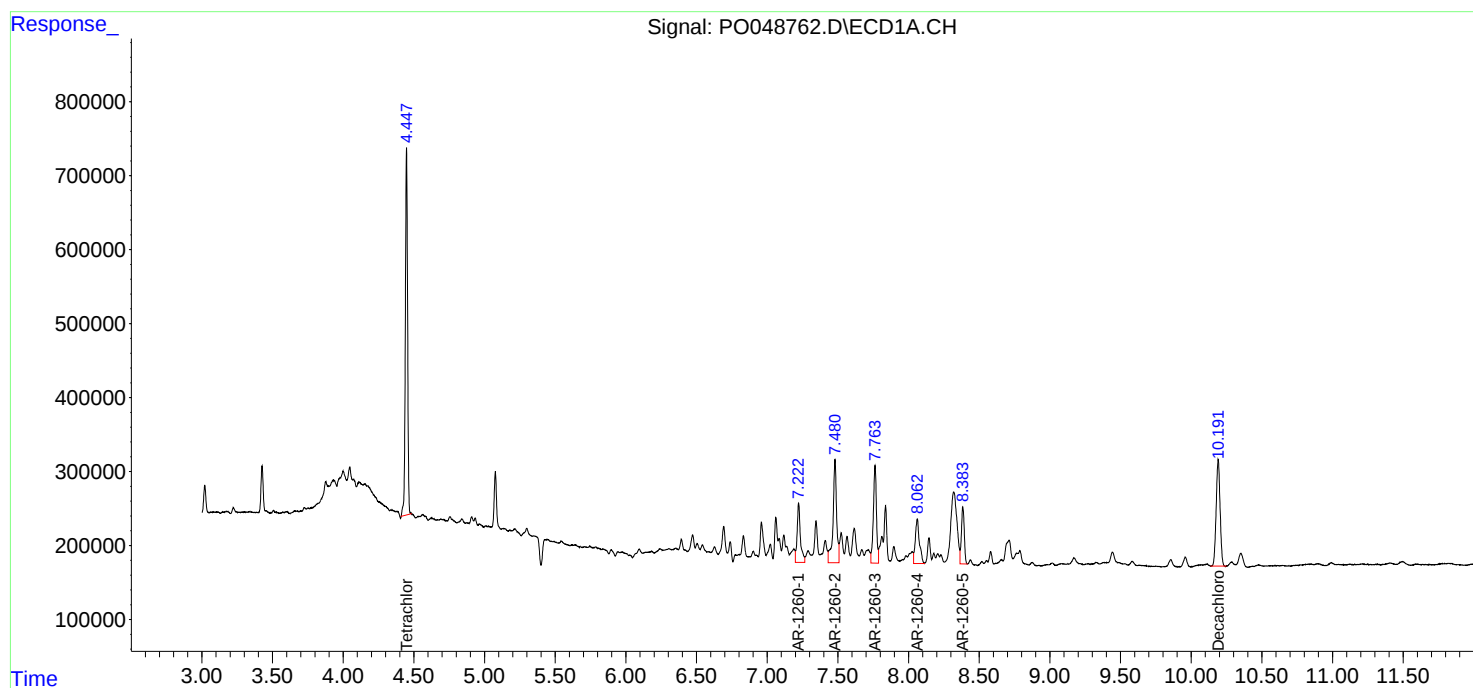

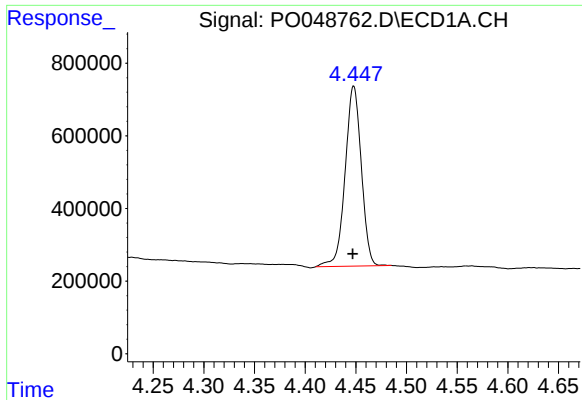


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 5500087
Conc: 45.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-3


Manual Integrations
APPROVED

Sohil
9/6/2018 2:21:31 PM

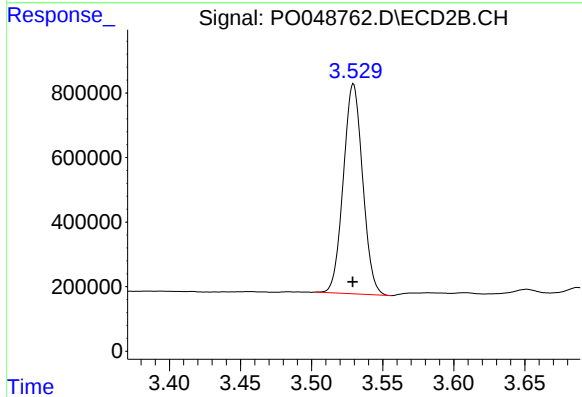


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 6147895
Conc: 39.33 ng/ml

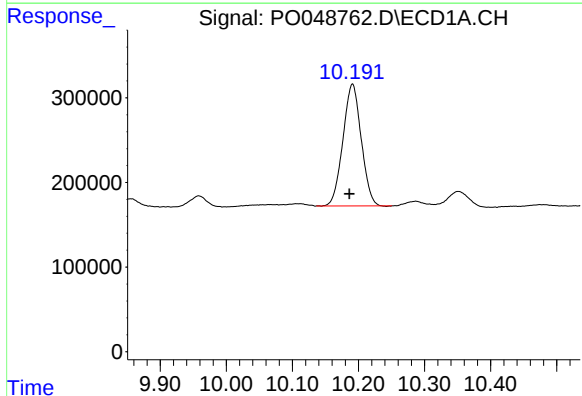


#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: 0.005 min
Response: 2768825
Conc: 19.84 ng/ml

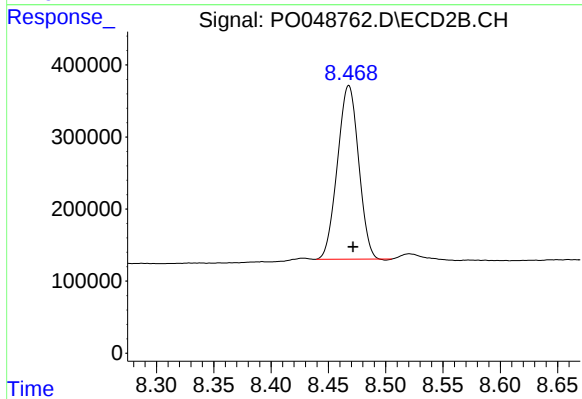

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: -0.004 min
Response: 3099291
Conc: 20.96 ng/ml

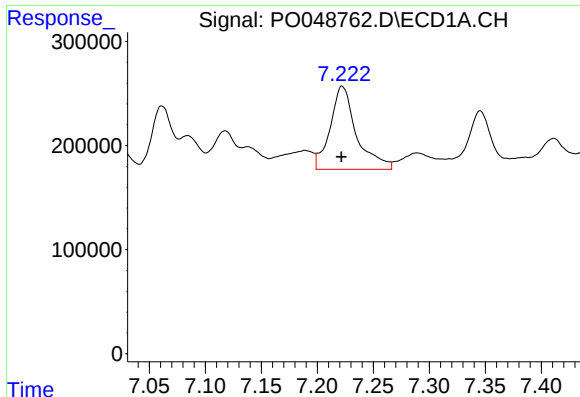


#31 AR-1260-1

R.T.: 7.223 min
Delta R.T.: 0.001 min
Response: 1308935
Conc: 158.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-3


Manual Integrations
APPROVED

Sohil
9/6/2018 2:21:31 PM

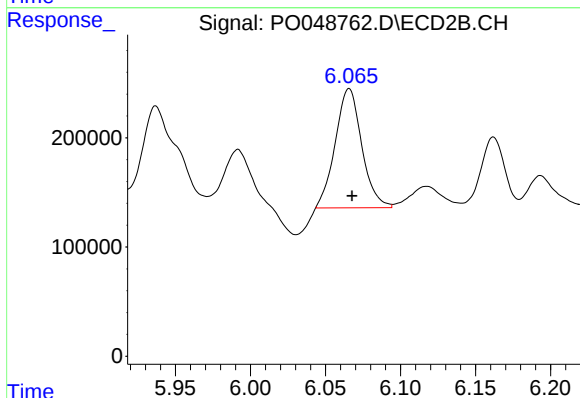


#31 AR-1260-1

R.T.: 6.065 min
Delta R.T.: -0.002 min
Response: 1347242
Conc: 129.42 ng/ml m

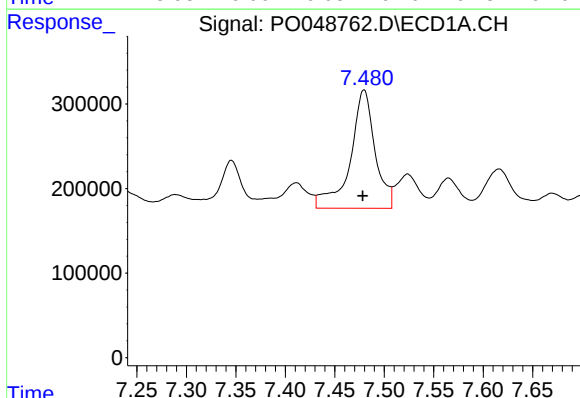


#32 AR-1260-2

R.T.: 7.480 min
Delta R.T.: 0.001 min
Response: 2443764
Conc: 248.69 ng/ml

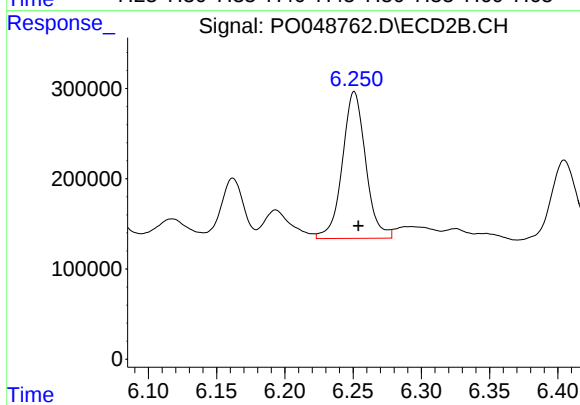

#32 AR-1260-2

R.T.: 6.250 min
Delta R.T.: -0.003 min
Response: 1938381
Conc: 154.79 ng/ml m

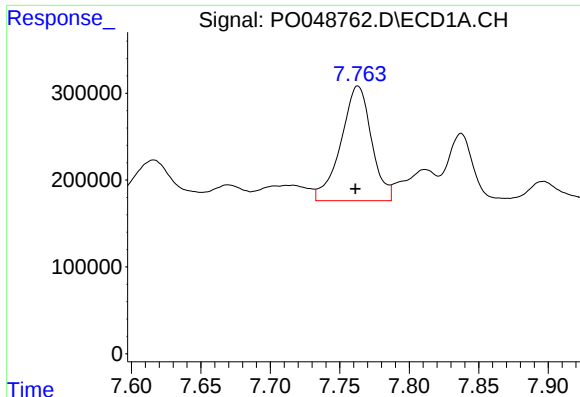


#33 AR-1260-3

R.T.: 7.763 min
Delta R.T.: 0.002 min
Response: 2026599
Conc: 169.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-3


Manual Integrations
APPROVED

Sohil
9/6/2018 2:21:31 PM

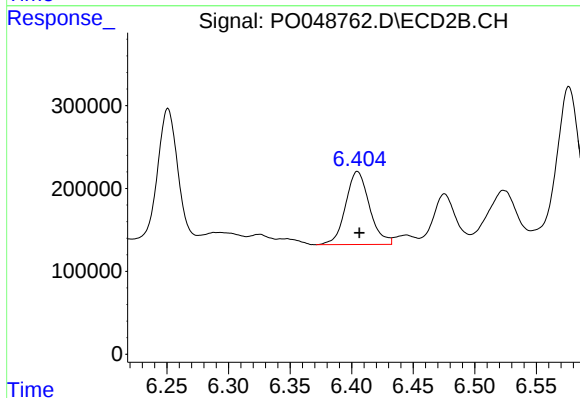


#33 AR-1260-3

R.T.: 6.405 min
Delta R.T.: -0.001 min
Response: 1189705
Conc: 100.28 ng/ml

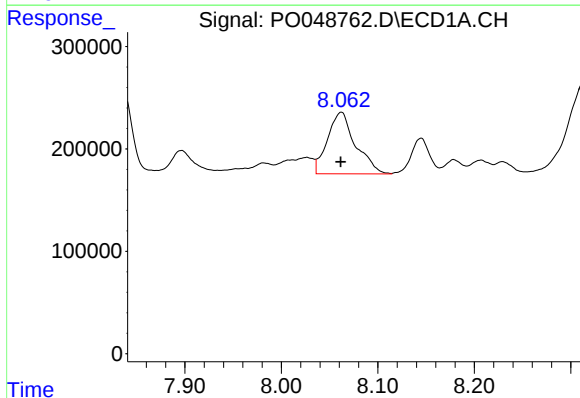


#34 AR-1260-4

R.T.: 8.062 min
Delta R.T.: 0.000 min
Response: 1214179
Conc: 141.46 ng/ml

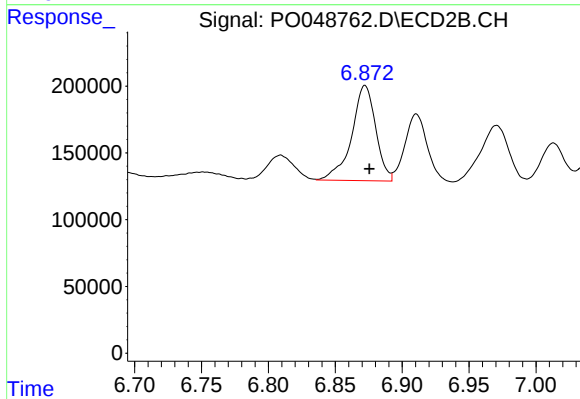

#34 AR-1260-4

R.T.: 6.872 min
Delta R.T.: -0.003 min
Response: 893381
Conc: 94.43 ng/ml

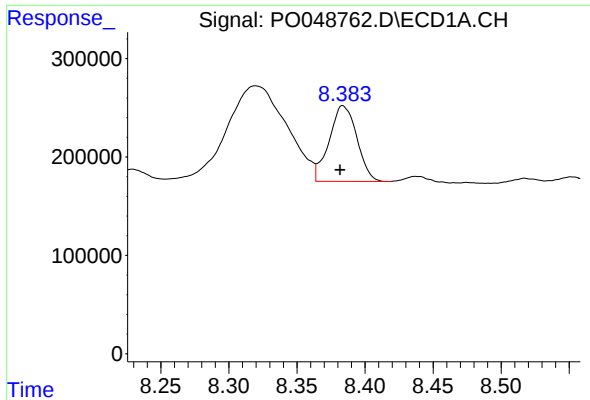


#35 AR-1260-5

R.T.: 8.384 min
Delta R.T.: 0.003 min
Response: 1092806
Conc: 65.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-3

Manual Integrations
APPROVED

Sohil
9/6/2018 2:21:31 PM

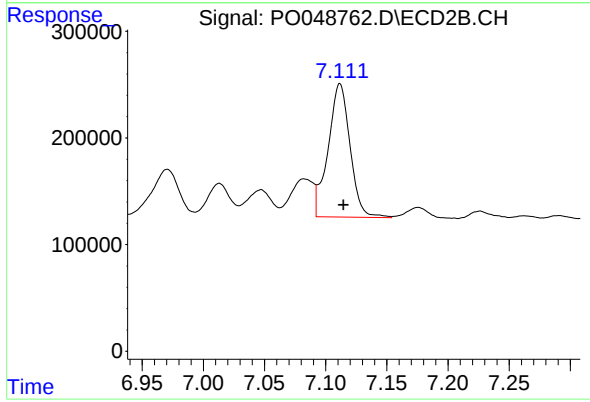

#35 AR-1260-5

R.T.: 7.112 min
Delta R.T.: -0.003 min
Response: 1561531
Conc: 71.91 ng/ml