

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090519\
 Data File : P0060380.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2019 11:47
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 9/6/2019 2:33:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 12:51:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 05 12:44:29 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.105	3.485	804062	727512	22.965	20.211
2) SA Decachlor...	9.549	8.332	1223527	895854	22.999m	22.218m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090519\
Data File : PO060380.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2019 11:47
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
9/6/2019 2:33:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 12:51:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 05 12:44:29 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

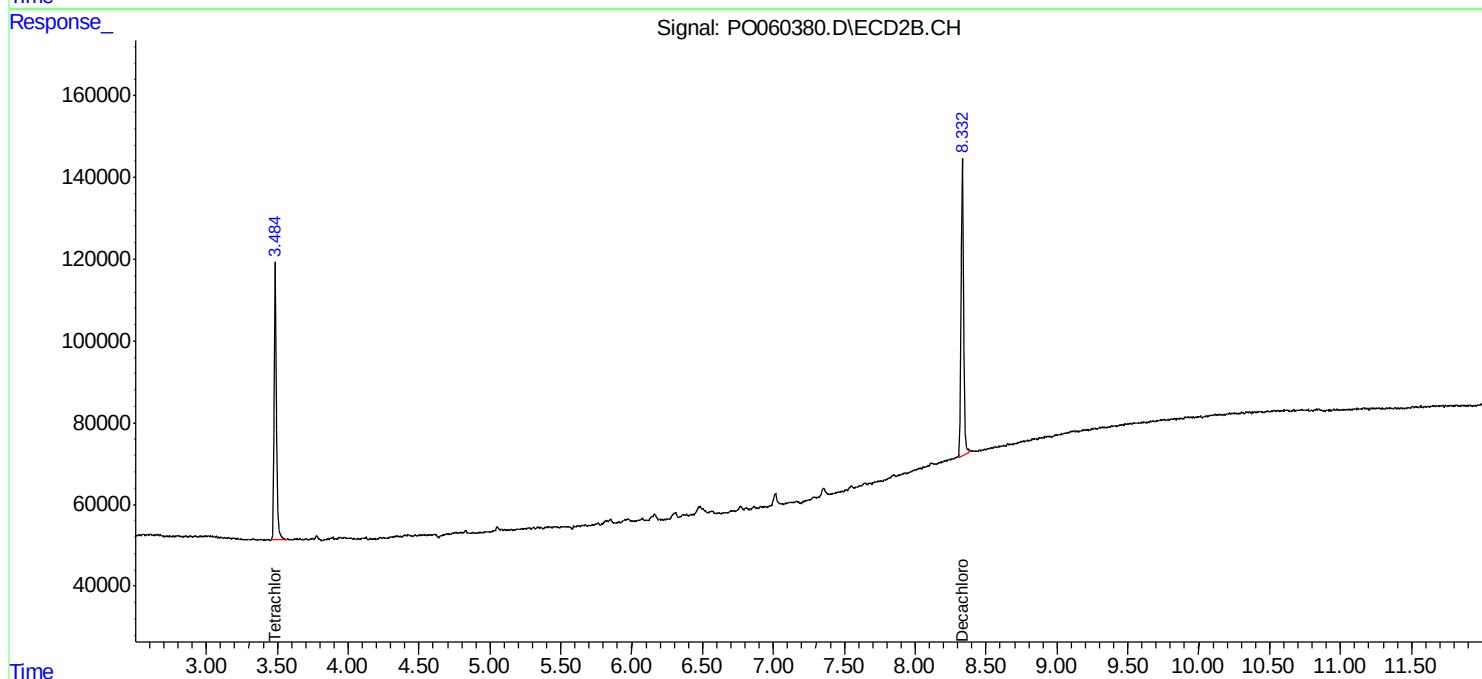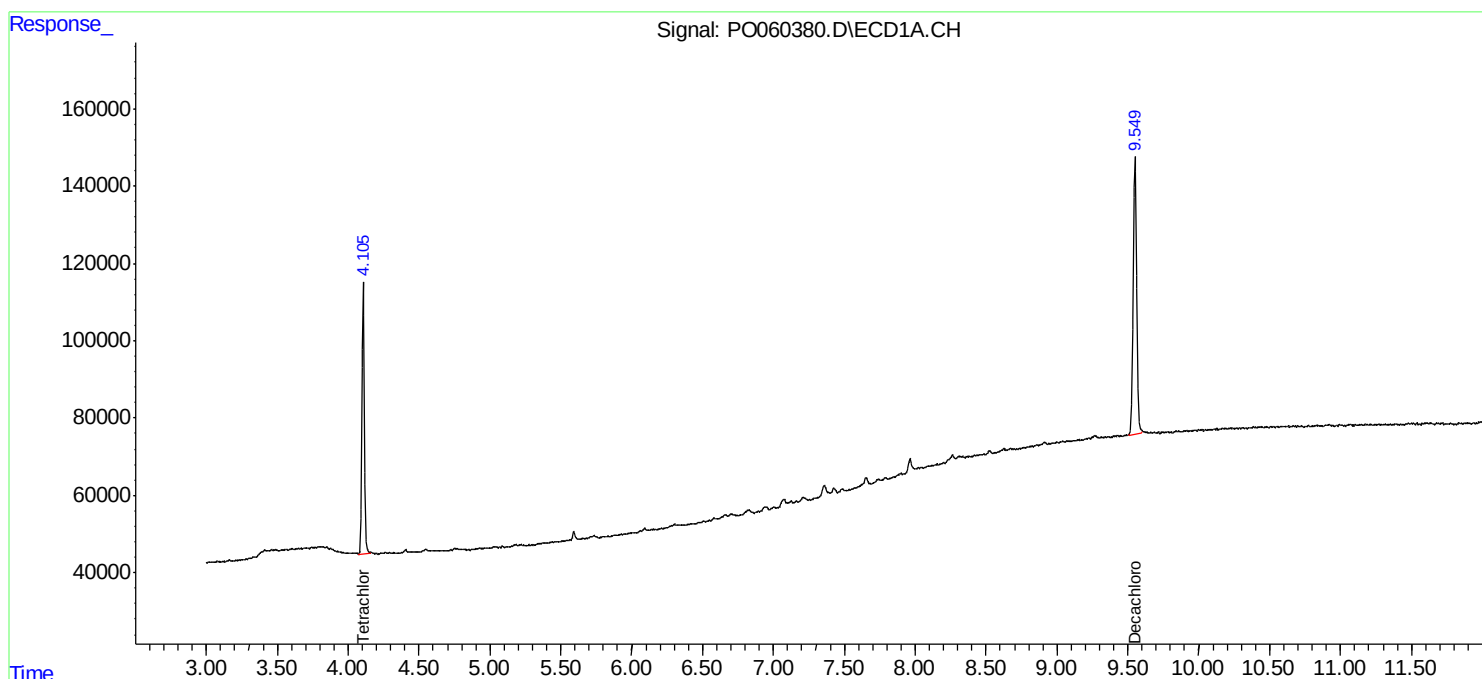

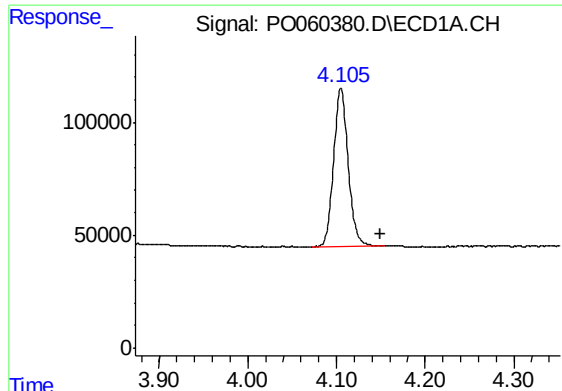


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: -0.045 min
Response: 804062
Conc: 22.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
9/6/2019 2:33:28 PM

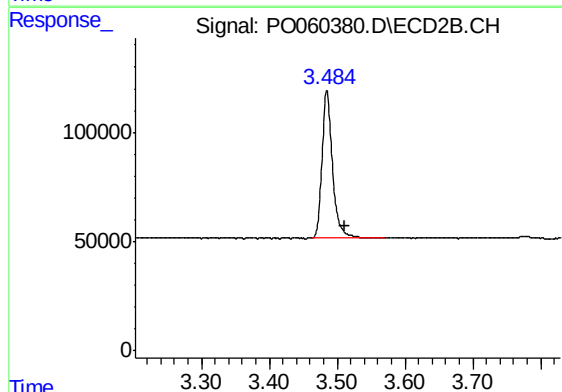


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: -0.025 min
Response: 727512
Conc: 20.21 ng/ml

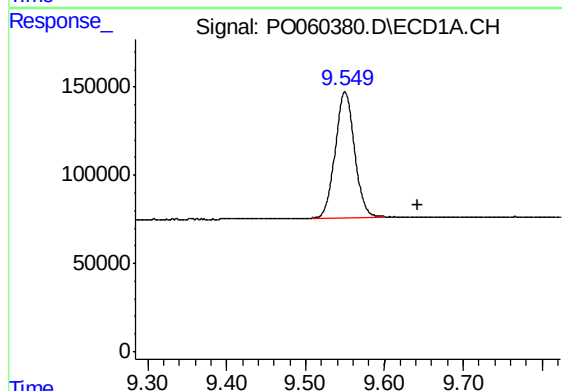

#2 Decachlorobiphenyl

R.T.: 9.549 min
Delta R.T.: -0.093 min
Response: 1223527
Conc: 23.00 ng/ml m

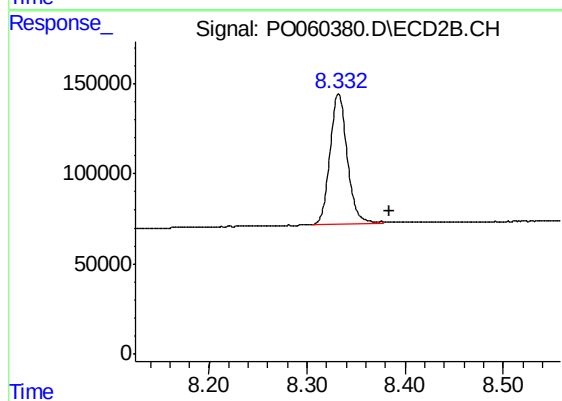

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.052 min
Response: 895854
Conc: 22.22 ng/ml m