

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090519\
 Data File : P0060385.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2019 13:30
 Operator : SM/AJ
 Sample : K4655-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-15-S

Manual Integrations
 APPROVED

Ankita
 9/6/2019 4:25:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 11:27:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 05 17:14:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.106	3.486	1154540	961747	32.975m	26.718
2)	SA Decachlor...	9.551	8.334	1281761	929844	24.093m	23.061m
Target Compounds							
26)	L6 AR-1254-1	6.091	5.331	69219	46543	33.176m	19.623m#
27)	L6 AR-1254-2	6.306	5.478	132456	42439	39.702	20.225m#
28)	L6 AR-1254-3	6.676	5.866	170890	76624	48.159m	22.788m#
29)	L6 AR-1254-4	6.950	6.077	84785	48457	28.784m	23.502m
30)	L6 AR-1254-5	7.362	6.484	163318	137246	52.813m	44.202m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090519\
Data File : PO060385.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2019 13:30
Operator : SM/AJ
Sample : K4655-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-15-S


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 11:27:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 05 17:14:47 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

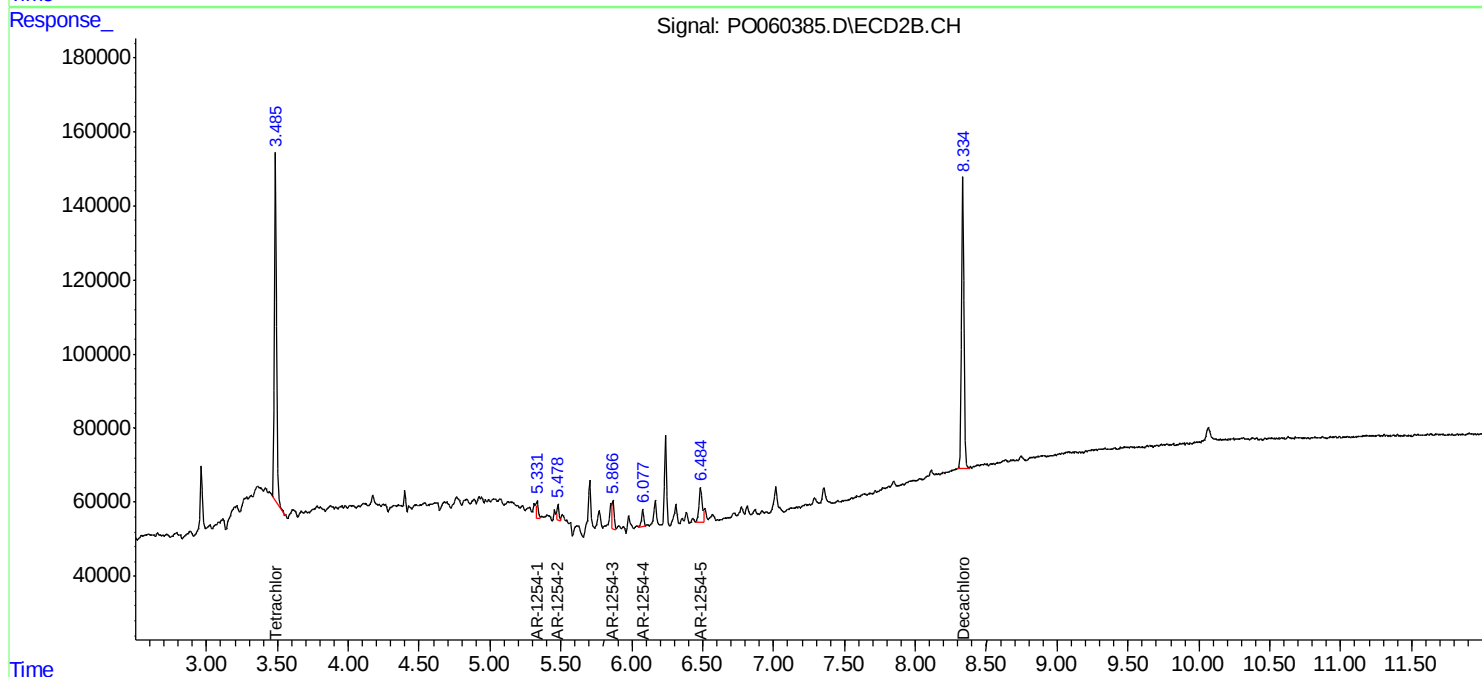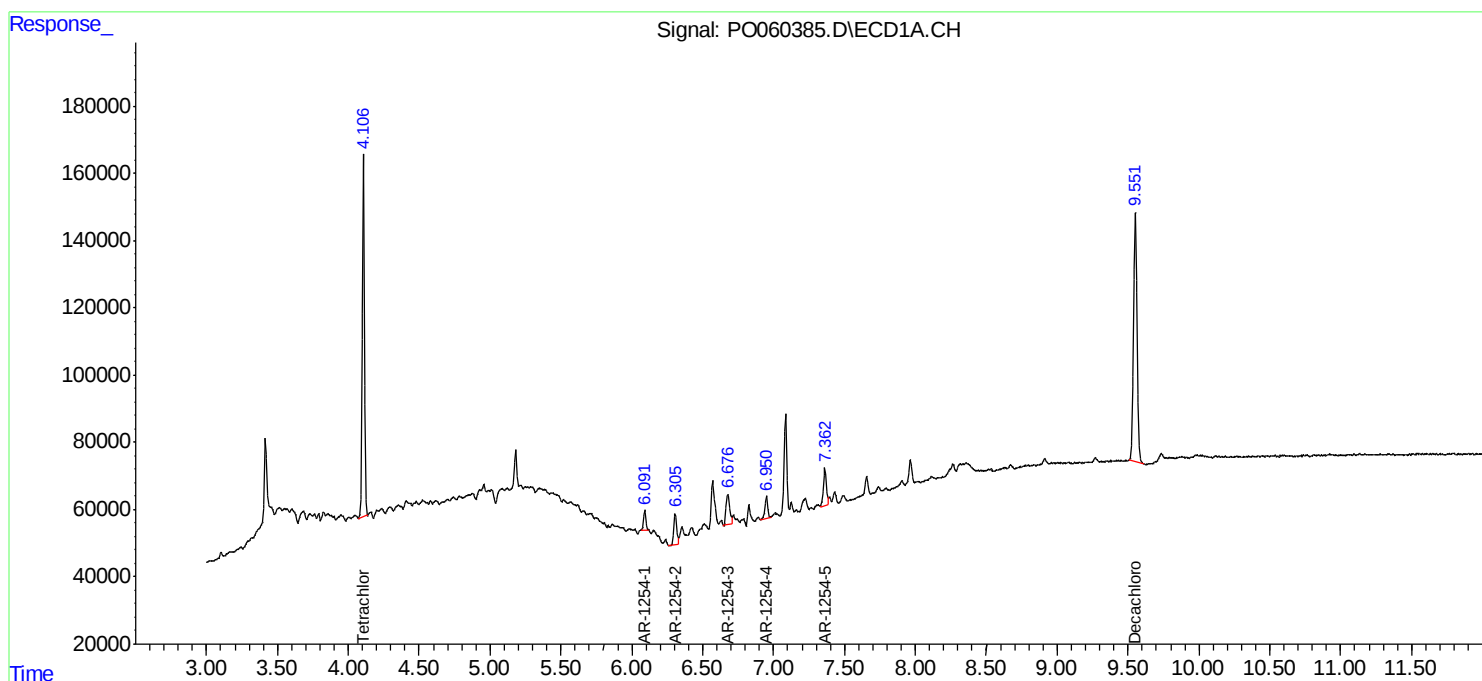

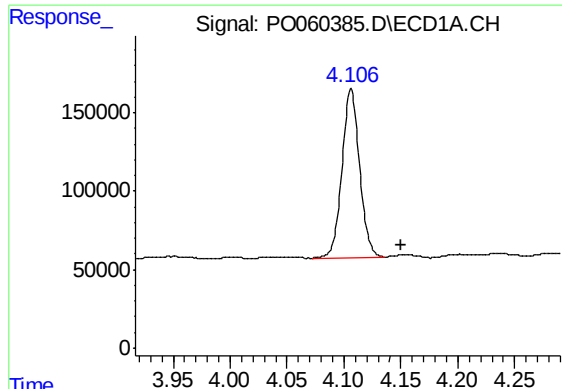


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.044 min
Response: 1154540
Conc: 32.98 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:40 PM

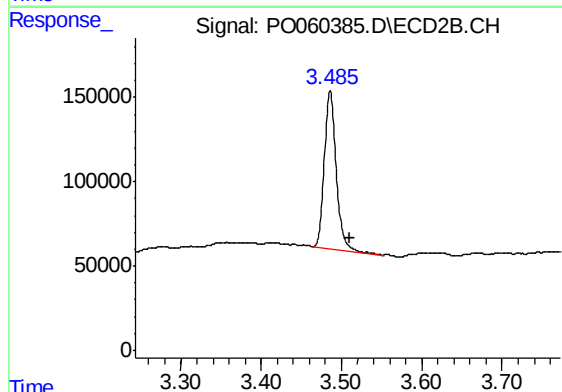


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.024 min
Response: 961747
Conc: 26.72 ng/ml

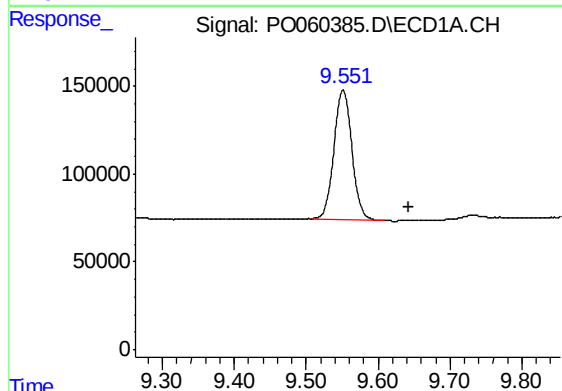


#2 Decachlorobiphenyl

R.T.: 9.551 min
Delta R.T.: -0.091 min
Response: 1281761
Conc: 24.09 ng/ml m

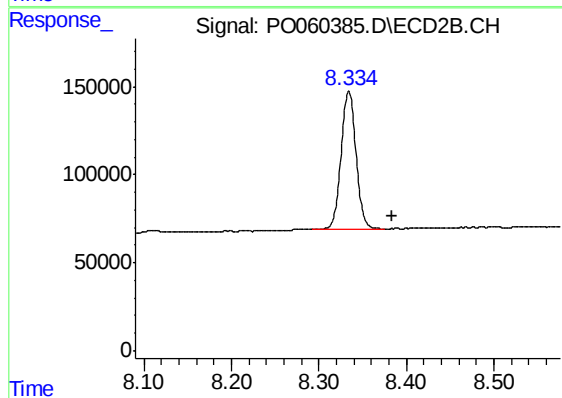

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.051 min
Response: 929844
Conc: 23.06 ng/ml m

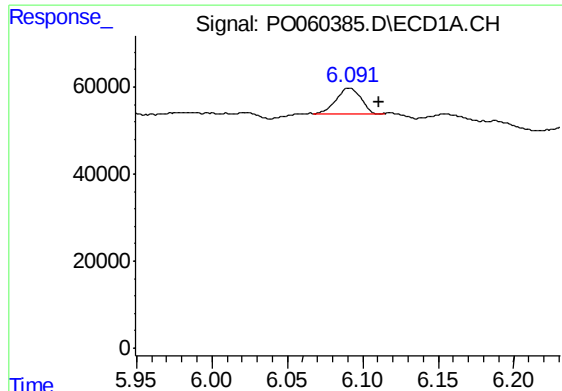


#26 AR-1254-1

R.T.: 6.091 min
Delta R.T.: -0.019 min
Response: 69219
Conc: 33.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:40 PM

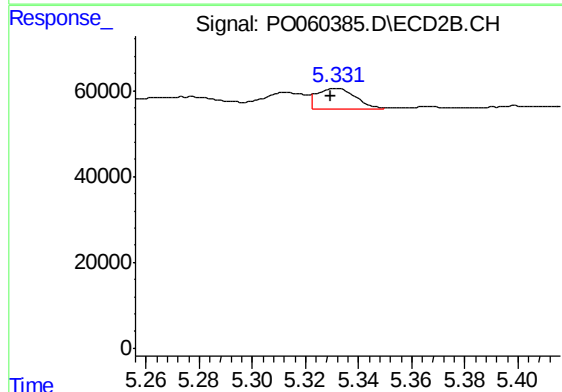


#26 AR-1254-1

R.T.: 5.331 min
Delta R.T.: 0.002 min
Response: 46543
Conc: 19.62 ng/ml m

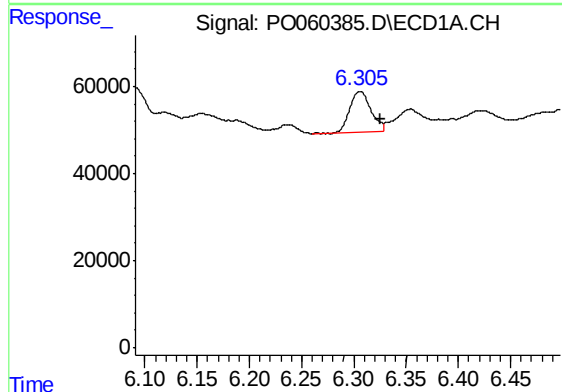


#27 AR-1254-2

R.T.: 6.306 min
Delta R.T.: -0.019 min
Response: 132456
Conc: 39.70 ng/ml

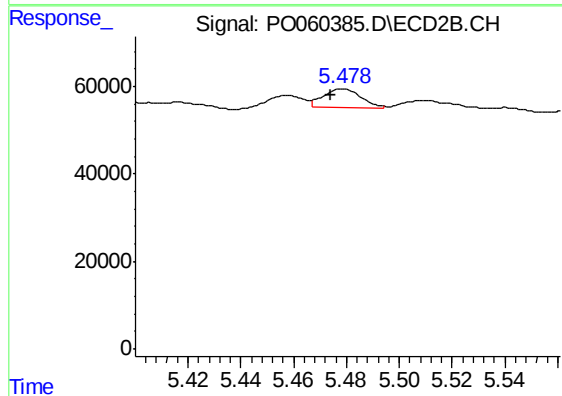

#27 AR-1254-2

R.T.: 5.478 min
Delta R.T.: 0.005 min
Response: 42439
Conc: 20.23 ng/ml m

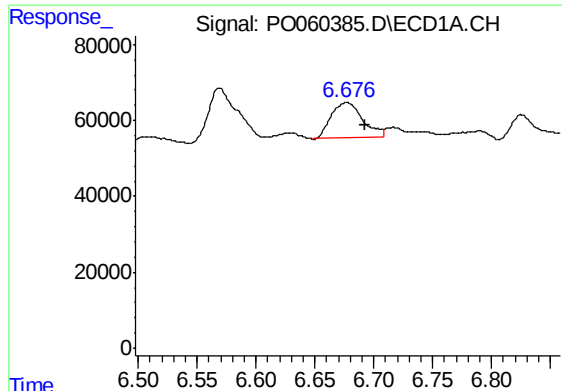


#28 AR-1254-3

R.T.: 6.676 min
Delta R.T.: -0.016 min
Response: 170890
Conc: 48.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:40 PM

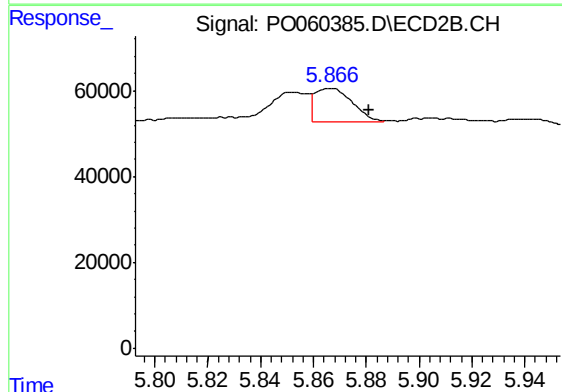


#28 AR-1254-3

R.T.: 5.866 min
Delta R.T.: -0.015 min
Response: 76624
Conc: 22.79 ng/ml m

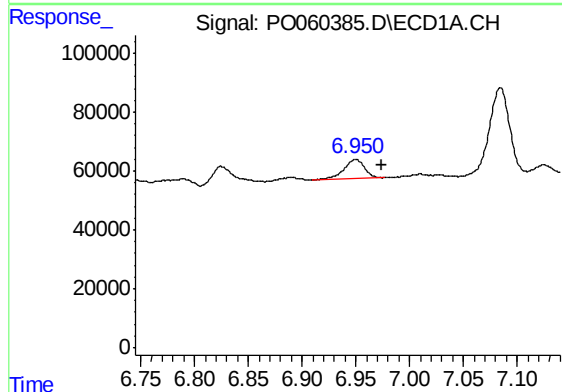


#29 AR-1254-4

R.T.: 6.950 min
Delta R.T.: -0.024 min
Response: 84785
Conc: 28.78 ng/ml m

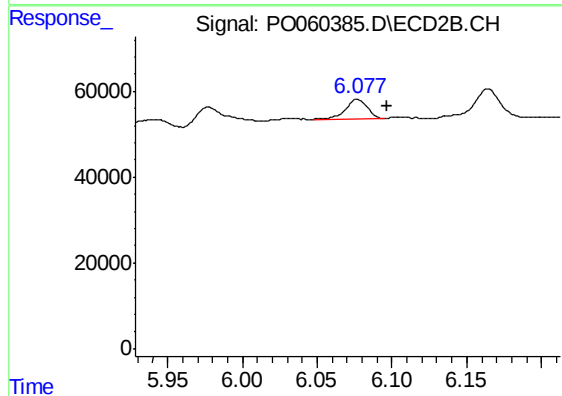

#29 AR-1254-4

R.T.: 6.077 min
Delta R.T.: -0.020 min
Response: 48457
Conc: 23.50 ng/ml m

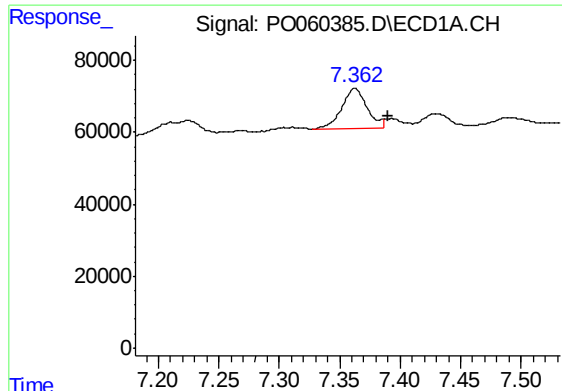


#30 AR-1254-5

R.T.: 7.362 min
Delta R.T.: -0.028 min
Response: 163318
Conc: 52.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-S

Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:40 PM

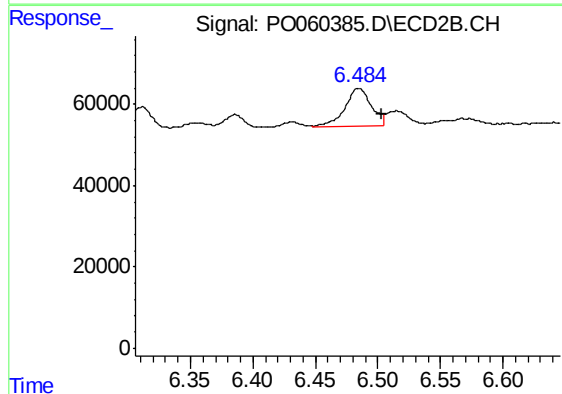

#30 AR-1254-5

R.T.: 6.484 min
Delta R.T.: -0.020 min
Response: 137246
Conc: 44.20 ng/ml m