

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090519\
 Data File : P0060386.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2019 13:47
 Operator : SM/AJ
 Sample : K4655-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-15-D

Manual Integrations
 APPROVED

Ankita
 9/6/2019 4:25:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 11:45:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 05 17:14:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.106	3.486	1308504	1088241	37.372m	30.233
2) SA Decachlor...	9.550	8.334	1368466	1011634	25.723m	25.089m
Target Compounds						
26) L6 AR-1254-1	6.094	5.333	335223	168997	160.669m	71.253m#
27) L6 AR-1254-2	6.303	5.478	203958	61960	61.134m	29.529m#
28) L6 AR-1254-3	6.667	5.850	212127	216010	59.780m	64.241m
29) L6 AR-1254-4	6.949	6.076	208239	119705	70.697m	58.058m
30) L6 AR-1254-5	7.363	6.484	329413	255977	106.523m	82.441m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090519\
Data File : PO060386.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2019 13:47
Operator : SM/AJ
Sample : K4655-07
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 11:45:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 05 17:14:47 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

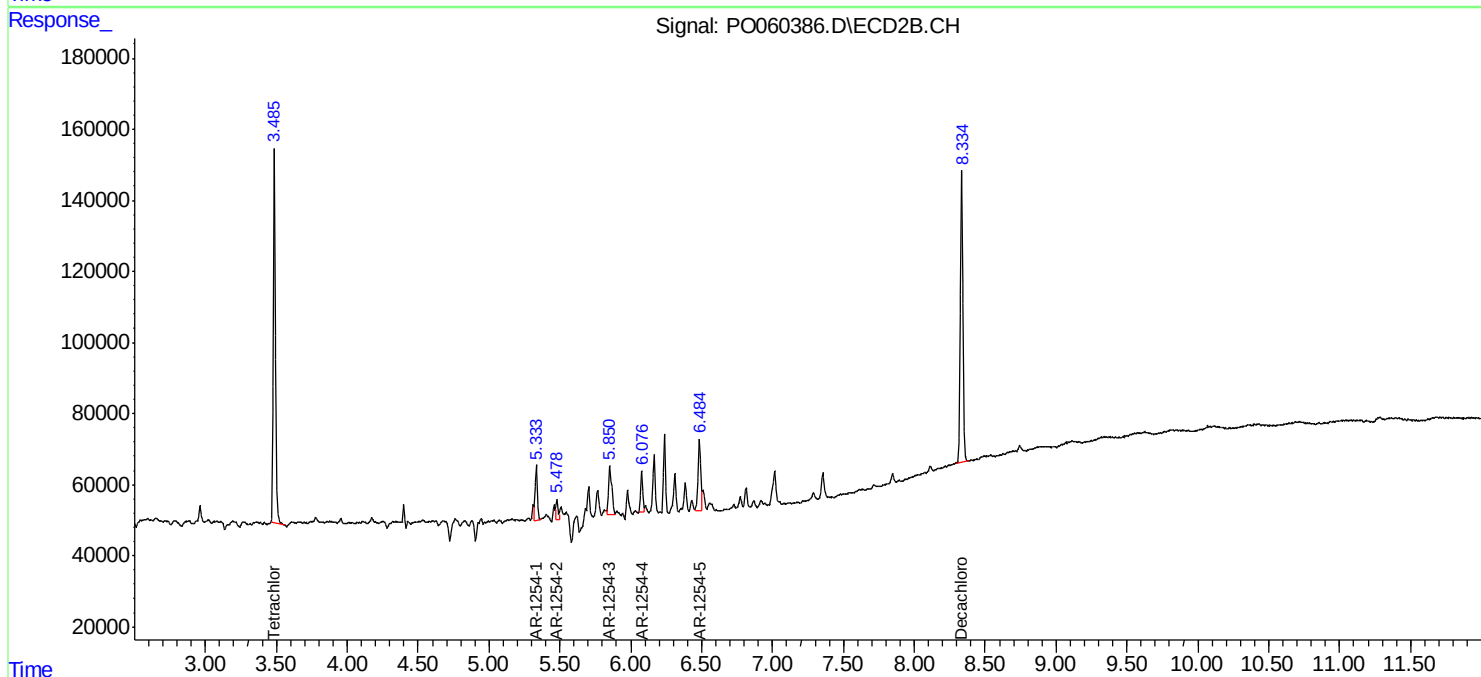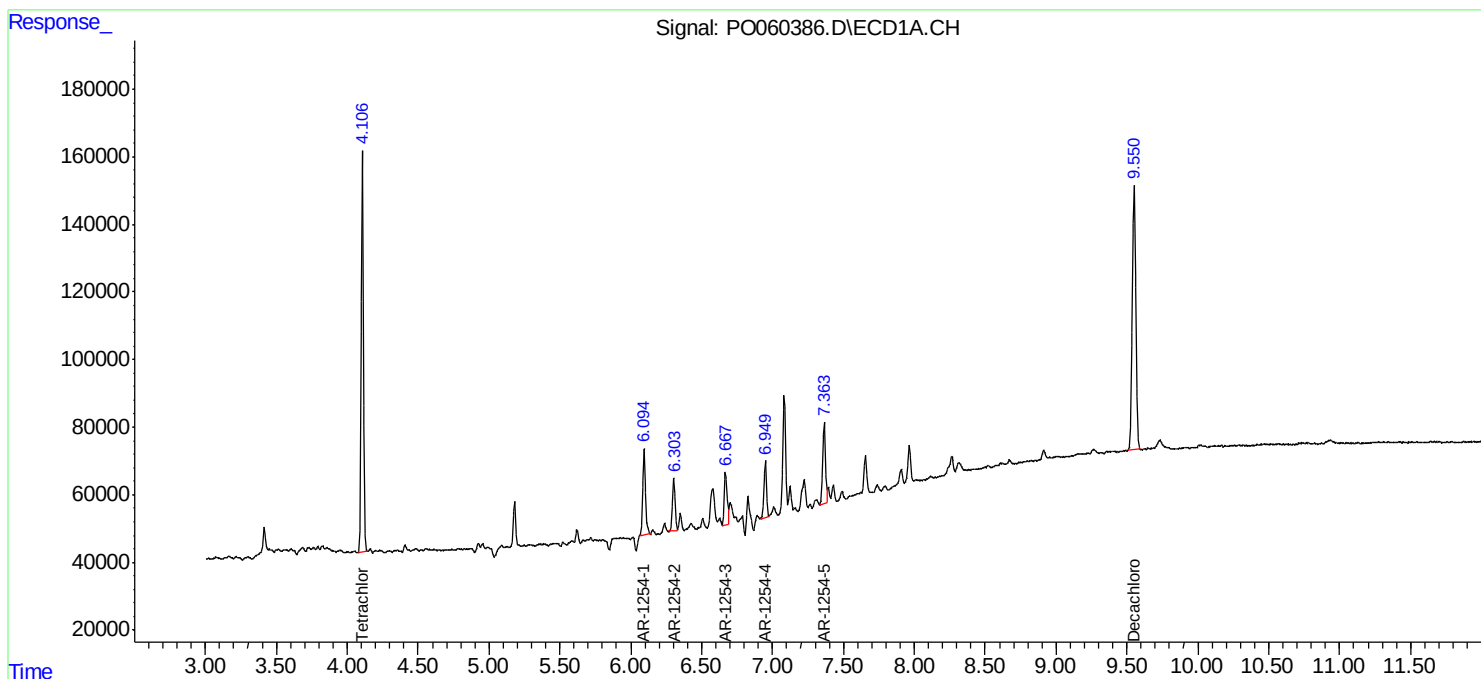

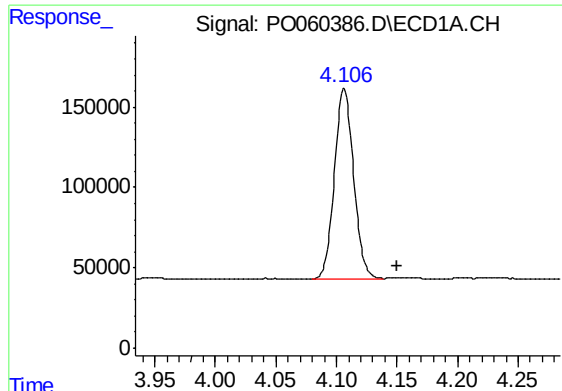


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.044 min
Response: 1308504
Conc: 37.37 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:42 PM

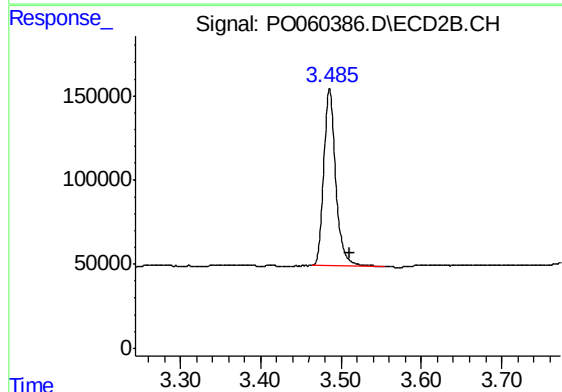


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.025 min
Response: 1088241
Conc: 30.23 ng/ml

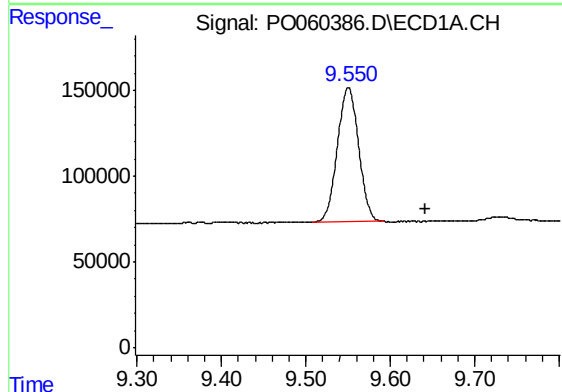


#2 Decachlorobiphenyl

R.T.: 9.550 min
Delta R.T.: -0.092 min
Response: 1368466
Conc: 25.72 ng/ml m

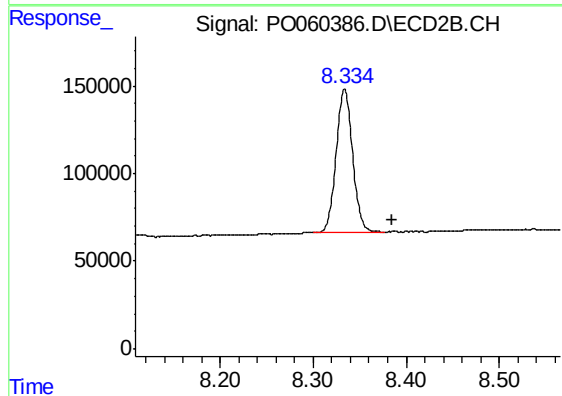

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.051 min
Response: 1011634
Conc: 25.09 ng/ml m

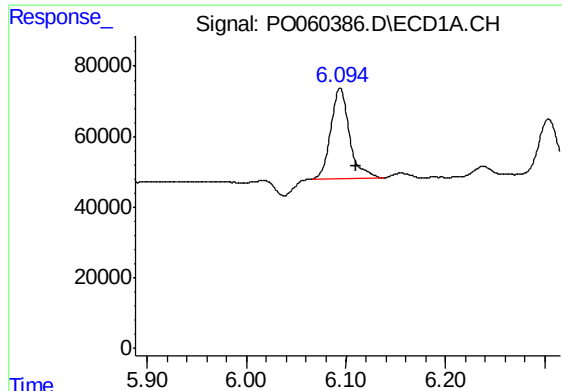


#26 AR-1254-1

R.T.: 6.094 min
Delta R.T.: -0.017 min
Response: 335223
Conc: 160.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:42 PM

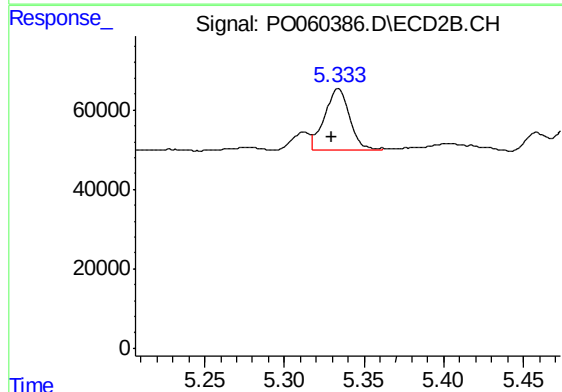


#26 AR-1254-1

R.T.: 5.333 min
Delta R.T.: 0.004 min
Response: 168997
Conc: 71.25 ng/ml m

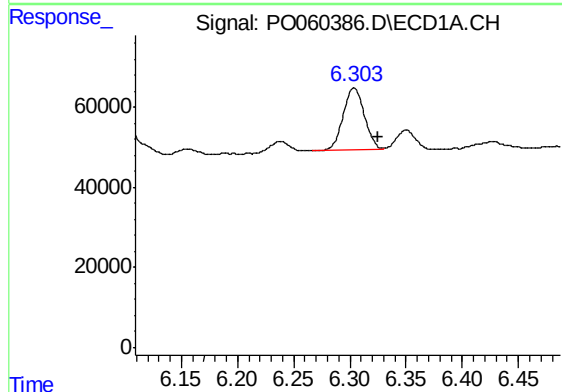


#27 AR-1254-2

R.T.: 6.303 min
Delta R.T.: -0.022 min
Response: 203958
Conc: 61.13 ng/ml m

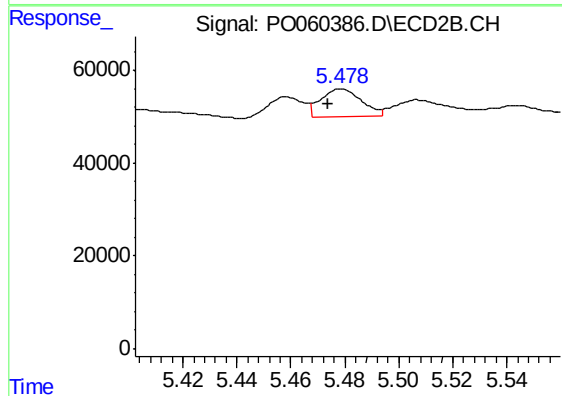

#27 AR-1254-2

R.T.: 5.478 min
Delta R.T.: 0.004 min
Response: 61960
Conc: 29.53 ng/ml m

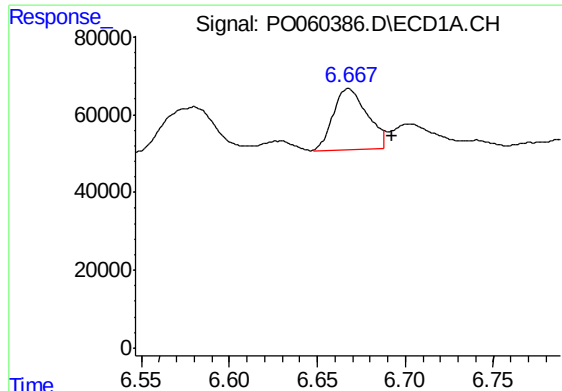


#28 AR-1254-3

R.T.: 6.667 min
Delta R.T.: -0.025 min
Response: 212127
Conc: 59.78 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:42 PM

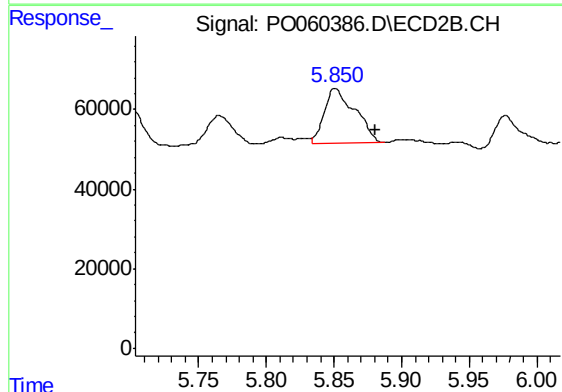


#28 AR-1254-3

R.T.: 5.850 min
Delta R.T.: -0.031 min
Response: 216010
Conc: 64.24 ng/ml m

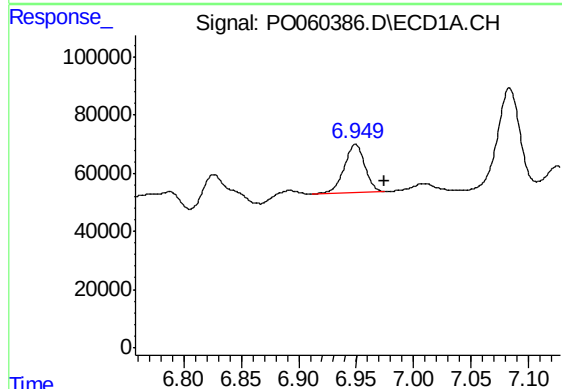


#29 AR-1254-4

R.T.: 6.949 min
Delta R.T.: -0.025 min
Response: 208239
Conc: 70.70 ng/ml m

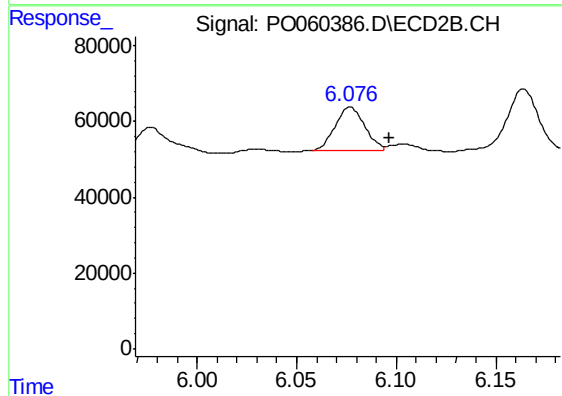

#29 AR-1254-4

R.T.: 6.076 min
Delta R.T.: -0.020 min
Response: 119705
Conc: 58.06 ng/ml m

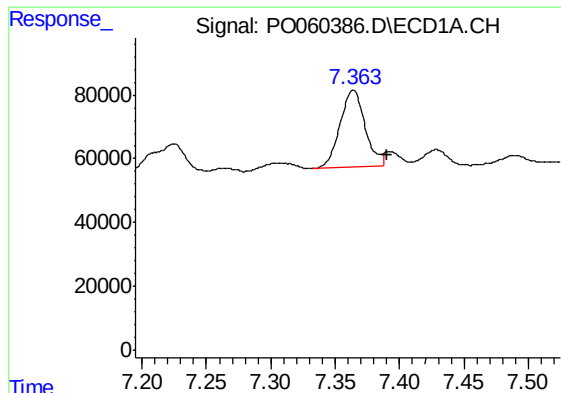


#30 AR-1254-5

R.T.: 7.363 min
Delta R.T.: -0.027 min
Response: 329413
Conc: 106.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-D

Manual Integrations
APPROVED

Ankita
9/6/2019 4:25:42 PM

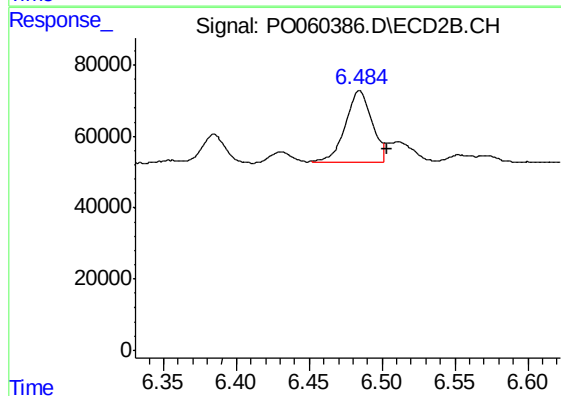

#30 AR-1254-5

R.T.: 6.484 min
Delta R.T.: -0.019 min
Response: 255977
Conc: 82.44 ng/ml m