

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090519\
 Data File : P0060406.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2019 19:48
 Operator : SM/AJ
 Sample : K4679-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WS-SB11-COMP

Manual Integrations
 APPROVED

Ankita
 9/6/2019 2:34:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 01:37:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 05 17:14:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.101	3.485	1076280	980100	30.740m	27.228
2)	SA Decachlor...	9.545	8.331	1162229	862954	21.846m	21.402m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090519\
Data File : P0060406.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2019 19:48
Operator : SM/AJ
Sample : K4679-08
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WS-SB11-COMP


Manual Integrations
APPROVED

Ankita
9/6/2019 2:34:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 01:37:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 05 17:14:47 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

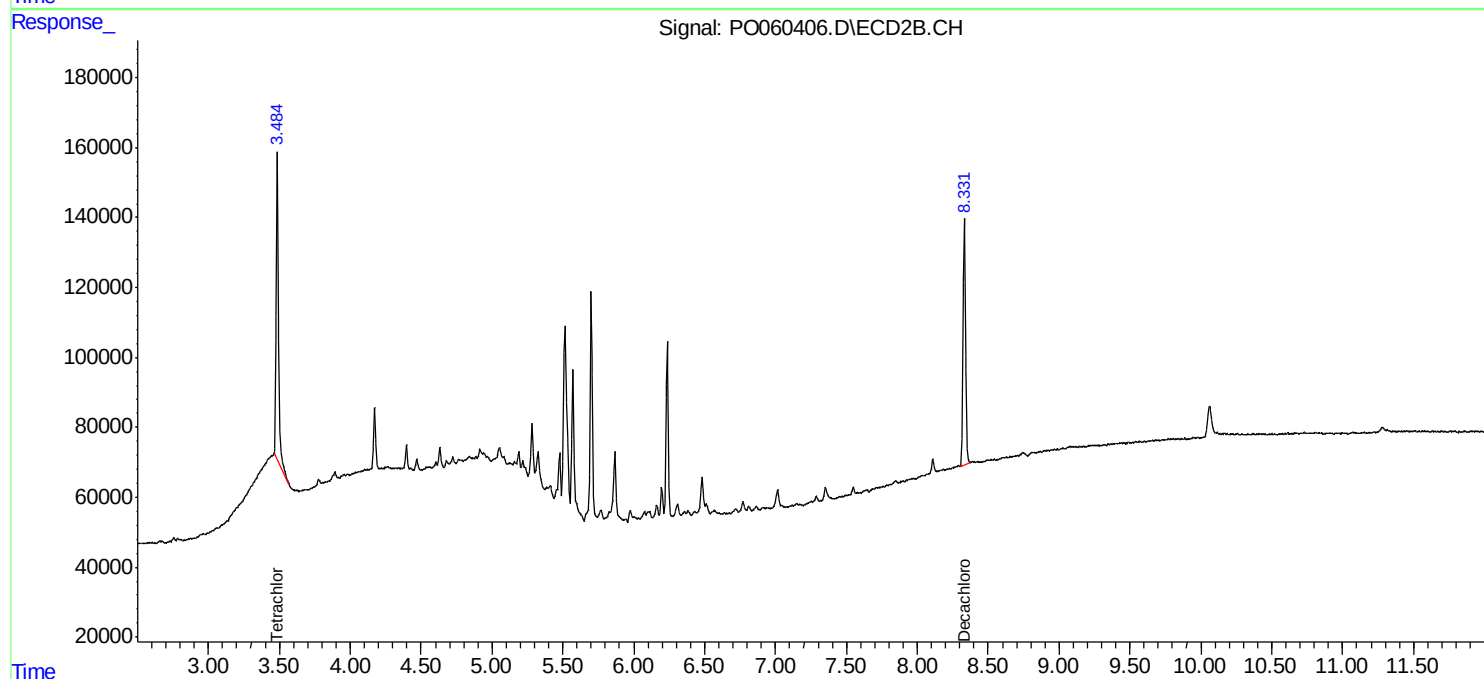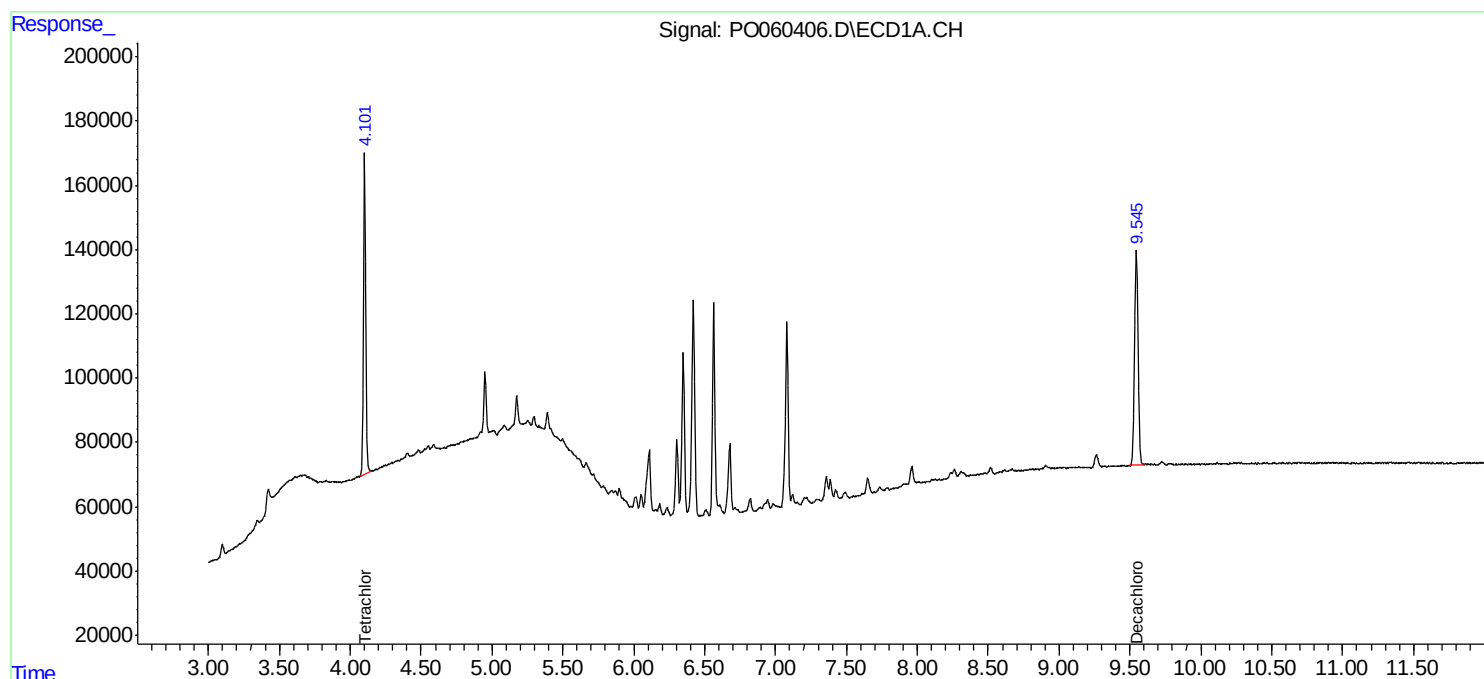

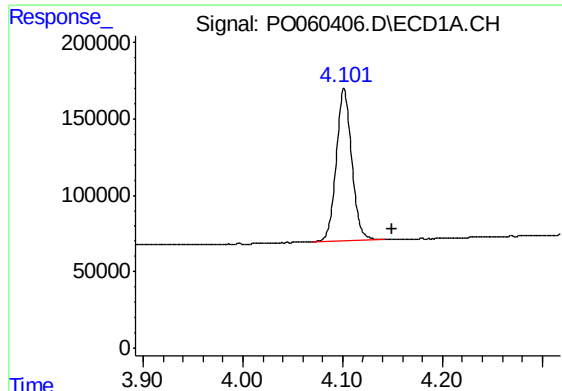


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.049 min
Response: 1076280
Conc: 30.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
WS-SB11-COMP


Manual Integrations
APPROVED

Ankita
9/6/2019 2:34:58 PM

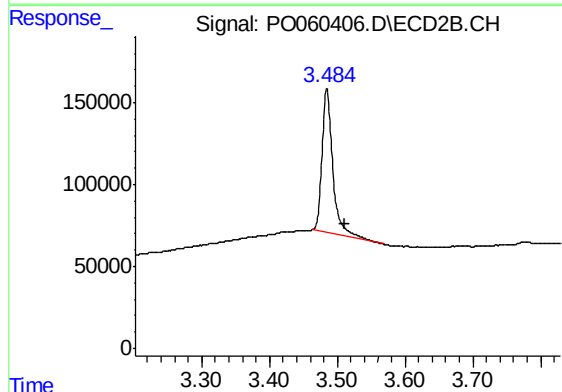


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: -0.026 min
Response: 980100
Conc: 27.23 ng/ml

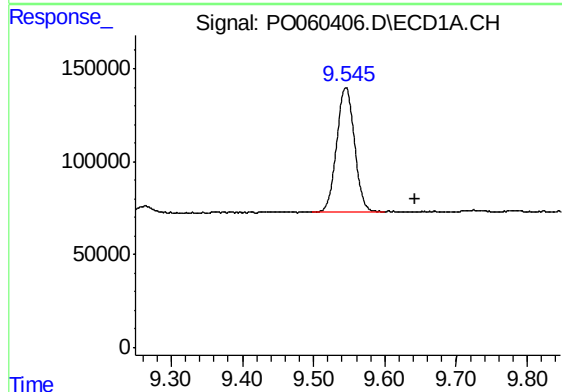

#2 Decachlorobiphenyl

R.T.: 9.545 min
Delta R.T.: -0.097 min
Response: 1162229
Conc: 21.85 ng/ml m

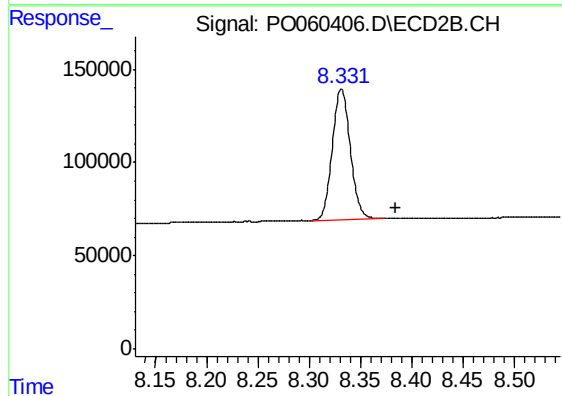

#2 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.053 min
Response: 862954
Conc: 21.40 ng/ml m