

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090524\
 Data File : P0106178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2024 13:39
 Operator : YP/AJ
 Sample : P3840-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1901

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/06/2024
 Supervised By :Ankita Jodhani 09/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 14:50:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.453	3.716	196.2E6	61684602	21.509	22.831m
2) SA Decachlor...	10.192	8.746	120.9E6	51766649	22.279	23.713

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090524\
Data File : PO106178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2024 13:39
Operator : YP/AJ
Sample : P3840-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1901


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2024
Supervised By :Ankita Jodhani 09/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 14:50:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

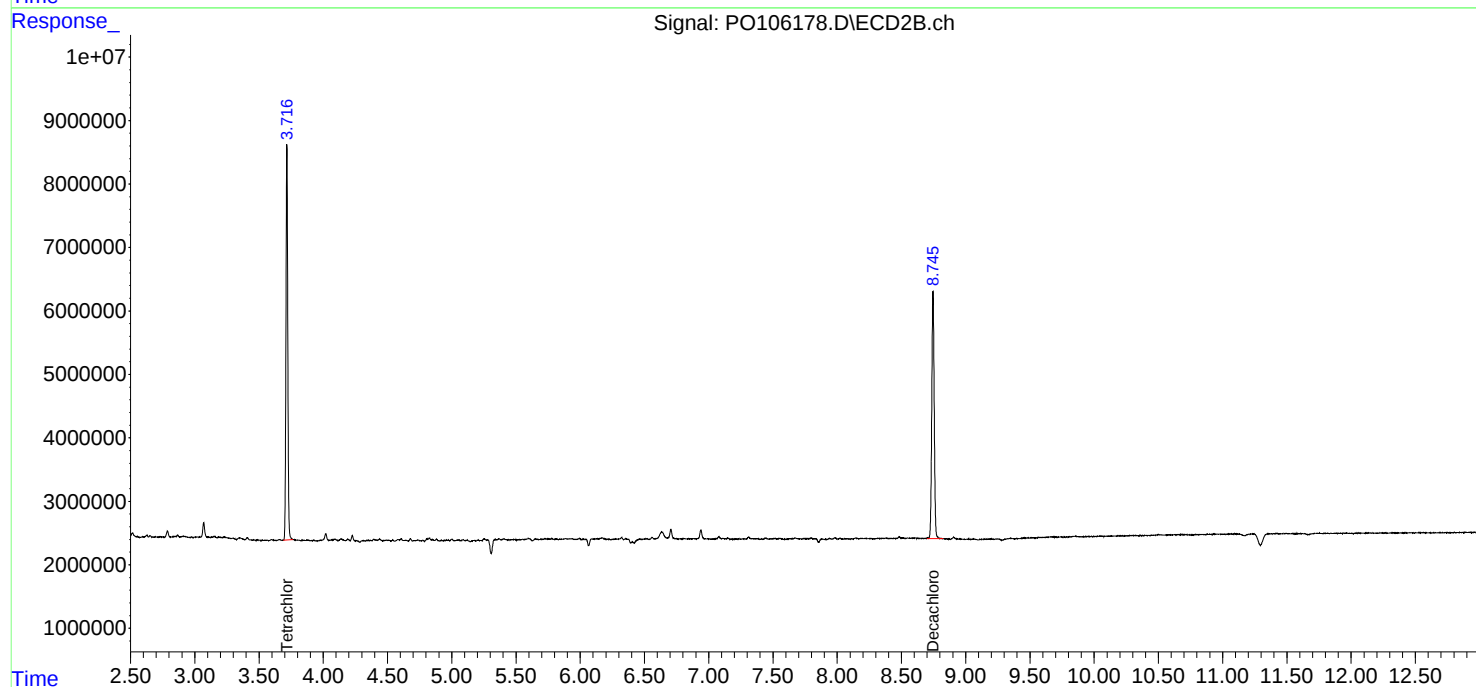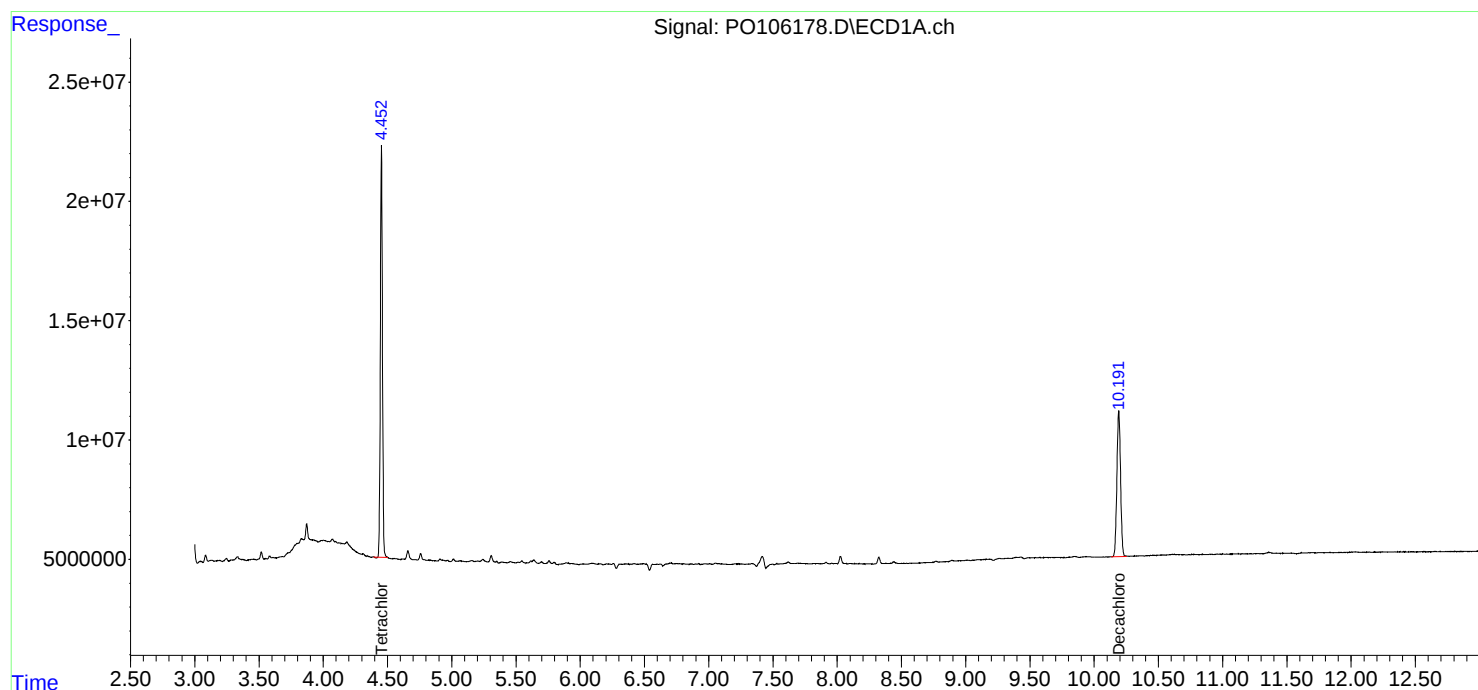

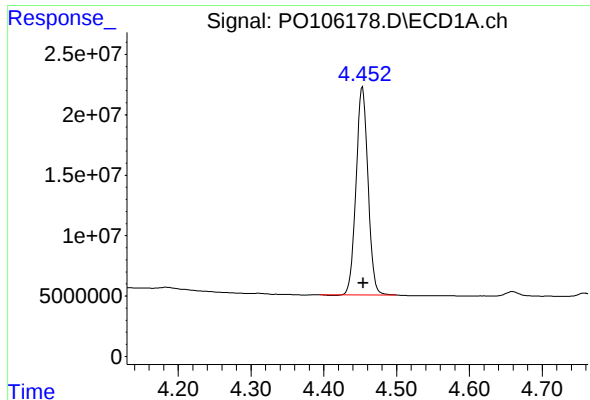


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 196230686
Conc: 21.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
1901


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2024
Supervised By :Ankita Jodhani 09/06/2024

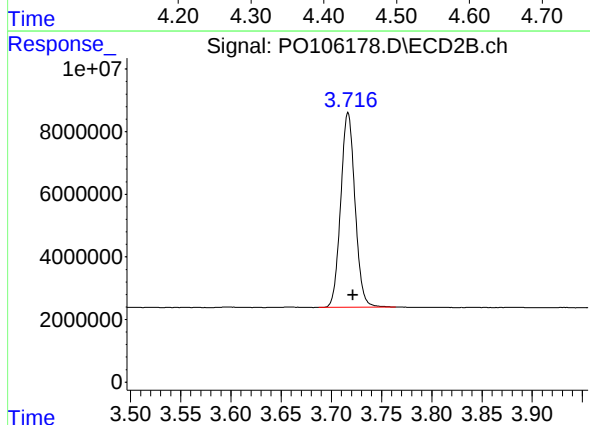


#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: -0.005 min
Response: 61684602
Conc: 22.83 ng/ml

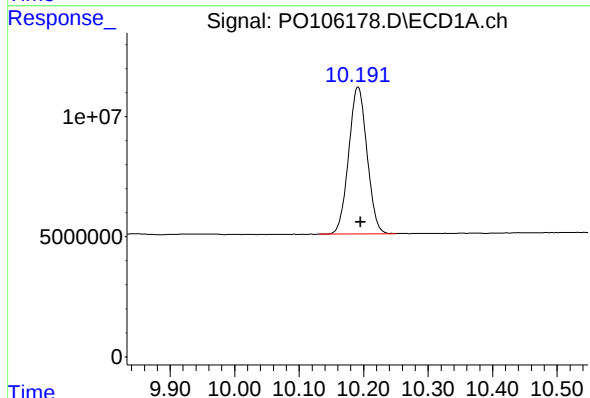

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.004 min
Response: 120908863
Conc: 22.28 ng/ml

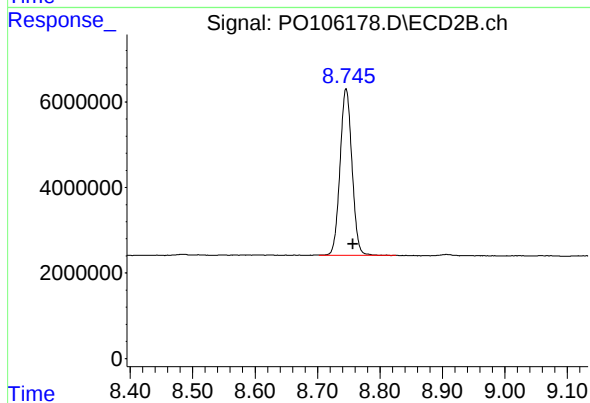

#2 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.011 min
Response: 51766649
Conc: 23.71 ng/ml